


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092018\
 Data File : BG036843.D
 Acq On : 20 Sep 2018 14:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 20 20:07:11 2018

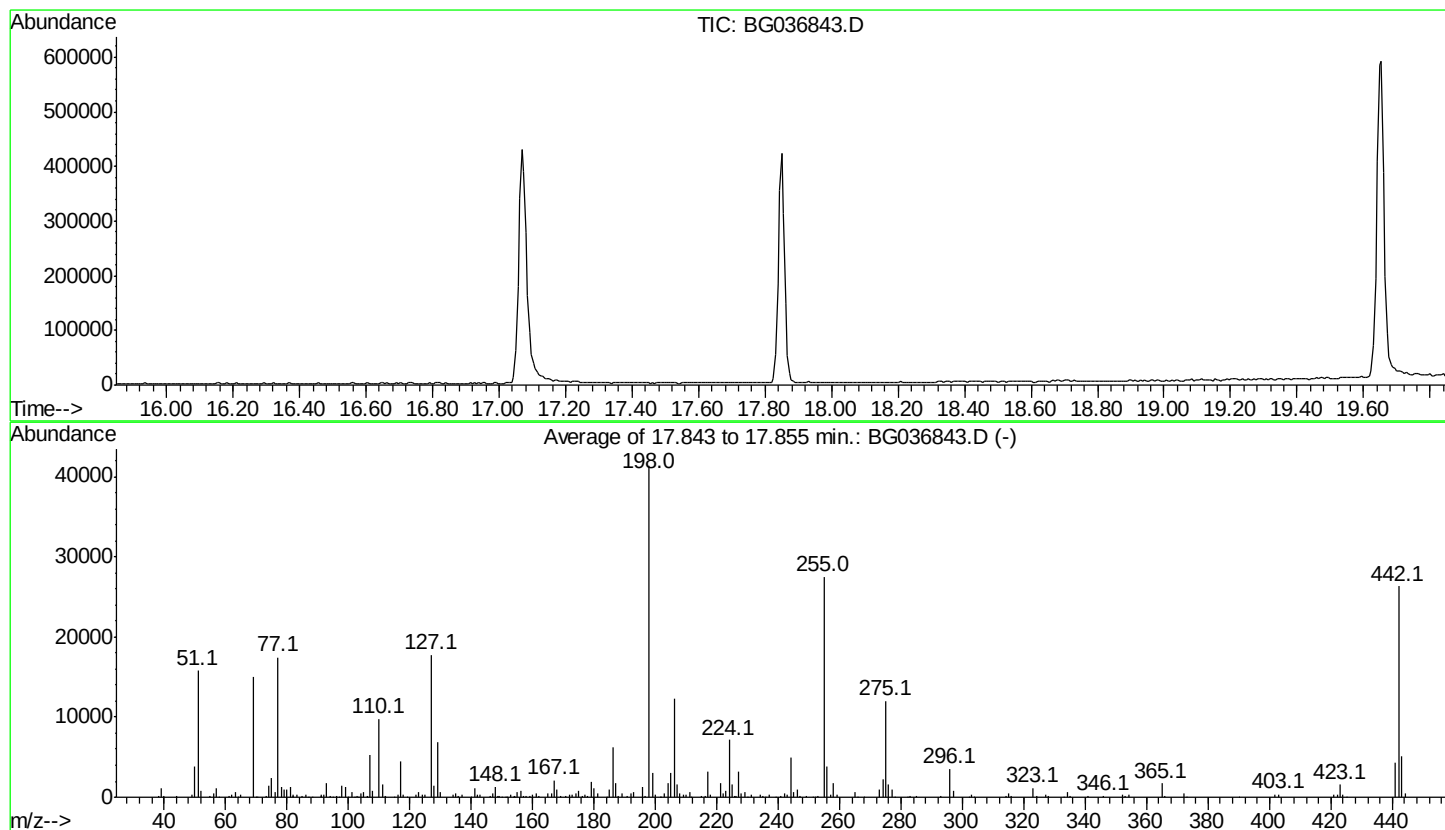

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	15760	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.1	14945	PASS
70	69	0.00	2	0.4	53	PASS
127	198	10	80	43.0	17791	PASS
197	198	0.00	2	0.2	88	PASS
198	198	100	100	100.0	41365	PASS
199	198	5	9	7.5	3094	PASS
275	198	10	60	29.1	12017	PASS
365	198	1	100	4.1	1716	PASS
441	198	0.01	100	10.6	4390	PASS
442	198	50	100	63.6	26301	PASS
443	442	15	24	19.5	5135	PASS