
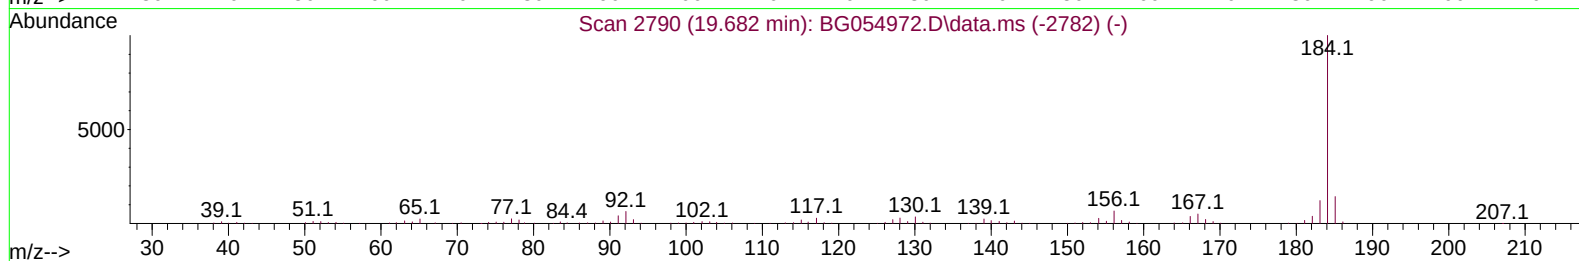
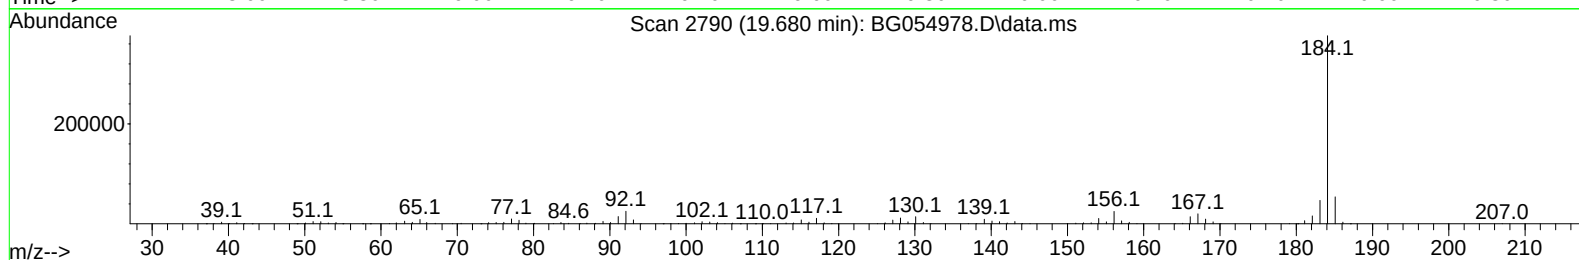


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092022\
Data File : BG054978.D
Acq On : 20 Sep 2022 8:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 18:55:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

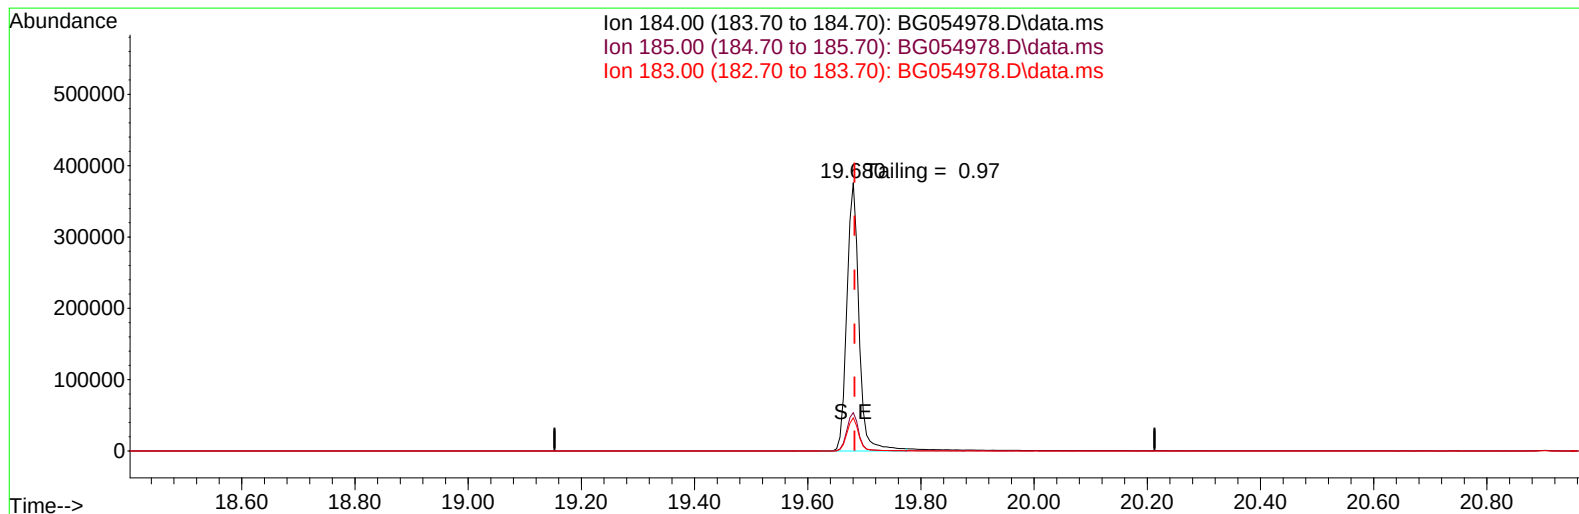




TIC: BG054978.D\data.ms

(77) Benzidine**19.680min (-0.002) 26744.38 ng****response 563886**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.31
183.00	12.30	12.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092022\
Data File : BG054978.D
Acq On : 20 Sep 2022 8:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 18:55:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

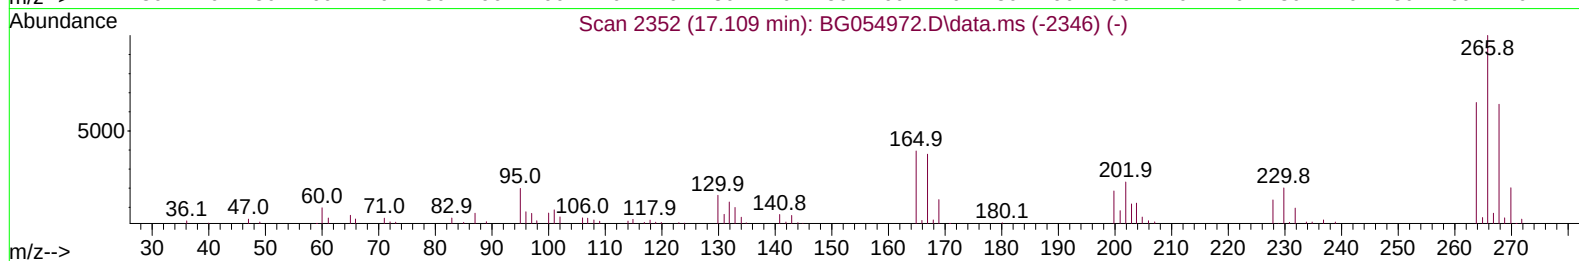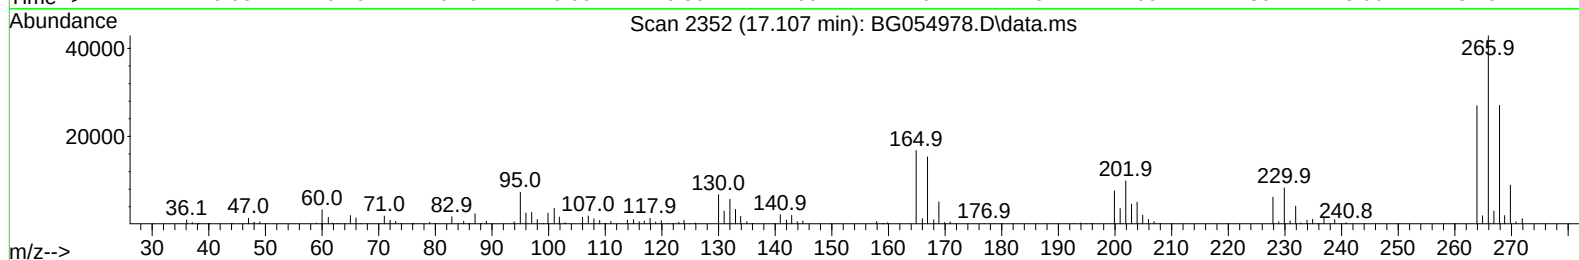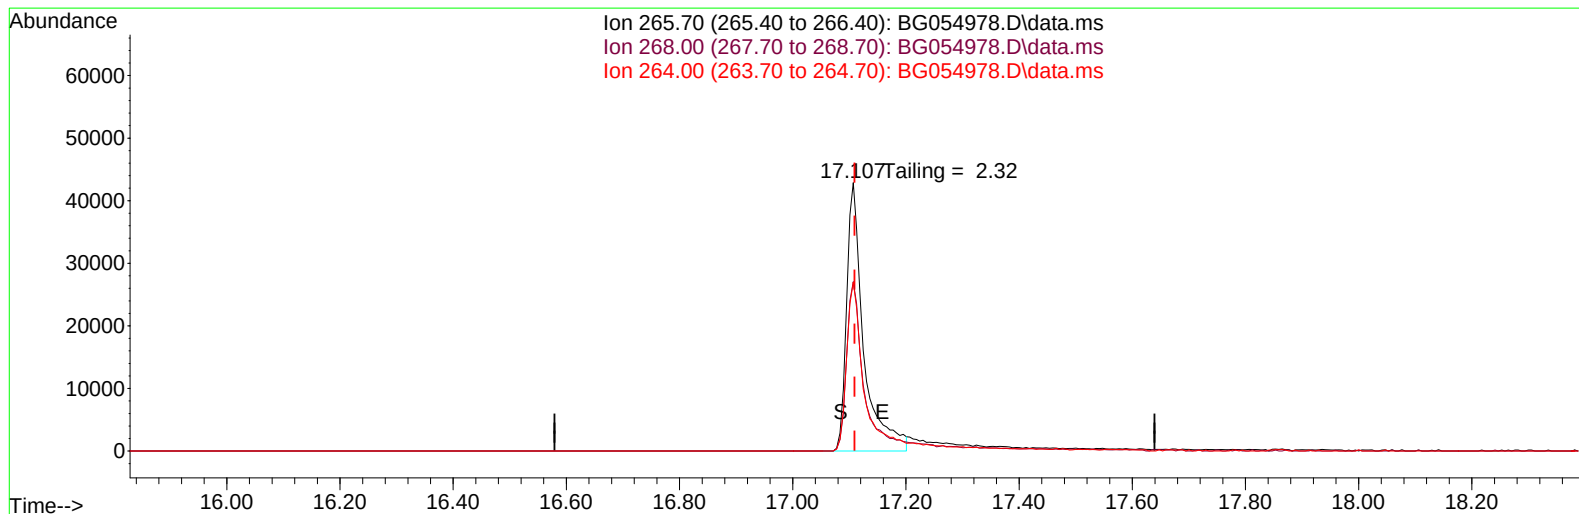

TIC: BG054978.D\data.ms

(70) Pentachlorophenol (C)

17.107min (-0.002) 3761.59 ng

response 99610

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.10
264.00	61.70	62.92
0.00	0.00	0.00