
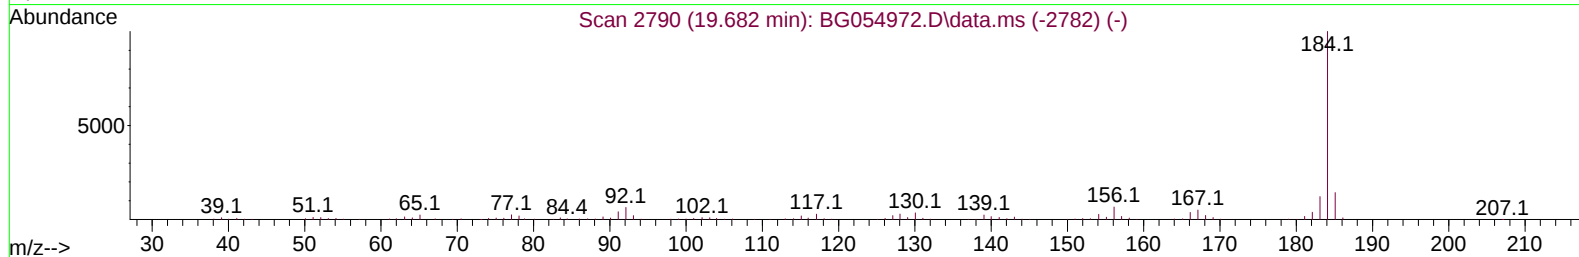
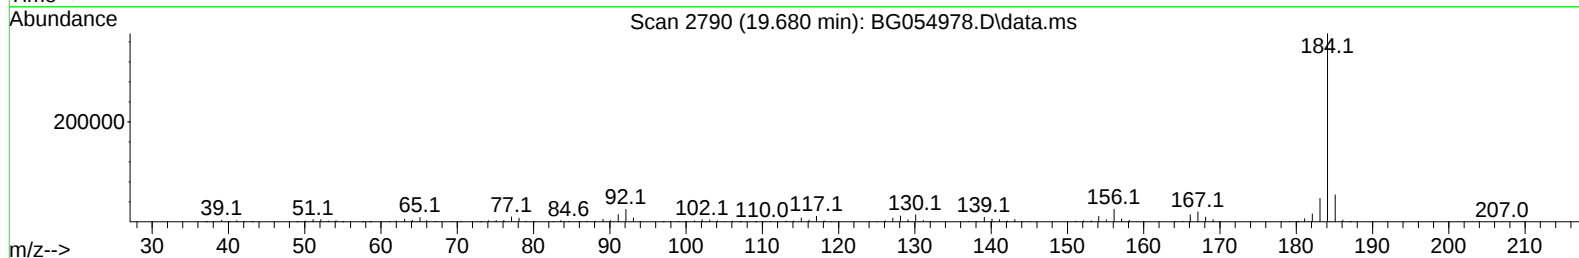


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092022\
Data File : BG054978.D
Acq On : 20 Sep 2022 8:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 20 18:55:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

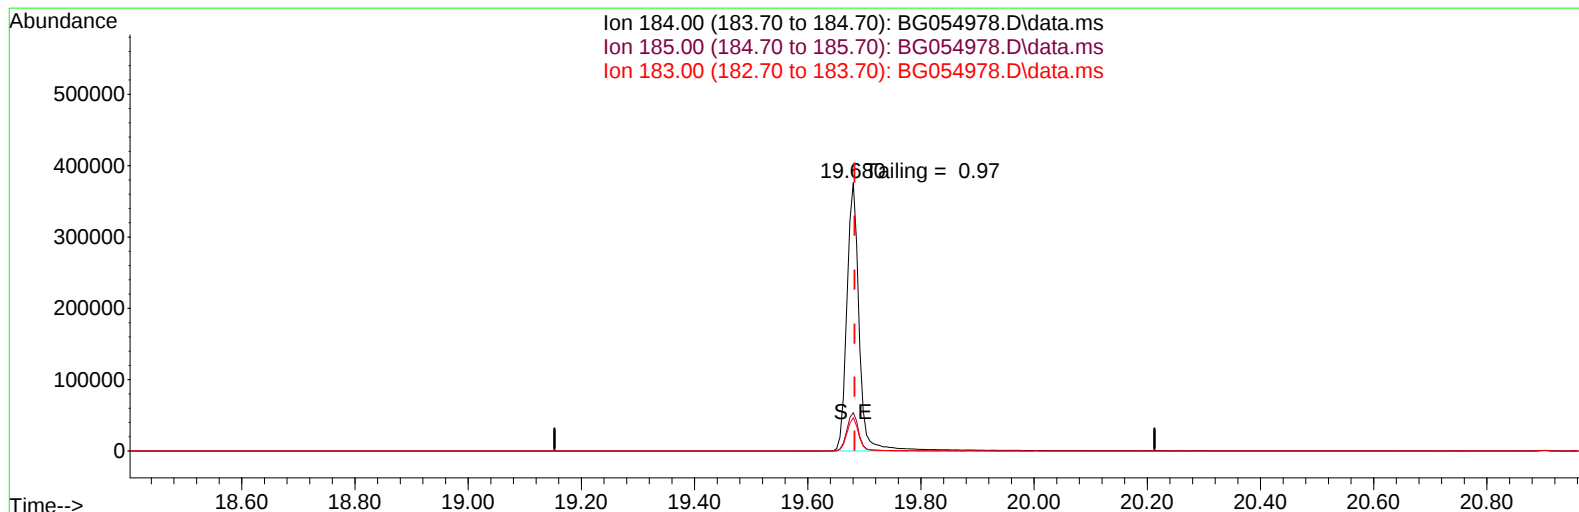

TIC: BG054978.D\data.ms

(77) Benzidine

19.680min (-0.002) 26744.38 ng




response 563886

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.31
183.00	12.30	12.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092022\
Data File : BG054978.D
Acq On : 20 Sep 2022 8:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 20 18:55:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

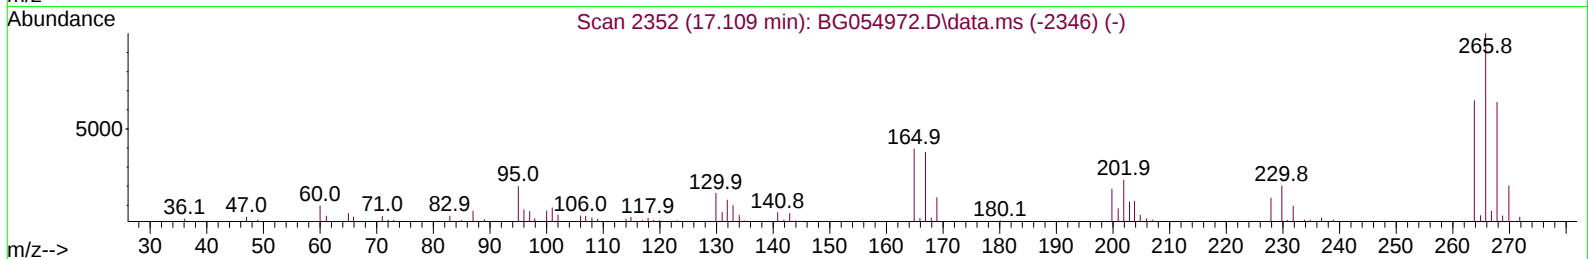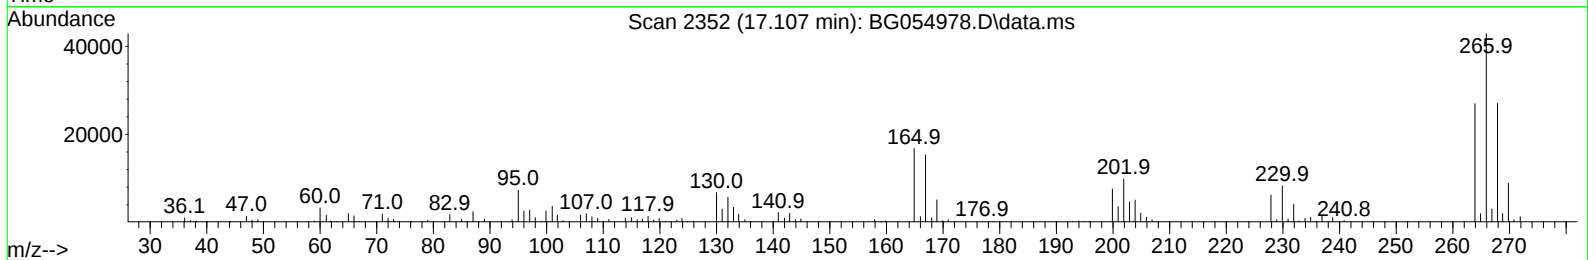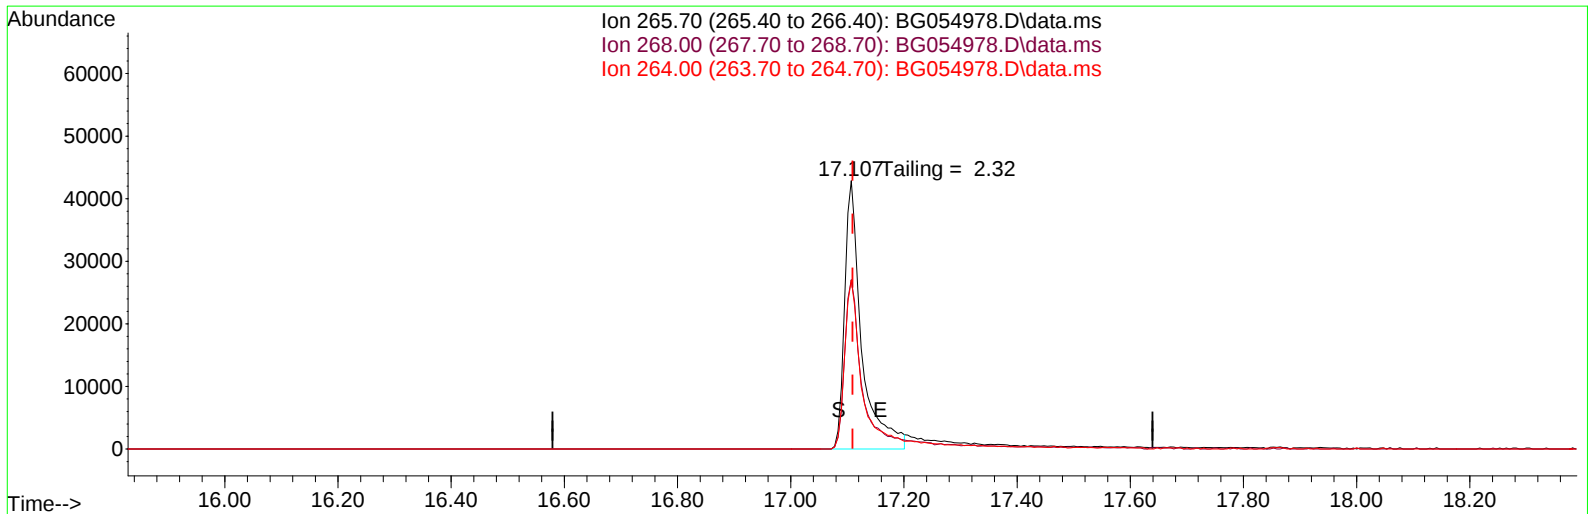

TIC: BG054978.D\data.ms

(70) Pentachlorophenol (C)

17.107min (-0.002) 3761.59 ng

response 99610


Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.10
264.00	61.70	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092022\
 Data File : BG054978.D
 Acq On : 20 Sep 2022 8:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 19 17:41:40 2022

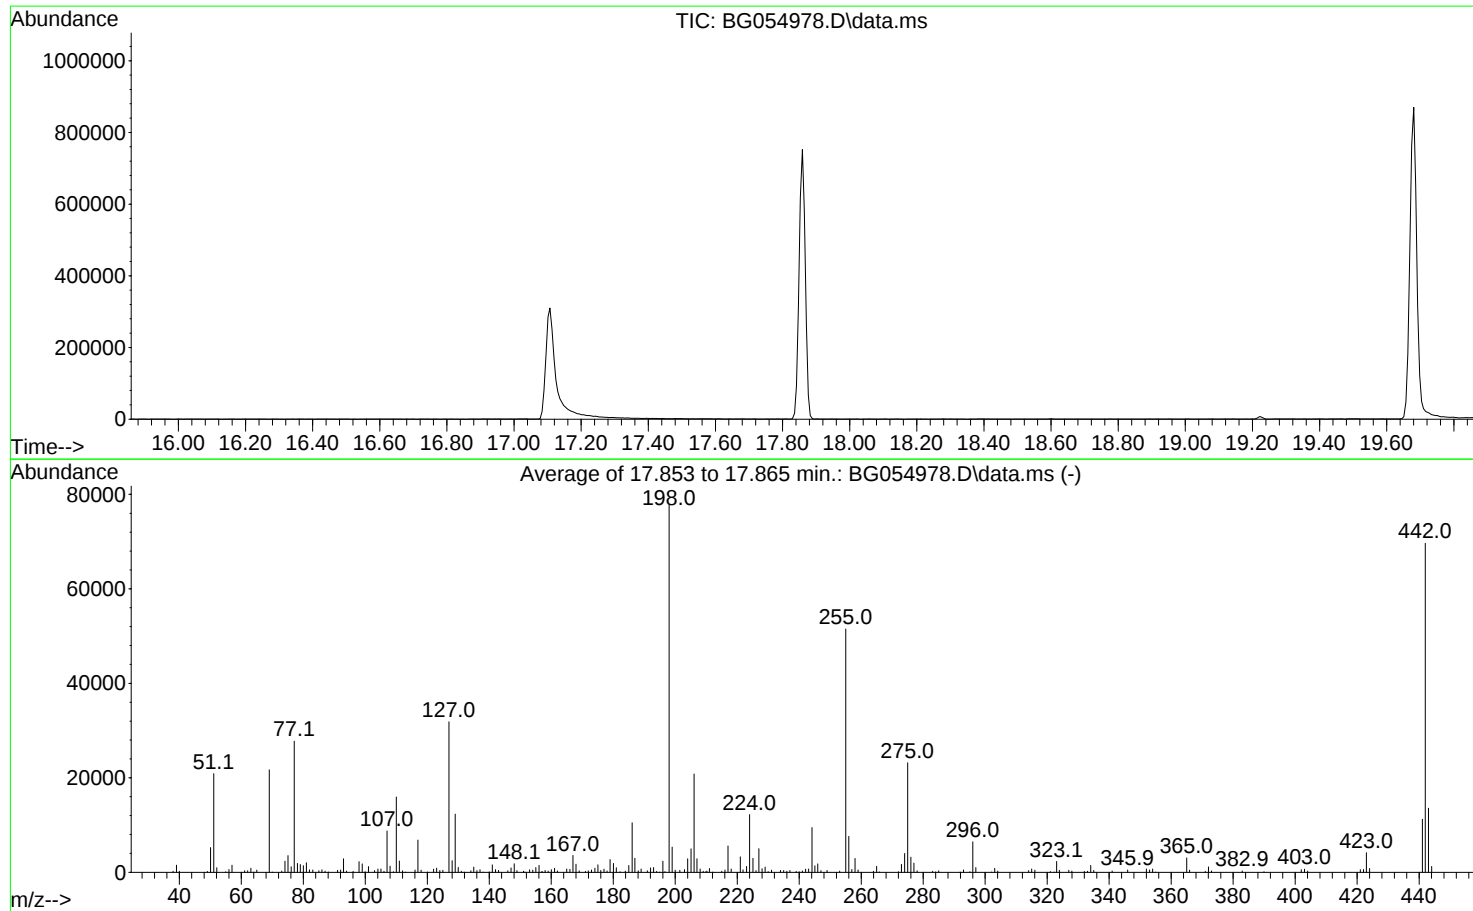

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	20892	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.9	21698	PASS
70	69	0.00	2	0.3	57	PASS
127	198	10	80	40.9	31851	PASS
197	198	0.00	2	0.2	153	PASS
198	198	100	100	100.0	77867	PASS
199	198	5	9	6.9	5339	PASS
275	198	10	60	29.8	23168	PASS
365	198	1	100	3.9	3039	PASS
441	198	0.01	100	14.4	11236	PASS
442	442	50	100	100.0	69640	PASS
443	442	15	24	19.5	13562	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2022	BNA_G	BG054978.D
Compound Name	Response	Retention Time
DDT	285134	20.9
DDD	10807	20.46
DDE	0	19.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10807	295941	3.65

Instrument :
BNA_G
ClientSampleId :
DFTPP