

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059127.D
 Acq On : 21 Sep 2023 3:02
 Operator : MA/JU
 Sample : 04344-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJH3

Quant Time: Sep 21 04:17:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 20 04:25:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.295	152	32697	20.000	ng/ul	0.00
20) Naphthalene-d8	11.139	136	168989	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.922	164	111991	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.672	188	261799	20.000	ng/ul	0.00
79) Chrysene-d12	21.991	240	233026	20.000	ng/ul	0.00
88) Perylene-d12	25.539	264	275800	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.606	96	4208	5.037	ng/uL	0.00
4) Pyridine-d5	4.041	84	31237	12.746	ng/ul	0.00
7) Phenol-d5	7.408	99	23535	7.320	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.613	67	73297	37.150	ng/ul	0.00
11) 2-Chlorophenol-d4	7.807	132	64459	27.168	ng/ul	0.00
15) 4-Methylphenol-d8	8.976	113	43989	17.180	ng/ul	0.00
21) Nitrobenzene-d5	9.493	128	47123	36.137	ng/ul	0.00
24) 2-Nitrophenol-d4	10.210	143	48458	36.786	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.733	165	84371	33.737	ng/ul	0.00
31) 4-Chloroaniline-d4	11.280	131	121282	31.072	ng/ul	0.00
46) Dimethylphthalate-d6	14.317	166	320168	37.173	ng/ul	0.00
49) Acenaphthylene-d8	14.629	160	366059	34.905	ng/ul	0.00
54) 4-Nitrophenol-d4	15.093	143	11947	7.603	ng/ul	0.00
60) Fluorene-d10	15.915	176	291588	36.985	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.015	200	58244	39.132	ng/ul	0.00
73) Anthracene-d10	17.778	188	497741	41.785	ng/ul	0.00
81) Pyrene-d10	20.046	212	589707	43.296	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.298	264	595102	44.189	ng/ul	0.00
Target Compounds						
					Qvalue	
34) Caprolactam	12.067	113	14346	15.496	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059127.D
Acq On : 21 Sep 2023 3:02
Operator : MA/JU
Sample : 04344-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJH3

Quant Time: Sep 21 04:17:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 20 04:25:24 2023
Response via : Initial Calibration

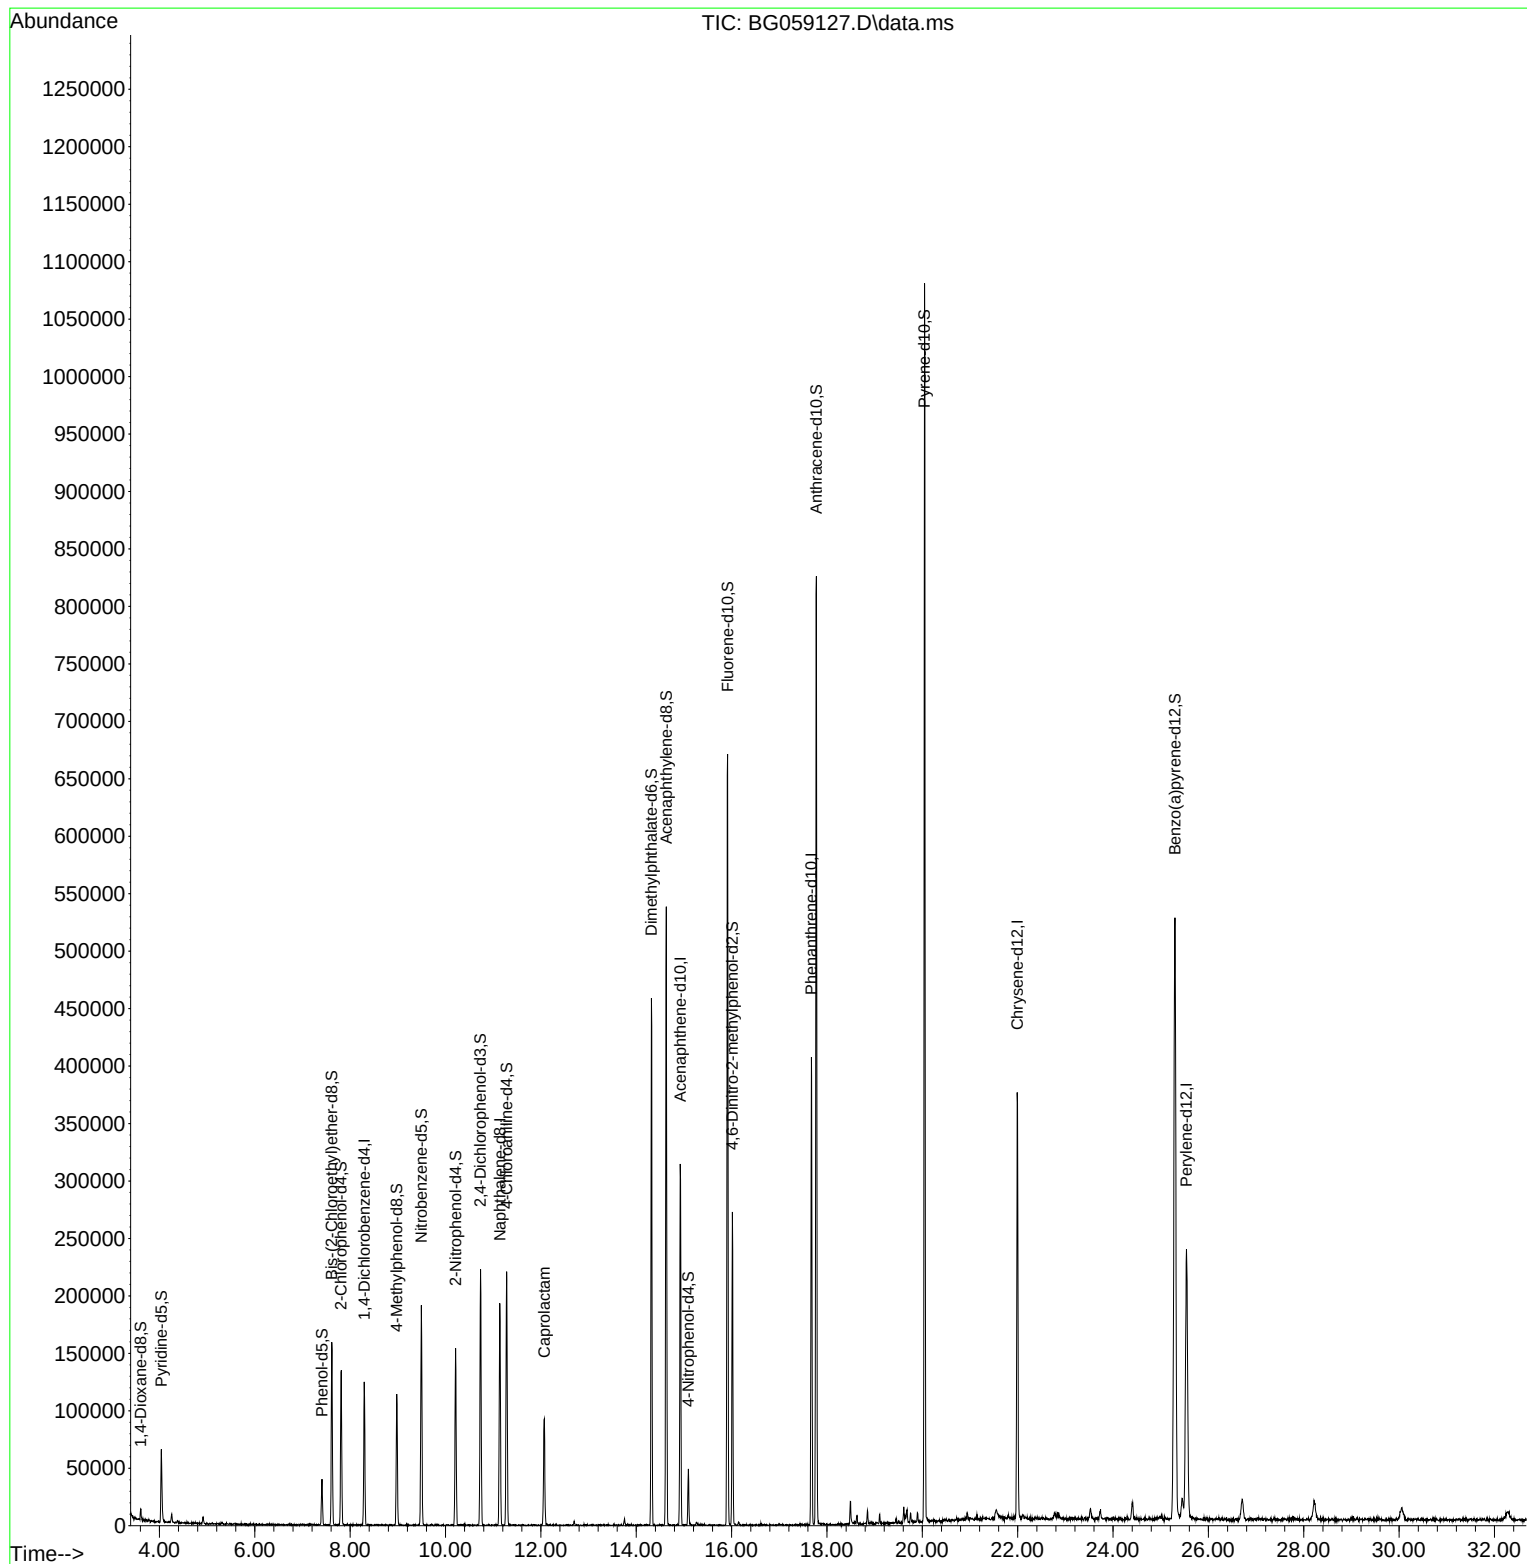

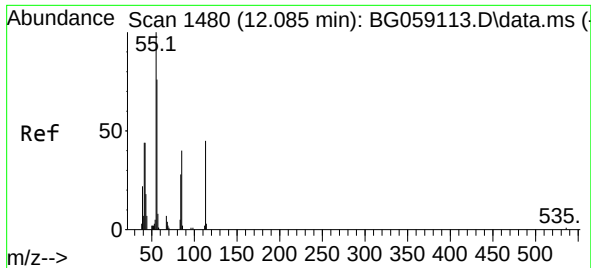

#34
Caprolactam
Concen: 15.496 ng/ul
RT: 12.067 min Scan# 14
Delta R.T. -0.029 min
Lab File: BG059127.D
Acq: 21 Sep 2023 3:02

Instrument :
BNA_G
ClientSampleId :
BBJH3

Tgt Ion	Ratio	Lower	Upper
113	100		
55	235.6	157.6	236.4
56	178.0	112.3	168.5

