

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059132.D
 Acq On : 21 Sep 2023 7:05
 Operator : MA/JU
 Sample : 04344-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBHMO

Quant Time: Sep 21 07:40:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 20 04:25:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.300	152	31056	20.000	ng/ul	0.00
20) Naphthalene-d8	11.138	136	153079	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.922	164	97662	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.671	188	231973	20.000	ng/ul	0.00
79) Chrysene-d12	21.996	240	198414	20.000	ng/ul	0.00
88) Perylene-d12	25.545	264	237295	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.606	96	4061	5.118	ng/uL	0.00
4) Pyridine-d5	4.040	84	32510	13.967	ng/ul	0.00
7) Phenol-d5	7.407	99	25907	8.484	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.613	67	68906	36.770	ng/ul	0.00
11) 2-Chlorophenol-d4	7.807	132	62866	27.897	ng/ul	0.00
15) 4-Methylphenol-d8	8.976	113	45965	18.900	ng/ul	0.00
21) Nitrobenzene-d5	9.493	128	43580	36.894	ng/ul	0.00
24) 2-Nitrophenol-d4	10.210	143	45182	37.864	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.733	165	76694	33.854	ng/ul	0.00
31) 4-Chloroaniline-d4	11.279	131	103036	29.141	ng/ul	0.00
46) Dimethylphthalate-d6	14.317	166	292228	38.907	ng/ul	0.00
49) Acenaphthylene-d8	14.628	160	339092	37.078	ng/ul	0.00
54) 4-Nitrophenol-d4	15.098	143	10405	7.593	ng/ul	0.00
60) Fluorene-d10	15.909	176	264853	38.523	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.015	200	48471	36.753	ng/ul	0.00
73) Anthracene-d10	17.771	188	424850	40.251	ng/ul	0.00
81) Pyrene-d10	20.045	212	469085	40.448	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.292	264	465960	40.214	ng/ul	0.00
Target Compounds						
					Qvalue	
34) Caprolactam	12.066	113	5871	7.001	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059132.D
Acq On : 21 Sep 2023 7:05
Operator : MA/JU
Sample : 04344-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBHM0

Quant Time: Sep 21 07:40:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 20 04:25:24 2023
Response via : Initial Calibration

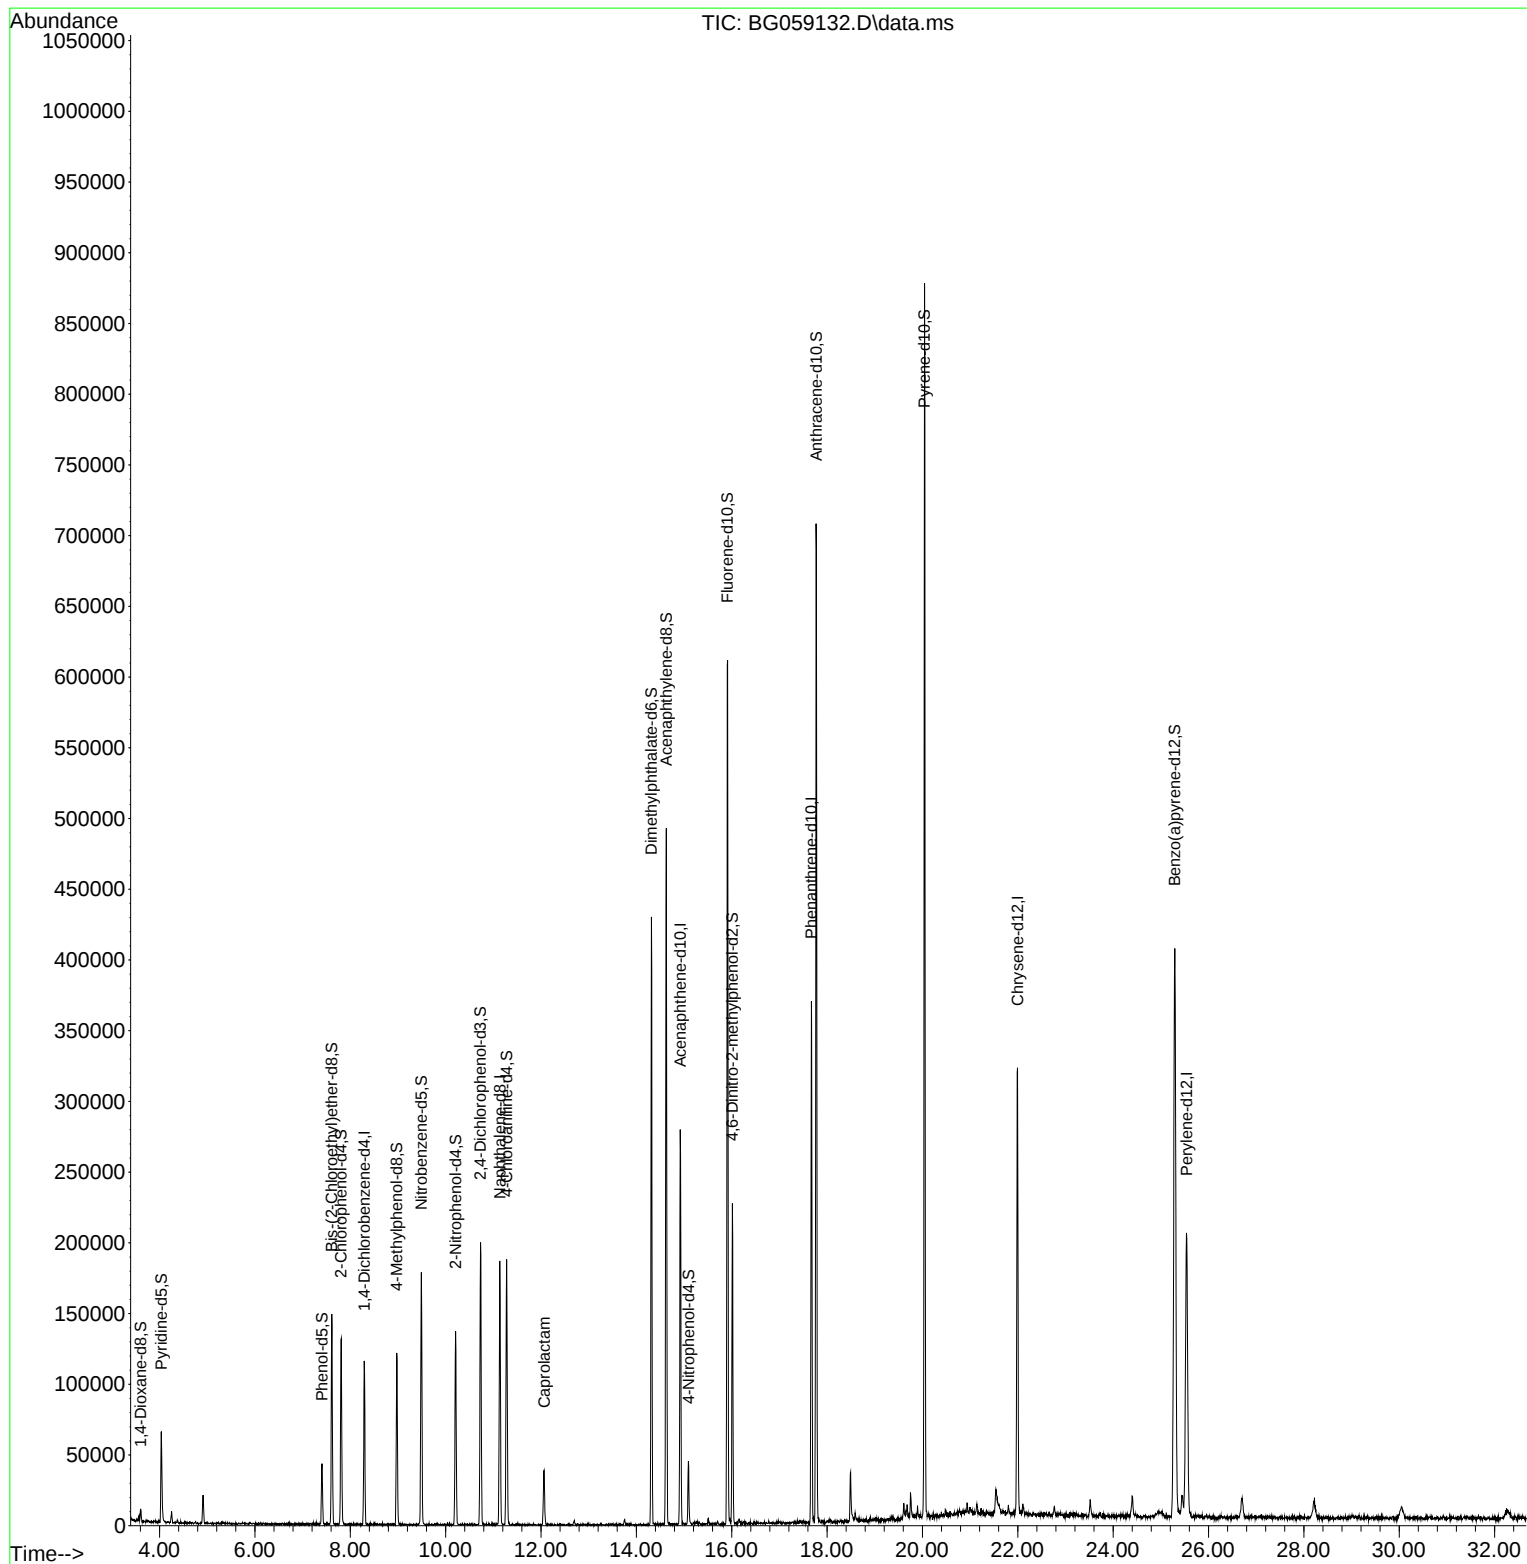

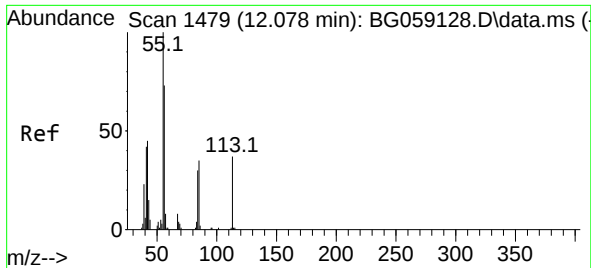

#34

Caprolactam

Concen: 7.001 ng/ul

RT: 12.066 min Scan# 14

Delta R.T. -0.029 min

Lab File: BG059132.D


Acq: 21 Sep 2023 7:05

Instrument :

BNA_G

ClientSampleId :

BBHM0

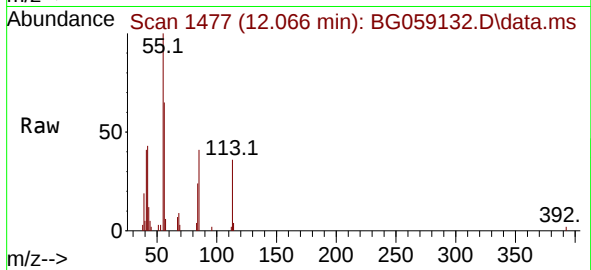

Tgt Ion:113 Resp: 5871

Ion Ratio Lower Upper

113 100

55 280.7 157.6 236.4#

56 181.2 112.3 168.5#

