

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059135.D
 Acq On : 21 Sep 2023 9:06
 Operator : MA/JU
 Sample : 04344-09
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBHR8

Quant Time: Sep 21 09:41:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 20 04:25:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.294	152	32279	20.000	ng/ul	0.00
20) Naphthalene-d8	11.138	136	159902	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.928	164	103766	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.677	188	247331	20.000	ng/ul	0.00
79) Chrysene-d12	21.996	240	210249	20.000	ng/ul	# 0.00
88) Perylene-d12	25.545	264	244644	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.606	96	3149	3.819	ng/uL	0.00
4) Pyridine-d5	4.035	84	28323	11.707	ng/ul	-0.01
7) Phenol-d5	7.407	99	24325	7.664	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.613	67	66391	34.086	ng/ul	0.00
11) 2-Chlorophenol-d4	7.813	132	60777	25.948	ng/ul	0.00
15) 4-Methylphenol-d8	8.976	113	45071	17.830	ng/ul	0.00
21) Nitrobenzene-d5	9.493	128	43510	35.263	ng/ul	0.00
24) 2-Nitrophenol-d4	10.210	143	44057	35.346	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.733	165	83455	35.267	ng/ul	0.00
31) 4-Chloroaniline-d4	11.285	131	92224	24.970	ng/ul	0.00
46) Dimethylphthalate-d6	14.323	166	326852	40.957	ng/ul	0.00
49) Acenaphthylene-d8	14.628	160	355687	36.605	ng/ul	0.00
54) 4-Nitrophenol-d4	15.098	143	11098	7.622	ng/ul	0.00
60) Fluorene-d10	15.915	176	281772	38.573	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.021	200	55200	39.256	ng/ul	0.00
73) Anthracene-d10	17.777	188	474471	42.161	ng/ul	0.00
81) Pyrene-d10	20.045	212	534305	43.478	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.298	264	522632	43.750	ng/ul	0.00
Target Compounds						
34) Caprolactam	12.072	113	14555	16.615	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059135.D
Acq On : 21 Sep 2023 9:06
Operator : MA/JU
Sample : 04344-09
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBHR8

Quant Time: Sep 21 09:41:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 20 04:25:24 2023
Response via : Initial Calibration

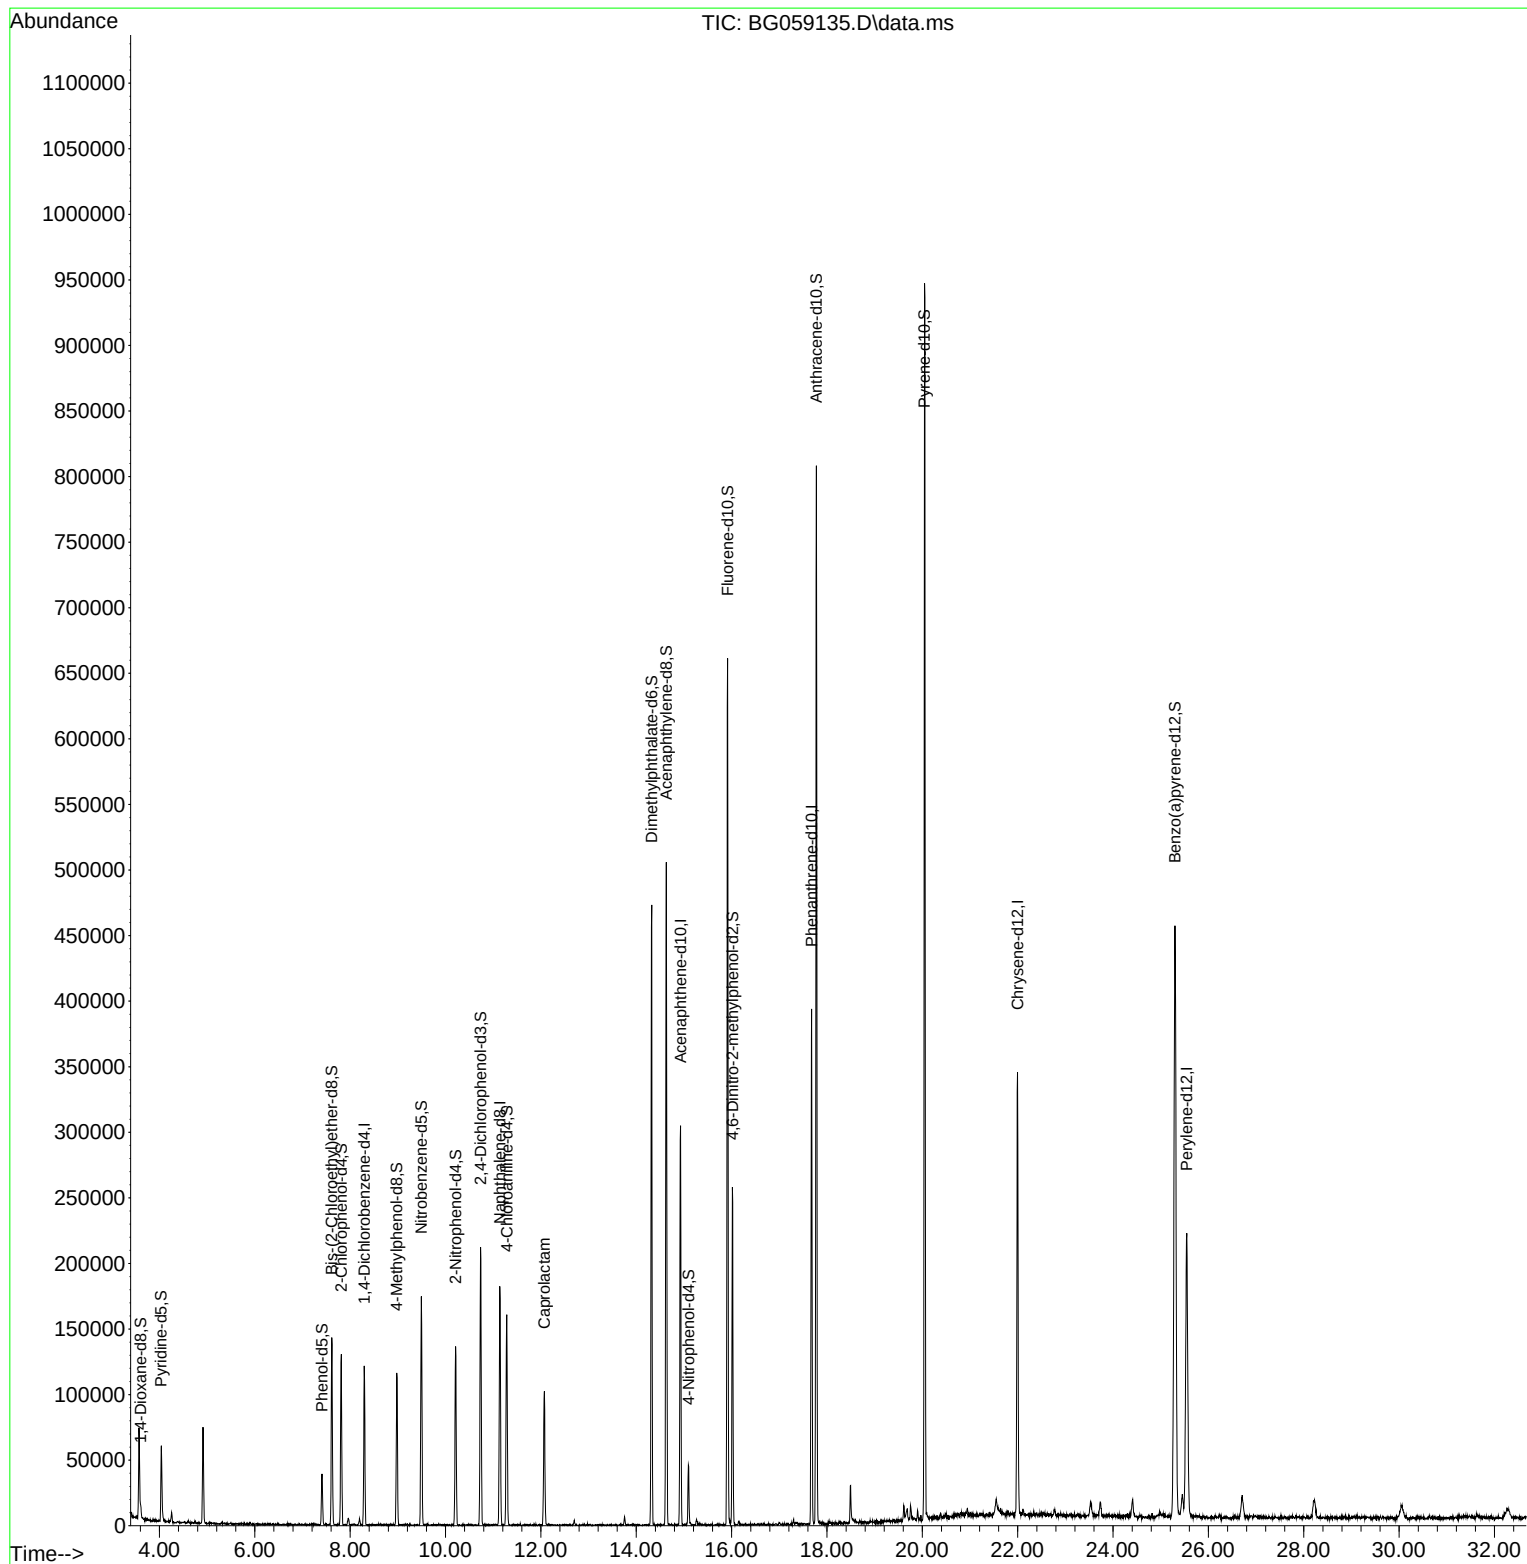

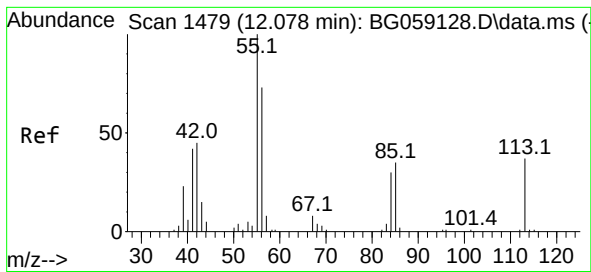

#34
 Caprolactam
 Concen: 16.615 ng/ul
 RT: 12.072 min Scan# 14
 Delta R.T. -0.023 min
 Lab File: BG059135.D
 Acq: 21 Sep 2023 9:06

Instrument :
 BNA_G
 ClientSampleId :
 BBHR8

Tgt Ion:113 Resp: 14555
 Ion Ratio Lower Upper
 113 100
 55 291.7 157.6 236.4#
 56 178.9 112.3 168.5#

