

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059102.D
 Acq On : 20 Sep 2023 10:00
 Operator : MA/JU
 Sample : PB155502BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK502

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.605	33	37	44	rVB2	10362	14357	1.54%	0.148%
2	4.040	106	111	123	rVB	86490	143908	15.41%	1.485%
3	4.381	163	169	173	rBV4	2115	3669	0.39%	0.038%
4	4.974	268	270	273	rVB	1325	1456	0.16%	0.015%
5	6.807	578	582	586	rVB	1137	1470	0.16%	0.015%
6	6.937	600	604	608	rBV	1462	2066	0.22%	0.021%
7	7.407	676	684	691	rBV	140779	238514	25.54%	2.462%
8	7.618	714	720	728	rVB	120131	194942	20.87%	2.012%
9	7.812	745	753	761	rBV	127118	217927	23.33%	2.249%
10	8.300	829	836	845	rVB	97937	168832	18.08%	1.743%
11	8.975	945	951	960	rBV	174149	296914	31.79%	3.065%
12	9.492	1031	1039	1047	rVB	137441	242736	25.99%	2.506%
13	10.209	1153	1161	1171	rBB2	107461	191104	20.46%	1.973%
14	10.732	1243	1250	1260	rBV	162346	294629	31.54%	3.041%
15	11.143	1311	1320	1328	rVB	151453	275205	29.47%	2.841%
16	11.284	1337	1344	1353	rVB	133142	236481	25.32%	2.441%
17	12.706	1580	1586	1590	rBB2	2495	4799	0.51%	0.050%
18	13.758	1757	1765	1769	rBV3	4006	5791	0.62%	0.060%
19	14.322	1855	1861	1867	rVB	349662	490629	52.53%	5.064%
20	14.628	1906	1913	1920	rBV	381217	602635	64.52%	6.221%
21	14.927	1957	1964	1972	rBB	264900	396137	42.41%	4.089%
22	15.092	1986	1992	2002	rBV	150233	246274	26.37%	2.542%
23	15.914	2126	2132	2139	rVB	512759	747210	80.00%	7.713%
24	16.020	2142	2150	2158	rBV	153038	229629	24.59%	2.370%
25	16.149	2168	2172	2175	rBV2	2083	2996	0.32%	0.031%
26	17.677	2424	2432	2438	rBV	335685	492547	52.74%	5.084%
27	17.777	2442	2449	2457	rVV	571057	833369	89.23%	8.602%
28	19.216	2690	2694	2697	rVB2	957	1607	0.17%	0.017%
29	19.293	2702	2707	2709	rBV2	1128	1743	0.19%	0.018%
30	19.616	2757	2762	2765	rBV3	8207	10090	1.08%	0.104%
31	19.680	2768	2773	2778	rVB2	5259	7991	0.86%	0.082%
32	19.910	2808	2812	2815	rBV2	1143	1443	0.15%	0.015%
33	20.051	2829	2836	2844	rBV	659380	933997	100.00%	9.641%
34	20.127	2847	2849	2851	rVB2	1754	1411	0.15%	0.015%
35	20.297	2876	2878	2882	rVB2	1178	1584	0.17%	0.016%
36	20.356	2886	2888	2893	rVB	2248	2131	0.23%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059102.D
 Acq On : 20 Sep 2023 10:00
 Operator : MA/JU
 Sample : PB155502BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK502

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

37	20.403	2893	2896	2897	rBV	1884	1467	0.16%	0.015%
38	20.491	2907	2911	2912	rVB2	1812	1805	0.19%	0.019%
39	20.626	2931	2934	2937	rBV2	1741	2549	0.27%	0.026%
40	20.715	2945	2949	2950	rBV2	1598	1898	0.20%	0.020%

41	20.732	2950	2952	2955	rVV2	1451	1509	0.16%	0.016%
42	20.779	2955	2960	2961	rBV4	2131	3051	0.33%	0.031%
43	20.938	2985	2987	2990	rVB3	2398	2837	0.30%	0.029%
44	20.967	2990	2992	2995	rVB4	2200	2136	0.23%	0.022%
45	21.232	3033	3037	3038	rBV2	1336	1470	0.16%	0.015%

46	21.531	3084	3088	3090	rBV4	1952	2679	0.29%	0.028%
47	21.596	3097	3099	3100	rBV2	1773	1430	0.15%	0.015%
48	21.995	3160	3167	3177	rVB	269319	482892	51.70%	4.984%
49	22.113	3185	3187	3191	rVB2	2667	3024	0.32%	0.031%
50	22.236	3206	3208	3211	rVB3	1947	1521	0.16%	0.016%

51	22.277	3213	3215	3216	rBV2	1893	1873	0.20%	0.019%
52	22.542	3258	3260	3261	rBV	1991	1467	0.16%	0.015%
53	22.718	3288	3290	3293	rVB3	1569	1763	0.19%	0.018%
54	22.765	3296	3298	3299	rBV2	4148	2614	0.28%	0.027%
55	22.859	3312	3314	3318	rVB3	2045	2419	0.26%	0.025%

56	23.529	3423	3428	3435	rBV5	6905	14511	1.55%	0.150%
57	24.210	3542	3544	3546	rBV2	2087	2069	0.22%	0.021%
58	24.304	3558	3560	3561	rBV2	1990	1466	0.16%	0.015%
59	24.351	3566	3568	3572	rBV4	1926	1728	0.19%	0.018%
60	24.410	3572	3578	3586	rBV5	8237	20509	2.20%	0.212%

61	24.763	3637	3638	3642	rVB3	1671	1704	0.18%	0.018%
62	24.839	3649	3651	3654	rBV2	1556	1946	0.21%	0.020%
63	25.027	3680	3683	3686	rBV5	2259	3090	0.33%	0.032%
64	25.297	3717	3729	3746	rBV2	300032	916303	98.11%	9.458%
65	25.450	3750	3755	3756	rBV3	8956	11274	1.21%	0.116%

66	25.550	3762	3772	3785	rVB2	168968	534293	57.21%	5.515%
67	25.938	3836	3838	3840	rVB3	2199	1856	0.20%	0.019%
68	26.073	3859	3861	3864	rBV4	1957	2061	0.22%	0.021%
69	26.108	3864	3867	3872	rVB3	2057	3357	0.36%	0.035%
70	26.449	3923	3925	3928	rVB4	1666	1477	0.16%	0.015%

71	26.649	3955	3959	3961	rBV3	2004	3052	0.33%	0.032%
72	26.713	3965	3970	3971	rBV4	9590	11848	1.27%	0.122%
73	27.548	4110	4112	4115	rBV3	1588	1606	0.17%	0.017%
74	27.612	4120	4123	4124	rBV	1665	1753	0.19%	0.018%
75	27.800	4151	4155	4157	rBV4	2082	2870	0.31%	0.030%

76	27.900	4171	4172	4173	rBV	2379	1520	0.16%	0.016%
----	--------	------	------	------	-----	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059102.D
 Acq On : 20 Sep 2023 10:00
 Operator : MA/JU
 Sample : PB155502BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK502

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

77	28.071	4199	4201	4205	rBV2	1601	1924	0.21%	0.020%
78	28.106	4205	4207	4211	rBV5	1761	2353	0.25%	0.024%
79	28.253	4223	4232	4241	rVB8	10698	35862	3.84%	0.370%
80	28.476	4268	4270	4273	rVB3	1791	2124	0.23%	0.022%
81	28.576	4286	4287	4289	rBV2	2076	1565	0.17%	0.016%
82	28.635	4296	4297	4300	rBV2	1636	1914	0.20%	0.020%
83	28.811	4326	4327	4331	rVB4	1814	1629	0.17%	0.017%
84	28.858	4331	4335	4337	rBV2	1785	2595	0.28%	0.027%
85	29.340	4415	4417	4419	rBV2	1620	1526	0.16%	0.016%
86	29.363	4419	4421	4423	rBV	1693	1437	0.15%	0.015%
87	29.428	4430	4432	4436	rVB3	1965	1753	0.19%	0.018%
88	30.033	4531	4535	4536	rBV4	3904	4736	0.51%	0.049%
89	30.250	4568	4572	4573	rBV3	2005	2451	0.26%	0.025%
90	30.474	4608	4610	4613	rVB2	2303	2165	0.23%	0.022%
91	30.503	4613	4615	4616	rBV2	1821	1438	0.15%	0.015%
92	30.550	4619	4623	4626	rBV2	2653	3260	0.35%	0.034%
93	30.603	4630	4632	4635	rBV3	2021	2656	0.28%	0.027%
94	30.867	4675	4677	4679	rVB2	2626	2215	0.24%	0.023%
95	30.991	4697	4698	4702	rBV4	1684	2191	0.23%	0.023%
96	31.067	4709	4711	4713	rBV2	1880	1461	0.16%	0.015%
97	31.672	4810	4814	4817	rBV3	2902	3523	0.38%	0.036%
98	32.048	4876	4878	4880	rVB2	2205	1861	0.20%	0.019%
99	32.248	4906	4912	4914	rBV4	2709	4849	0.52%	0.050%
100	32.589	4968	4970	4972	rBV2	1310	1471	0.16%	0.015%




Sum of corrected areas: 9687879

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059102.D
Acq On : 20 Sep 2023 10:00
Operator : MA/JU
Sample : PB155502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

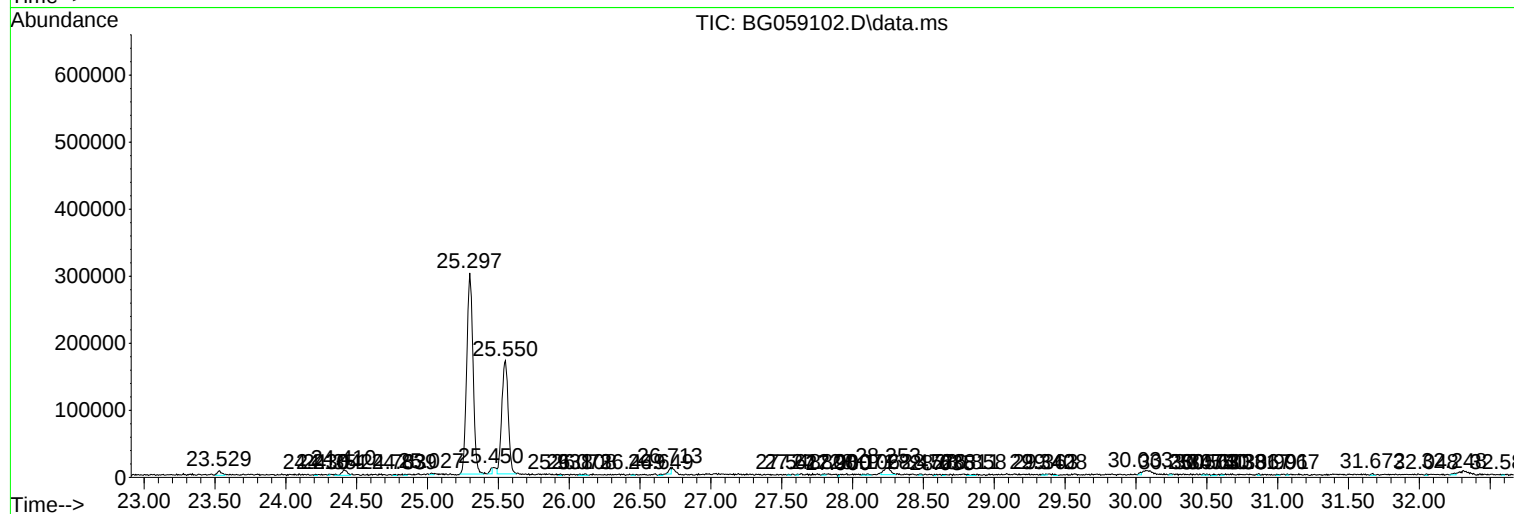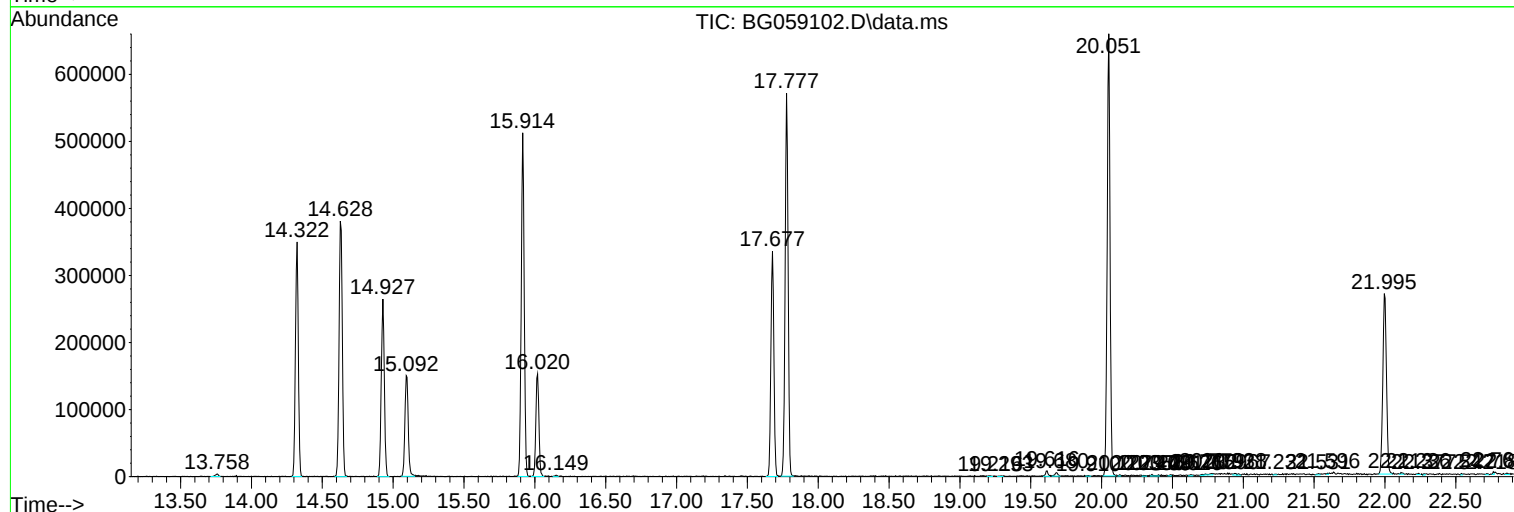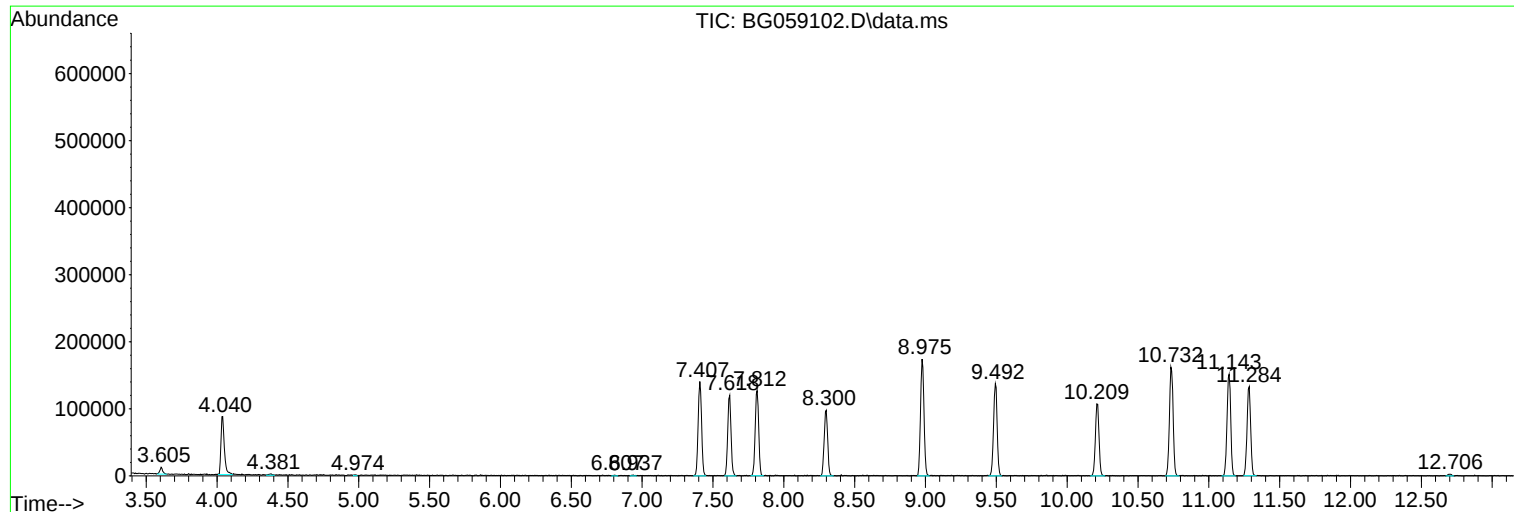

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059102.D
Acq On : 20 Sep 2023 10:00
Operator : MA/JU
Sample : PB155502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059102.D
Acq On : 20 Sep 2023 10:00
Operator : MA/JU
Sample : PB155502BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK502

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc