

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059115.D
 Acq On : 20 Sep 2023 18:49
 Operator : MA/JU
 Sample : PB155510BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK510

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.608	34	37	44	rVB	8890	12913	1.39%	0.131%
2	4.037	105	110	123	rBV	130031	219018	23.58%	2.229%
3	4.378	166	168	171	rVB3	2063	2309	0.25%	0.024%
4	5.782	404	407	410	rVB2	1056	1623	0.17%	0.017%
5	5.911	426	429	432	rBV	1129	1601	0.17%	0.016%
6	6.035	447	450	453	rBV	1056	1685	0.18%	0.017%
7	7.410	677	684	695	rBV	144988	245128	26.39%	2.495%
8	7.615	712	719	729	rVB	118928	195740	21.08%	1.992%
9	7.809	746	752	760	rBV	128067	224912	24.22%	2.289%
10	8.297	829	835	842	rVB	110832	190129	20.47%	1.935%
11	8.978	944	951	959	rBV	171719	289735	31.20%	2.949%
12	9.313	1005	1008	1011	rBV	1087	1498	0.16%	0.015%
13	9.489	1030	1038	1050	rVB2	133184	236931	25.51%	2.411%
14	10.212	1153	1161	1169	rBV2	105359	189663	20.42%	1.930%
15	10.735	1241	1250	1259	rBB	160070	284762	30.66%	2.898%
16	11.140	1312	1319	1326	rBV	173285	310513	33.43%	3.160%
17	11.281	1335	1343	1352	rBV	173137	315668	33.99%	3.213%
18	12.697	1579	1584	1587	rBV2	2292	3317	0.36%	0.034%
19	13.749	1759	1763	1769	rBV2	2486	3267	0.35%	0.033%
20	14.319	1854	1860	1867	rVB	320826	448871	48.33%	4.568%
21	14.630	1906	1913	1922	rVB	341723	557287	60.01%	5.672%
22	14.924	1956	1963	1971	rVB	284515	429670	46.26%	4.373%
23	15.095	1985	1992	2000	rBV	153171	238229	25.65%	2.425%
24	15.195	2005	2009	2013	rVB2	1369	2018	0.22%	0.021%
25	15.911	2124	2131	2139	rVB	465266	692277	74.54%	7.046%
26	16.017	2142	2149	2155	rBV	160452	222110	23.92%	2.261%
27	17.674	2425	2431	2440	rVB	362538	539720	58.11%	5.493%
28	17.774	2440	2448	2457	rBV2	516689	791234	85.20%	8.053%
29	18.050	2492	2495	2499	rVB	1225	1575	0.17%	0.016%
30	18.532	2575	2577	2581	rVB2	1899	2076	0.22%	0.021%
31	18.579	2581	2585	2587	rBV	1181	1550	0.17%	0.016%
32	19.613	2756	2761	2765	rBV2	7312	9410	1.01%	0.096%
33	19.678	2768	2772	2776	rVB2	6407	8197	0.88%	0.083%
34	20.048	2829	2835	2844	rVV	657380	922678	99.35%	9.391%
35	20.694	2944	2945	2947	rVB	2231	1447	0.16%	0.015%
36	20.717	2947	2949	2952	rBV2	2084	2765	0.30%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059115.D
 Acq On : 20 Sep 2023 18:49
 Operator : MA/JU
 Sample : PB155510BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK510

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

37	20.947	2985	2988	2991	rVB2	3130	3103	0.33%	0.032%
38	20.970	2991	2992	2995	rBV3	2395	1682	0.18%	0.017%
39	21.029	3000	3002	3005	rBV2	1588	1714	0.18%	0.017%
40	21.123	3016	3018	3020	rBV3	1581	1595	0.17%	0.016%

41	21.240	3036	3038	3041	rVB3	2423	2197	0.24%	0.022%
42	21.540	3085	3089	3092	rBV6	3255	4251	0.46%	0.043%
43	21.992	3159	3166	3173	rBV2	311420	552776	59.52%	5.626%
44	22.345	3222	3226	3227	rVB2	1806	1597	0.17%	0.016%
45	22.357	3227	3228	3231	rBV2	1783	1526	0.16%	0.016%

46	22.433	3239	3241	3247	rBV4	1790	2761	0.30%	0.028%
47	22.480	3247	3249	3251	rVB	2108	1527	0.16%	0.016%
48	22.521	3251	3256	3258	rBV4	2186	4245	0.46%	0.043%
49	22.639	3274	3276	3278	rVB	2402	1764	0.19%	0.018%
50	22.756	3293	3296	3297	rBV	3173	3027	0.33%	0.031%

51	23.391	3403	3404	3407	rVB2	2465	1988	0.21%	0.020%
52	23.514	3423	3425	3426	rBV2	3999	3744	0.40%	0.038%
53	23.820	3475	3477	3479	rBV2	2021	2023	0.22%	0.021%
54	23.861	3481	3484	3485	rVB2	2382	1900	0.20%	0.019%
55	23.878	3485	3487	3490	rBV5	2001	2239	0.24%	0.023%

56	24.137	3529	3531	3534	rVB3	1886	2256	0.24%	0.023%
57	24.166	3534	3536	3537	rBV	2192	1495	0.16%	0.015%
58	24.401	3574	3576	3582	rVB7	4758	7616	0.82%	0.078%
59	24.642	3615	3617	3620	rVB4	1820	1966	0.21%	0.020%
60	24.672	3620	3622	3623	rBV2	2548	1686	0.18%	0.017%

61	25.294	3716	3728	3742	rBV2	303705	928722	100.00%	9.452%
62	25.430	3749	3751	3752	rBV2	2848	2698	0.29%	0.027%
63	25.541	3760	3770	3782	rVB2	198453	594204	63.98%	6.048%
64	25.670	3790	3792	3794	rBV3	2403	2234	0.24%	0.023%
65	26.117	3866	3868	3870	rBV2	2531	2270	0.24%	0.023%

66	26.387	3910	3914	3917	rBV4	2124	3075	0.33%	0.031%
67	26.452	3923	3925	3927	rBV2	1884	1494	0.16%	0.015%
68	26.499	3932	3933	3936	rBV2	2782	2034	0.22%	0.021%
69	26.628	3952	3955	3957	rBV3	1848	2582	0.28%	0.026%
70	26.693	3960	3966	3968	rBV5	5967	9356	1.01%	0.095%

71	27.357	4077	4079	4081	rBV2	1553	1672	0.18%	0.017%
72	27.762	4146	4148	4151	rBV2	2492	2554	0.28%	0.026%
73	27.909	4171	4173	4175	rBV3	1766	2027	0.22%	0.021%
74	27.962	4180	4182	4183	rVV2	2515	1762	0.19%	0.018%
75	27.997	4186	4188	4191	rBV4	2391	3167	0.34%	0.032%

76	28.027	4191	4193	4195	rBV2	2201	1880	0.20%	0.019%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059115.D
 Acq On : 20 Sep 2023 18:49
 Operator : MA/JU
 Sample : PB155510BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK510

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

77	28.050	4195	4197	4203	rVB6	1910	2027	0.22%	0.021%
78	28.126	4209	4210	4213	rBV2	1498	1487	0.16%	0.015%
79	28.185	4217	4220	4221	rBV3	2427	2525	0.27%	0.026%
80	28.502	4273	4274	4277	rVB3	2702	1774	0.19%	0.018%
81	28.978	4353	4355	4356	rVB	2700	1890	0.20%	0.019%
82	28.996	4356	4358	4359	rBV2	2159	1552	0.17%	0.016%
83	29.043	4362	4366	4369	rBV5	2081	3502	0.38%	0.036%
84	29.172	4386	4388	4389	rBV	3122	1748	0.19%	0.018%
85	29.396	4425	4426	4432	rVB2	2880	4027	0.43%	0.041%
86	29.437	4432	4433	4436	rBV2	2029	1814	0.20%	0.018%
87	29.707	4477	4479	4483	rBV3	1858	2257	0.24%	0.023%
88	30.195	4561	4562	4564	rBV2	1905	1632	0.18%	0.017%
89	30.289	4576	4578	4581	rVB2	1837	1566	0.17%	0.016%
90	31.123	4718	4720	4723	rBV3	1564	1643	0.18%	0.017%
91	31.317	4751	4753	4756	rBV	1805	1822	0.20%	0.019%
92	31.793	4832	4834	4837	rVB2	1646	1921	0.21%	0.020%
93	31.934	4856	4858	4861	rBV4	2266	3158	0.34%	0.032%
94	32.345	4927	4928	4931	rVB3	3197	2453	0.26%	0.025%
95	32.369	4931	4932	4936	rVB3	3315	2519	0.27%	0.026%
96	32.404	4936	4938	4941	rBV3	1842	2085	0.22%	0.021%
97	32.474	4949	4950	4953	rVB2	2938	2394	0.26%	0.024%
98	32.504	4953	4955	4956	rBV2	1847	1555	0.17%	0.016%
99	32.545	4958	4962	4964	rBV4	1595	2465	0.27%	0.025%
100	32.574	4964	4967	4969	rBV3	1474	1749	0.19%	0.018%




Sum of corrected areas: 9825500

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059115.D
Acq On : 20 Sep 2023 18:49
Operator : MA/JU
Sample : PB155510BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

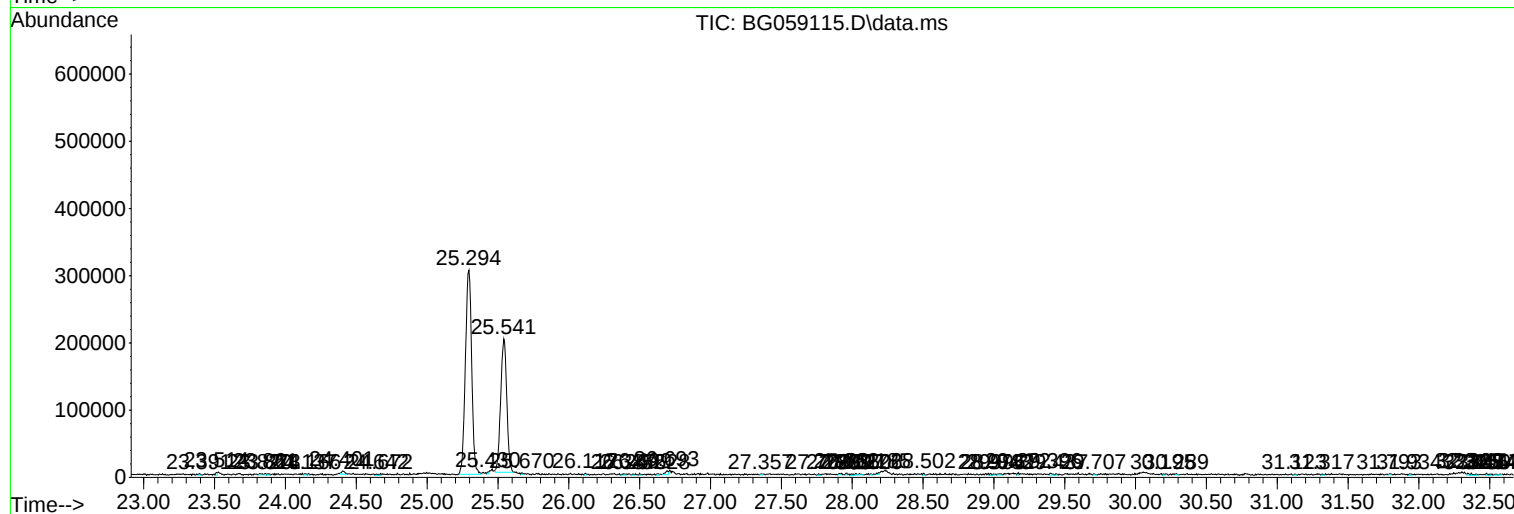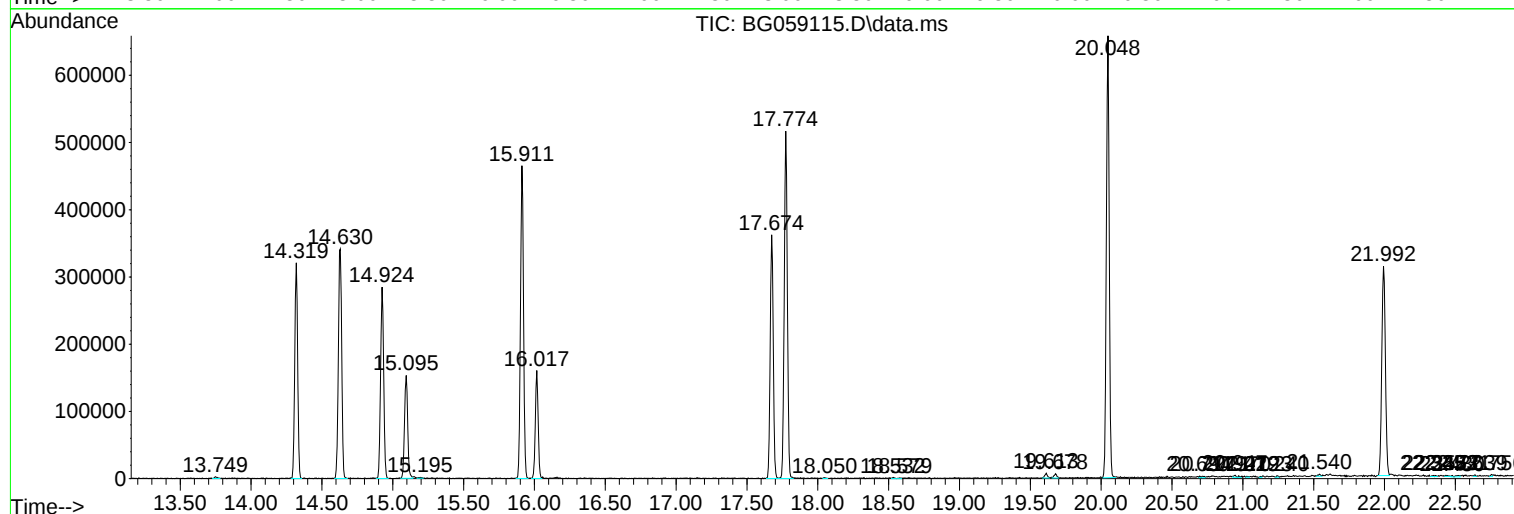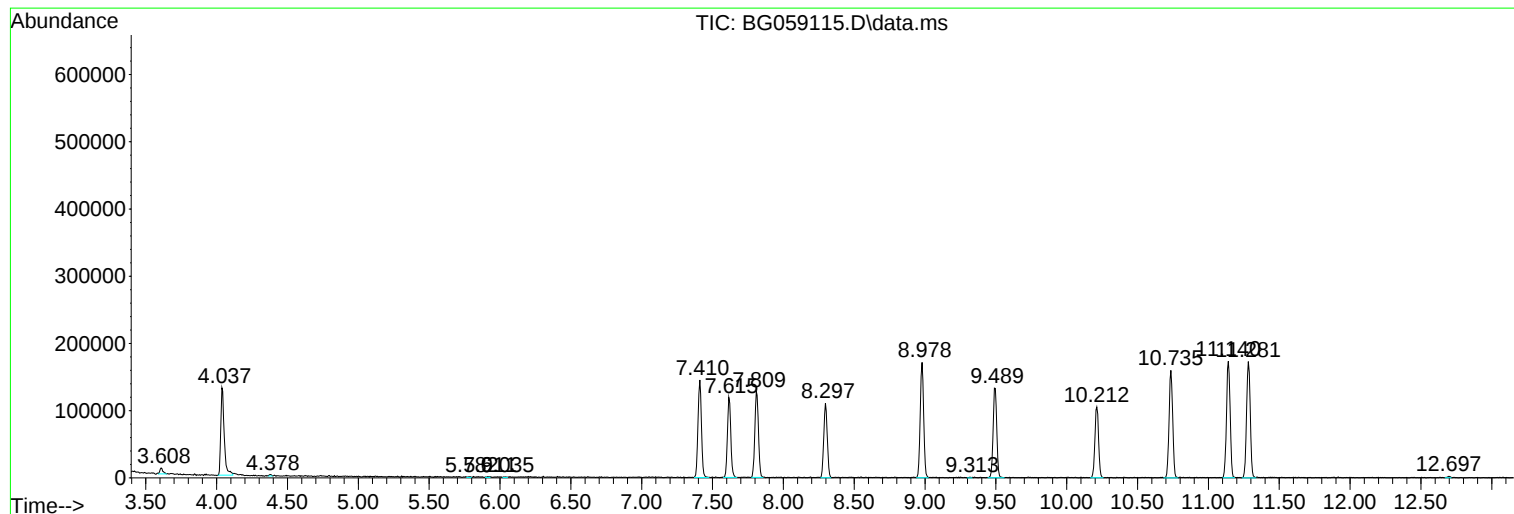

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059115.D
Acq On : 20 Sep 2023 18:49
Operator : MA/JU
Sample : PB155510BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059115.D
Acq On : 20 Sep 2023 18:49
Operator : MA/JU
Sample : PB155510BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK510

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc