

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059127.D
 Acq On : 21 Sep 2023 3:02
 Operator : MA/JU
 Sample : 04344-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.606	34	37	44	rVB3	10539	15647	0.99%	0.117%
2	3.777	64	66	71	rVB5	2373	3408	0.22%	0.026%
3	4.041	106	111	120	rBV	63062	102445	6.47%	0.769%
4	4.258	142	148	153	rBV3	7723	12172	0.77%	0.091%
5	4.382	164	169	174	rVB4	2544	4725	0.30%	0.035%
6	4.916	255	260	265	rBV3	5875	8429	0.53%	0.063%
7	7.408	677	684	691	rVB	40030	65096	4.11%	0.488%
8	7.613	711	719	728	rBV	159480	265745	16.77%	1.994%
9	7.813	745	753	762	rBV	134782	231370	14.60%	1.736%
10	8.295	828	835	844	rBV	124819	205955	13.00%	1.546%
11	8.976	944	951	960	rVB	114439	198491	12.53%	1.489%
12	9.493	1031	1039	1046	rBV	191353	335609	21.18%	2.518%
13	10.210	1154	1161	1168	rBV	154460	264467	16.69%	1.985%
14	10.733	1241	1250	1260	rBV	223128	387734	24.47%	2.910%
15	11.139	1312	1319	1326	rBV	193005	345209	21.79%	2.590%
16	11.280	1335	1343	1352	rVB	220865	400512	25.28%	3.005%
17	12.073	1468	1478	1484	rBV	92990	178625	11.27%	1.340%
18	12.696	1579	1584	1588	rVB	3973	5565	0.35%	0.042%
19	13.753	1758	1764	1768	rBV2	6115	9506	0.60%	0.071%
20	14.317	1853	1860	1867	rVB	458717	661690	41.76%	4.965%
21	14.629	1906	1913	1920	rBV2	538027	820916	51.81%	6.160%
22	14.922	1957	1963	1970	rBV	314429	492525	31.09%	3.696%
23	15.093	1987	1992	2000	rBV2	48882	71963	4.54%	0.540%
24	15.263	2017	2021	2026	rBV4	2475	3903	0.25%	0.029%
25	15.915	2125	2132	2139	rBV	670503	1037303	65.47%	7.784%
26	16.015	2143	2149	2158	rBV	272314	390306	24.63%	2.929%
27	16.150	2165	2172	2175	rBV2	2971	5237	0.33%	0.039%
28	17.449	2392	2393	2398	rBV	1584	2536	0.16%	0.019%
29	17.672	2424	2431	2441	rBV	407419	627245	39.59%	4.707%
30	17.778	2441	2449	2457	rBV2	825133	1272238	80.30%	9.547%
31	17.913	2468	2472	2475	rBV	1339	2182	0.14%	0.016%
32	18.489	2567	2570	2580	rBV3	19875	30923	1.95%	0.232%
33	18.630	2590	2594	2597	rBV4	6939	9624	0.61%	0.072%
34	18.847	2628	2631	2637	rBV	12059	15572	0.98%	0.117%
35	19.106	2671	2675	2678	rBV2	8281	9131	0.58%	0.069%
36	19.441	2730	2732	2734	rBV2	3162	2986	0.19%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059127.D
 Acq On : 21 Sep 2023 3:02
 Operator : MA/JU
 Sample : 04344-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBJH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

37	19.499	2739	2742	2745	rBV2	2663	2893	0.18%	0.022%
38	19.611	2755	2761	2764	rBV3	15107	22004	1.39%	0.165%
39	19.640	2764	2766	2767	rVV2	6548	5521	0.35%	0.041%
40	19.681	2769	2773	2779	rVB2	11483	17870	1.13%	0.134%
41	19.752	2782	2785	2789	rBV5	8289	11427	0.72%	0.086%
42	19.893	2806	2809	2814	rBV4	8095	10660	0.67%	0.080%
43	20.046	2829	2835	2842	rBV	1077150	1535084	96.89%	11.519%
44	20.251	2867	2870	2875	rBV3	3084	4929	0.31%	0.037%
45	20.428	2899	2900	2903	rBV2	2490	2536	0.16%	0.019%
46	20.939	2985	2987	2991	rVB5	6102	7496	0.47%	0.056%
47	20.992	2995	2996	2999	rBV3	2524	3106	0.20%	0.023%
48	21.144	3020	3022	3025	rVB4	4237	3373	0.21%	0.025%
49	21.550	3085	3091	3097	rBV6	7849	23066	1.46%	0.173%
50	21.685	3112	3114	3118	rVB3	3174	3152	0.20%	0.024%
51	21.732	3120	3122	3123	rBV2	2882	2297	0.14%	0.017%
52	21.991	3160	3166	3176	rVB2	369955	643918	40.64%	4.832%
53	22.766	3296	3298	3300	rBV2	3607	3754	0.24%	0.028%
54	22.825	3306	3308	3310	rBV3	3979	3367	0.21%	0.025%
55	22.995	3335	3337	3342	rVB5	2159	2814	0.18%	0.021%
56	23.524	3422	3427	3433	rVB4	8221	15825	1.00%	0.119%
57	23.736	3457	3463	3468	rBV4	9392	17694	1.12%	0.133%
58	23.877	3485	3487	3490	rBV4	2529	3080	0.19%	0.023%
59	23.953	3497	3500	3502	rBV3	1971	2134	0.13%	0.016%
60	24.012	3508	3510	3513	rVB4	3190	2213	0.14%	0.017%
61	24.399	3571	3576	3577	rBV4	12373	16549	1.04%	0.124%
62	24.899	3657	3661	3662	rBV3	2137	2757	0.17%	0.021%
63	25.298	3716	3729	3746	rBV2	522610	1584356	100.00%	11.889%
64	25.445	3749	3754	3760	rVV3	16387	43964	2.77%	0.330%
65	25.539	3761	3770	3782	rVB	232421	717961	45.32%	5.388%
66	26.709	3960	3969	3977	rBV5	16518	50204	3.17%	0.377%
67	27.231	4055	4058	4061	rBV4	2029	2730	0.17%	0.020%
68	28.160	4214	4216	4217	rBV	2648	2188	0.14%	0.016%
69	28.213	4218	4225	4228	rBV7	14249	29976	1.89%	0.225%
70	29.041	4365	4366	4368	rVB2	3838	2121	0.13%	0.016%
71	29.382	4422	4424	4426	rBV2	1914	2089	0.13%	0.016%
72	29.476	4439	4440	4443	rBV3	3054	2752	0.17%	0.021%
73	29.811	4495	4497	4499	rBV2	2373	2371	0.15%	0.018%
74	29.852	4503	4504	4508	rBV3	2218	2428	0.15%	0.018%
75	30.016	4528	4532	4533	rBV3	5971	6114	0.39%	0.046%
76	30.710	4648	4650	4653	rVB	2791	2309	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059127.D
Acq On : 21 Sep 2023 3:02
Operator : MA/JU
Sample : 04344-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJH3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Title : SVOA CALIBRATION

77	31.121	4718	4720	4722	rBV2	2063	2302	0.15%	0.017%
78	31.456	4774	4777	4778	rBV	2236	2333	0.15%	0.018%
79	32.613	4971	4974	4976	rBV3	2557	3323	0.21%	0.025%



Sum of corrected areas: 13326030

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059127.D
Acq On : 21 Sep 2023 3:02
Operator : MA/JU
Sample : 04344-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

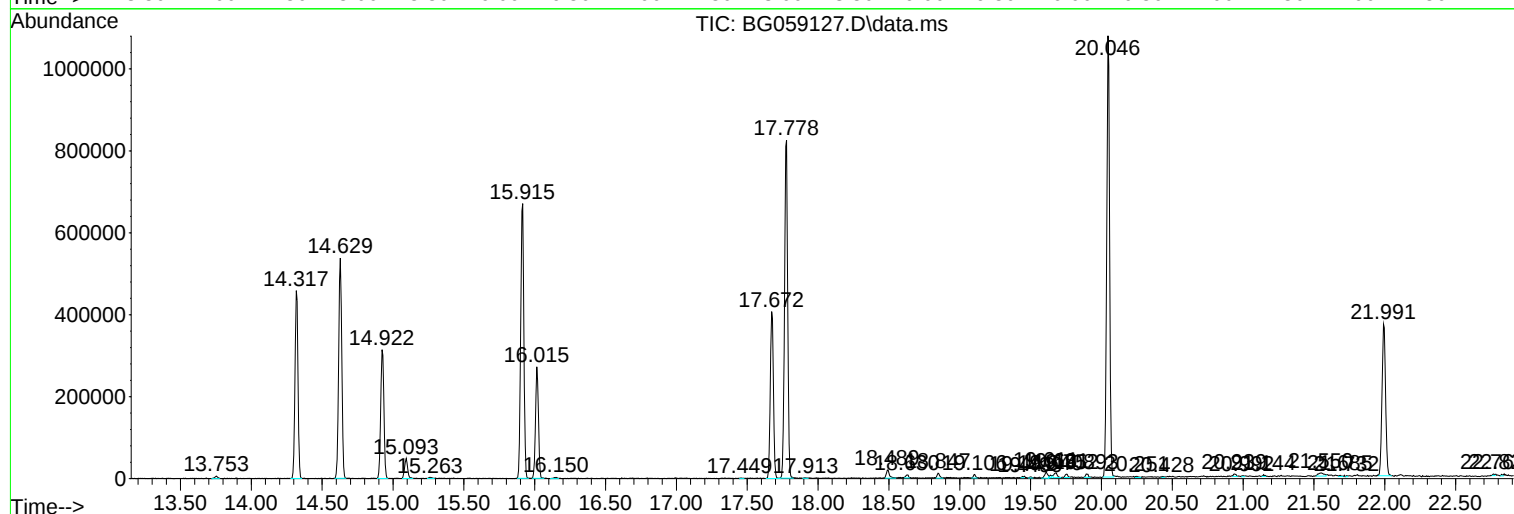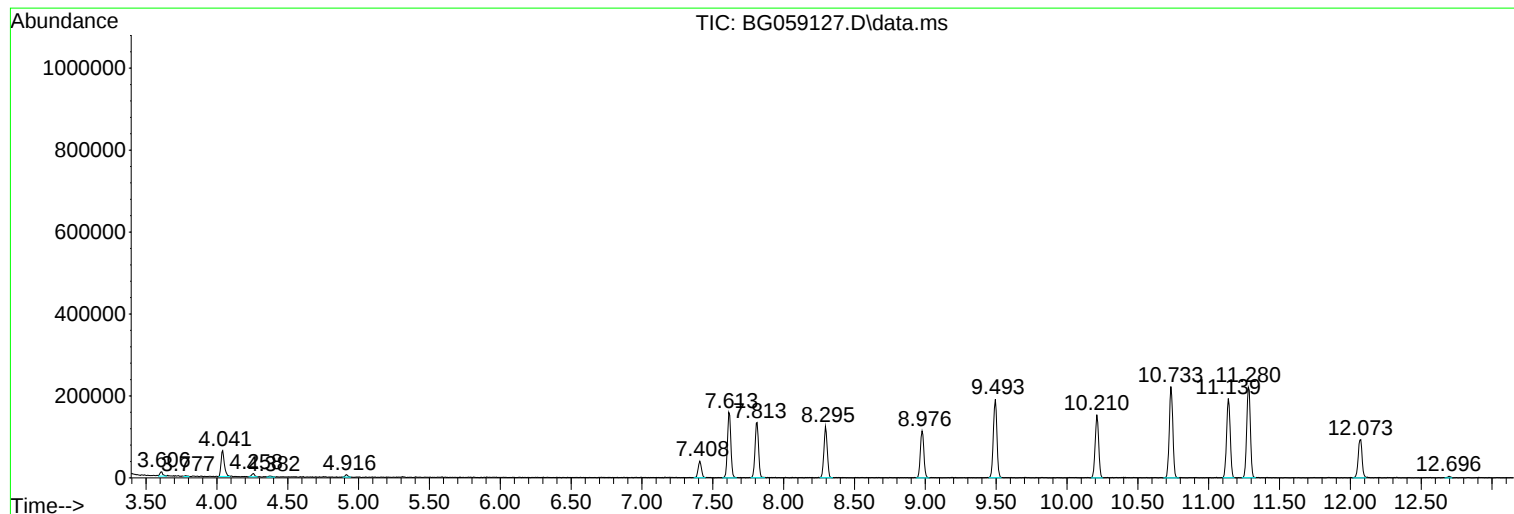

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059127.D
Acq On : 21 Sep 2023 3:02
Operator : MA/JU
Sample : 04344-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059127.D
Acq On : 21 Sep 2023 3:02
Operator : MA/JU
Sample : 04344-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBJH3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc