

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059129.D
 Acq On : 21 Sep 2023 5:03
 Operator : MA/JU
 Sample : PB155513BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK513

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059129.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.605	33	37	43	rVB3	11653	17065	1.38%	0.128%
2	4.039	106	111	122	rBV	168893	283390	22.85%	2.133%
3	4.374	164	168	172	rBV4	1696	3048	0.25%	0.023%
4	5.079	283	288	290	rVB4	1480	2292	0.18%	0.017%
5	5.667	384	388	390	rBV	1212	1854	0.15%	0.014%
6	6.137	463	468	469	rBV	1436	1770	0.14%	0.013%
7	7.406	678	684	693	rVB	189880	322189	25.98%	2.426%
8	7.617	711	720	727	rBV	150532	249373	20.11%	1.877%
9	7.811	745	753	759	rBV	175772	298013	24.03%	2.244%
10	8.293	829	835	843	rVB	147162	244597	19.73%	1.841%
11	8.975	944	951	961	rVB	219738	386327	31.16%	2.908%
12	9.492	1032	1039	1046	rBV	178648	311484	25.12%	2.345%
13	10.209	1154	1161	1168	rVB2	139153	249553	20.13%	1.879%
14	10.731	1243	1250	1260	rBV	219005	378739	30.54%	2.851%
15	11.137	1311	1319	1326	rBV	217307	389983	31.45%	2.936%
16	11.284	1336	1344	1351	rBV	221827	410728	33.12%	3.092%
17	12.694	1580	1584	1588	rBV2	3309	4590	0.37%	0.035%
18	13.751	1761	1764	1770	rVB2	5390	7792	0.63%	0.059%
19	14.315	1854	1860	1867	rBV	419068	630502	50.85%	4.747%
20	14.627	1905	1913	1921	rBV	504382	772849	62.33%	5.818%
21	14.927	1955	1964	1971	rBB	371753	587595	47.39%	4.424%
22	15.097	1985	1993	2000	rBV	208546	333156	26.87%	2.508%
23	15.197	2008	2010	2012	rVB	2131	1894	0.15%	0.014%
24	15.914	2125	2132	2141	rVB	630211	951179	76.71%	7.161%
25	16.019	2143	2150	2157	rVV	223012	324299	26.15%	2.441%
26	16.149	2169	2172	2177	rVB	3003	4426	0.36%	0.033%
27	17.676	2424	2432	2438	rBV	475241	724316	58.41%	5.453%
28	17.776	2442	2449	2457	rVV2	676299	1077342	86.88%	8.110%
29	18.593	2586	2588	2592	rVB2	1169	1711	0.14%	0.013%
30	19.609	2756	2761	2766	rVB4	8966	13183	1.06%	0.099%
31	19.680	2768	2773	2778	rVB4	8406	12209	0.98%	0.092%
32	19.897	2806	2810	2813	rBV3	1854	2762	0.22%	0.021%
33	20.050	2829	2836	2842	rBV	831627	1226508	98.91%	9.233%
34	20.696	2944	2946	2948	rBV3	1731	1855	0.15%	0.014%
35	20.937	2985	2987	2990	rBV3	2787	3176	0.26%	0.024%
36	20.996	2995	2997	3000	rVB3	3016	2698	0.22%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059129.D
 Acq On : 21 Sep 2023 5:03
 Operator : MA/JU
 Sample : PB155513BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK513

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

37	21.155	3022	3024	3027	rBV2	1680	2151	0.17%	0.016%
38	21.254	3038	3041	3042	rBV2	1996	1976	0.16%	0.015%
39	21.536	3086	3089	3091	rBV4	3711	4994	0.40%	0.038%
40	21.848	3140	3142	3146	rVB4	1524	1932	0.16%	0.015%

41	21.995	3160	3167	3174	rBV2	401481	713481	57.54%	5.371%
42	22.206	3199	3203	3204	rBV3	2000	2328	0.19%	0.018%
43	22.341	3224	3226	3228	rBV3	1994	1738	0.14%	0.013%
44	22.359	3228	3229	3234	rVB5	2596	1958	0.16%	0.015%
45	22.770	3295	3299	3301	rBV5	4134	5737	0.46%	0.043%

46	22.982	3331	3335	3336	rBV3	2410	2398	0.19%	0.018%
47	23.522	3422	3427	3430	rVV5	6973	10663	0.86%	0.080%
48	23.552	3430	3432	3434	rVB	2311	1640	0.13%	0.012%
49	23.793	3471	3473	3475	rVB2	2261	1637	0.13%	0.012%
50	23.816	3475	3477	3479	rVB3	2258	1712	0.14%	0.013%

51	23.992	3505	3507	3509	rBV2	1817	1993	0.16%	0.015%
52	24.204	3541	3543	3546	rBV4	2032	1910	0.15%	0.014%
53	24.404	3572	3577	3585	rVB6	12127	27333	2.20%	0.206%
54	24.703	3627	3628	3632	rBV3	1829	2717	0.22%	0.020%
55	24.921	3663	3665	3668	rBV4	2606	2669	0.22%	0.020%

56	24.956	3668	3671	3672	rBV3	3114	3372	0.27%	0.025%
57	25.291	3717	3728	3745	rVB2	423644	1239969	100.00%	9.335%
58	25.402	3745	3747	3748	rBV2	3301	3185	0.26%	0.024%
59	25.449	3748	3755	3760	rVV5	14774	43760	3.53%	0.329%
60	25.538	3760	3770	3785	rVB	263461	810162	65.34%	6.099%

61	26.348	3907	3908	3911	rVB3	3286	1925	0.16%	0.014%
62	26.372	3911	3912	3916	rBV3	2425	2333	0.19%	0.018%
63	26.425	3919	3921	3923	rBV2	1972	1890	0.15%	0.014%
64	26.707	3961	3969	3976	rBV4	14785	41196	3.32%	0.310%
65	27.036	4023	4025	4030	rBV3	1403	2081	0.17%	0.016%

66	27.600	4119	4121	4124	rBV3	2711	1971	0.16%	0.015%
67	27.735	4140	4144	4146	rBV2	1848	2568	0.21%	0.019%
68	28.082	4199	4203	4204	rBV3	1861	2149	0.17%	0.016%
69	28.217	4215	4226	4238	rVB7	16452	62644	5.05%	0.472%
70	28.334	4244	4246	4250	rBV3	2370	3030	0.24%	0.023%

71	28.887	4338	4340	4342	rBV2	1702	1747	0.14%	0.013%
72	29.269	4404	4405	4408	rVB3	2872	1734	0.14%	0.013%
73	29.298	4408	4410	4412	rBV2	2507	1962	0.16%	0.015%
74	29.316	4412	4413	4415	rBV2	2207	1618	0.13%	0.012%
75	29.985	4525	4527	4528	rBV2	2137	1735	0.14%	0.013%

76	30.403	4597	4598	4600	rBV2	2598	1992	0.16%	0.015%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059129.D
Acq On : 21 Sep 2023 5:03
Operator : MA/JU
Sample : PB155513BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK513

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Title : SVOA CALIBRATION

77	30.502	4613	4615	4616	rBV2	1867	1649	0.13%	0.012%
78	30.573	4625	4627	4631	rVB5	2382	2012	0.16%	0.015%
79	31.519	4786	4788	4791	rBV4	1668	1635	0.13%	0.012%
80	31.895	4851	4852	4855	rBV3	2807	2724	0.22%	0.021%
81	32.012	4870	4872	4874	rBV2	1676	1616	0.13%	0.012%
82	32.148	4893	4895	4896	rBV2	2964	2702	0.22%	0.020%
83	32.247	4909	4912	4914	rBV4	5770	8290	0.67%	0.062%
84	32.441	4943	4945	4947	rBV2	1572	1665	0.13%	0.013%
85	32.559	4964	4965	4968	rBV3	2440	2599	0.21%	0.020%




Sum of corrected areas: 13283329

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059129.D
Acq On : 21 Sep 2023 5:03
Operator : MA/JU
Sample : PB155513BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

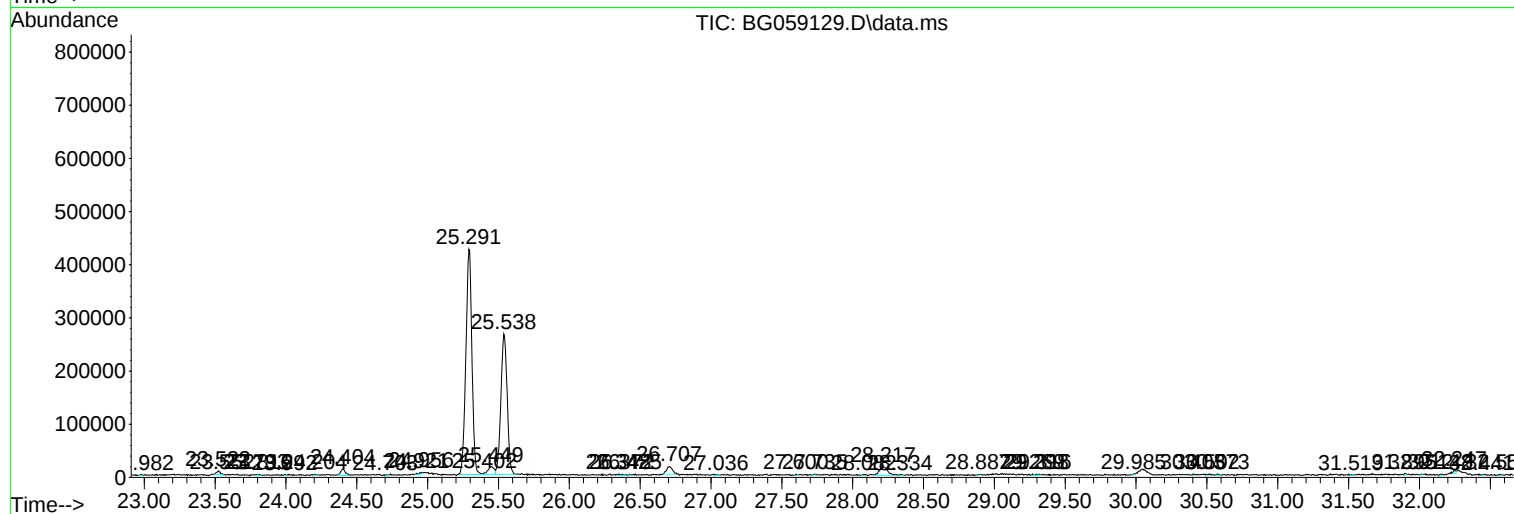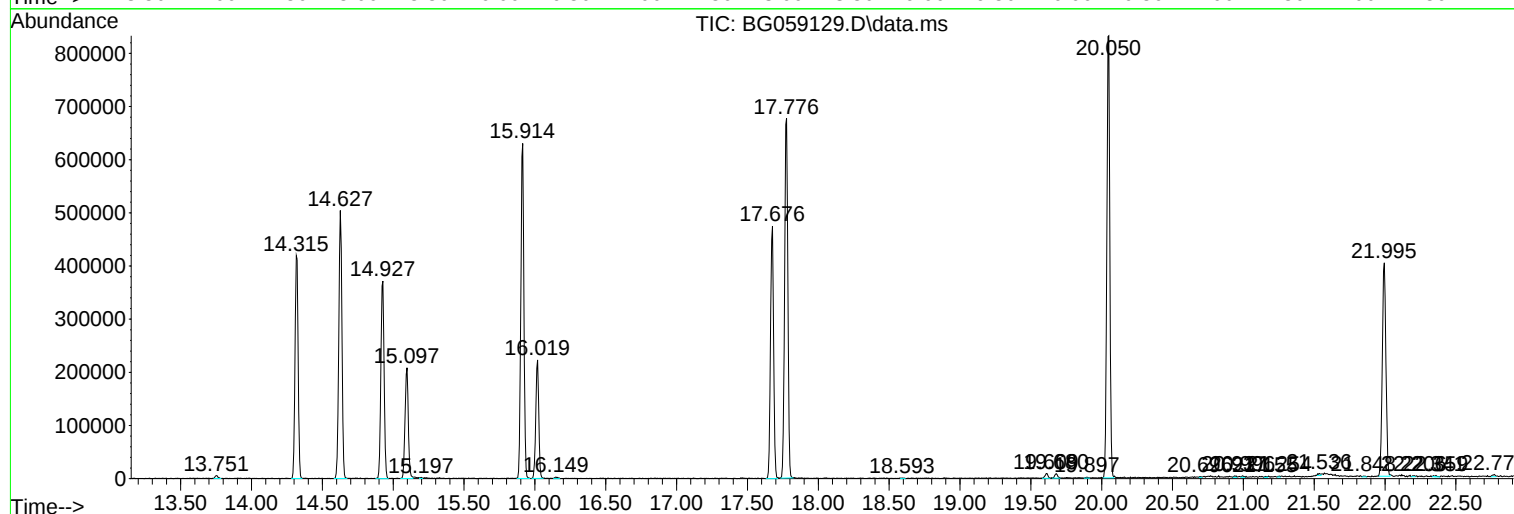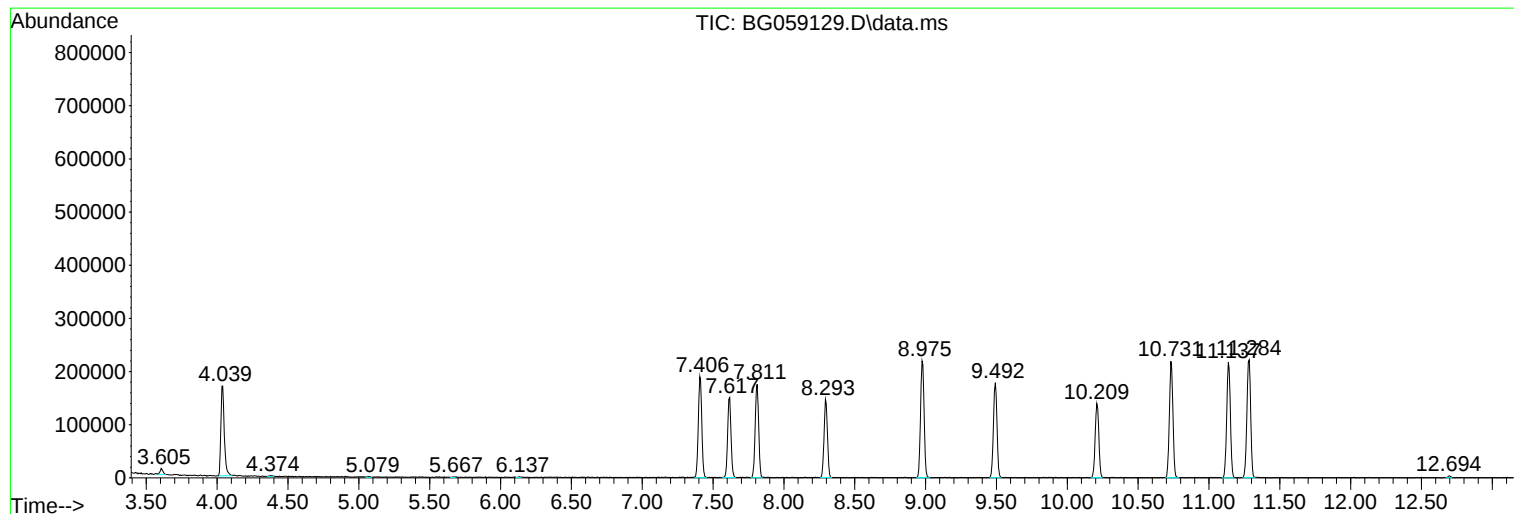

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059129.D
Acq On : 21 Sep 2023 5:03
Operator : MA/JU
Sample : PB155513BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059129.D
Acq On : 21 Sep 2023 5:03
Operator : MA/JU
Sample : PB155513BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc