

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059130.D
 Acq On : 21 Sep 2023 5:44
 Operator : MA/JU
 Sample : PB155516BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK516

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.608	34	37	42	rVB3	10880	15448	1.30%	0.138%
2	3.996	102	103	105	rBV	2721	2154	0.18%	0.019%
3	4.037	105	110	123	rVB	115254	179045	15.09%	1.602%
4	4.372	165	167	171	rBV4	1559	2350	0.20%	0.021%
5	6.522	530	533	537	rVB2	1029	1601	0.13%	0.014%
6	6.763	572	574	578	rVB	1248	1589	0.13%	0.014%
7	7.409	677	684	694	rVB	166311	283091	23.86%	2.534%
8	7.615	713	719	727	rVB	137130	223084	18.80%	1.997%
9	7.809	745	752	759	rBV	153783	261224	22.02%	2.338%
10	8.297	828	835	844	rVB	102440	171474	14.45%	1.535%
11	8.426	853	857	861	rBV	1399	1668	0.14%	0.015%
12	8.978	943	951	959	rBV2	208888	355472	29.96%	3.181%
13	9.489	1031	1038	1046	rBV	157447	279000	23.51%	2.497%
14	10.212	1153	1161	1167	rBV	126741	224708	18.94%	2.011%
15	10.729	1241	1249	1259	rBV	192635	345145	29.09%	3.089%
16	11.140	1311	1319	1327	rVB	152053	276283	23.28%	2.473%
17	11.281	1335	1343	1350	rBV	152766	279525	23.56%	2.502%
18	12.127	1484	1487	1491	rBV	1507	1910	0.16%	0.017%
19	12.691	1576	1583	1592	rVB3	3310	5444	0.46%	0.049%
20	13.749	1759	1763	1769	rVB2	4662	6643	0.56%	0.059%
21	14.319	1854	1860	1867	rVB	406663	563004	47.45%	5.039%
22	14.625	1904	1912	1919	rBV	432742	700881	59.07%	6.273%
23	14.924	1956	1963	1972	rBV	262491	396193	33.39%	3.546%
24	15.095	1985	1992	1999	rBV	206485	317384	26.75%	2.841%
25	15.911	2124	2131	2138	rBV	605003	868435	73.19%	7.772%
26	16.017	2142	2149	2158	rBV	209604	302407	25.49%	2.706%
27	16.146	2168	2171	2175	rBV2	3189	4142	0.35%	0.037%
28	17.674	2424	2431	2437	rBV	349659	505975	42.64%	4.528%
29	17.774	2440	2448	2455	rBV2	657294	986956	83.18%	8.833%
30	17.991	2482	2485	2488	rVB2	1673	1813	0.15%	0.016%
31	18.837	2626	2629	2633	rBV	1048	1700	0.14%	0.015%
32	19.607	2756	2760	2766	rVB3	9686	12655	1.07%	0.113%
33	19.677	2768	2772	2777	rVB2	6928	11410	0.96%	0.102%
34	19.901	2807	2810	2813	rVB2	1558	1643	0.14%	0.015%
35	20.048	2828	2835	2842	rBV	803616	1153676	97.23%	10.325%
36	20.694	2942	2945	2946	rBV2	1820	2071	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059130.D
 Acq On : 21 Sep 2023 5:44
 Operator : MA/JU
 Sample : PB155516BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK516

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

37	20.935	2984	2986	2988	rBV2	2881	2764	0.23%	0.025%
38	21.082	3006	3011	3013	rBV2	1916	2731	0.23%	0.024%
39	21.311	3049	3050	3053	rBV	1793	1846	0.16%	0.017%
40	21.552	3083	3091	3094	rBV7	3019	8693	0.73%	0.078%

41	21.992	3158	3166	3173	rBV	298246	530738	44.73%	4.750%
42	22.274	3210	3214	3215	rBV3	2490	2739	0.23%	0.025%
43	22.962	3328	3331	3334	rVB3	1850	1813	0.15%	0.016%
44	23.279	3384	3385	3387	rVB	3203	1814	0.15%	0.016%
45	23.520	3424	3426	3430	rVB4	3615	4983	0.42%	0.045%

46	23.579	3434	3436	3441	rVB4	2109	2480	0.21%	0.022%
47	23.749	3461	3465	3467	rBV3	1677	2186	0.18%	0.020%
48	24.025	3508	3512	3514	rBV4	1363	1642	0.14%	0.015%
49	24.061	3516	3518	3520	rBV3	1478	1569	0.13%	0.014%
50	24.207	3541	3543	3544	rBV2	2085	1580	0.13%	0.014%

51	24.337	3562	3565	3568	rBV3	2053	2262	0.19%	0.020%
52	24.407	3570	3577	3582	rVB5	8271	17515	1.48%	0.157%
53	24.619	3610	3613	3614	rVB2	1717	1583	0.13%	0.014%
54	24.666	3619	3621	3624	rVB3	1935	2201	0.19%	0.020%
55	24.701	3624	3627	3629	rBV3	2218	2873	0.24%	0.026%

56	25.294	3715	3728	3742	rBV3	382178	1186559	100.00%	10.620%
57	25.447	3751	3754	3755	rBV3	4929	4725	0.40%	0.042%
58	25.541	3759	3770	3780	rVB3	189536	575439	48.50%	5.150%
59	25.717	3797	3800	3801	rBV3	2127	1894	0.16%	0.017%
60	25.759	3806	3807	3809	rBV2	2779	1715	0.14%	0.015%

61	26.669	3959	3962	3963	rBV2	3685	4207	0.35%	0.038%
62	26.693	3963	3966	3968	rVV4	6272	8220	0.69%	0.074%
63	26.763	3976	3978	3981	rVB2	1792	2068	0.17%	0.019%
64	26.863	3992	3995	3996	rBV2	2054	2152	0.18%	0.019%
65	27.016	4018	4021	4022	rBV2	2122	1697	0.14%	0.015%

66	27.222	4055	4056	4058	rBV	2387	2264	0.19%	0.020%
67	27.415	4087	4089	4091	rBV2	1589	1629	0.14%	0.015%
68	27.480	4098	4100	4103	rBV2	2376	2279	0.19%	0.020%
69	28.167	4214	4217	4218	rBV3	3220	3336	0.28%	0.030%
70	28.185	4218	4220	4221	rBV2	3861	3363	0.28%	0.030%

71	28.203	4221	4223	4224	rBV2	3721	2981	0.25%	0.027%
72	28.655	4295	4300	4302	rBV4	1570	2733	0.23%	0.024%
73	29.014	4359	4361	4363	rBV2	2100	1555	0.13%	0.014%
74	29.719	4478	4481	4483	rVB3	1938	1931	0.16%	0.017%
75	29.907	4511	4513	4515	rBV2	1853	1913	0.16%	0.017%

76	29.954	4519	4521	4524	rBV3	1885	2250	0.19%	0.020%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059130.D
Acq On : 21 Sep 2023 5:44
Operator : MA/JU
Sample : PB155516BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK516

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Title : SVOA CALIBRATION

77	29.995	4524	4528	4529	rBV2	3262	3222	0.27%	0.029%
78	30.012	4529	4531	4532	rBV	2313	1533	0.13%	0.014%
79	30.036	4532	4535	4536	rBV2	3256	3364	0.28%	0.030%
80	30.459	4605	4607	4609	rVB2	2029	1568	0.13%	0.014%
81	30.518	4616	4617	4620	rVB2	2022	1749	0.15%	0.016%
82	31.252	4740	4742	4743	rBV	2610	2187	0.18%	0.020%
83	32.004	4868	4870	4871	rBV2	2130	1750	0.15%	0.016%
84	32.457	4945	4947	4950	rBV2	1881	1868	0.16%	0.017%




Sum of corrected areas: 11173366

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059130.D
Acq On : 21 Sep 2023 5:44
Operator : MA/JU
Sample : PB155516BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

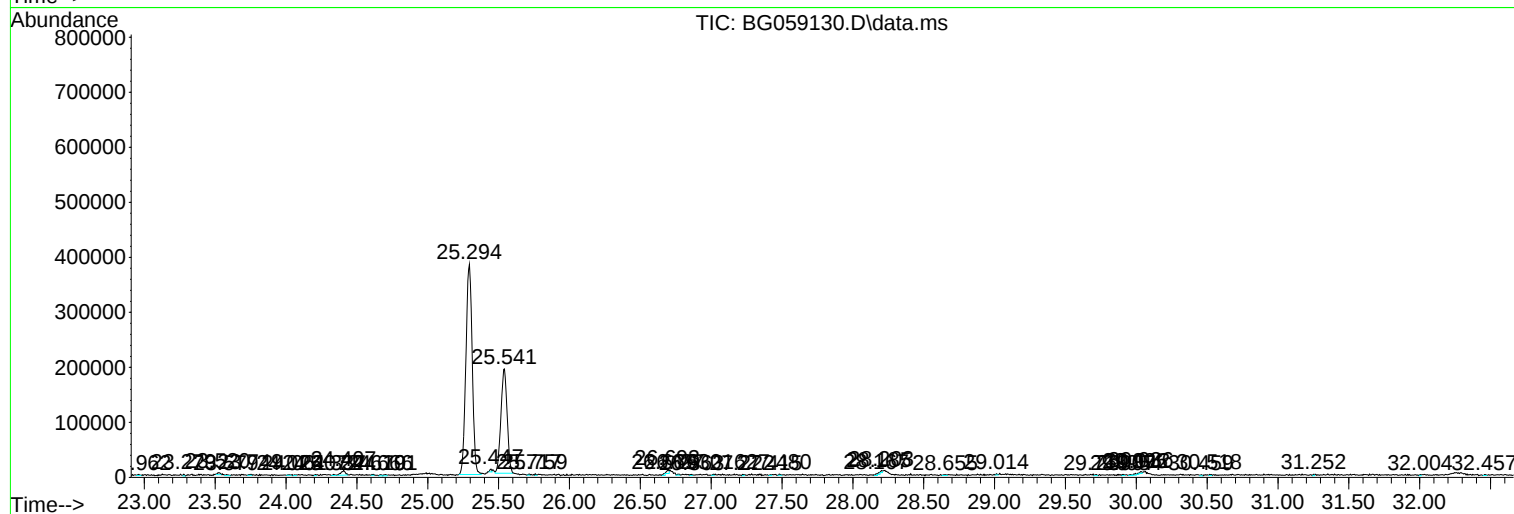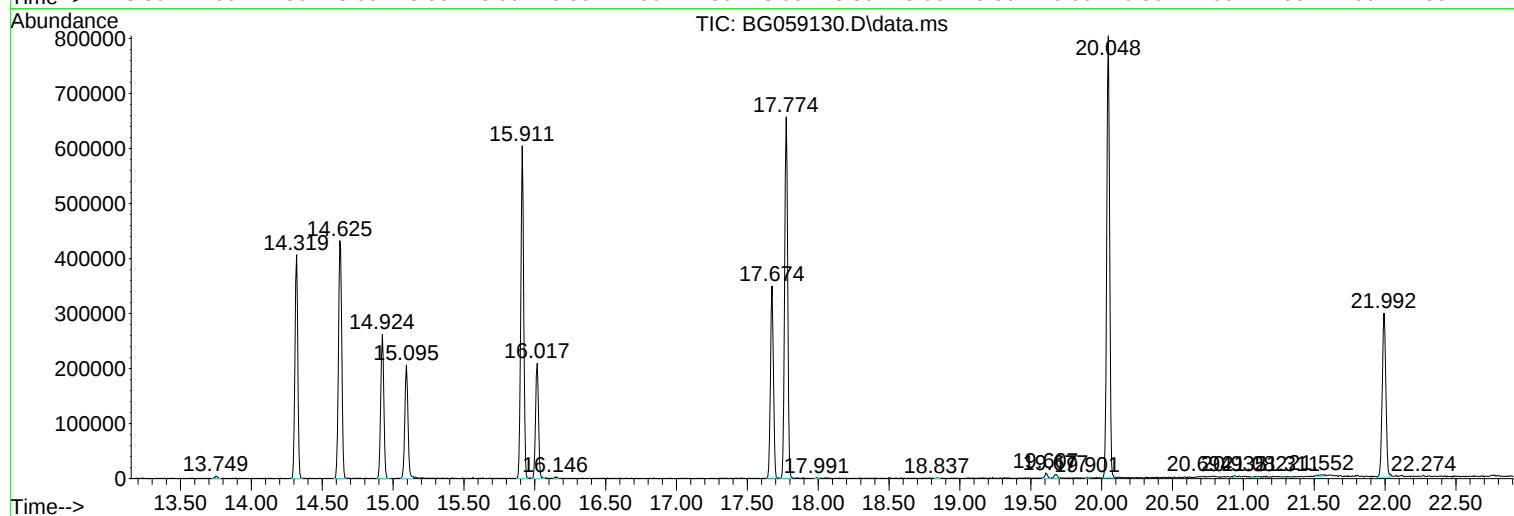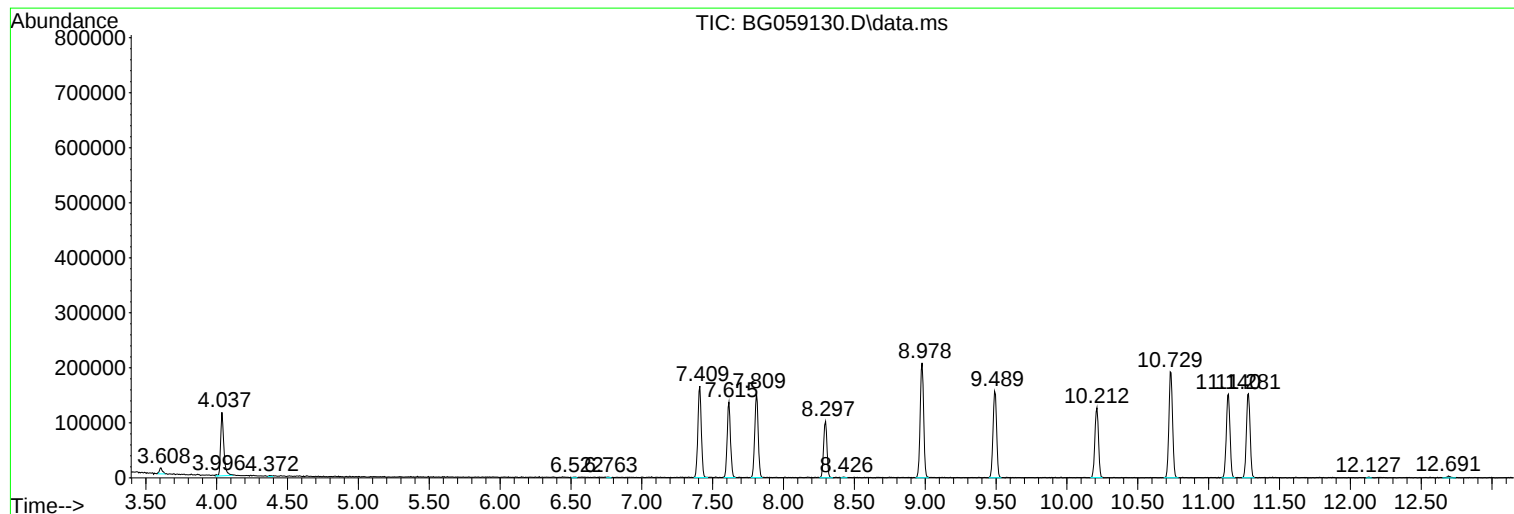

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059130.D
Acq On : 21 Sep 2023 5:44
Operator : MA/JU
Sample : PB155516BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059130.D
Acq On : 21 Sep 2023 5:44
Operator : MA/JU
Sample : PB155516BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK516

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------