

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059143.D
 Acq On : 21 Sep 2023 17:20
 Operator : MA/JU
 Sample : PB155604BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.610	34	38	42	rVB3	8429	11908	1.18%	0.117%
2	4.039	106	111	122	rBV	142685	227419	22.51%	2.237%
3	4.292	151	154	156	rBV2	1716	1685	0.17%	0.017%
4	4.627	208	211	214	rBV3	1045	1410	0.14%	0.014%
5	4.750	227	232	233	rBV4	1444	1696	0.17%	0.017%
6	5.831	414	416	421	rVB	1187	1598	0.16%	0.016%
7	6.390	508	511	514	rBV	1280	1519	0.15%	0.015%
8	6.630	549	552	554	rBV2	1591	1923	0.19%	0.019%
9	7.406	678	684	691	rBV	143524	250107	24.75%	2.460%
10	7.612	713	719	729	rVB	117254	196131	19.41%	1.929%
11	7.811	746	753	760	rBV2	134520	228152	22.58%	2.244%
12	7.964	778	779	783	rBV	948	1357	0.13%	0.013%
13	8.005	783	786	788	rVV2	1488	1718	0.17%	0.017%
14	8.064	792	796	797	rVB	1279	1568	0.16%	0.015%
15	8.293	828	835	842	rVB	99422	170114	16.84%	1.673%
16	8.493	866	869	872	rBV	1135	1518	0.15%	0.015%
17	8.975	944	951	964	rVB	171657	301043	29.79%	2.961%
18	9.492	1031	1039	1047	rVB	135428	233813	23.14%	2.300%
19	10.209	1154	1161	1169	rVB2	111040	195747	19.37%	1.925%
20	10.731	1243	1250	1259	rBV	173155	302235	29.91%	2.973%
21	11.137	1312	1319	1327	rVB	156428	280109	27.72%	2.755%
22	11.278	1337	1343	1352	rVB	184307	327539	32.42%	3.222%
23	12.700	1579	1585	1589	rBV2	3017	5147	0.51%	0.051%
24	13.346	1694	1695	1702	rBV	1025	1596	0.16%	0.016%
25	13.428	1706	1709	1713	rVB	1112	1387	0.14%	0.014%
26	13.751	1758	1764	1769	rBV5	3966	6454	0.64%	0.063%
27	14.316	1854	1860	1867	rBV	320671	481277	47.63%	4.734%
28	14.627	1904	1913	1920	rBV	385145	594955	58.88%	5.852%
29	14.927	1957	1964	1971	rVB	255041	397371	39.33%	3.908%
30	15.097	1986	1993	2007	rBV	163485	264688	26.20%	2.603%
31	15.914	2124	2132	2139	rBV	484535	734158	72.66%	7.221%
32	16.014	2144	2149	2156	rBV	161259	239340	23.69%	2.354%
33	16.143	2168	2171	2177	rVB	2487	3884	0.38%	0.038%
34	16.190	2177	2179	2185	rBV	1099	1382	0.14%	0.014%
35	17.071	2326	2329	2333	rBV	886	1521	0.15%	0.015%
36	17.465	2393	2396	2399	rBV	1148	1484	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059143.D
 Acq On : 21 Sep 2023 17:20
 Operator : MA/JU
 Sample : PB155604BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

37	17.676	2425	2432	2439	rBV	327673	509132	50.39%	5.008%
38	17.776	2441	2449	2459	rVV	562246	858022	84.92%	8.439%
39	17.876	2461	2466	2469	rVB	1168	2041	0.20%	0.020%
40	17.905	2469	2471	2477	rBV3	1888	2472	0.24%	0.024%

41	18.652	2594	2598	2601	rBV	825	1370	0.14%	0.013%
42	19.139	2677	2681	2682	rBV	1181	1502	0.15%	0.015%
43	19.609	2756	2761	2768	rBV3	6884	12027	1.19%	0.118%
44	19.674	2768	2772	2777	rVV2	6899	9425	0.93%	0.093%
45	19.897	2807	2810	2814	rBV2	2604	3178	0.31%	0.031%

46	20.044	2829	2835	2843	rVB	667190	968840	95.89%	9.529%
47	20.191	2858	2860	2864	rVB4	1660	1665	0.16%	0.016%
48	20.256	2869	2871	2874	rVB3	2026	1828	0.18%	0.018%
49	20.497	2909	2912	2917	rVB3	2065	2843	0.28%	0.028%
50	20.567	2922	2924	2927	rBV2	1315	1655	0.16%	0.016%

51	20.802	2960	2964	2966	rBV2	1800	2383	0.24%	0.023%
52	20.867	2974	2975	2977	rBV2	2426	1662	0.16%	0.016%
53	21.507	3081	3084	3085	rBV3	2390	2095	0.21%	0.021%
54	21.807	3133	3135	3138	rBV3	2217	1603	0.16%	0.016%
55	21.995	3159	3167	3177	rBV	296808	528492	52.31%	5.198%

56	22.365	3228	3230	3232	rBV3	1623	1436	0.14%	0.014%
57	22.500	3251	3253	3255	rVB3	2450	1780	0.18%	0.018%
58	22.524	3255	3257	3258	rBV2	2456	1348	0.13%	0.013%
59	22.559	3261	3263	3264	rBV	2213	1349	0.13%	0.013%
60	22.759	3294	3297	3299	rBV3	4296	5911	0.59%	0.058%

61	22.811	3304	3306	3309	rBV3	2627	2154	0.21%	0.021%
62	22.870	3315	3316	3320	rVB4	3462	3514	0.35%	0.035%
63	23.017	3339	3341	3342	rVB2	3453	1894	0.19%	0.019%
64	23.516	3423	3426	3427	rBV2	4178	4430	0.44%	0.044%
65	24.133	3529	3531	3532	rBV	2086	1738	0.17%	0.017%

66	24.398	3569	3576	3581	rBV6	9877	24620	2.44%	0.242%
67	24.556	3601	3603	3604	rBV2	3220	2433	0.24%	0.024%
68	24.633	3614	3616	3617	rBV2	2783	1834	0.18%	0.018%
69	24.709	3627	3629	3632	rBV3	3151	3292	0.33%	0.032%
70	25.291	3716	3728	3743	rBV2	339189	1010402	100.00%	9.938%

71	25.538	3759	3770	3781	rVB3	193792	584131	57.81%	5.745%
72	25.943	3837	3839	3841	rBV3	2063	2058	0.20%	0.020%
73	26.066	3858	3860	3863	rBV3	2184	2222	0.22%	0.022%
74	26.196	3880	3882	3883	rBV2	2739	1945	0.19%	0.019%
75	26.254	3890	3892	3893	rBV2	2602	1825	0.18%	0.018%

76	26.319	3901	3903	3905	rBV2	2137	1966	0.19%	0.019%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059143.D
 Acq On : 21 Sep 2023 17:20
 Operator : MA/JU
 Sample : PB155604BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

77	26.343	3905	3907	3908	rBV	2663	1510	0.15%	0.015%
78	26.689	3963	3966	3982	rVB8	12988	40061	3.96%	0.394%
79	26.860	3993	3995	3996	rBV2	2392	1873	0.19%	0.018%
80	26.942	4007	4009	4013	rBV5	2469	2951	0.29%	0.029%
81	27.265	4063	4064	4067	rBV2	2983	2721	0.27%	0.027%
82	27.477	4096	4100	4101	rBV4	2187	2180	0.22%	0.021%
83	27.529	4108	4109	4112	rVB3	2580	1603	0.16%	0.016%
84	27.606	4120	4122	4124	rBV3	2702	2186	0.22%	0.022%
85	27.988	4185	4187	4191	rBV4	2123	3627	0.36%	0.036%
86	28.205	4217	4224	4229	rBV5	11615	31655	3.13%	0.311%
87	28.470	4267	4269	4272	rBV4	1811	1828	0.18%	0.018%
88	28.534	4276	4280	4281	rBV4	1855	2229	0.22%	0.022%
89	28.710	4308	4310	4313	rBV3	2142	1790	0.18%	0.018%
90	29.415	4428	4430	4433	rBV2	2429	1859	0.18%	0.018%
91	29.539	4449	4451	4453	rBV2	1974	1843	0.18%	0.018%
92	29.645	4467	4469	4470	rBV2	2102	1762	0.17%	0.017%
93	30.209	4564	4565	4568	rBV2	1464	1529	0.15%	0.015%
94	30.984	4695	4697	4698	rBV	2759	1410	0.14%	0.014%
95	31.143	4722	4724	4726	rBV2	2315	1614	0.16%	0.016%
96	31.466	4778	4779	4781	rBV2	2582	1825	0.18%	0.018%
97	31.736	4823	4825	4827	rVB2	2274	1432	0.14%	0.014%
98	32.124	4889	4891	4894	rBV3	2611	2839	0.28%	0.028%
99	32.200	4902	4904	4905	rBV2	3626	2231	0.22%	0.022%
100	32.459	4946	4948	4953	rVB5	2536	2925	0.29%	0.029%




Sum of corrected areas: 10166953

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059143.D
Acq On : 21 Sep 2023 17:20
Operator : MA/JU
Sample : PB155604BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK604

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

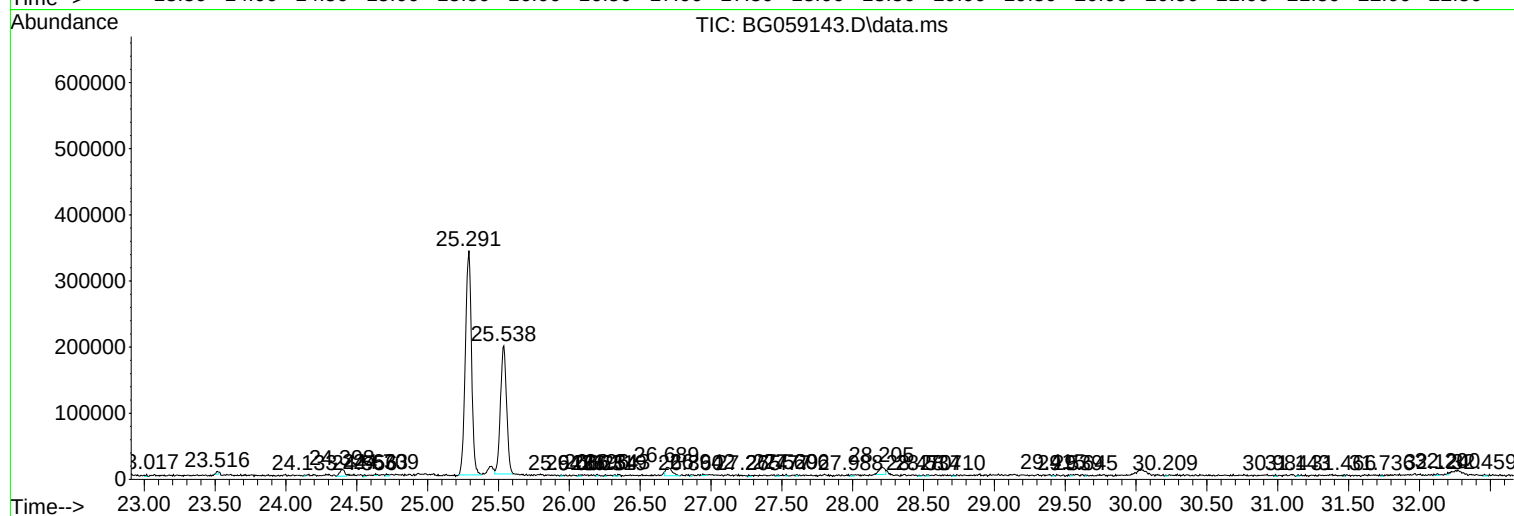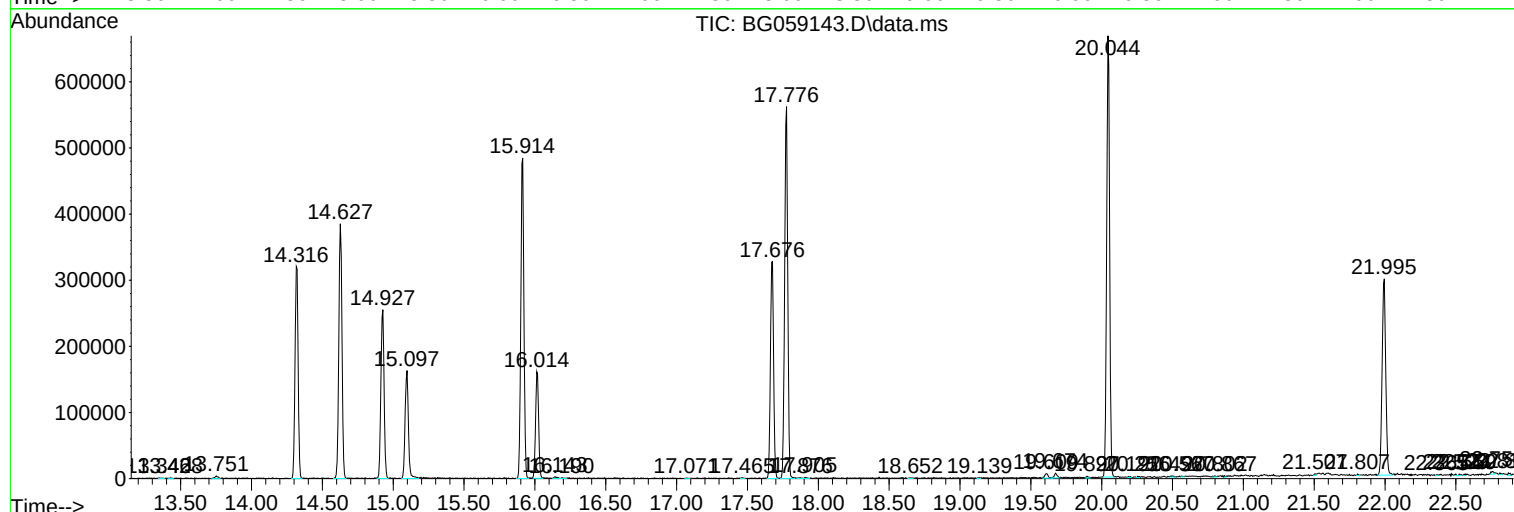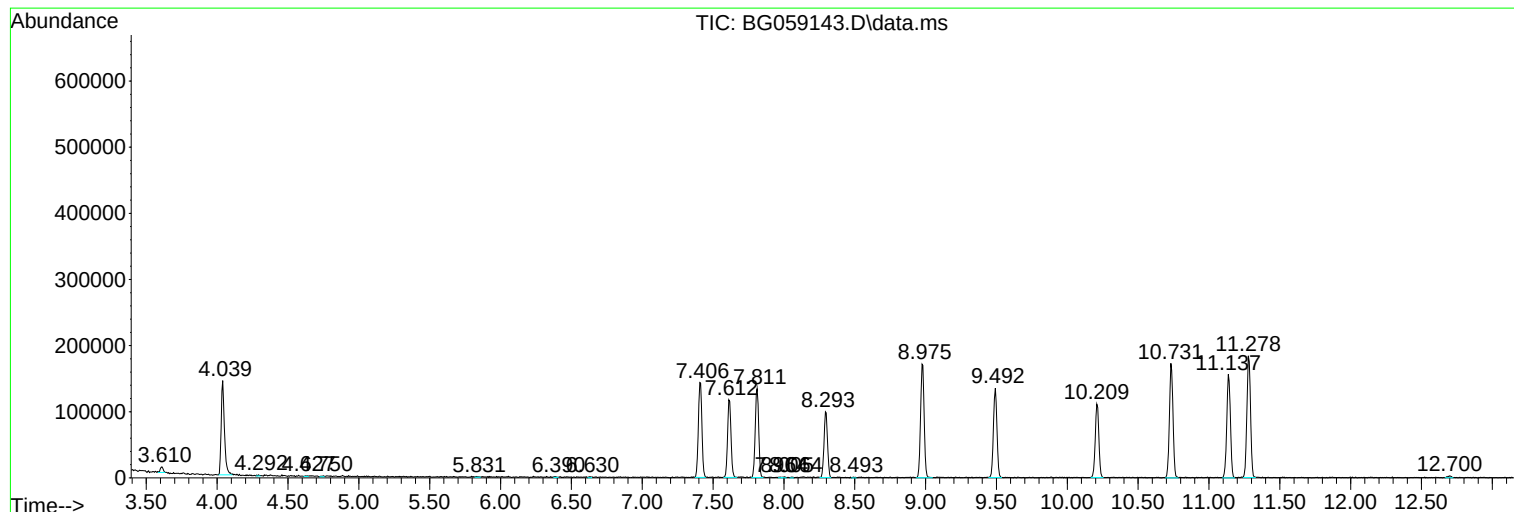

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059143.D
Acq On : 21 Sep 2023 17:20
Operator : MA/JU
Sample : PB155604BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK604

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059143.D
Acq On : 21 Sep 2023 17:20
Operator : MA/JU
Sample : PB155604BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK604

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc