

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059155.D
 Acq On : 22 Sep 2023 8:24
 Operator : MA/JU
 Sample : PB155604BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.603	32	36	42	rVB3	16066	23725	1.66%	0.169%
2	3.885	82	84	87	rBV3	2137	2622	0.18%	0.019%
3	4.031	105	109	121	rBV	203215	339289	23.72%	2.410%
4	4.372	164	167	174	rBV4	3718	4990	0.35%	0.035%
5	4.742	228	230	234	rVB4	1564	1971	0.14%	0.014%
6	5.077	283	287	288	rBV	1885	1756	0.12%	0.012%
7	5.306	322	326	328	rBV2	1935	1817	0.13%	0.013%
8	6.464	520	523	526	rBV2	1581	1717	0.12%	0.012%
9	7.192	644	647	651	rVB	1820	1791	0.13%	0.013%
10	7.410	675	684	691	rBV	205296	353023	24.68%	2.507%
11	7.610	709	718	726	rBV	157408	264227	18.48%	1.877%
12	7.803	744	751	759	rBV	190740	328496	22.97%	2.333%
13	8.291	826	834	843	rBV	120105	201173	14.07%	1.429%
14	8.973	943	950	961	rBV2	234539	427054	29.86%	3.033%
15	9.137	976	978	984	rVB2	1503	2282	0.16%	0.016%
16	9.490	1026	1038	1045	rBV	209582	368529	25.77%	2.618%
17	9.760	1083	1084	1089	rBV	2043	1905	0.13%	0.014%
18	10.207	1153	1160	1169	rVB	163122	299418	20.94%	2.127%
19	10.283	1169	1173	1176	rVB	1696	2574	0.18%	0.018%
20	10.318	1176	1179	1180	rBV	1555	1761	0.12%	0.013%
21	10.729	1242	1249	1257	rBV	254476	446261	31.20%	3.170%
22	10.941	1281	1285	1288	rVB	1857	2014	0.14%	0.014%
23	11.135	1310	1318	1327	rBV	188508	338434	23.66%	2.404%
24	11.276	1335	1342	1350	rBV	261420	480731	33.61%	3.415%
25	11.505	1378	1381	1385	rVB	1228	1784	0.12%	0.013%
26	11.587	1391	1395	1397	rBV	1487	1807	0.13%	0.013%
27	11.987	1458	1463	1464	rBV	1574	2515	0.18%	0.018%
28	12.480	1543	1547	1548	rVB	1902	1990	0.14%	0.014%
29	12.610	1566	1569	1575	rVB2	1920	3607	0.25%	0.026%
30	12.704	1577	1585	1588	rVB3	5500	10912	0.76%	0.078%
31	13.191	1667	1668	1671	rBV3	2395	2342	0.16%	0.017%
32	13.749	1759	1763	1767	rBV3	5818	9451	0.66%	0.067%
33	13.890	1785	1787	1791	rVB3	2469	2109	0.15%	0.015%
34	14.319	1853	1860	1867	rBV	524322	753614	52.69%	5.353%
35	14.625	1906	1912	1921	rVB	609905	983811	68.79%	6.988%
36	14.854	1948	1951	1954	rBV	1621	1988	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059155.D
 Acq On : 22 Sep 2023 8:24
 Operator : MA/JU
 Sample : PB155604BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK604

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

37	14.925	1956	1963	1972	rVB	350825	552458	38.63%	3.924%
38	15.001	1972	1976	1978	rBV	2287	2306	0.16%	0.016%
39	15.095	1986	1992	2001	rBV	273246	420316	29.39%	2.985%
40	15.853	2118	2121	2124	rBV	1344	1878	0.13%	0.013%

41	15.912	2124	2131	2138	rVV	697100	1014168	70.91%	7.203%
42	16.017	2143	2149	2155	rBV	196529	295850	20.69%	2.101%
43	16.147	2169	2171	2174	rVB2	2401	2404	0.17%	0.017%
44	16.599	2243	2248	2249	rBV	1356	2017	0.14%	0.014%
45	16.687	2260	2263	2265	rBV	1997	2298	0.16%	0.016%

46	16.793	2278	2281	2285	rVB	1597	2472	0.17%	0.018%
47	17.563	2410	2412	2420	rVB3	1891	2964	0.21%	0.021%
48	17.674	2422	2431	2438	rVV	422528	634832	44.39%	4.509%
49	17.774	2440	2448	2457	rVB	815446	1216897	85.09%	8.643%
50	18.062	2492	2497	2501	rBV2	2189	4945	0.35%	0.035%

51	18.133	2506	2509	2512	rVB	2145	2405	0.17%	0.017%
52	18.162	2512	2514	2517	rBV	1857	2029	0.14%	0.014%
53	18.491	2565	2570	2573	rBV3	9176	12028	0.84%	0.085%
54	18.650	2595	2597	2602	rBV3	1852	2062	0.14%	0.015%
55	18.702	2604	2606	2608	rBV	2045	1872	0.13%	0.013%

56	18.885	2633	2637	2640	rVB	1452	1838	0.13%	0.013%
57	19.525	2745	2746	2749	rVB	2394	1751	0.12%	0.012%
58	19.549	2749	2750	2753	rBV2	1402	1742	0.12%	0.012%
59	19.613	2757	2761	2764	rVV4	11004	15656	1.09%	0.111%
60	19.678	2767	2772	2780	rVB2	11704	20673	1.45%	0.147%

61	19.754	2783	2785	2788	rBV3	3787	3040	0.21%	0.022%
62	20.048	2829	2835	2841	rBV	894757	1319324	92.25%	9.371%
63	20.230	2865	2866	2868	rBV2	2172	1754	0.12%	0.012%
64	20.295	2875	2877	2878	rBV2	2355	2313	0.16%	0.016%
65	20.465	2904	2906	2907	rBV2	2744	1726	0.12%	0.012%

66	20.606	2929	2930	2932	rBV2	4038	2497	0.17%	0.018%
67	20.659	2937	2939	2941	rBV3	3490	4100	0.29%	0.029%
68	21.335	3052	3054	3055	rBV3	4418	2890	0.20%	0.021%
69	21.793	3130	3132	3134	rBV3	5072	4826	0.34%	0.034%
70	21.993	3159	3166	3176	rVB2	361367	620280	43.37%	4.406%

71	24.396	3569	3575	3581	rBV5	27094	60484	4.23%	0.430%
72	25.295	3715	3728	3745	rBV2	464688	1430159	100.00%	10.158%
73	25.536	3761	3769	3781	rVB2	228402	674672	47.17%	4.792%
74	28.209	4216	4224	4226	rBV5	19041	45533	3.18%	0.323%
75	28.415	4257	4259	4260	rBV2	4814	3429	0.24%	0.024%

76	28.708	4307	4309	4310	rVB	4936	2039	0.14%	0.014%
----	--------	------	------	------	-----	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059155.D
Acq On : 22 Sep 2023 8:24
Operator : MA/JU
Sample : PB155604BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK604

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Title : SVOA CALIBRATION

77	29.807	4495	4496	4497	rBV	5084	2413	0.17%	0.017%
78	31.476	4778	4780	4782	rBV3	4790	6010	0.42%	0.043%




Sum of corrected areas: 14078840

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059155.D
Acq On : 22 Sep 2023 8:24
Operator : MA/JU
Sample : PB155604BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK604

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

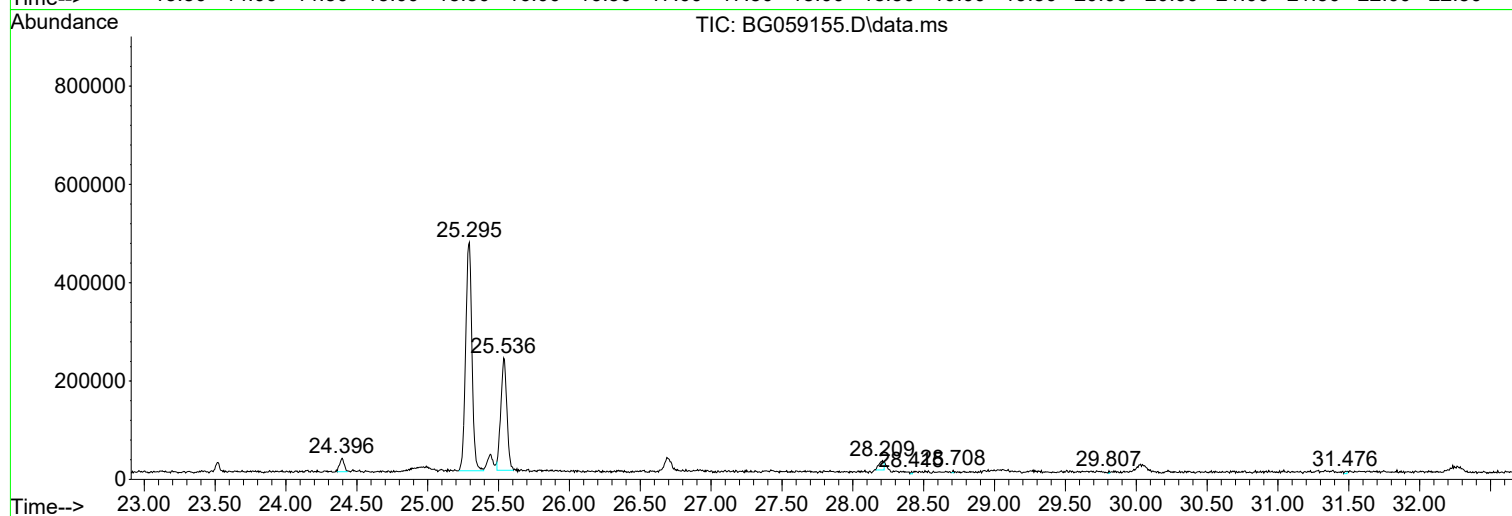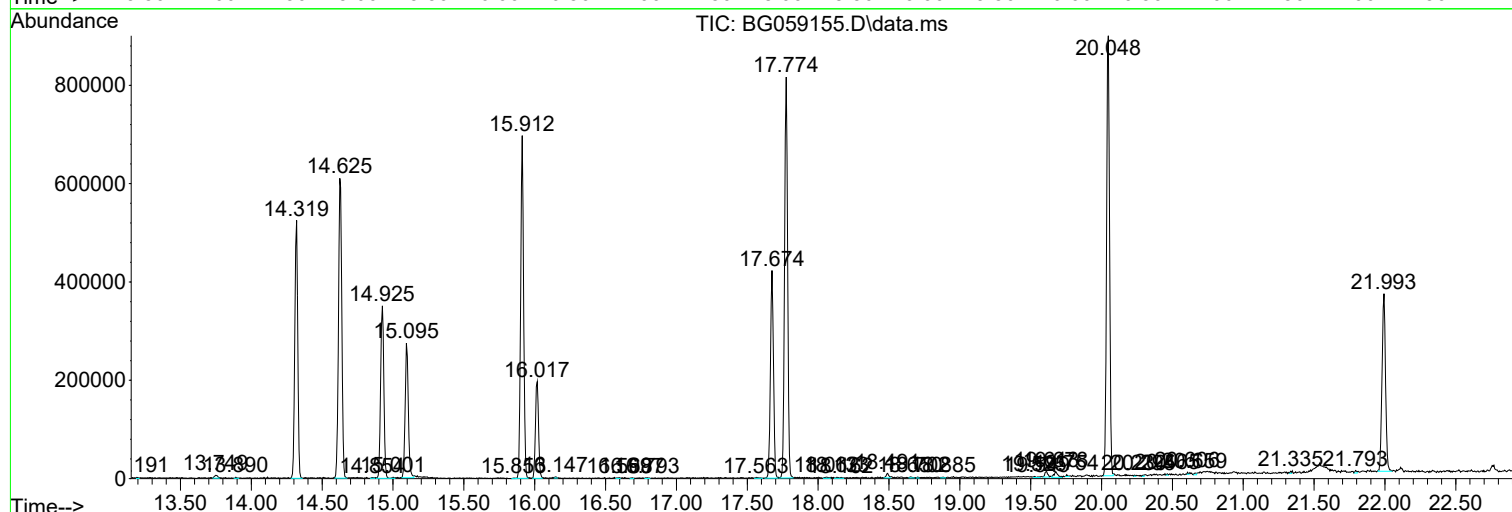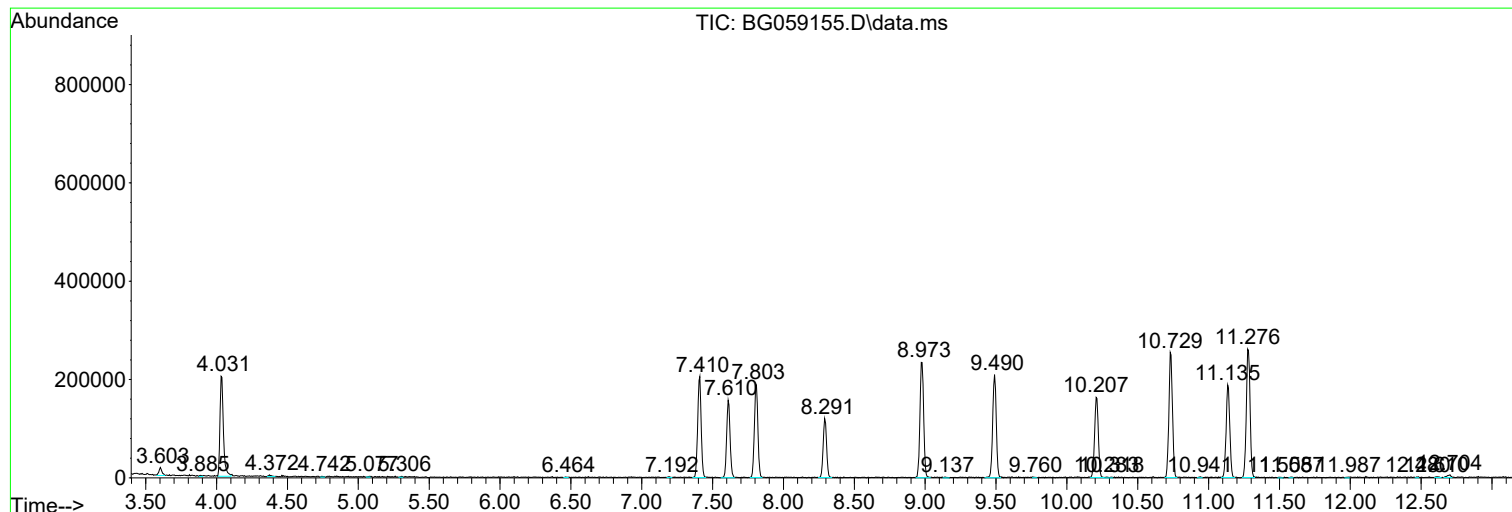

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059155.D
Acq On : 22 Sep 2023 8:24
Operator : MA/JU
Sample : PB155604BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK604

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059155.D
Acq On : 22 Sep 2023 8:24
Operator : MA/JU
Sample : PB155604BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK604

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc