

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059162.D
 Acq On : 22 Sep 2023 13:52
 Operator : MA/JU
 Sample : PB155687BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.040	107	111	123	rBV	131637	217784	23.01%	2.170%
2	5.756	401	403	405	rBV2	2114	1655	0.17%	0.016%
3	5.791	407	409	414	rVB4	2209	2614	0.28%	0.026%
4	6.120	463	465	468	rVB3	1828	1492	0.16%	0.015%
5	6.654	555	556	560	rVB2	2091	1631	0.17%	0.016%
6	6.837	585	587	590	rVB2	2005	1405	0.15%	0.014%
7	7.412	678	685	691	rVB	150525	254311	26.87%	2.534%
8	7.612	713	719	729	rVB	108667	191959	20.29%	1.913%
9	7.812	746	753	761	rVB	134234	237782	25.13%	2.369%
10	7.900	766	768	772	rVB2	1602	1523	0.16%	0.015%
11	7.935	772	774	777	rBV3	1146	1392	0.15%	0.014%
12	8.047	792	793	796	rVB2	1716	1604	0.17%	0.016%
13	8.294	828	835	844	rBV	117806	201929	21.34%	2.012%
14	8.540	874	877	881	rVB4	1350	1633	0.17%	0.016%
15	8.975	945	951	963	rVB2	179744	314656	33.25%	3.135%
16	9.081	968	969	974	rVB2	1521	1741	0.18%	0.017%
17	9.492	1031	1039	1048	rBV	142664	250726	26.50%	2.498%
18	9.627	1060	1062	1065	rVB2	1731	1493	0.16%	0.015%
19	9.692	1072	1073	1078	rBV3	1632	1668	0.18%	0.017%
20	10.209	1153	1161	1169	rBV	113869	206167	21.79%	2.054%
21	10.274	1169	1172	1175	rBV3	1302	1754	0.19%	0.017%
22	10.468	1203	1205	1209	rVB2	2226	1661	0.18%	0.017%
23	10.732	1244	1250	1260	rBV	177311	322207	34.05%	3.211%
24	10.797	1260	1261	1266	rVB	2569	2383	0.25%	0.024%
25	10.961	1285	1289	1292	rBV3	1053	1621	0.17%	0.016%
26	11.137	1311	1319	1331	rBV	187600	336647	35.58%	3.355%
27	11.284	1336	1344	1351	rBV	180727	338641	35.79%	3.374%
28	11.378	1358	1360	1364	rVB2	1921	1896	0.20%	0.019%
29	11.778	1425	1428	1431	rVB4	1704	1827	0.19%	0.018%
30	12.700	1576	1585	1589	rBV4	3557	6282	0.66%	0.063%
31	12.741	1589	1592	1595	rVB3	1026	1496	0.16%	0.015%
32	13.664	1747	1749	1756	rVB2	1199	1722	0.18%	0.017%
33	13.752	1760	1764	1769	rVV3	4392	7706	0.81%	0.077%
34	13.811	1771	1774	1778	rVB	1783	2024	0.21%	0.020%
35	13.887	1784	1787	1789	rBV	1670	1706	0.18%	0.017%
36	14.316	1853	1860	1866	rBV	367843	524877	55.47%	5.230%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059162.D
 Acq On : 22 Sep 2023 13:52
 Operator : MA/JU
 Sample : PB155687BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

37	14.387	1871	1872	1875	rVB	1906	1547	0.16%	0.015%
38	14.627	1906	1913	1922	rVB	412174	653425	69.05%	6.511%
39	14.733	1929	1931	1935	rVB2	1335	1705	0.18%	0.017%
40	14.786	1935	1940	1942	rBV3	1235	1851	0.20%	0.018%

41	14.921	1957	1963	1972	rVB	315865	503323	53.19%	5.015%
42	15.092	1985	1992	2003	rBV	95364	171087	18.08%	1.705%
43	15.368	2037	2039	2042	rVB2	1638	1646	0.17%	0.016%
44	15.691	2091	2094	2096	rBV2	1432	1768	0.19%	0.018%
45	15.908	2125	2131	2139	rBV	523379	804615	85.03%	8.018%

46	16.014	2143	2149	2156	rVV	127810	195344	20.64%	1.947%
47	16.143	2168	2171	2177	rVB3	3983	5390	0.57%	0.054%
48	16.355	2205	2207	2212	rBV2	1012	1700	0.18%	0.017%
49	17.266	2359	2362	2365	rBV2	1490	2165	0.23%	0.022%
50	17.342	2373	2375	2379	rBV3	1489	2066	0.22%	0.021%

51	17.677	2425	2432	2440	rBV	361374	567786	60.00%	5.658%
52	17.771	2441	2448	2456	rBV	536839	832980	88.03%	8.300%
53	18.059	2494	2497	2501	rBV3	1793	2432	0.26%	0.024%
54	18.217	2521	2524	2527	rBV	2379	2485	0.26%	0.025%
55	18.382	2549	2552	2556	rVB3	2087	2975	0.31%	0.030%

56	18.441	2556	2562	2564	rBV2	1365	1760	0.19%	0.018%
57	18.476	2564	2568	2569	rBV	1577	1575	0.17%	0.016%
58	18.576	2584	2585	2588	rBV	2113	1445	0.15%	0.014%
59	18.605	2588	2590	2592	rVB	1434	1465	0.15%	0.015%
60	18.629	2592	2594	2597	rBV	1687	1970	0.21%	0.020%

61	19.181	2685	2688	2689	rBV2	1546	1557	0.16%	0.016%
62	19.263	2699	2702	2704	rVB	2203	2022	0.21%	0.020%
63	19.298	2704	2708	2710	rBV3	1449	2110	0.22%	0.021%
64	19.392	2722	2724	2727	rBV2	1994	1552	0.16%	0.015%
65	19.522	2744	2746	2749	rVB2	1832	1579	0.17%	0.016%

66	19.604	2756	2760	2764	rBV5	9021	10664	1.13%	0.106%
67	19.675	2769	2772	2776	rVB2	5891	7518	0.79%	0.075%
68	19.780	2787	2790	2792	rBV	1222	1420	0.15%	0.014%
69	19.898	2806	2810	2812	rBV4	2800	3987	0.42%	0.040%
70	19.957	2817	2820	2823	rBV4	1409	2007	0.21%	0.020%

71	20.045	2829	2835	2847	rBV	634361	946299	100.00%	9.430%
72	20.197	2858	2861	2866	rBV3	2047	3183	0.34%	0.032%
73	20.286	2874	2876	2880	rVB4	3412	2224	0.24%	0.022%
74	20.397	2893	2895	2897	rVB3	2621	1491	0.16%	0.015%
75	20.438	2900	2902	2905	rVB3	2324	1967	0.21%	0.020%

76	20.691	2944	2945	2948	rBV3	3529	3114	0.33%	0.031%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
 Data File : BG059162.D
 Acq On : 22 Sep 2023 13:52
 Operator : MA/JU
 Sample : PB155687BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

77	20.985	2994	2995	2996	rBV	3540	1884	0.20%	0.019%
78	21.402	3063	3066	3067	rBV3	2977	3368	0.36%	0.034%
79	21.472	3075	3078	3079	rBV3	6228	6428	0.68%	0.064%
80	21.666	3109	3111	3114	rVB3	4843	3889	0.41%	0.039%
81	21.995	3160	3167	3174	rBV	269955	480823	50.81%	4.791%
82	22.454	3243	3245	3247	rBV3	3567	2401	0.25%	0.024%
83	22.571	3264	3265	3268	rVB2	5228	3372	0.36%	0.034%
84	23.300	3387	3389	3390	rBV2	3555	2096	0.22%	0.021%
85	23.611	3438	3442	3443	rBV4	4237	4954	0.52%	0.049%
86	24.281	3554	3556	3557	rBV	3549	2641	0.28%	0.026%
87	25.168	3705	3707	3710	rBV4	3456	2316	0.24%	0.023%
88	25.291	3716	3728	3741	rBV2	244361	780274	82.46%	7.775%
89	25.538	3760	3770	3784	rVB	158525	506022	53.47%	5.042%
90	26.596	3948	3950	3952	rBV3	4331	2565	0.27%	0.026%
91	27.730	4141	4143	4144	rBV2	3303	1626	0.17%	0.016%
92	27.894	4170	4171	4173	rBV2	3006	2212	0.23%	0.022%
93	27.971	4182	4184	4185	rBV	3981	3512	0.37%	0.035%
94	30.168	4556	4558	4560	rBV3	3846	3186	0.34%	0.032%
95	30.462	4606	4608	4611	rVB4	4524	4320	0.46%	0.043%
96	30.538	4619	4621	4622	rBV2	3369	2640	0.28%	0.026%
97	30.597	4629	4631	4633	rVB3	3907	2042	0.22%	0.020%
98	30.691	4646	4647	4648	rBV	3640	1967	0.21%	0.020%
99	31.549	4791	4793	4794	rBV2	4008	1859	0.20%	0.019%
100	31.960	4861	4863	4864	rBV2	3873	2193	0.23%	0.022%




Sum of corrected areas: 10035404

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059162.D
Acq On : 22 Sep 2023 13:52
Operator : MA/JU
Sample : PB155687BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK687

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

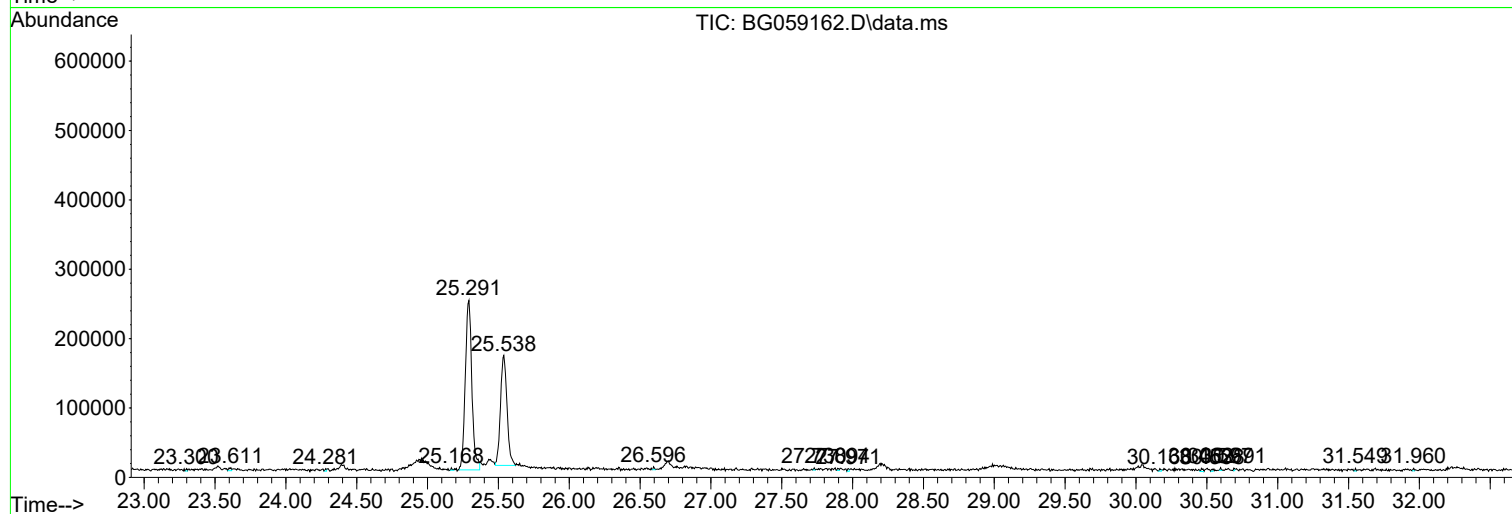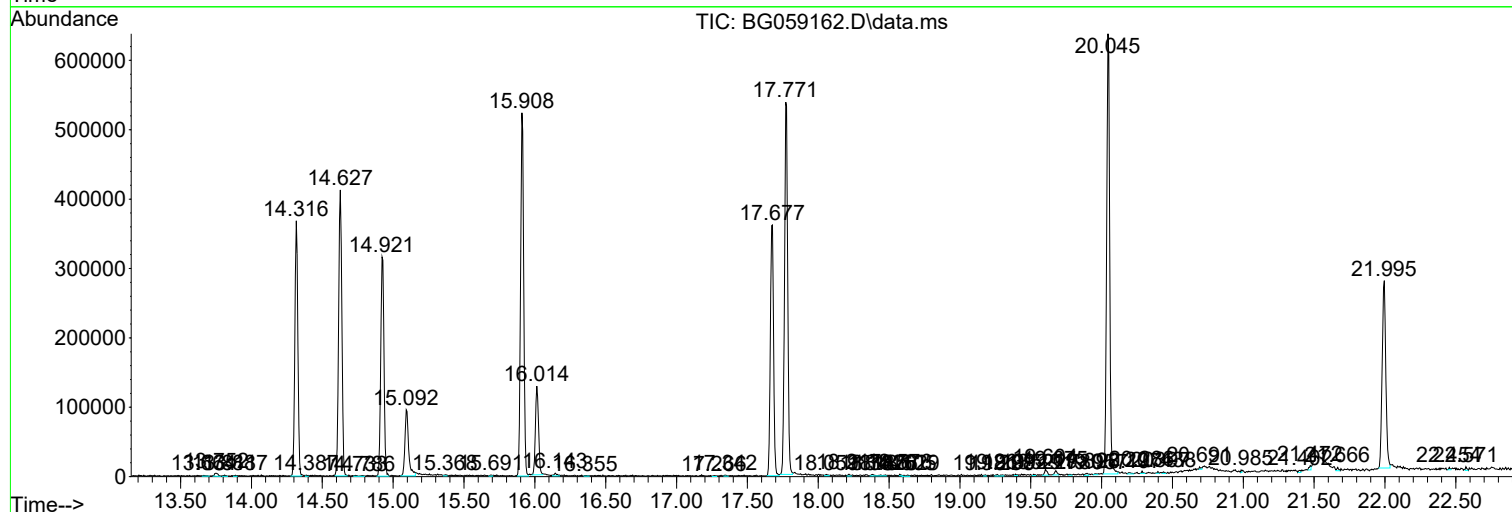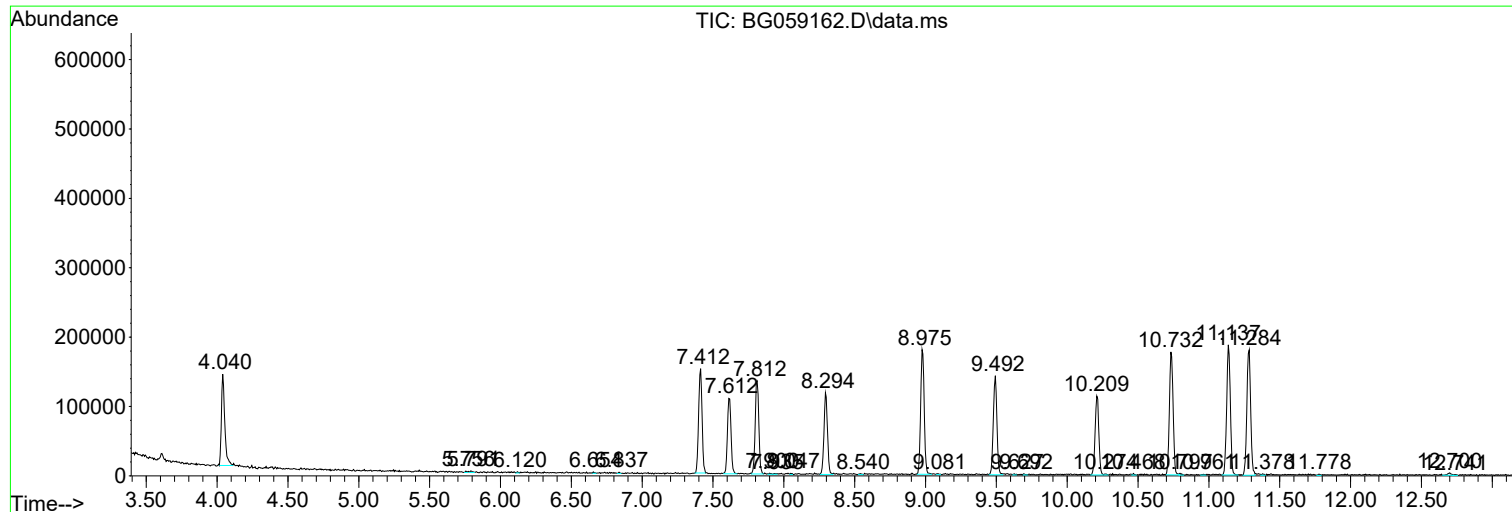

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059162.D
Acq On : 22 Sep 2023 13:52
Operator : MA/JU
Sample : PB155687BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK687

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092023\
Data File : BG059162.D
Acq On : 22 Sep 2023 13:52
Operator : MA/JU
Sample : PB155687BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK687

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------