

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG092118\
 Data File : BG036872.D
 Acq On : 21 Sep 2018 23:56
 Operator : JU/SJ
 Sample : J4777-30
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-04-092018-B

Quant Time: Sep 22 04:30:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 20 20:07:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	39056	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	157052	20.00	ng	0.00
38) Acenaphthene-d10	14.67	164	106198	20.00	ng	0.00
63) Phenanthrene-d10	17.42	188	290346	20.00	ng	0.00
75) Chrysene-d12	21.68	240	323607	20.00	ng	0.00
86) Perylene-d12	24.90	264	322715	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	247006	121.29	ng	0.00
7) Phenol-d6	7.21	99	317650	100.81	ng	0.00
23) Nitrobenzene-d5	9.21	82	248039	84.58	ng	0.00
41) 2,4,6-Tribromophenol	16.16	330	176546	138.95	ng	0.00
44) 2-Fluorobiphenyl	13.30	172	569242	79.83	ng	0.00
78) Terphenyl-d14	20.03	244	1192051	96.86	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.21	70	33080	12.620	ng	# 72
50) 2,6-Dinitrotoluene	14.67	165	12989	6.964	ng	# 20
56) 2,4-Dinitrotoluene	14.67	165	12989	4.991	ng	# 18
66) 4-Bromophenyl-phenylether	16.16	248	12048	3.648	ng	# 1
76) Benzidine	20.03	184	19637	2.007	ng	# 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG092118\
Data File : BG036872.D
Acq On : 21 Sep 2018 23:56
Operator : JU/SJ
Sample : J4777-30
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-04-092018-B

Quant Time: Sep 22 04:30:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 20 20:07:11 2018
Response via : Initial Calibration

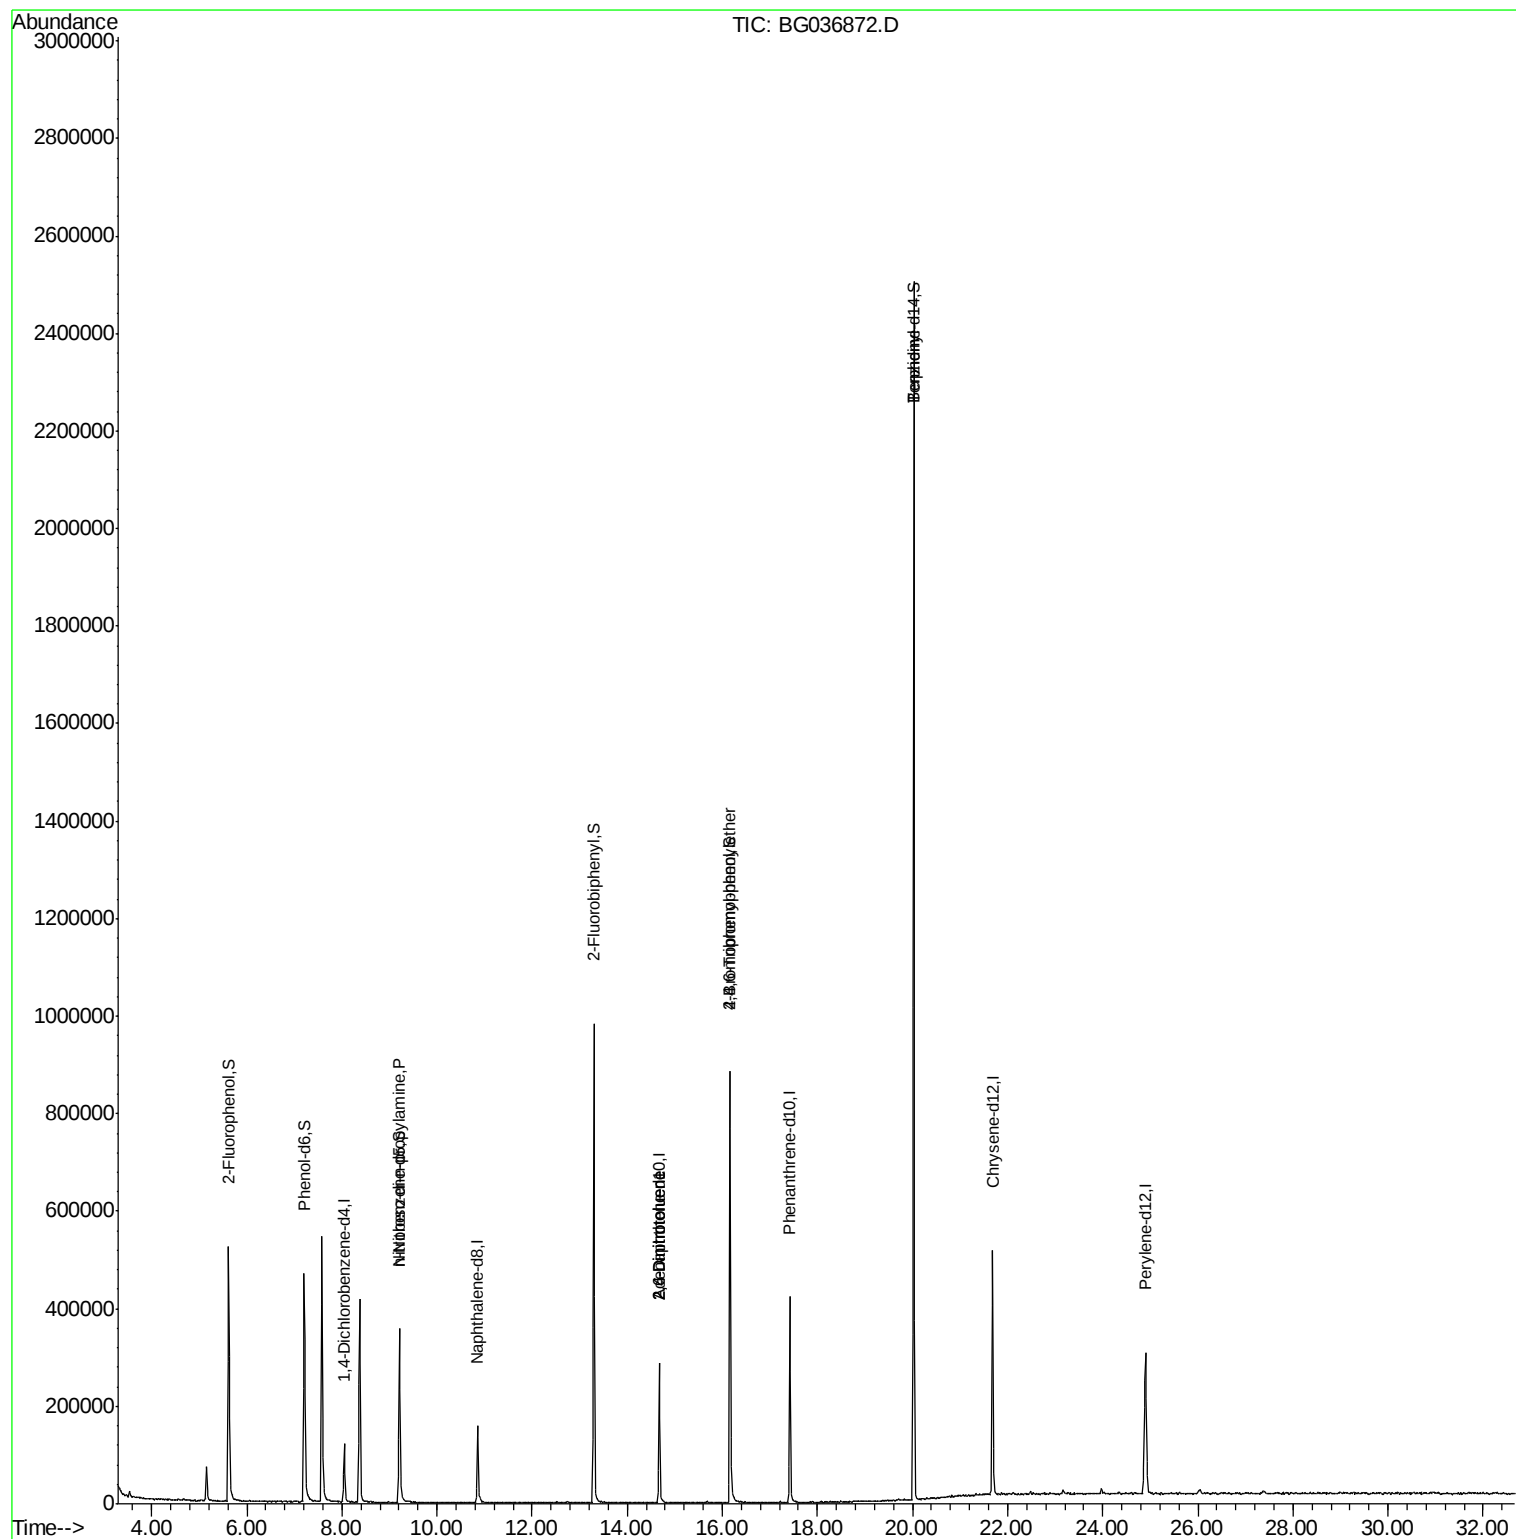

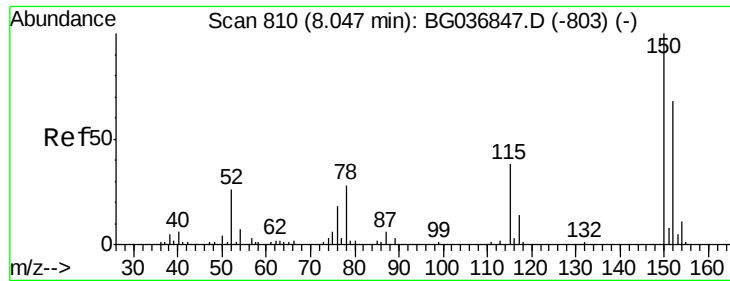


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 811
Delta R.T. 0.01 min
Lab File: BG036872.D
Acq: 21 Sep 2018 23:56

Instrument :
BNA_G
ClientSampleId :
PL-04-092018-B

Tgt Ion:152 Resp: 39056
Ion Ratio Lower Upper
152 100
150 149.8 119.5 179.3
115 58.3 44.5 66.7

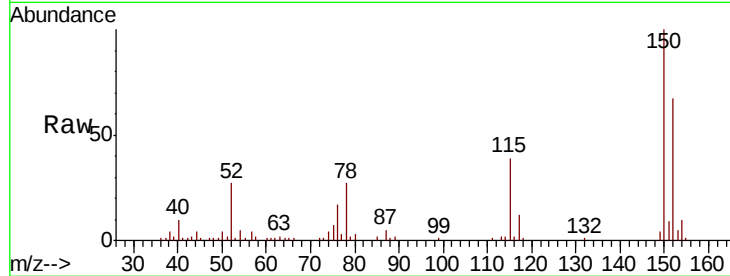


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

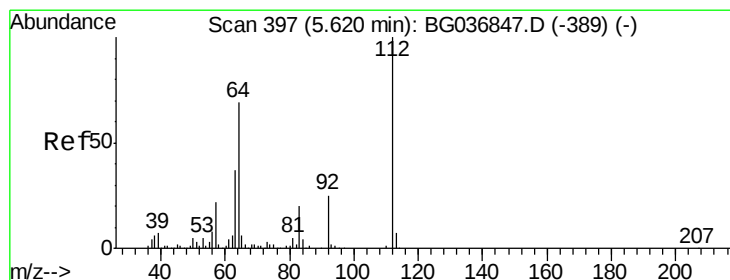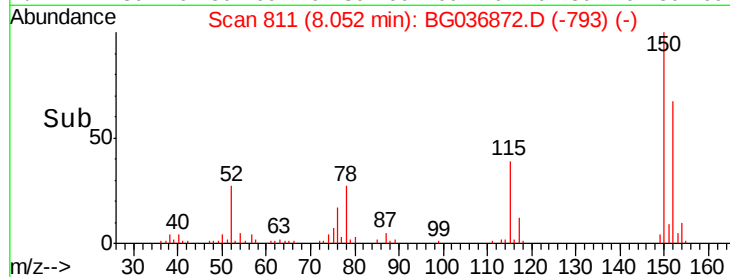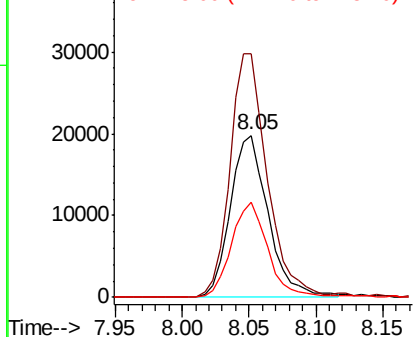



#5


2-Fluorophenol
Concen: 121.288 ng
RT: 5.62 min Scan# 397
Delta R.T. -0.00 min
Lab File: BG036872.D
Acq: 21 Sep 2018 23:56

Tgt Ion:112 Resp: 247006
Ion Ratio Lower Upper
112 100
64 73.7 57.2 85.8
63 37.7 30.8 46.2

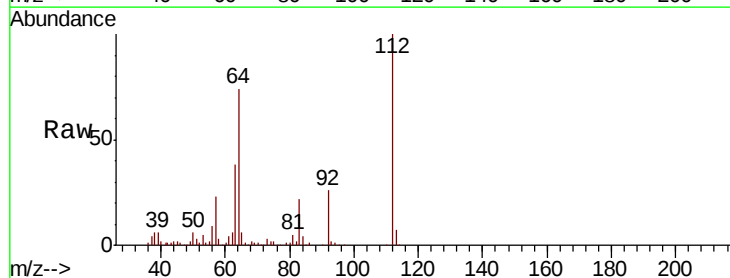

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

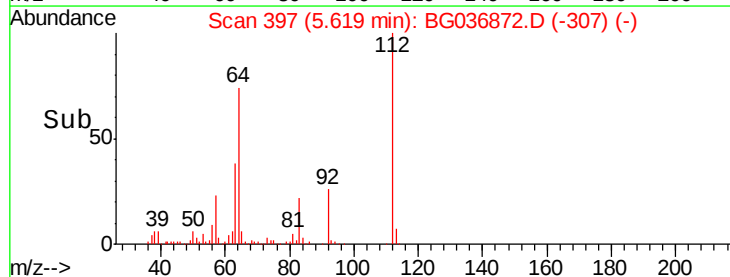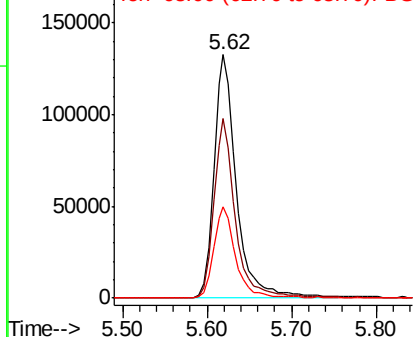

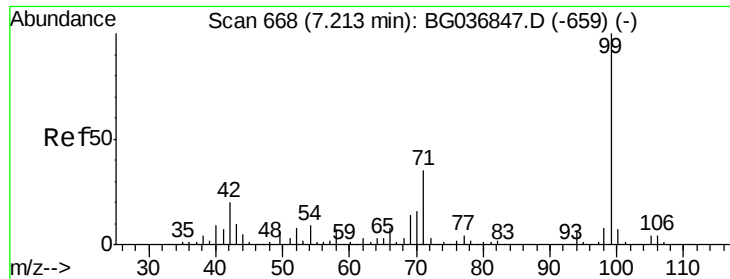

#7

Phenol-d6

Concen: 100.814 ng

RT: 7.21 min Scan# 667

Delta R.T. -0.01 min

Lab File: BG036872.D

Acq: 21 Sep 2018 23:56

Instrument :

BNA_G

ClientSampleId :

PL-04-092018-B


Tgt Ion: 99 Resp: 317650

Ion Ratio Lower Upper




99 100

42 19.6 16.5 24.7

71 35.5 29.4 44.2

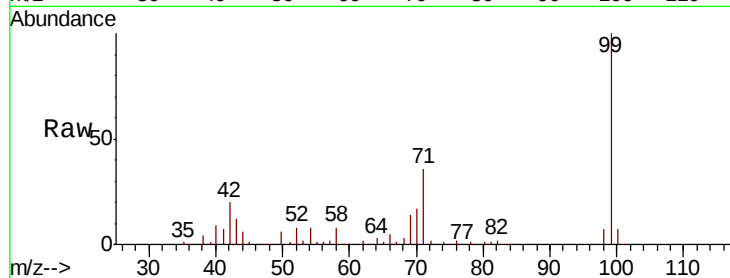

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

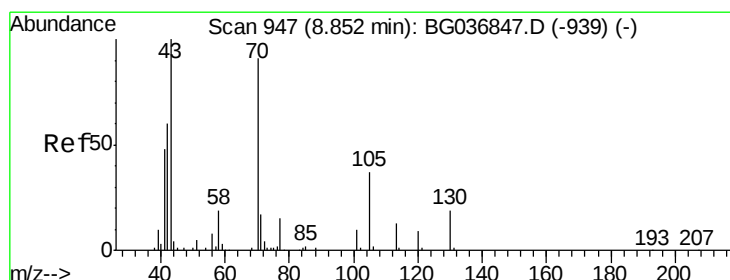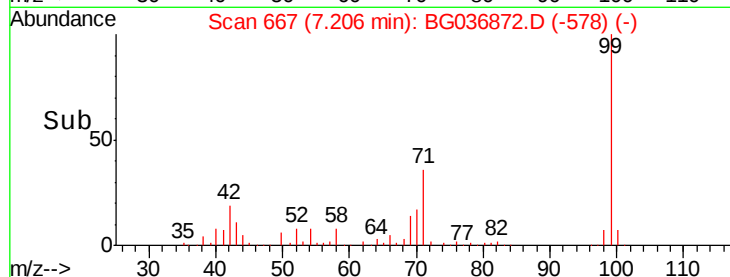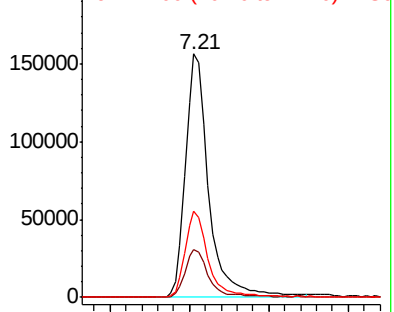

#19

n-Nitroso-di-n-propylamine

Concen: 12.620 ng

RT: 9.21 min Scan# 1008

Delta R.T. 0.36 min

Lab File: BG036872.D

Acq: 21 Sep 2018 23:56

Tgt Ion: 70 Resp: 33080


Ion Ratio Lower Upper

70 100



42 49.5 56.2 84.4#

101 0.0 7.8 11.6#

130 2.0 16.2 24.2#

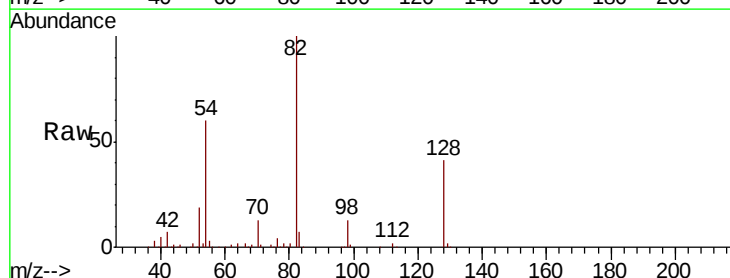

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

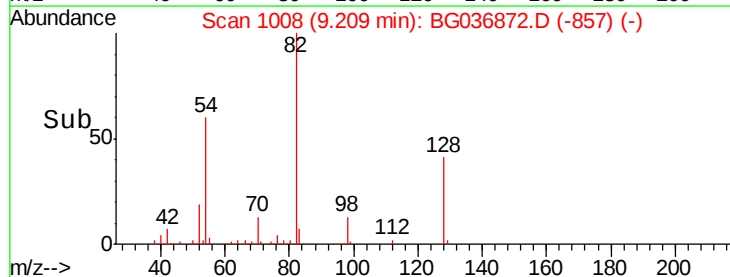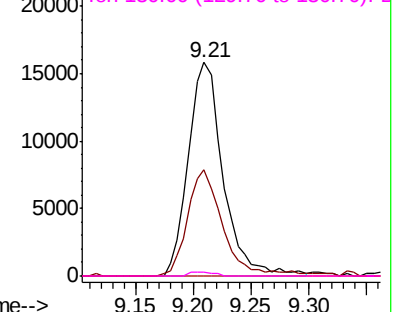







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.85 min Scan# 1288
Delta R.T. -0.00 min
Lab File: BG036872.D
Acq: 21 Sep 2018 23:56

Instrument :
BNA_G
ClientSampleId :
PL-04-092018-B

Tgt Ion:	136	Resp:	157052
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.8	13.2
54	11.1	9.2	13.8
68	6.3	5.8	8.6

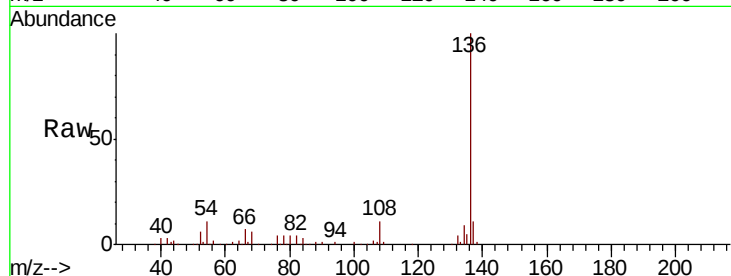


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BG
Ion 68.00 (67.70 to 68.70): BG

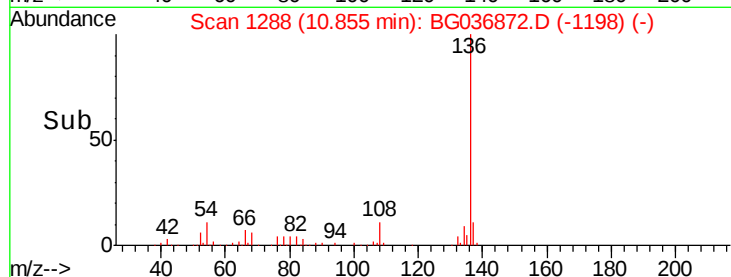
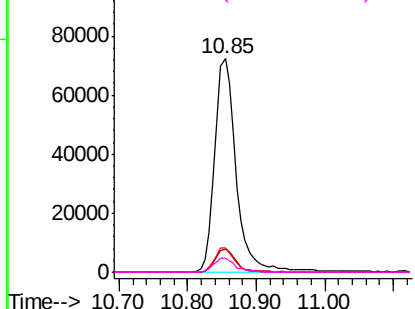



#23
Nitrobenzene-d5
Concen: 84.575 ng
RT: 9.21 min Scan# 1008
Delta R.T. -0.00 min
Lab File: BG036872.D
Acq: 21 Sep 2018 23:56

Tgt Ion:	82	Resp:	248039
Ion	Ratio	Lower	Upper
82	100		
128	41.0	33.3	49.9
54	59.5	45.1	67.7



Abundance Ion 82.00 (81.70 to 82.70): BG
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BG

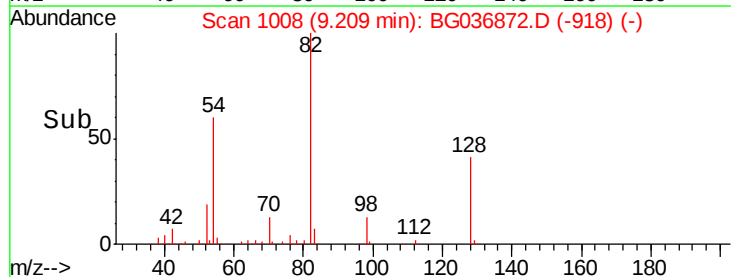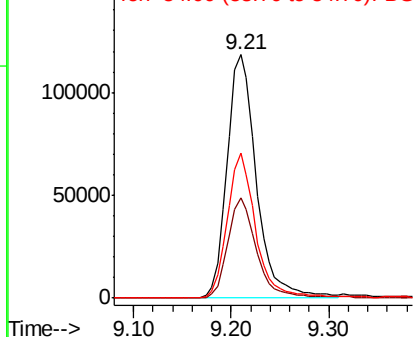

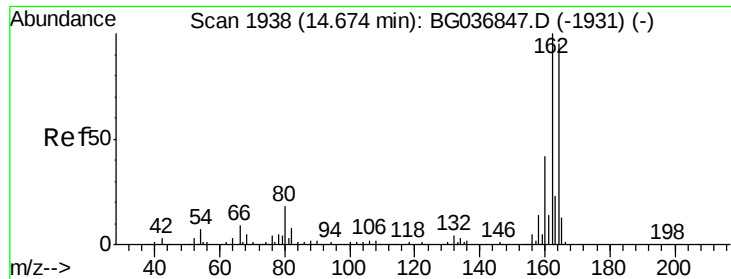

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.67 min Scan# 1938

Delta R.T. -0.00 min

Lab File: BG036872.D

Acq: 21 Sep 2018 23:56

Instrument :

BNA_G

ClientSampleId :

PL-04-092018-B





Tgt Ion:164 Resp: 106198

Ion Ratio Lower Upper

164 100

162 104.6 80.7 121.1

160 46.0 35.3 52.9

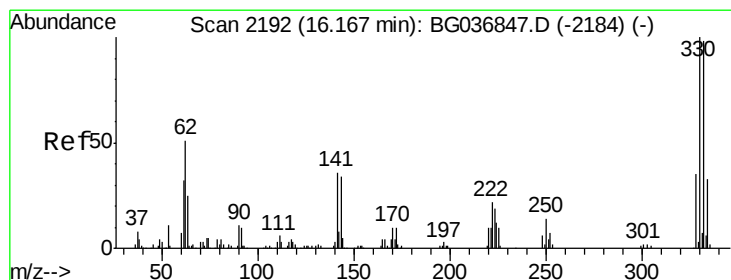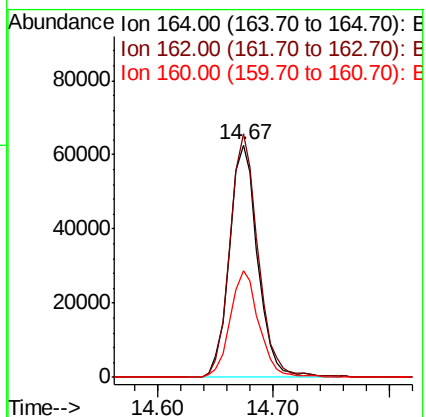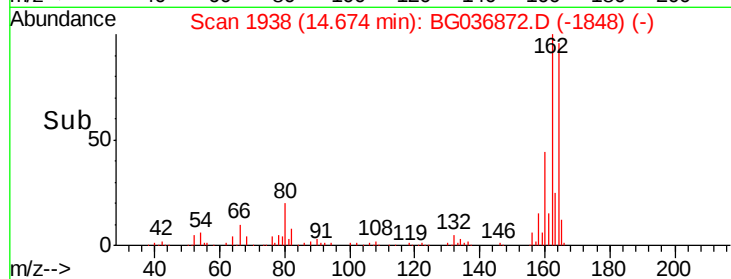

#41

2,4,6-Tribromophenol

Concen: 138.948 ng

RT: 16.16 min Scan# 2191

Delta R.T. -0.01 min

Lab File: BG036872.D

Acq: 21 Sep 2018 23:56




Tgt Ion:330 Resp: 176546

Ion Ratio Lower Upper

330 100

332 93.4 75.4 113.2

141 38.0 30.7 46.1


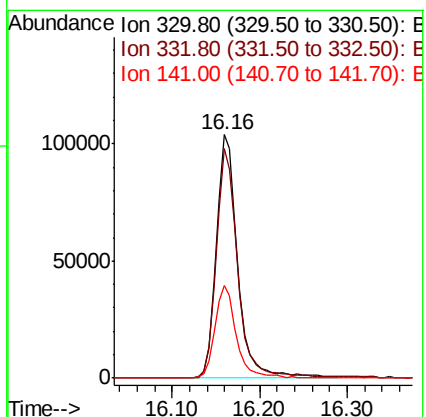
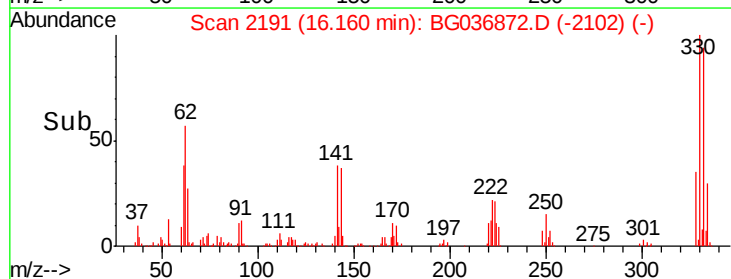
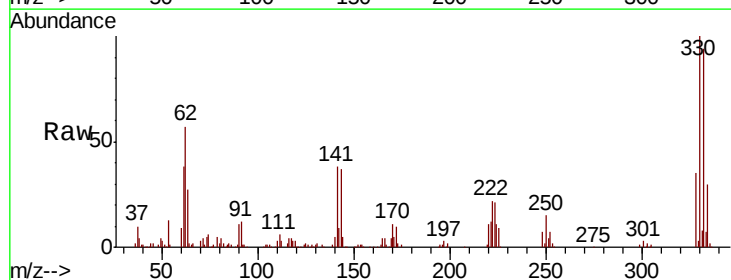




#44
 2-Fluorobiphenyl
 Concen: 79.834 ng
 RT: 13.30 min Scan# 1704
 Delta R.T. -0.00 min
 Lab File: BG036872.D
 Acq: 21 Sep 2018 23:56




Instrument :
 BNA_G
 ClientSampleId :
 PL-04-092018-B

Tgt Ion:172 Resp: 569242
 Ion Ratio Lower Upper
 172 100
 171 36.8 31.3 46.9
 170 24.2 21.0 31.6

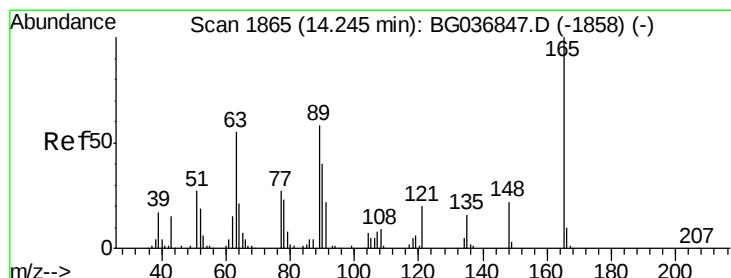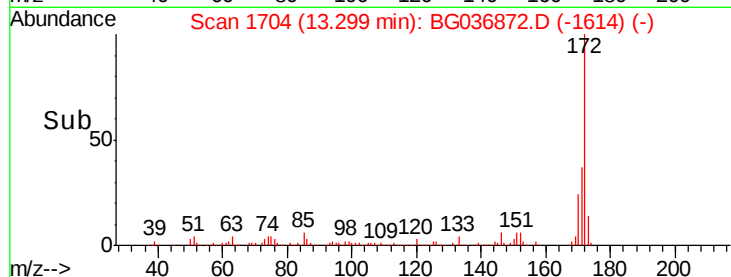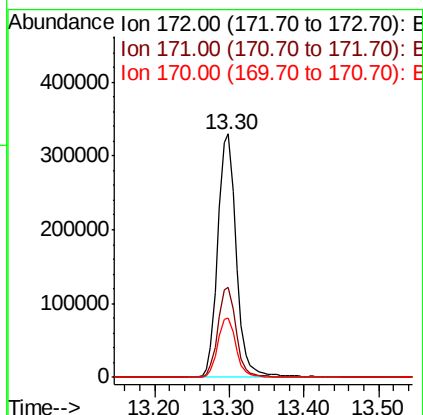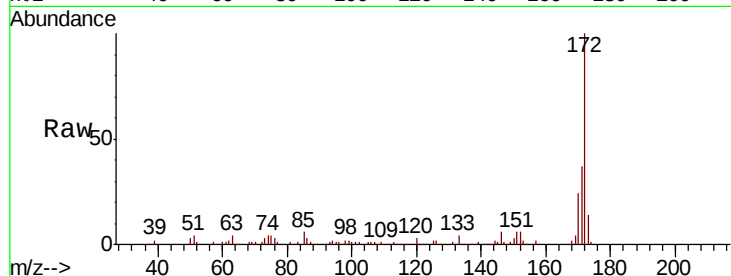

#50
 2,6-Dinitrotoluene
 Concen: 6.964 ng
 RT: 14.67 min Scan# 1938
 Delta R.T. 0.43 min
 Lab File: BG036872.D
 Acq: 21 Sep 2018 23:56

Tgt Ion:165 Resp: 12989
 Ion Ratio Lower Upper
 165 100
 63 0.0 50.1 75.1#
 89 0.0 47.8 71.6#

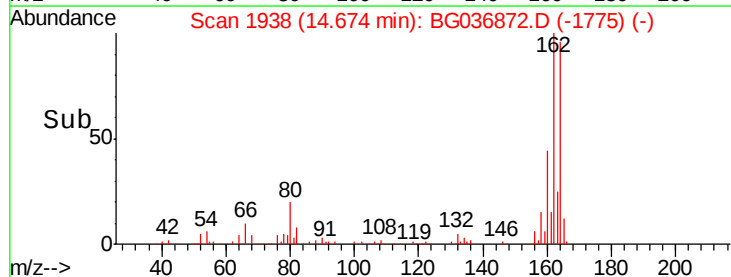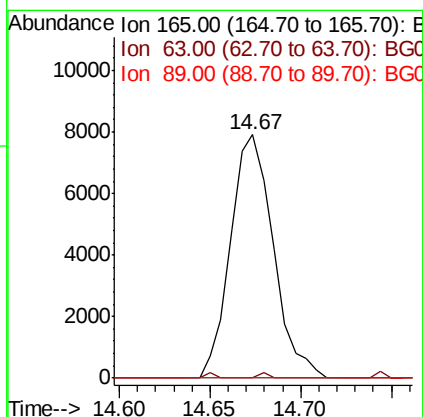







#56
2,4-Dinitrotoluene
Concen: 4.991 ng
RT: 14.67 min Scan# 1938
Delta R.T. -0.36 min
Lab File: BG036872.D
Acq: 21 Sep 2018 23:56

Instrument :
BNA_G
ClientSampleId :
PL-04-092018-B

Tgt Ion:	165	Resp:	12989
Ion	Ratio	Lower	Upper
165	100		
63	0.0	40.1	60.1#
89	0.0	63.7	95.5#
182	0.0	2.5	3.7#




Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BGC
Ion 89.00 (88.70 to 89.70): BGC
Ion 182.00 (181.70 to 182.70): E

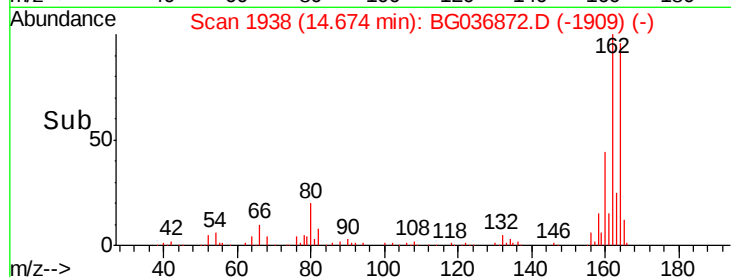
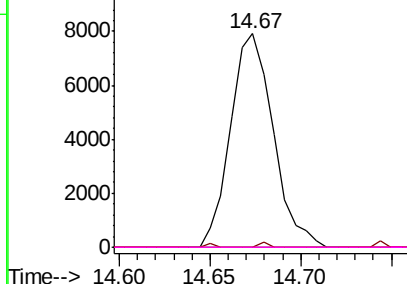



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.42 min Scan# 2405
Delta R.T. -0.00 min
Lab File: BG036872.D
Acq: 21 Sep 2018 23:56

Tgt Ion:	188	Resp:	290346
Ion	Ratio	Lower	Upper
188	100		
94	7.6	6.7	10.1
80	8.8	8.1	12.1



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

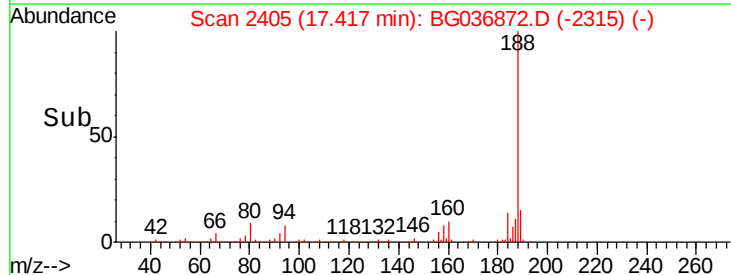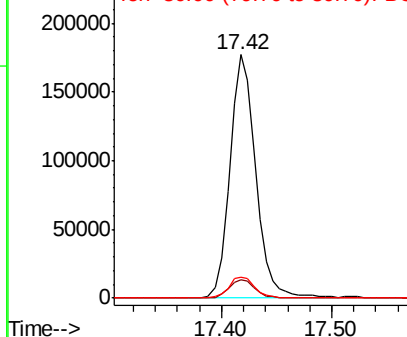


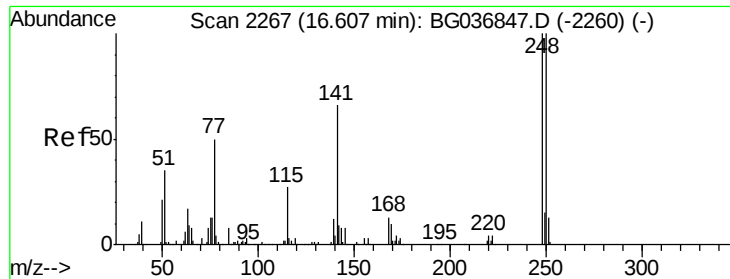




#66
 4-Bromophenyl-phenylether
 Concen: 3.648 ng
 RT: 16.16 min Scan# 2191
 Delta R.T. -0.45 min
 Lab File: BG036872.D
 Acq: 21 Sep 2018 23:56

Instrument :
 BNA_G
 ClientSampleId :
 PL-04-092018-B

Tgt Ion:248 Resp: 12048
 Ion Ratio Lower Upper
 248 100
 250 219.2 78.1 117.1#
 141 561.7 53.7 80.5#

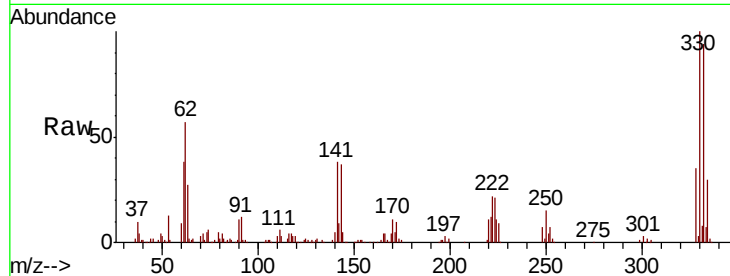


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

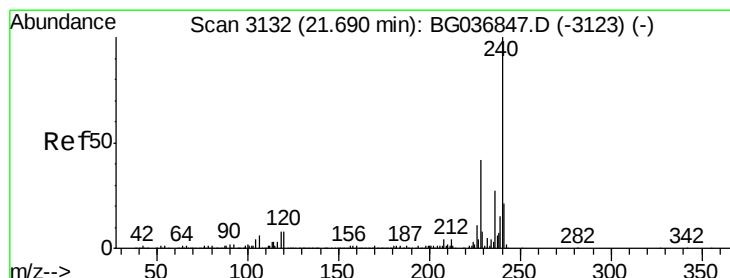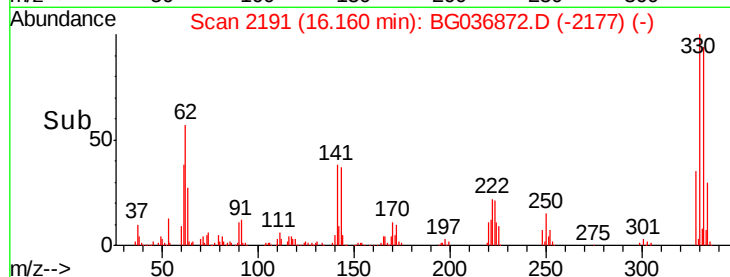
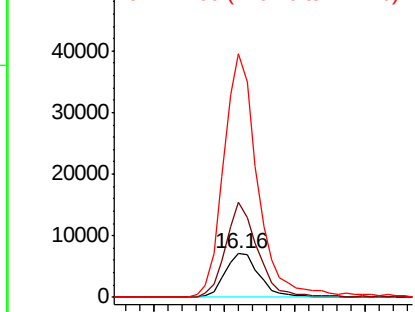


#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.68 min Scan# 3131
 Delta R.T. -0.01 min
 Lab File: BG036872.D
 Acq: 21 Sep 2018 23:56

Tgt Ion:240 Resp: 323607
 Ion Ratio Lower Upper
 240 100
 120 7.6 6.9 10.3
 236 26.8 21.2 31.8

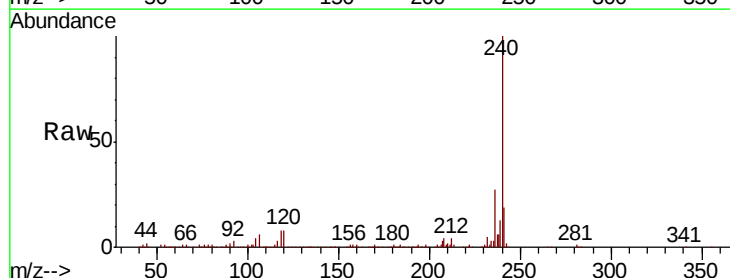

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



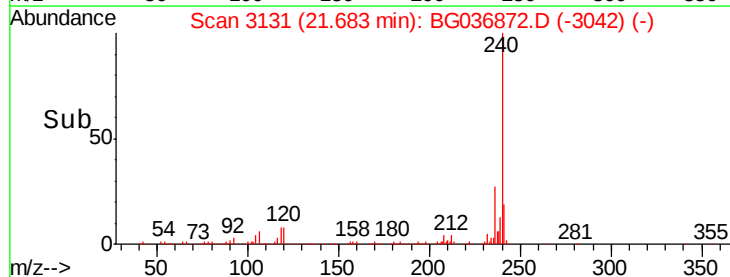
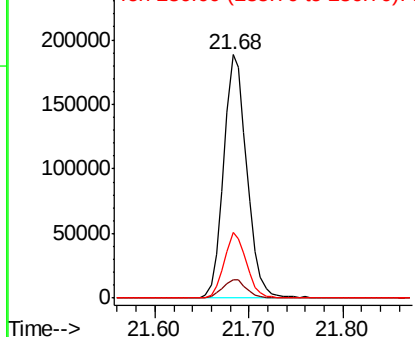




#76
Benzidine
Concen: 2.007 ng
RT: 20.03 min Scan# 2849
Delta R.T. 0.38 min
Lab File: BG036872.D
Acq: 21 Sep 2018 23:56




Instrument :
BNA_G
ClientSampleId :
PL-04-092018-B


Tgt Ion:184 Resp: 19637
Ion Ratio Lower Upper
184 100
185 18.4 12.6 18.8
183 10.8 10.9 16.3#

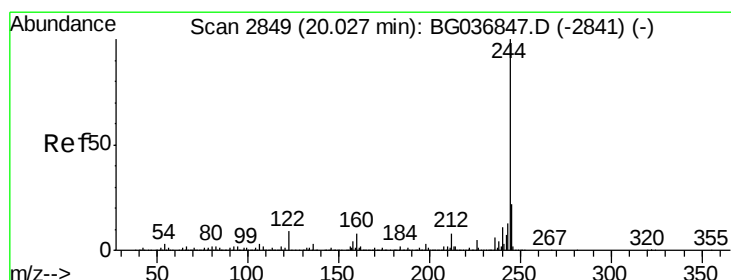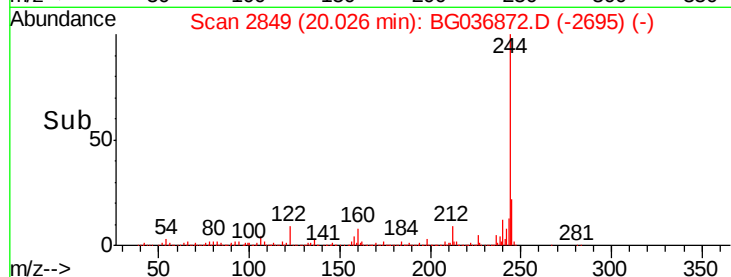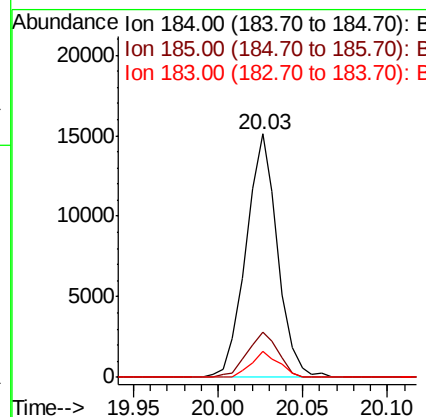

#78
Terphenyl-d14
Concen: 96.861 ng
RT: 20.03 min Scan# 2849
Delta R.T. -0.00 min
Lab File: BG036872.D
Acq: 21 Sep 2018 23:56

Tgt Ion:244 Resp: 1192051
Ion Ratio Lower Upper
244 100
212 8.6 7.0 10.6
122 9.0 7.1 10.7

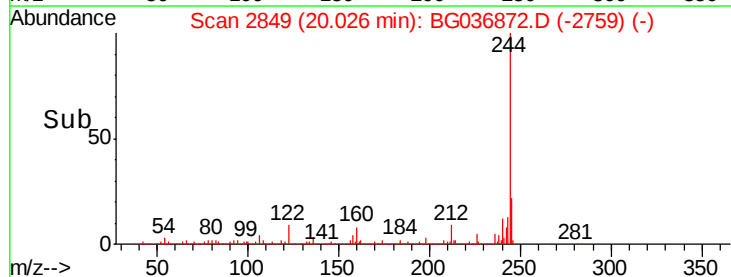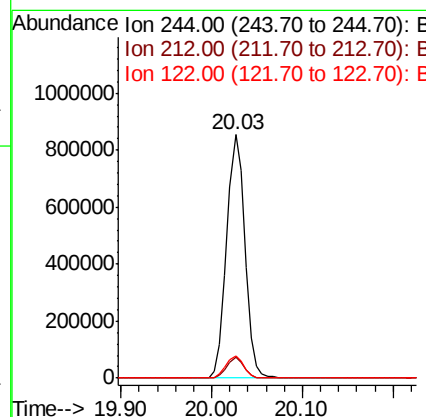


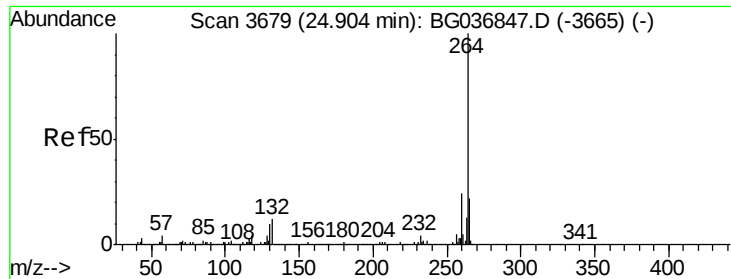

#86
Perylene-d12
Concen: 20.000 ng
RT: 24.90 min Scan# 3678
Delta R.T. -0.01 min
Lab File: BG036872.D
Acq: 21 Sep 2018 23:56

Instrument :
BNA_G
ClientSampleId :
PL-04-092018-B

Tgt Ion:	264	Resp:	322715
Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.6	29.4
265	21.8	17.4	26.0



Abundance Ion 264.00 (263.70 to 264.70): E
150000 Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

