

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092118\
 Data File : BG036894.D
 Acq On : 22 Sep 2018 14:53
 Operator : JU/SJ
 Sample : J4778-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Sep 24 03:55:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 20 20:07:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	39185	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	166230	20.00	ng	0.00
38) Acenaphthene-d10	14.67	164	113507	20.00	ng	0.00
63) Phenanthrene-d10	17.41	188	302539	20.00	ng	0.00
75) Chrysene-d12	21.68	240	329531	20.00	ng	-0.01
86) Perylene-d12	24.89	264	330690	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	259147	126.83	ng	0.00
7) Phenol-d6	7.21	99	338382	107.04	ng	0.00
23) Nitrobenzene-d5	9.21	82	269122	86.70	ng	0.00
41) 2,4,6-Tribromophenol	16.16	330	178632	131.54	ng	0.00
44) 2-Fluorobiphenyl	13.30	172	612665	80.39	ng	0.00
78) Terphenyl-d14	20.02	244	1219838	97.34	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.21	70	37020	14.077	ng	# 74
50) 2,6-Dinitrotoluene	14.68	165	14879	7.464	ng	# 20
56) 2,4-Dinitrotoluene	14.68	165	14879	5.349	ng	# 18
66) 4-Bromophenyl-phenylether	16.16	248	12715	3.695	ng	# 1
76) Benzidine	20.02	184	21307	2.139	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092118\
Data File : BG036894.D
Acq On : 22 Sep 2018 14:53
Operator : JU/SJ
Sample : J4778-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Sep 24 03:55:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 20 20:07:11 2018
Response via : Initial Calibration

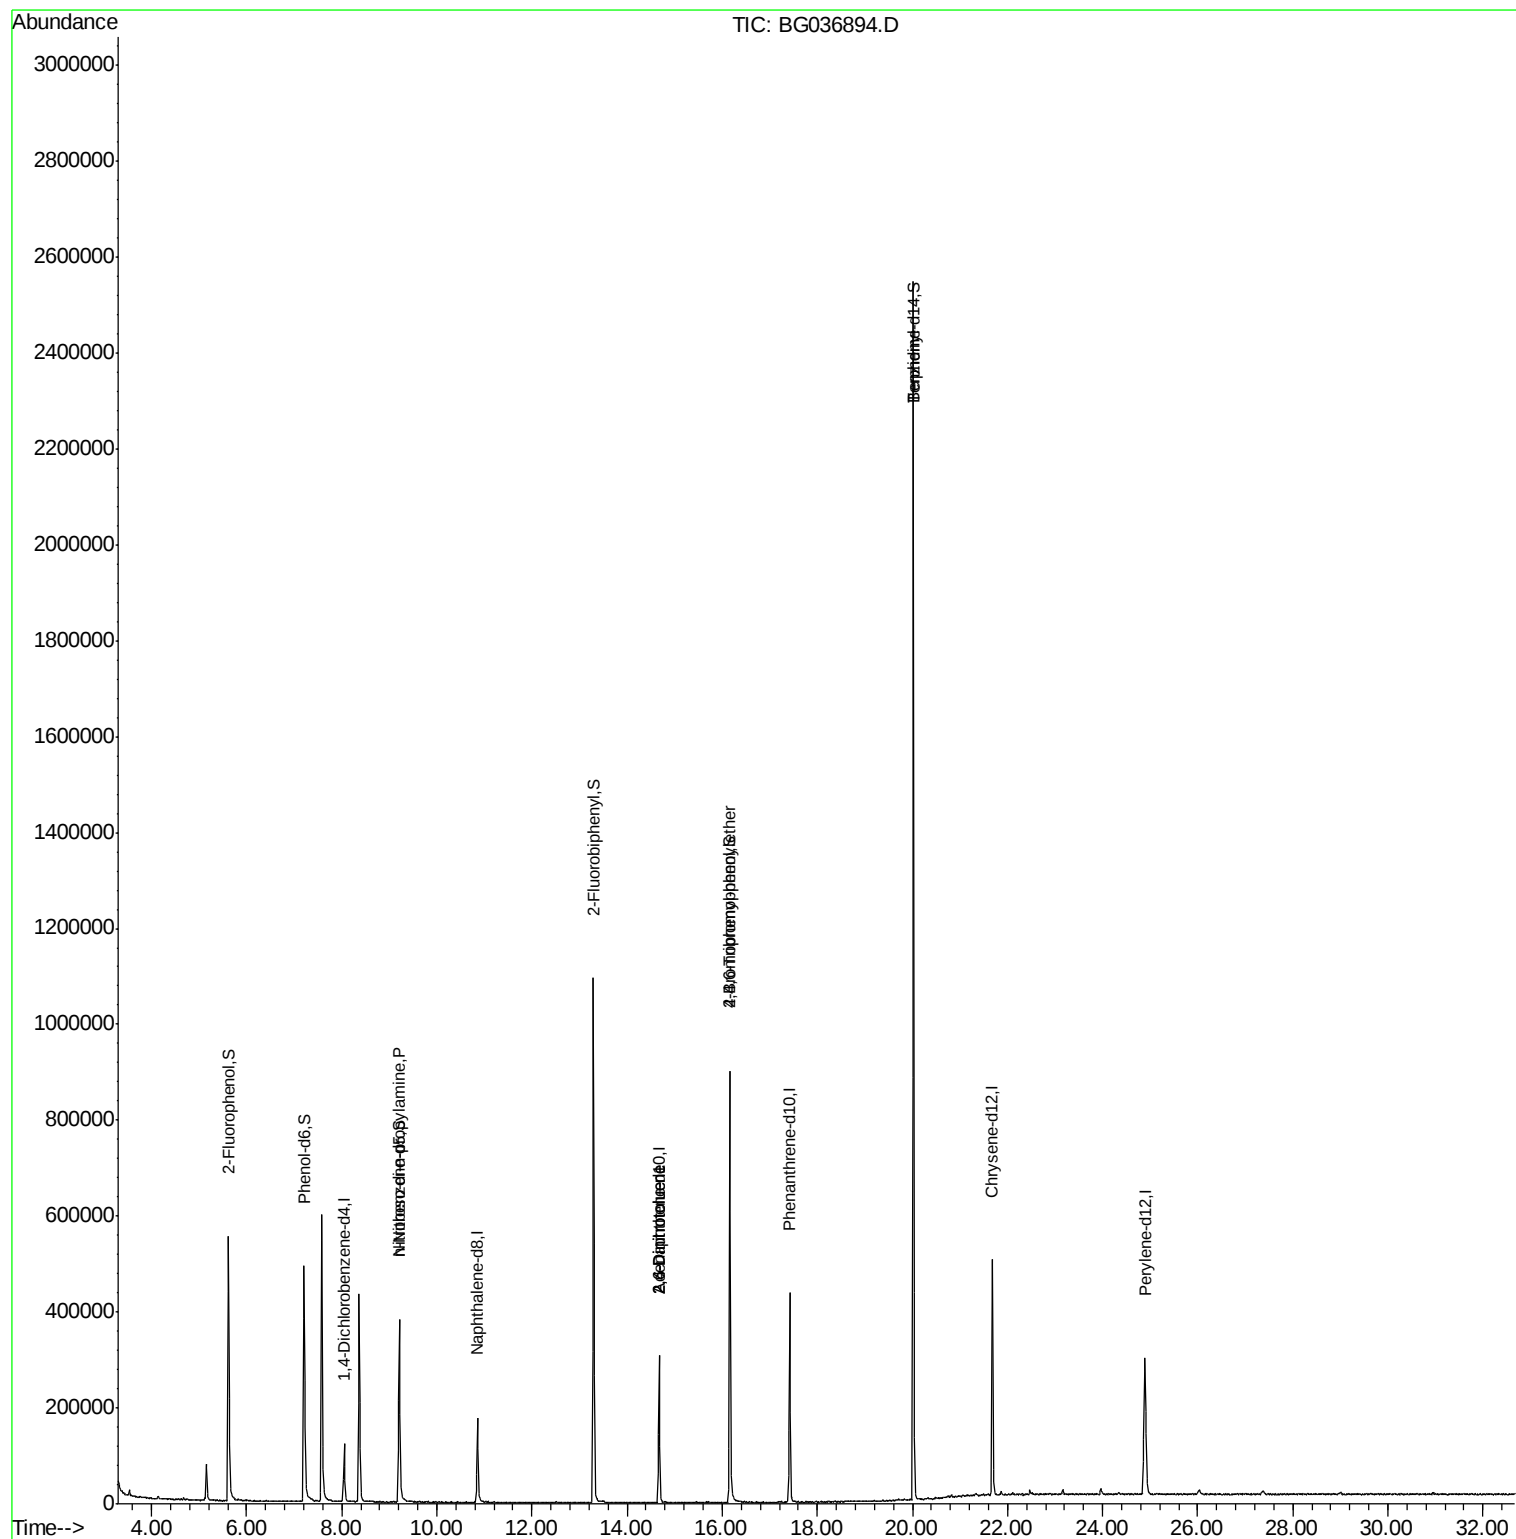

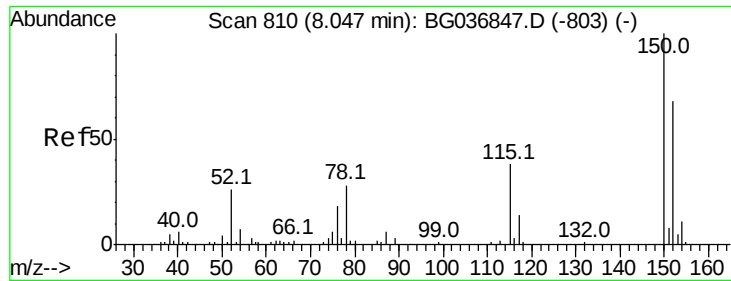


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.04 min Scan# 809
 Delta R.T. -0.00 min
 Lab File: BG036894.D
 Acq: 22 Sep 2018 14:53

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	144.8	119.5	179.3
115	60.2	44.5	66.7



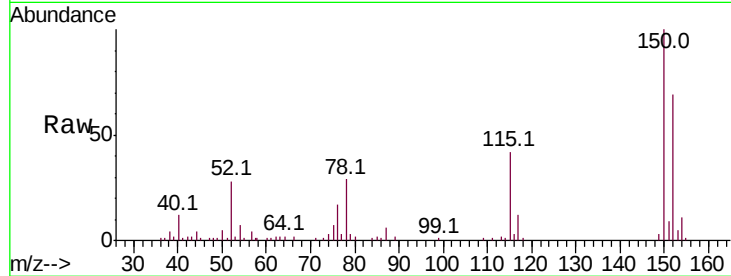


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

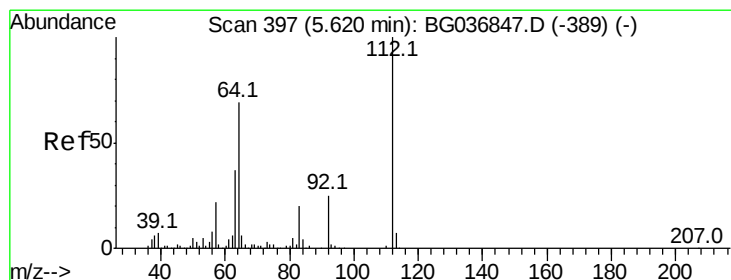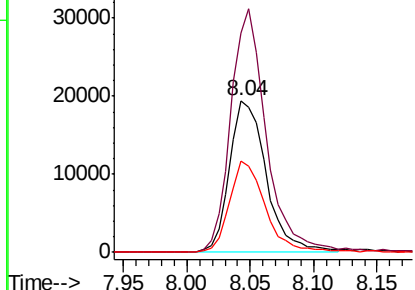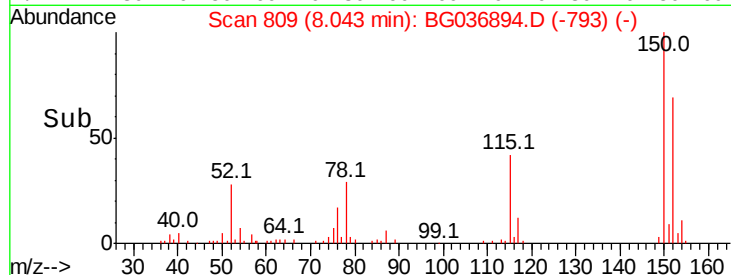

#5

2-Fluorophenol
 Concen: 126.831 ng
 RT: 5.62 min Scan# 396
 Delta R.T. -0.00 min
 Lab File: BG036894.D
 Acq: 22 Sep 2018 14:53

Tgt Ion	Ratio	Lower	Upper
112	100		
64	72.2	57.2	85.8
63	38.1	30.8	46.2






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

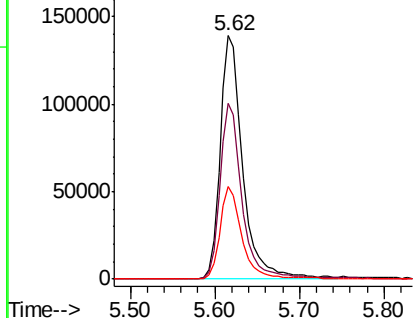

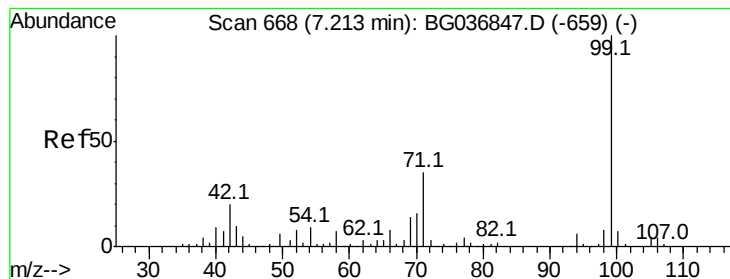

#7

Phenol-d6

Concen: 107.041 ng

RT: 7.21 min Scan# 667

Delta R.T. -0.00 min

Lab File: BG036894.D

Acq: 22 Sep 2018 14:53

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 338382

Ion Ratio Lower Upper




99 100

42 20.6 16.5 24.7

71 37.4 29.4 44.2

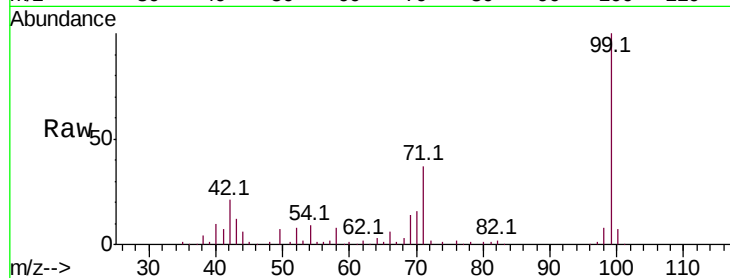

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

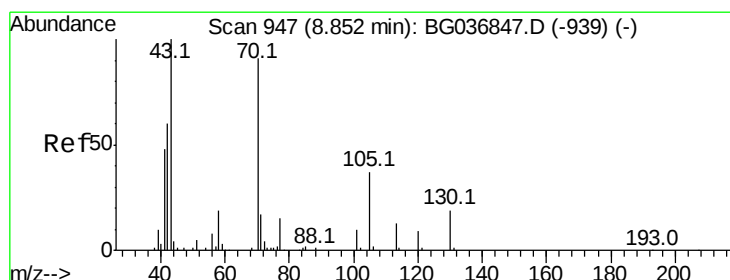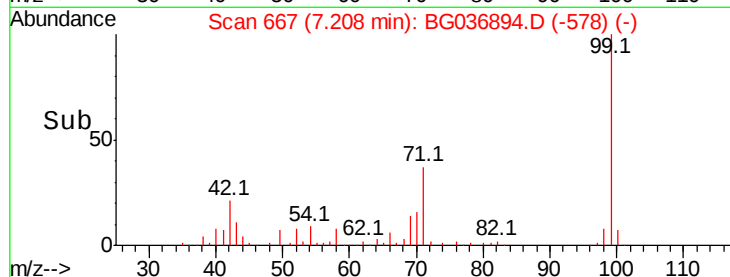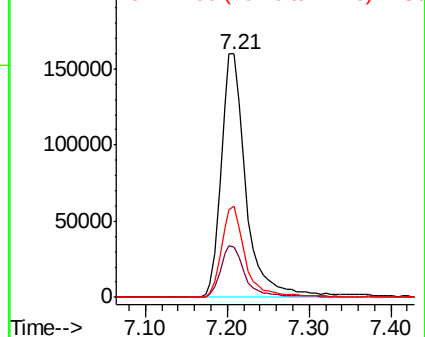

#19

n-Nitroso-di-n-propylamine

Concen: 14.077 ng

RT: 9.21 min Scan# 1007

Delta R.T. 0.35 min

Lab File: BG036894.D

Acq: 22 Sep 2018 14:53

Tgt Ion: 70 Resp: 37020


Ion Ratio Lower Upper

70 100



42 52.2 56.2 84.4#

101 0.0 7.8 11.6#

130 2.3 16.2 24.2#

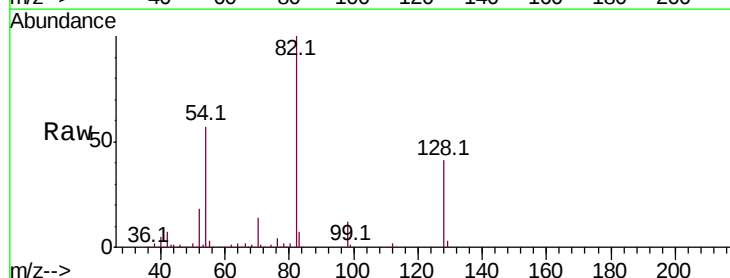

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

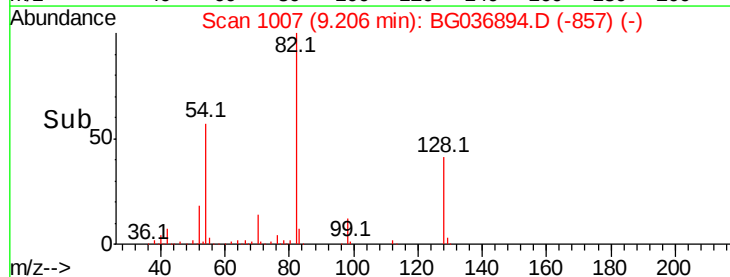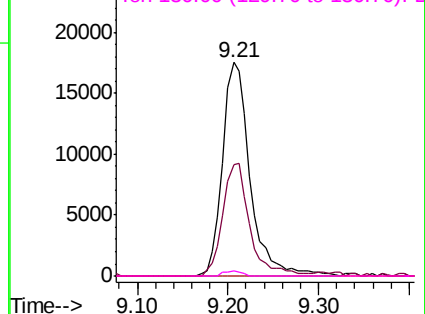







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.85 min Scan# 1287
Delta R.T. -0.00 min
Lab File: BG036894.D
Acq: 22 Sep 2018 14:53

Instrument :
BNA_G
ClientSampleId :

Tot Ion:	136	Resp:	166230
Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.8	13.2
54	11.0	9.2	13.8
68	6.4	5.8	8.6

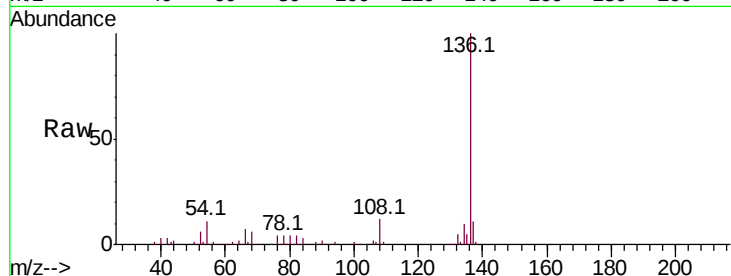


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


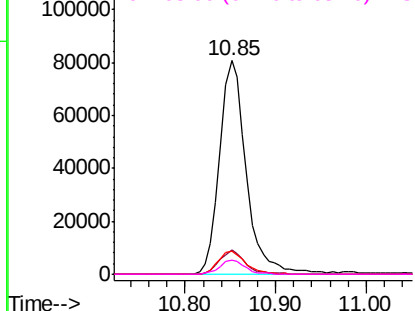



#23
Nitrobenzene-d5
Concen: 86.698 ng
RT: 9.21 min Scan# 1007
Delta R.T. -0.00 min
Lab File: BG036894.D
Acq: 22 Sep 2018 14:53

Tgt Ion:	82	Resp:	269122
Ion	Ratio	Lower	Upper
82	100		
128	40.9	33.3	49.9
54	56.8	45.1	67.7



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

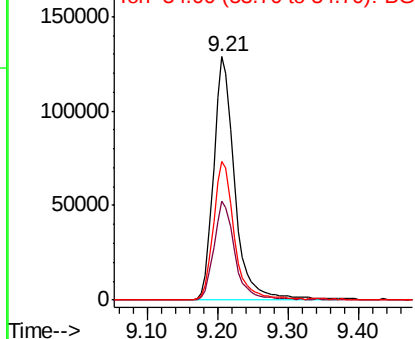



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.67 min Scan# 1937

Delta R.T. -0.00 min

Lab File: BG036894.D

Acq: 22 Sep 2018 14:53


Instrument :

BNA_G

ClientSampleId :

Tot Ion:164 Resp: 113507




Ion	Ratio	Lower	Upper
164	100		
162	102.9	80.7	121.1
160	46.0	35.3	52.9

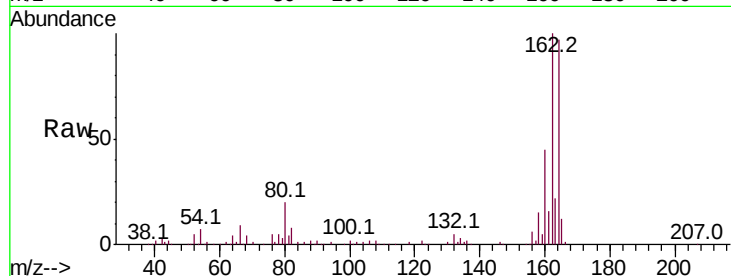

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

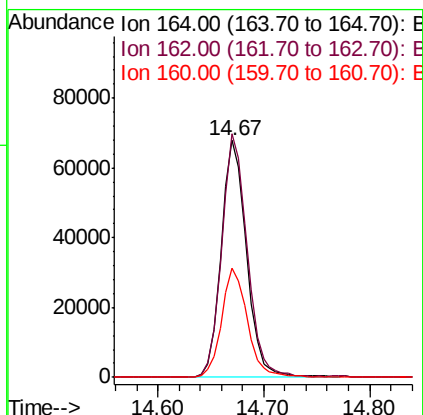

#41

2,4,6-Tribromophenol

Concen: 131.536 ng

RT: 16.16 min Scan# 2191


Delta R.T. -0.00 min

Lab File: BG036894.D

Acq: 22 Sep 2018 14:53

Tgt Ion:330 Resp: 178632



Ion	Ratio	Lower	Upper
330	100		
332	100.3	75.4	113.2
141	39.7	30.7	46.1



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



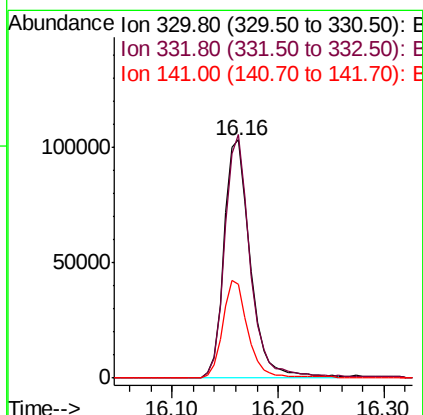





#44
 2-Fluorobiphenyl
 Concen: 80.391 ng
 RT: 13.30 min Scan# 1703
 Delta R.T. -0.00 min
 Lab File: BG036894.D
 Acq: 22 Sep 2018 14:53




Instrument :
 BNA_G
 ClientSampled :


Tot Ion:172 Resp: 612665
 Ion Ratio Lower Upper
 172 100
 171 37.7 31.3 46.9
 170 25.2 21.0 31.6

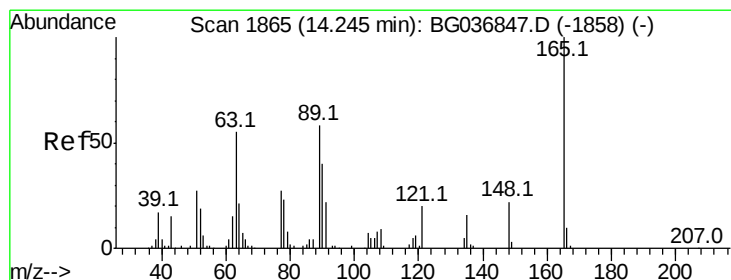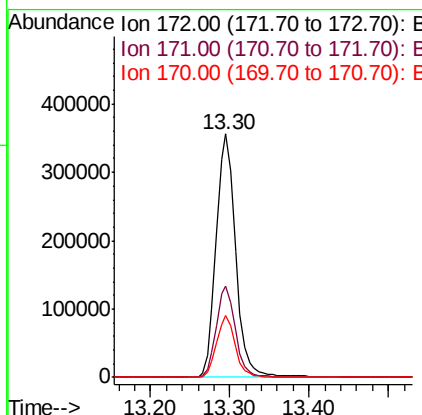

#50
 2,6-Dinitrotoluene
 Concen: 7.464 ng
 RT: 14.68 min Scan# 1938
 Delta R.T. 0.43 min
 Lab File: BG036894.D
 Acq: 22 Sep 2018 14:53

Tgt Ion:165 Resp: 14879
 Ion Ratio Lower Upper
 165 100
 63 0.0 50.1 75.1#
 89 0.0 47.8 71.6#

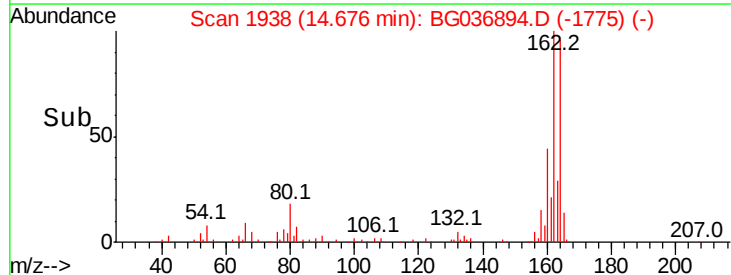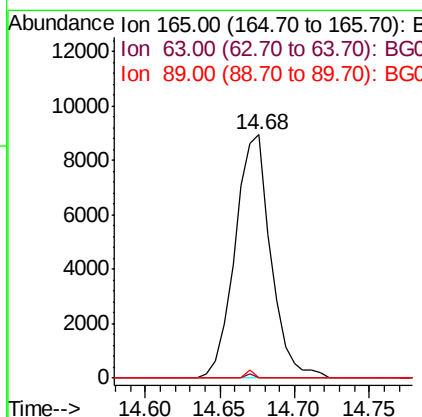


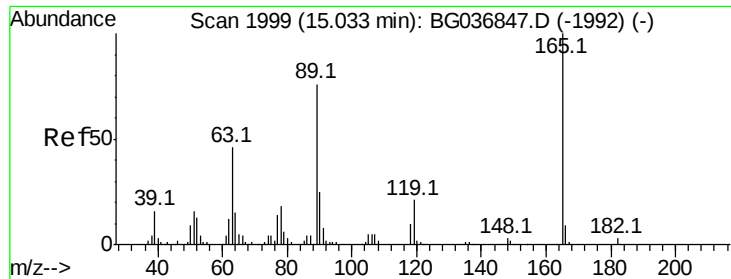

#56
2,4-Dinitrotoluene
Concen: 5.349 ng
RT: 14.68 min Scan# 1938
Delta R.T. -0.36 min
Lab File: BG036894.D
Acq: 22 Sep 2018 14:53

Instrument :
BNA_G
ClientSampled :

Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	40.1	60.1#
89	0.0	63.7	95.5#
182	0.0	2.5	3.7#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

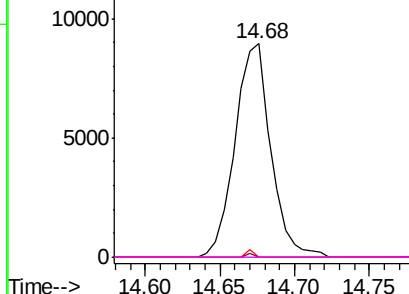




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.41 min Scan# 2404
Delta R.T. -0.00 min
Lab File: BG036894.D
Acq: 22 Sep 2018 14:53


Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.7	6.7	10.1
80	10.0	8.1	12.1

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

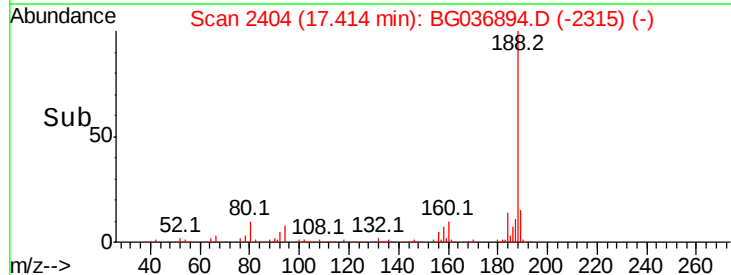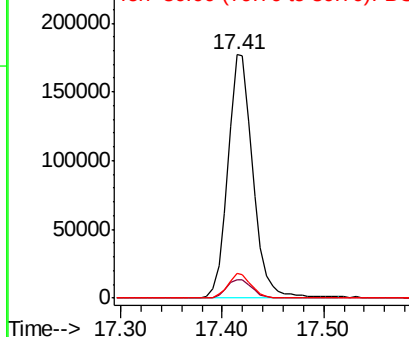


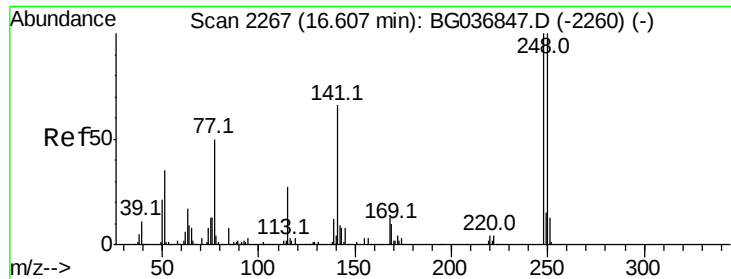




#66
 4-Bromophenyl-phenylether
 Concen: 3.695 ng
 RT: 16.16 min Scan# 2191
 Delta R.T. -0.44 min
 Lab File: BG036894.D
 Acq: 22 Sep 2018 14:53

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:248 Resp: 12715
 Ion Ratio Lower Upper
 248 100
 250 195.2 78.1 117.1#
 141 572.6 53.7 80.5#

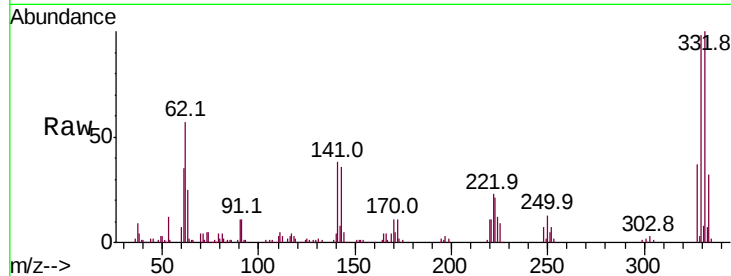


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E


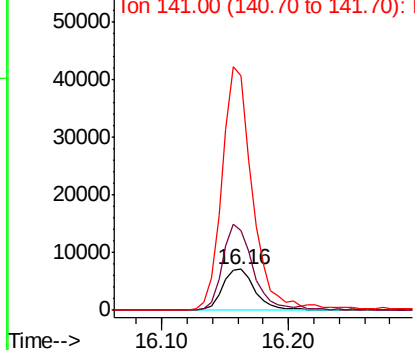



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.68 min Scan# 3130
 Delta R.T. -0.01 min
 Lab File: BG036894.D
 Acq: 22 Sep 2018 14:53

Tgt Ion:240 Resp: 329531
 Ion Ratio Lower Upper
 240 100
 120 8.1 6.9 10.3
 236 24.9 21.2 31.8



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

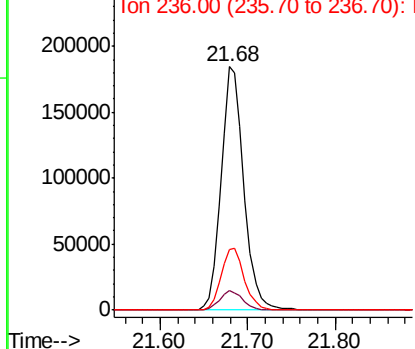

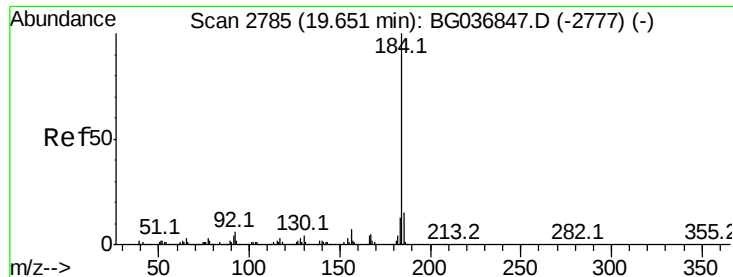

#76

Benzidine

Concen: 2.139 ng

RT: 20.02 min Scan# 2848

Delta R.T. 0.37 min

Lab File: BG036894.D

Acq: 22 Sep 2018 14:53

Instrument :

BNA_G

ClientSampleId :





Tot Ion:184 Resp: 21307

Ion Ratio Lower Upper

184 100

185 17.2 12.6 18.8

183 7.5 10.9 16.3#

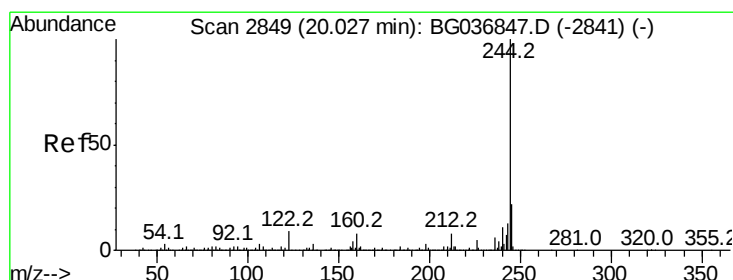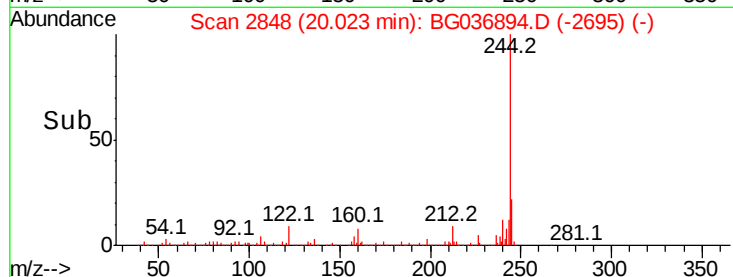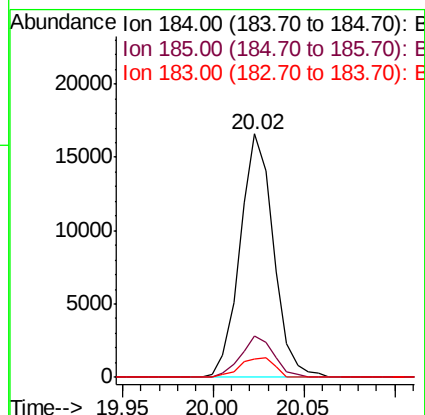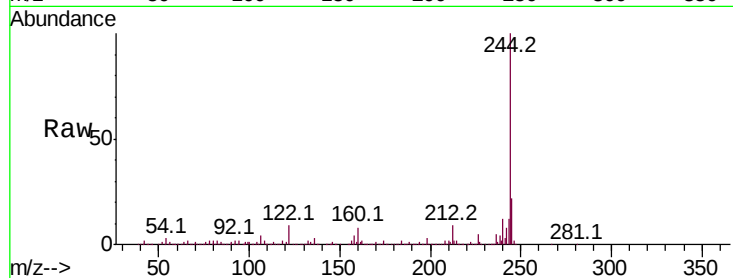

#78

Terphenyl-d14

Concen: 97.337 ng

RT: 20.02 min Scan# 2848

Delta R.T. -0.00 min

Lab File: BG036894.D

Acq: 22 Sep 2018 14:53




Tgt Ion:244 Resp: 1219838


Ion Ratio Lower Upper

244 100

212 8.5 7.0 10.6

122 9.4 7.1 10.7

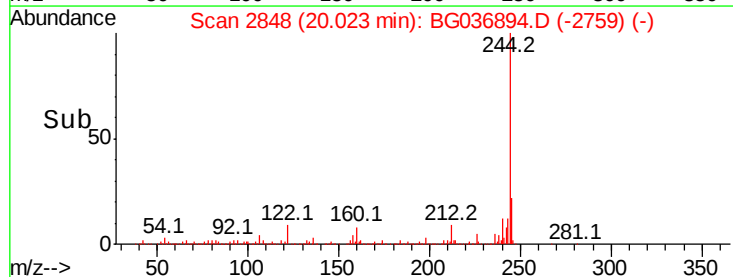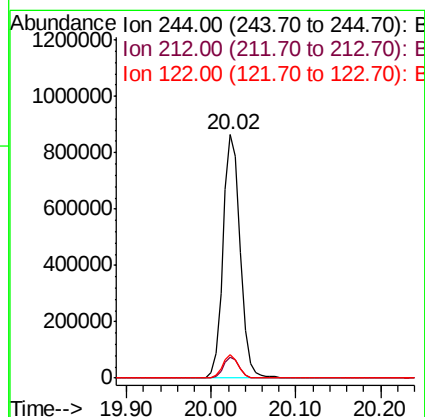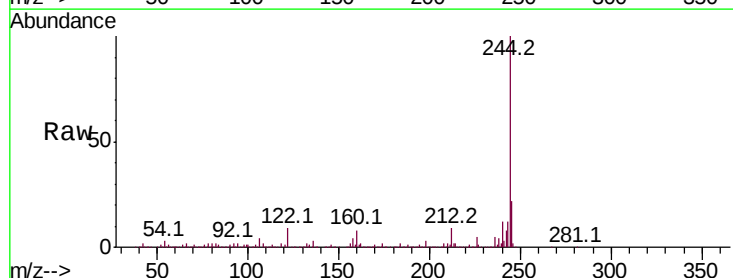


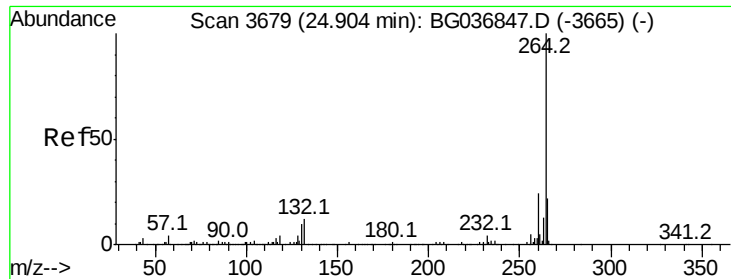

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.89 min Scan# 3677
Delta R.T. -0.01 min
Lab File: BG036894.D
Acq: 22 Sep 2018 14:53

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.6	29.4
265	22.7	17.4	26.0



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

