
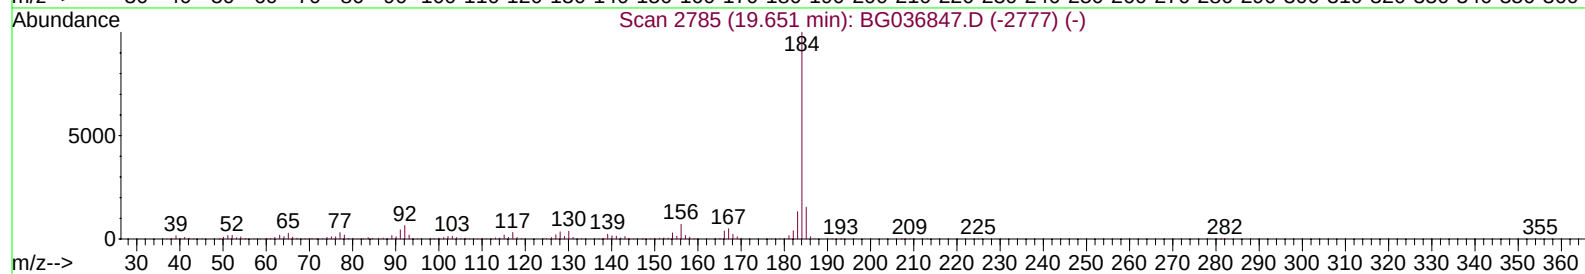
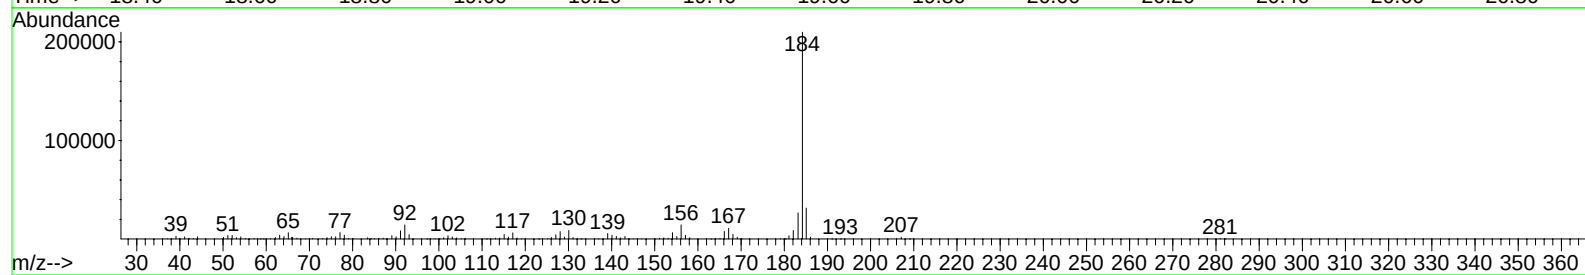


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092118\
 Data File : BG036852.D
 Acq On : 21 Sep 2018 8:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 18:21:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 20 20:07:11 2018
 Response via : Initial Calibration

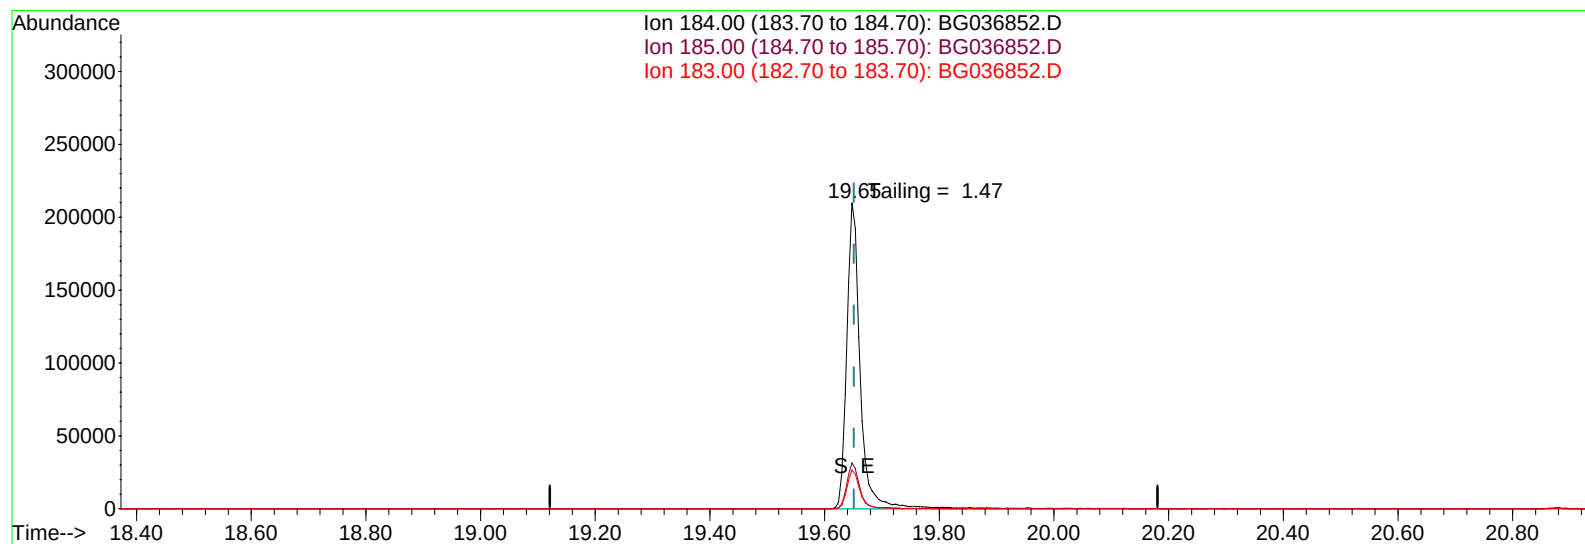

TIC: BG036852.D

(76) Benzidine




19.648min (-0.003) 7214.94ng

response 337409

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.02
183.00	13.60	12.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092118\
Data File : BG036852.D
Acq On : 21 Sep 2018 8:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 18:21:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 20 20:07:11 2018
Response via : Initial Calibration

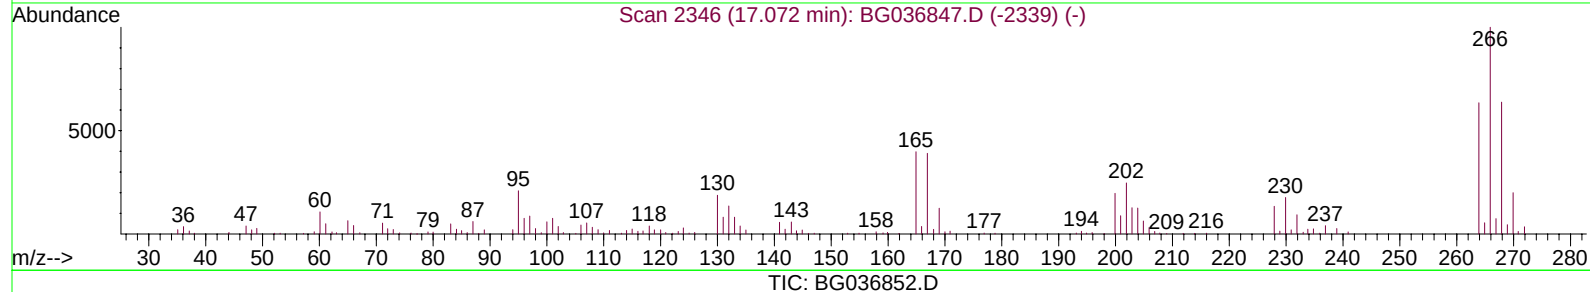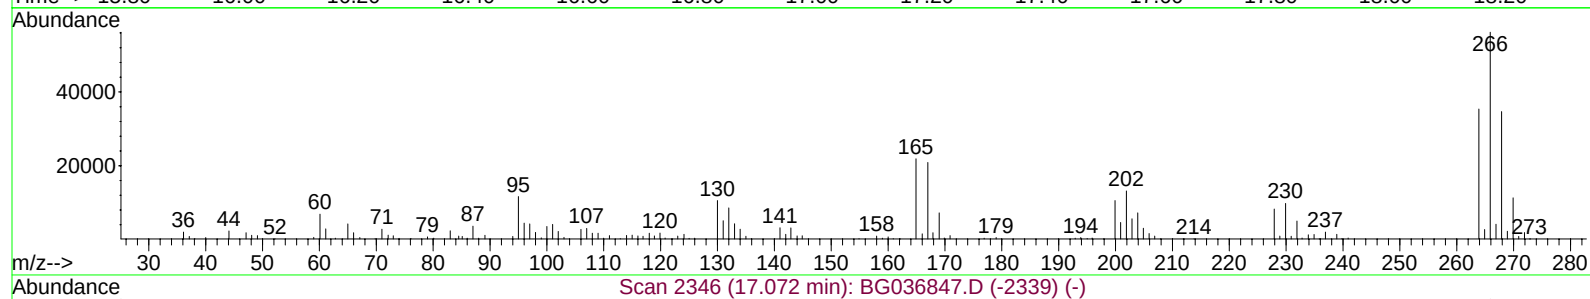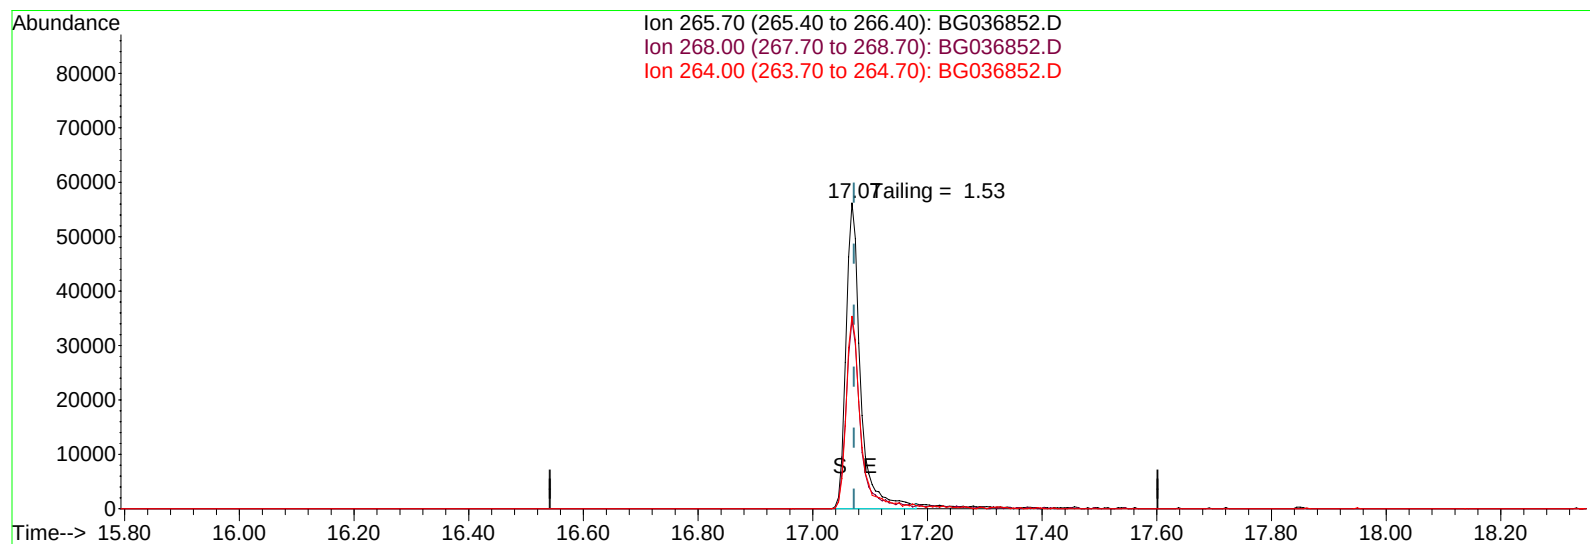

(69) Pentachlorophenol (C)

17.068min (-0.003) 10728.76ng

response 100419

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.75
264.00	61.10	62.93
0.00	0.00	0.00