

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092118\
 Data File : BG036866.D
 Acq On : 21 Sep 2018 20:02
 Operator : JU/SJ
 Sample : J4777-16
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-02-0920-18-C

Quant Time: Sep 22 05:01:27 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 20 20:07:11 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	38270	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	158438	20.00	ng	0.00
38) Acenaphthene-d10	14.67	164	106584	20.00	ng	0.00
63) Phenanthrene-d10	17.42	188	292950	20.00	ng	0.00
75) Chrysene-d12	21.69	240	323374	20.00	ng	0.00
86) Perylene-d12	24.89	264	314853	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	250570	125.57	ng	0.00
7) Phenol-d6	7.21	99	322320	104.40	ng	0.00
23) Nitrobenzene-d5	9.21	82	253755	85.77	ng	0.00
41) 2,4,6-Tribromophenol	16.16	330	184208	144.45	ng	0.00
44) 2-Fluorobiphenyl	13.30	172	582015	81.33	ng	0.00
78) Terphenyl-d14	20.02	244	1226461	99.73	ng	0.00
Target Compounds						
31) Naphthalene	10.91	128	20257	2.687	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092118\
Data File : BG036866.D
Acq On : 21 Sep 2018 20:02
Operator : JU/SJ
Sample : J4777-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-02-0920-18-C

Quant Time: Sep 22 05:01:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 20 20:07:11 2018
Response via : Initial Calibration

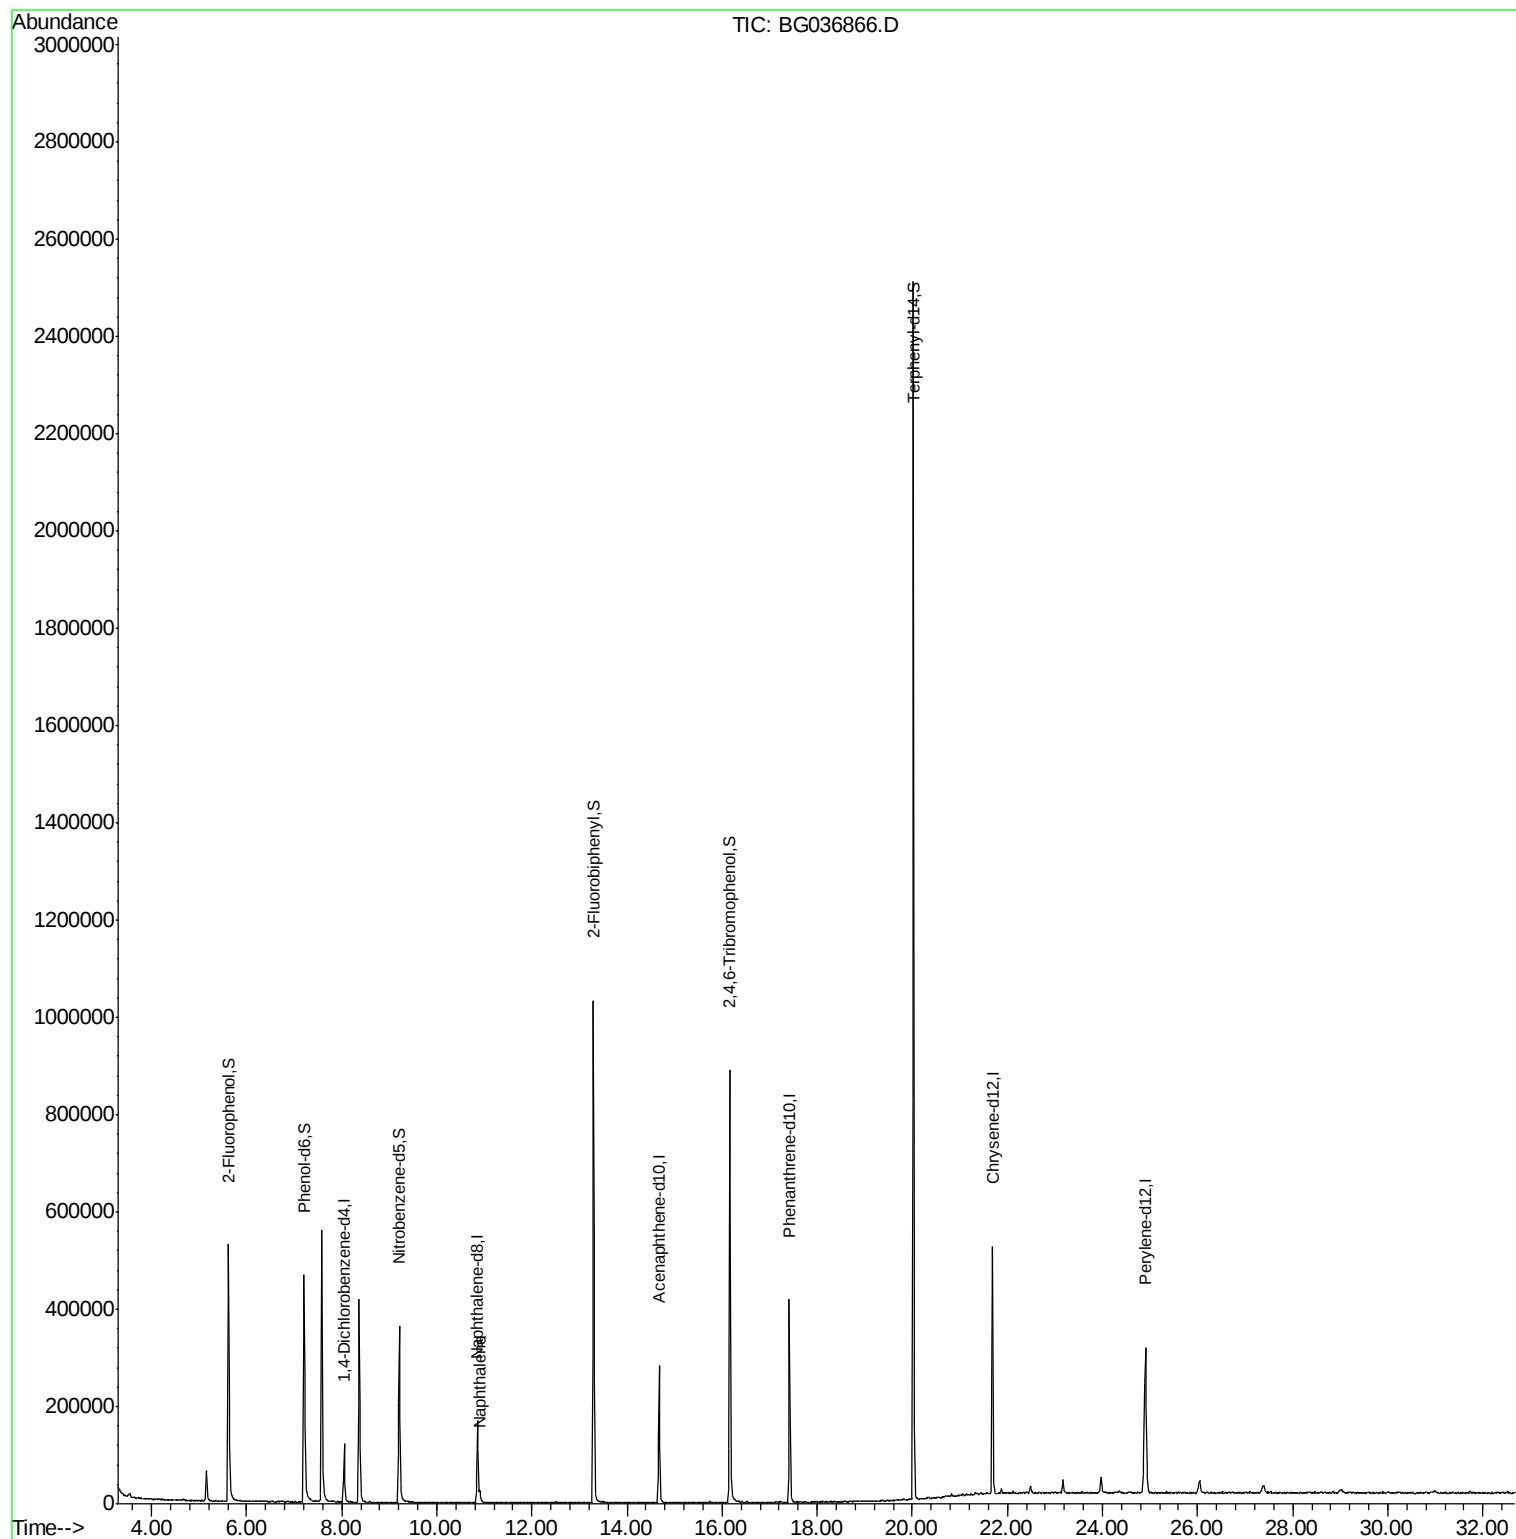

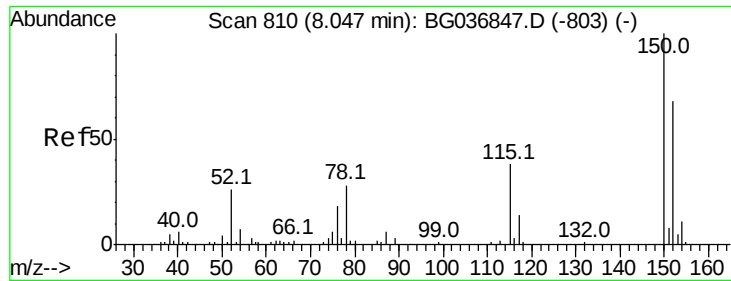


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.05 min Scan# 810
 Delta R.T. 0.00 min
 Lab File: BG036866.D
 Acq: 21 Sep 2018 20:02

Instrument :
 BNA_G
 ClientSampleId :
 PL-02-0920-18-C

Tot Ion	Ratio	Lower	Upper
152	100		
150	143.8	119.5	179.3
115	51.0	44.5	66.7



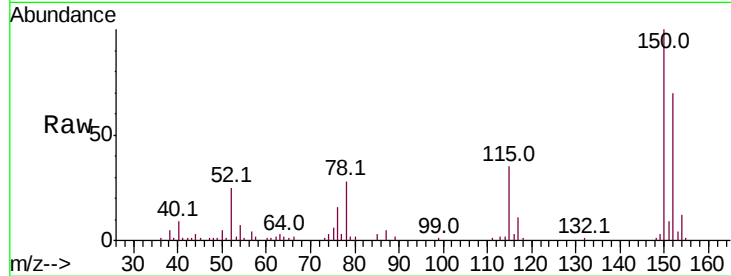


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

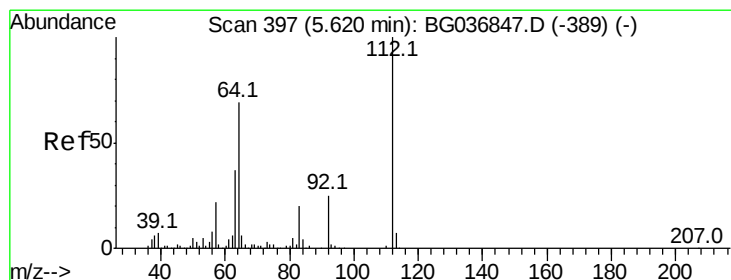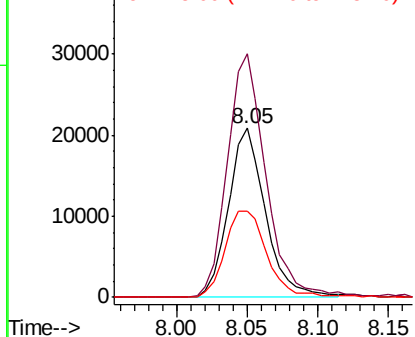

#5

2-Fluorophenol
 Concen: 125.565 ng
 RT: 5.62 min Scan# 396
 Delta R.T. -0.00 min
 Lab File: BG036866.D
 Acq: 21 Sep 2018 20:02

Tgt Ion	Ratio	Lower	Upper
112	100		
64	71.0	57.2	85.8
63	38.3	30.8	46.2





Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

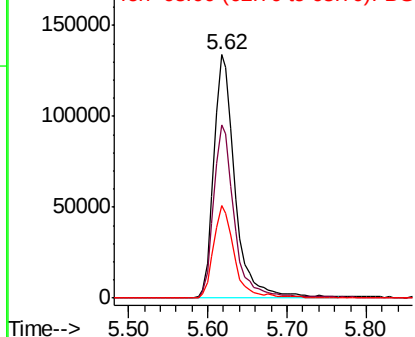



#7

Phenol-d6

Concen: 104.397 ng

RT: 7.21 min Scan# 667

Delta R.T. -0.00 min

Lab File: BG036866.D

Acq: 21 Sep 2018 20:02

Instrument :

BNA_G

ClientSampleId :

PL-02-0920-18-C



Tot Ion: 99 Resp: 322320

Ion Ratio Lower Upper

99 100

42 21.5 16.5 24.7



71 36.5 29.4 44.2

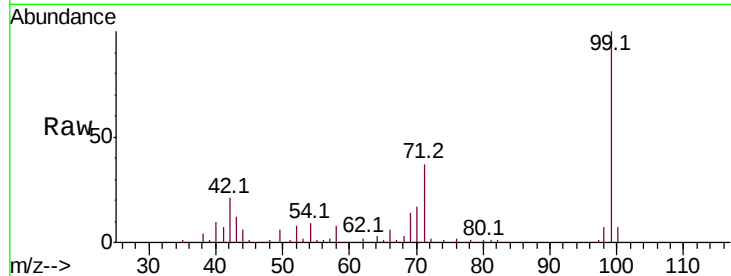

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

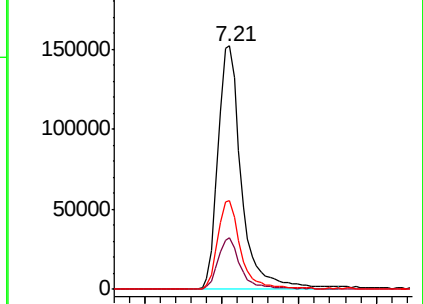

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1287

Delta R.T. -0.00 min

Lab File: BG036866.D

Acq: 21 Sep 2018 20:02

Tgt Ion: 136 Resp: 158438



Ion Ratio Lower Upper

136 100

137 10.6 8.8 13.2

54 11.1 9.2 13.8

68 7.4 5.8 8.6





Abundance Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC




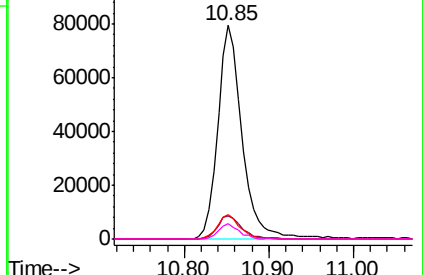


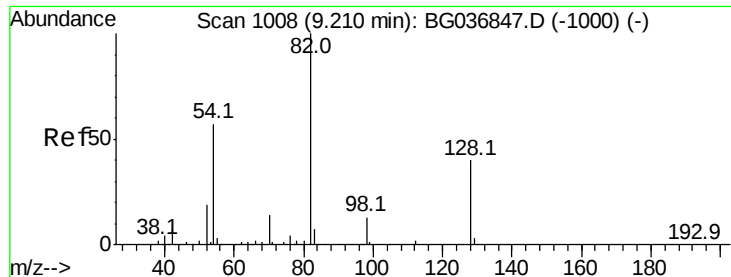

#23
Nitrobenzene-d5
Concen: 85.768 ng
RT: 9.21 min Scan# 1007
Delta R.T. -0.00 min
Lab File: BG036866.D
Acq: 21 Sep 2018 20:02




Instrument :
BNA_G
ClientSampleId :
PL-02-0920-18-C


Tot Ion	Ratio	Lower	Upper
82	100		
128	39.3	33.3	49.9
54	56.8	45.1	67.7

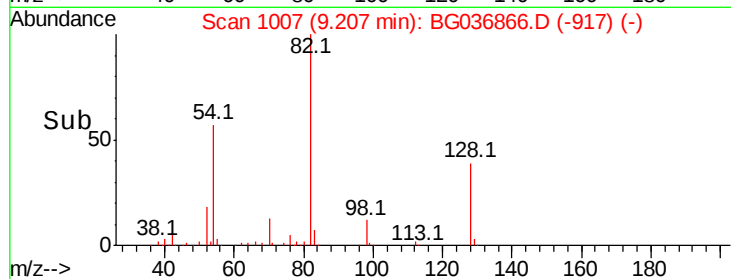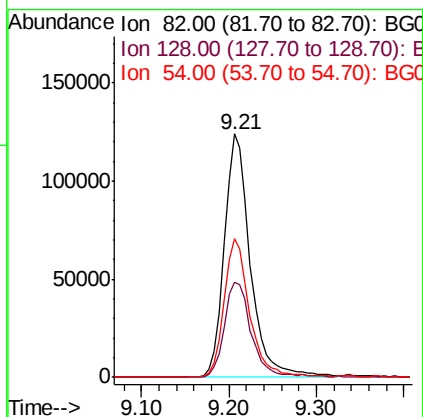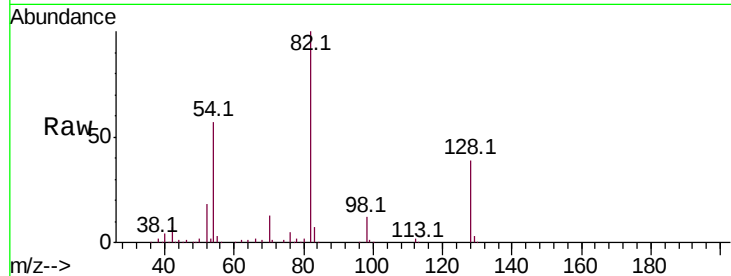

#31
Naphthalene
Concen: 2.687 ng
RT: 10.91 min Scan# 1296
Delta R.T. -0.00 min
Lab File: BG036866.D
Acq: 21 Sep 2018 20:02

Tgt Ion	Ratio	Lower	Upper
128	100		
129	11.0	9.4	14.2
127	12.2	11.0	16.4

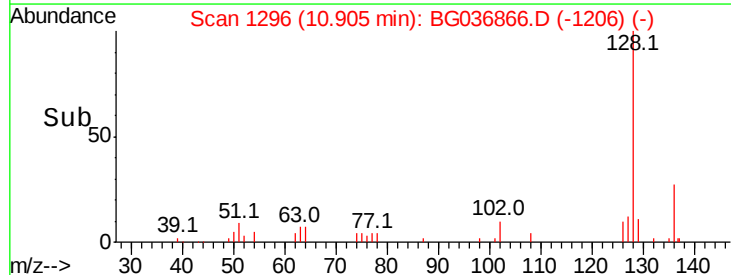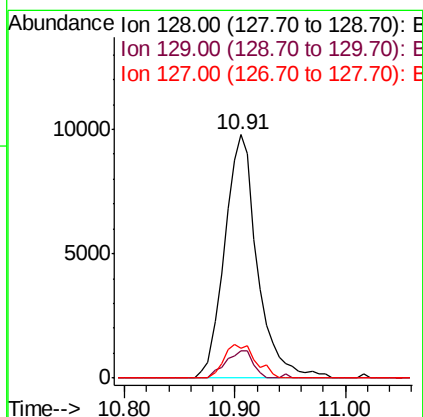



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.67 min Scan# 1937

Delta R.T. -0.00 min

Lab File: BG036866.D

Acq: 21 Sep 2018 20:02

Instrument :

BNA_G

ClientSampleId :

PL-02-0920-18-C





Tot Ion:164 Resp: 106584

Ion Ratio Lower Upper

164 100

162 106.7 80.7 121.1

160 44.2 35.3 52.9

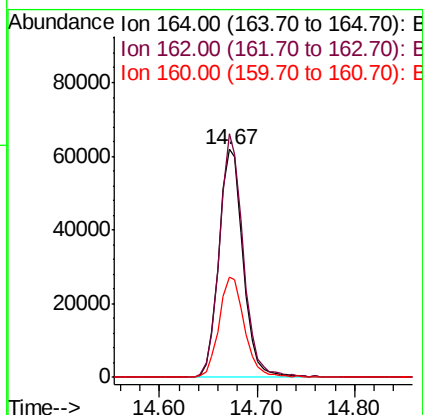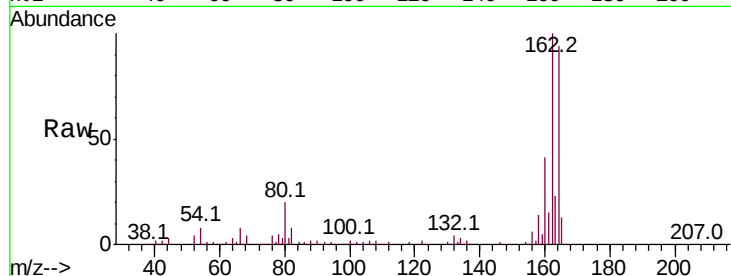

#41

2,4,6-Tribromophenol

Concen: 144.453 ng

RT: 16.16 min Scan# 2191

Delta R.T. -0.00 min

Lab File: BG036866.D

Acq: 21 Sep 2018 20:02




Tgt Ion:330 Resp: 184208

Ion Ratio Lower Upper

330 100

332 94.5 75.4 113.2

141 37.3 30.7 46.1


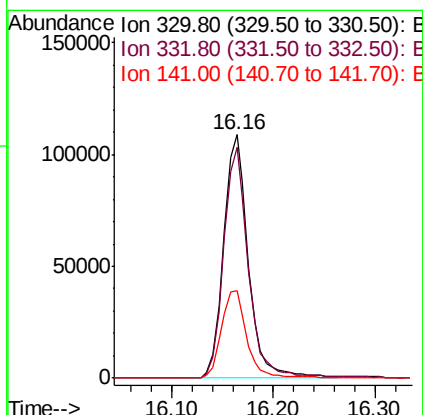






#44
 2-Fluorobiphenyl
 Concen: 81.330 ng
 RT: 13.30 min Scan# 1703
 Delta R.T. -0.00 min
 Lab File: BG036866.D
 Acq: 21 Sep 2018 20:02




Instrument :
 BNA_G
 ClientSampleId :
 PL-02-0920-18-C


Tot Ion:172 Resp: 582015
 Ion Ratio Lower Upper
 172 100
 171 36.4 31.3 46.9
 170 24.2 21.0 31.6

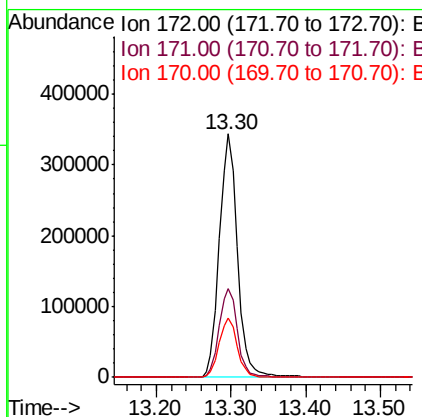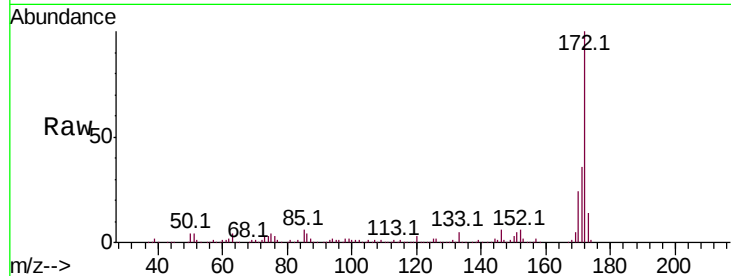

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.42 min Scan# 2404
 Delta R.T. -0.00 min
 Lab File: BG036866.D
 Acq: 21 Sep 2018 20:02

Tgt Ion:188 Resp: 292950
 Ion Ratio Lower Upper
 188 100
 94 8.3 6.7 10.1
 80 9.5 8.1 12.1

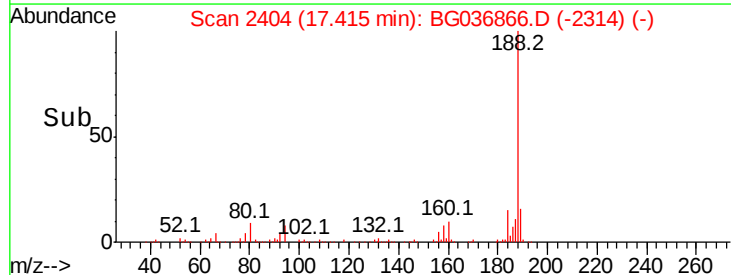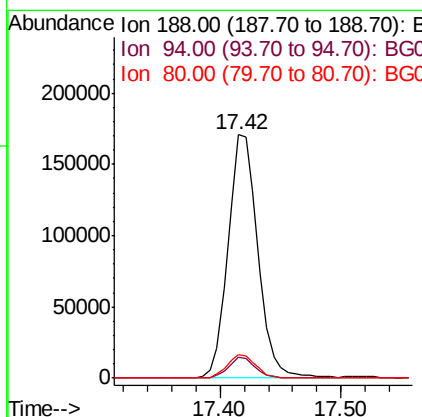

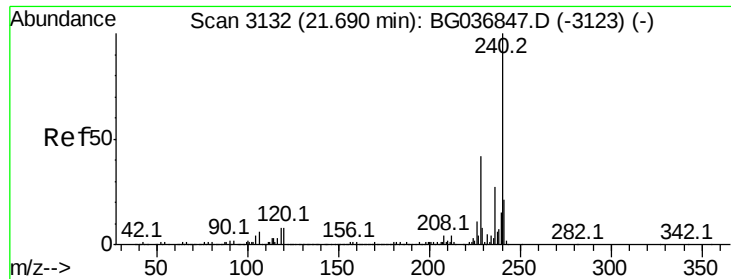

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3131

Delta R.T. -0.00 min

Lab File: BG036866.D

Acq: 21 Sep 2018 20:02

Instrument :

BNA_G

ClientSampleId :

PL-02-0920-18-C


Tot Ion:240 Resp: 323374

Ion Ratio Lower Upper

240 100

120 8.0 6.9 10.3




236 26.8 21.2 31.8

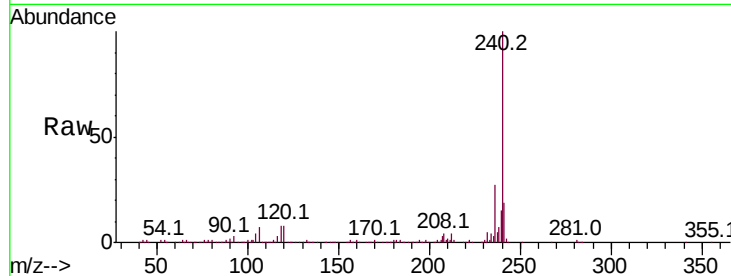

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

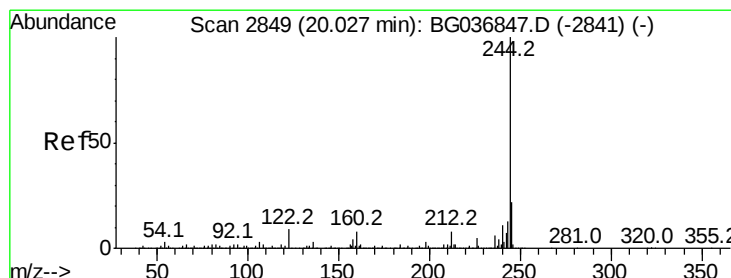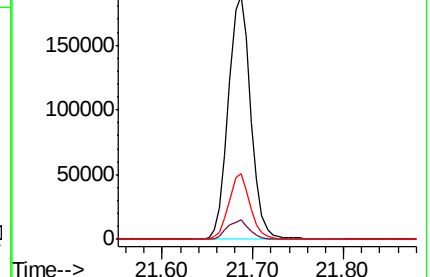

#78

Terphenyl-d14

Concen: 99.729 ng

RT: 20.02 min Scan# 2848

Delta R.T. -0.00 min

Lab File: BG036866.D

Acq: 21 Sep 2018 20:02


Tgt Ion:244 Resp: 1226461

Ion Ratio Lower Upper

244 100

212 8.7 7.0 10.6



122 9.2 7.1 10.7




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

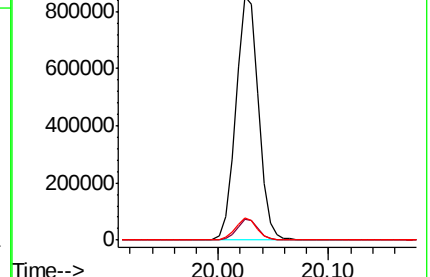


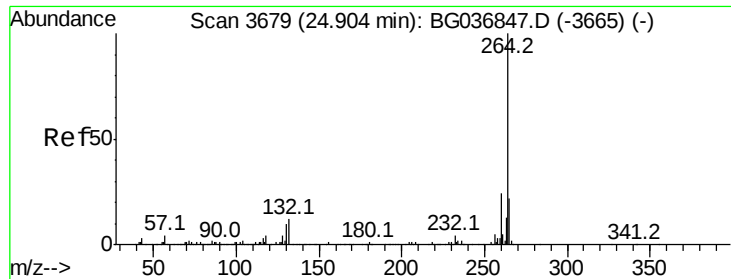

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 24.89 min Scan# 3677
 Delta R.T. -0.01 min
 Lab File: BG036866.D
 Acq: 21 Sep 2018 20:02

Instrument :
 BNA_G
 ClientSampleId :
 PL-02-0920-18-C

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.6	29.4
265	21.0	17.4	26.0

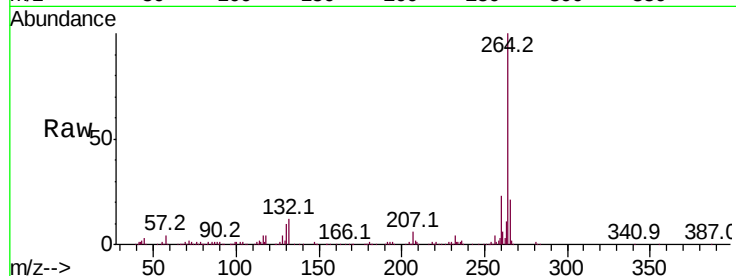

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

