

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092118\
 Data File : BG036874.D
 Acq On : 22 Sep 2018 1:14
 Operator : JU/SJ
 Sample : J4777-32
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PL-04-092018-D

Quant Time: Sep 22 05:10:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 20 20:07:11 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	40319	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	159801	20.00	ng	0.00
38) Acenaphthene-d10	14.67	164	105512	20.00	ng	0.00
63) Phenanthrene-d10	17.42	188	284101	20.00	ng	0.00
75) Chrysene-d12	21.68	240	316811	20.00	ng	0.00
86) Perylene-d12	24.90	264	312979	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	265988	126.52	ng	0.00
7) Phenol-d6	7.21	99	330856	101.72	ng	0.00
23) Nitrobenzene-d5	9.21	82	261044	87.48	ng	0.00
41) 2,4,6-Tribromophenol	16.16	330	171330	135.72	ng	0.00
44) 2-Fluorobiphenyl	13.29	172	587198	82.89	ng	0.00
78) Terphenyl-d14	20.03	244	1177366	97.72	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092118\
Data File : BG036874.D
Acq On : 22 Sep 2018 1:14
Operator : JU/SJ
Sample : J4777-32
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PL-04-092018-D

Quant Time: Sep 22 05:10:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 20 20:07:11 2018
Response via : Initial Calibration

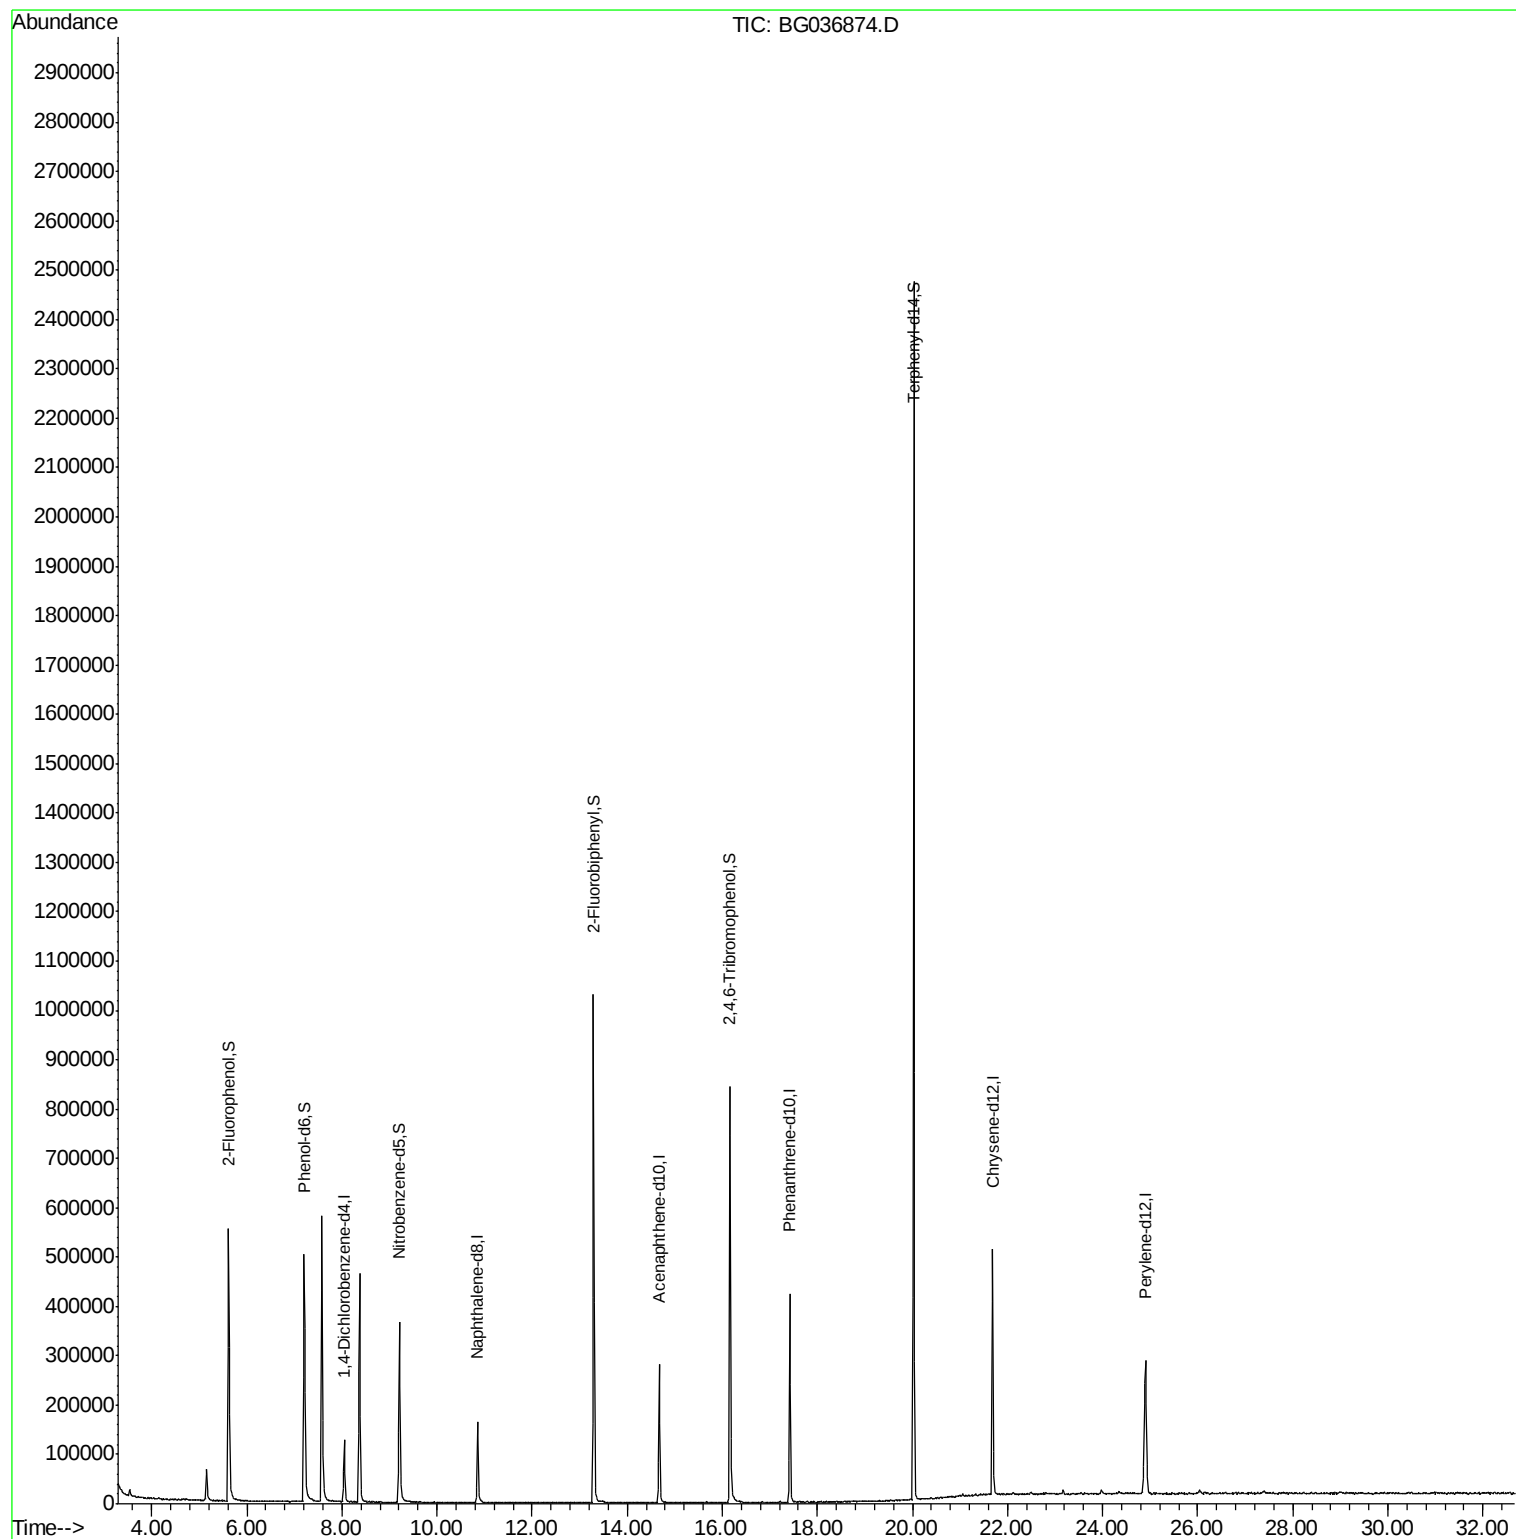

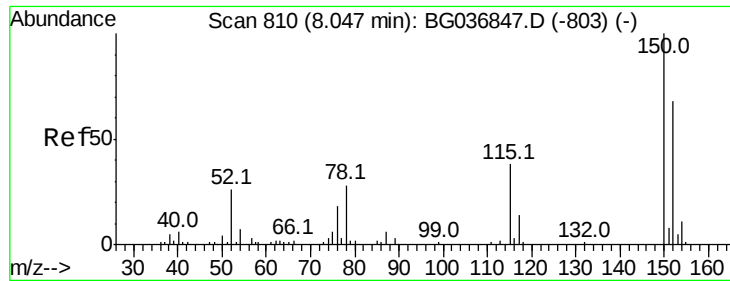


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.05 min Scan# 811
 Delta R.T. 0.01 min
 Lab File: BG036874.D
 Acq: 22 Sep 2018 1:14

Instrument :
 BNA_G
 ClientSampleId :
 PL-04-092018-D

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.0	119.5	179.3
115	53.5	44.5	66.7



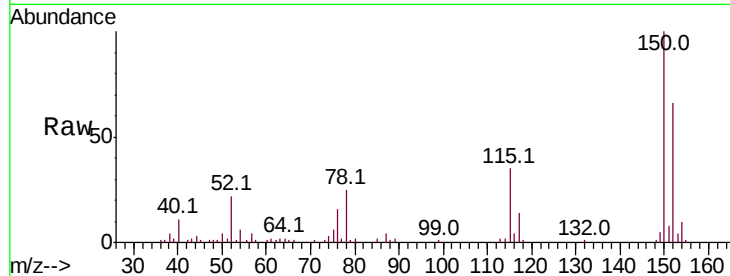


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

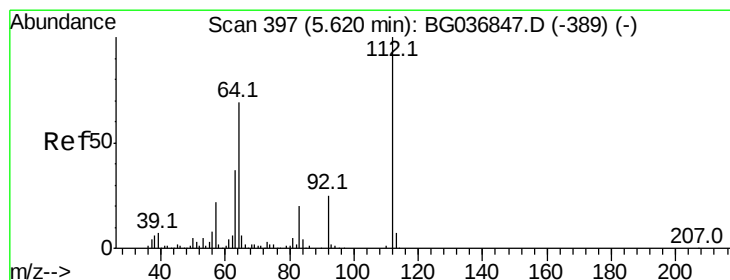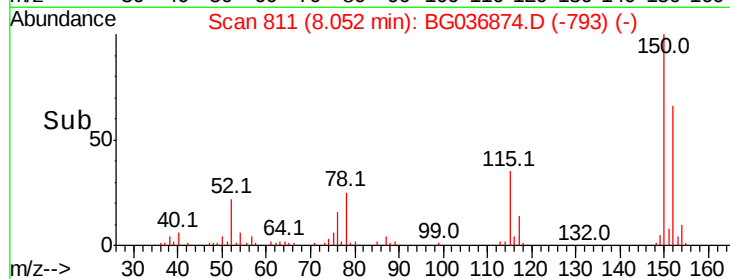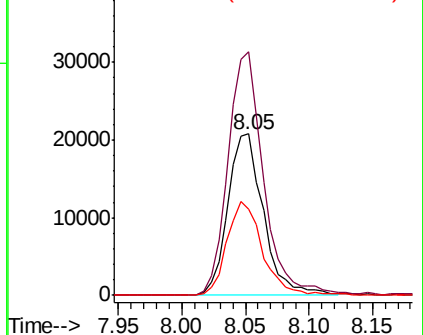

#5

2-Fluorophenol
 Concen: 126.518 ng
 RT: 5.62 min Scan# 397
 Delta R.T. -0.00 min
 Lab File: BG036874.D
 Acq: 22 Sep 2018 1:14

Tgt Ion	Ratio	Lower	Upper
112	100		
64	67.5	57.2	85.8
63	36.1	30.8	46.2


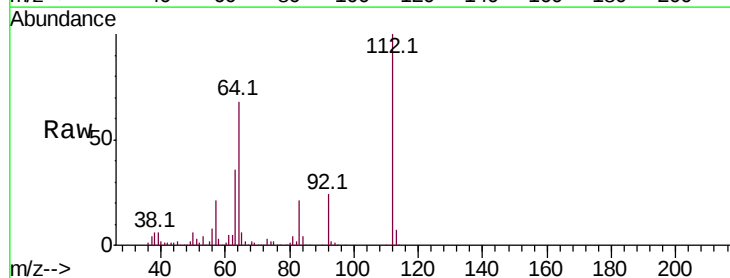


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

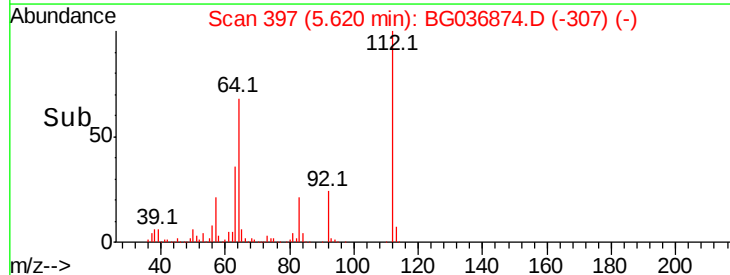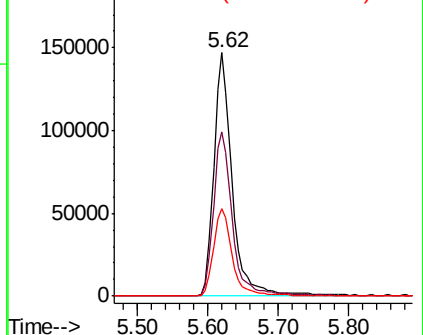



#7

Phenol-d6

Concen: 101.716 ng

RT: 7.21 min Scan# 667

Delta R.T. -0.01 min

Lab File: BG036874.D

Acq: 22 Sep 2018 1:14

Instrument :

BNA_G

ClientSampleId :

PL-04-092018-D


Tot Ion: 99 Resp: 330856

Ion Ratio Lower Upper




99 100

42 20.9 16.5 24.7

71 36.9 29.4 44.2

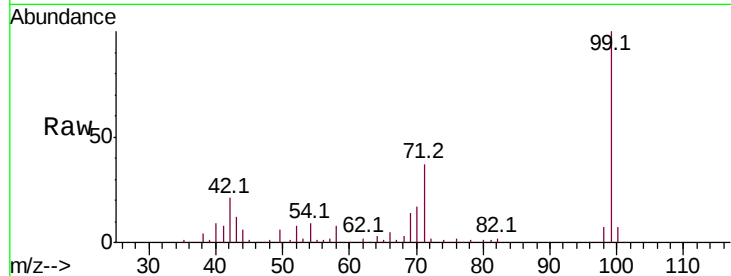

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

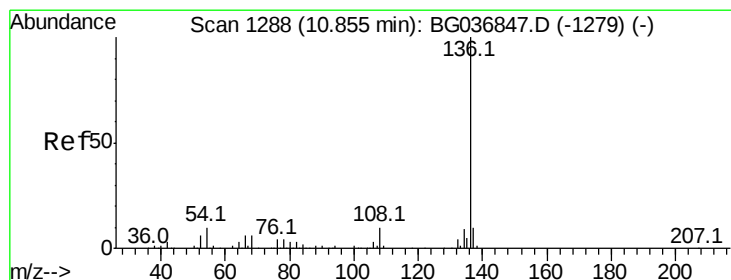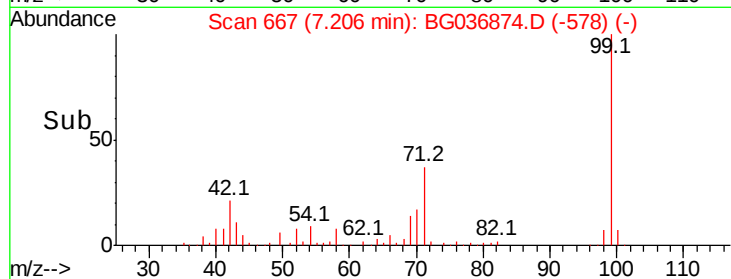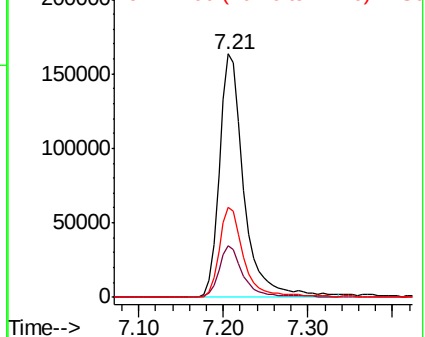

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.85 min Scan# 1288

Delta R.T. -0.00 min

Lab File: BG036874.D

Acq: 22 Sep 2018 1:14

Tgt Ion:136 Resp: 159801


Ion Ratio Lower Upper

136 100



137 10.6 8.8 13.2


54 10.2 9.2 13.8

68 6.9 5.8 8.6

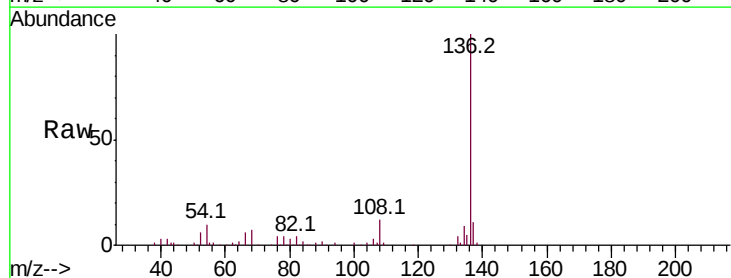

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

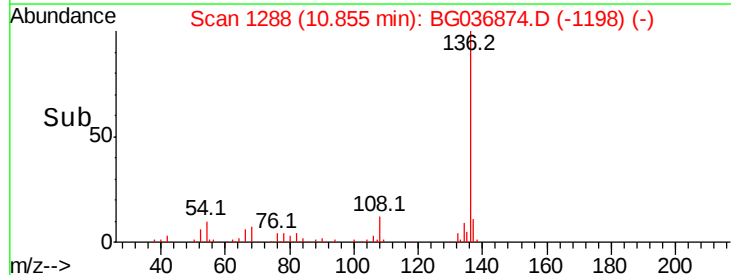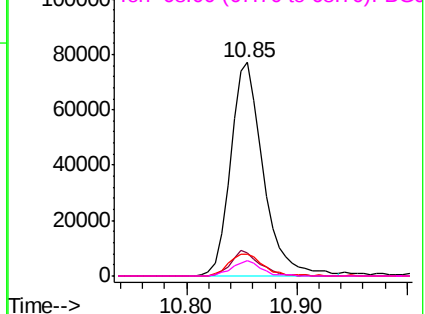


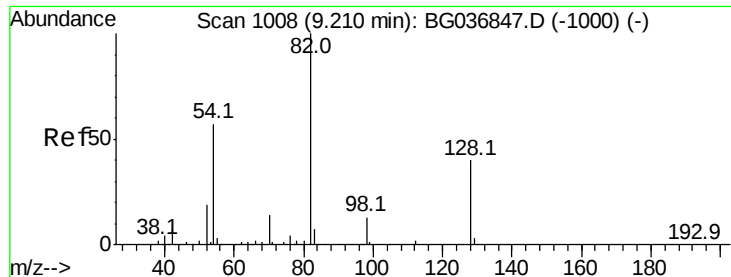




#23
Nitrobenzene-d5
Concen: 87.479 ng
RT: 9.21 min Scan# 1008
Delta R.T. -0.00 min
Lab File: BG036874.D
Acq: 22 Sep 2018 1:14

Instrument :
BNA_G
ClientSampleId :
PL-04-092018-D

Tot Ion	82	Resp	261044
Ion Ratio	Lower	Upper	
82	100		
128	41.5	33.3	49.9
54	56.7	45.1	67.7

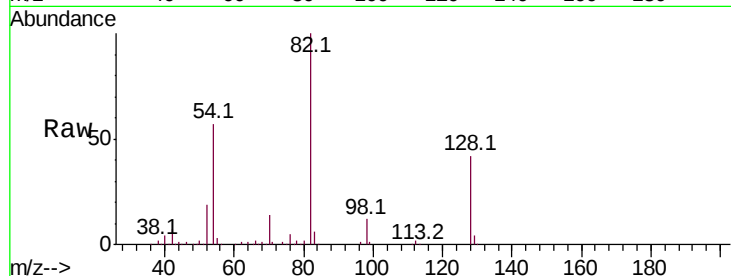


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

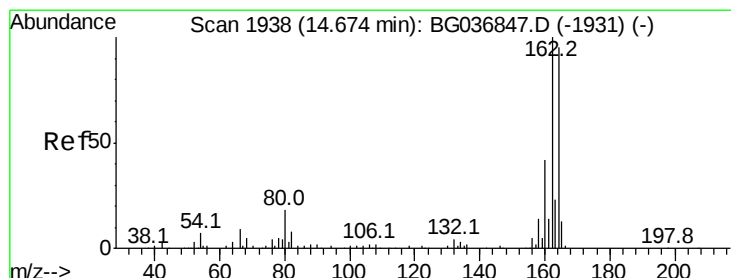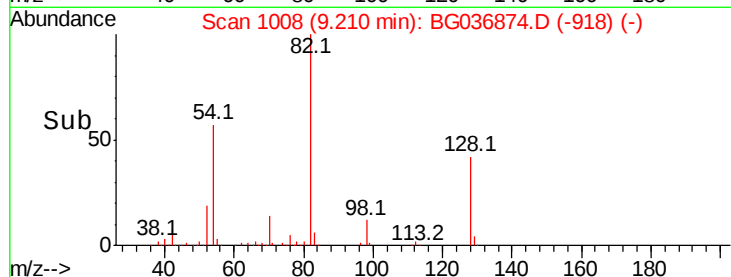
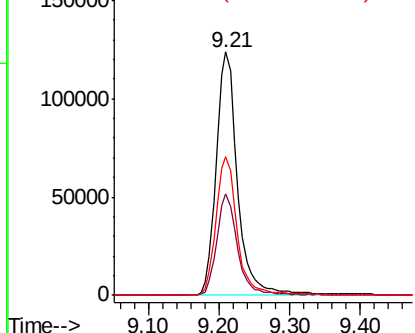


#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.67 min Scan# 1938
Delta R.T. -0.00 min
Lab File: BG036874.D
Acq: 22 Sep 2018 1:14

Tgt Ion	164	Resp	105512
Ion Ratio	Lower	Upper	
164	100		
162	101.2	80.7	121.1
160	45.5	35.3	52.9

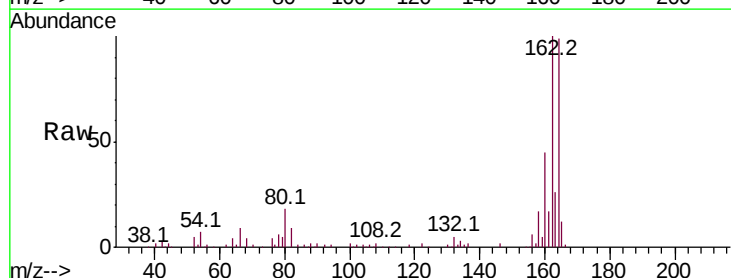

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

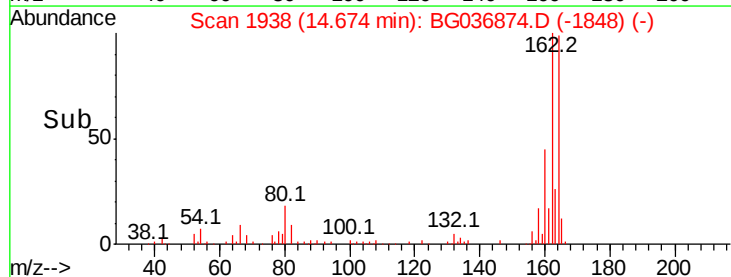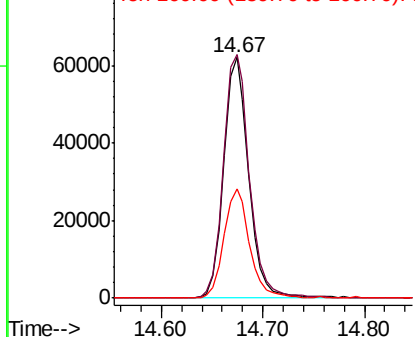







#41
 2,4,6-Tribromophenol
 Concen: 135.719 ng
 RT: 16.16 min Scan# 2191
 Delta R.T. -0.01 min
 Lab File: BG036874.D
 Acq: 22 Sep 2018 1:14

Instrument :
 BNA_G
 ClientSampleId :
 PL-04-092018-D

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	75.4	113.2
141	38.3	30.7	46.1

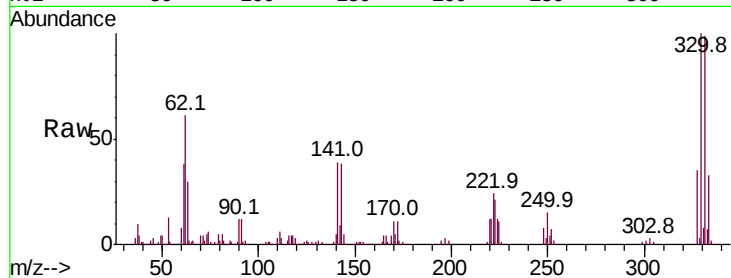


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

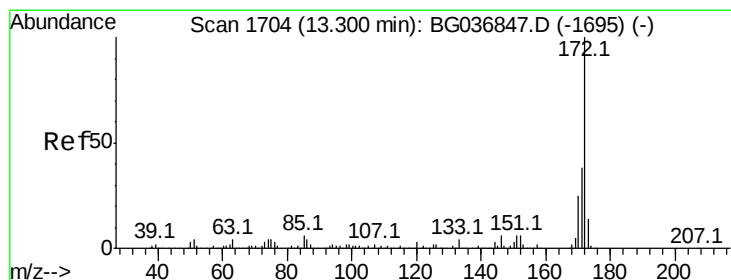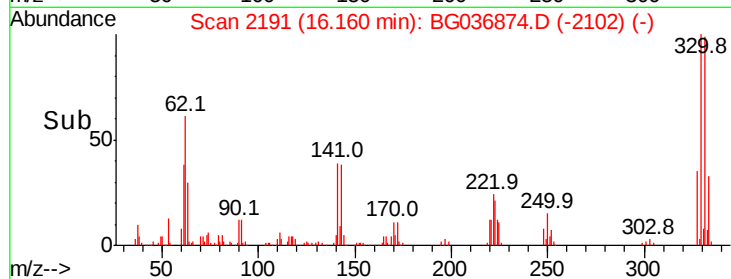
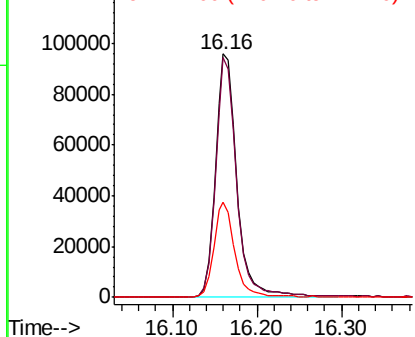


#44
 2-Fluorobiphenyl
 Concen: 82.888 ng
 RT: 13.29 min Scan# 1703
 Delta R.T. -0.01 min
 Lab File: BG036874.D
 Acq: 22 Sep 2018 1:14

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	31.3	46.9
170	24.2	21.0	31.6

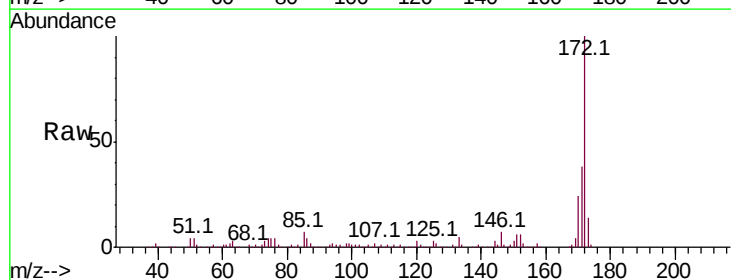

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



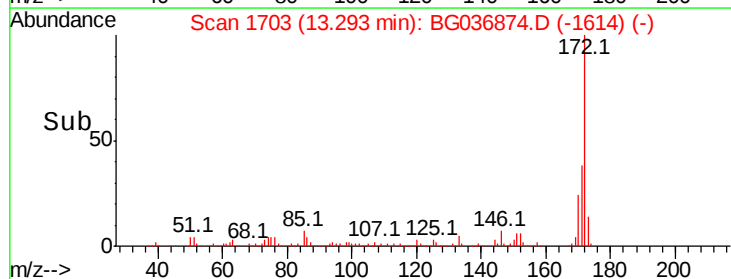
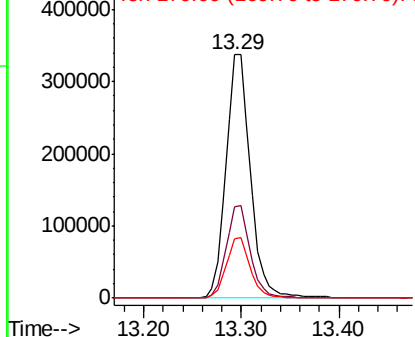




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.42 min Scan# 2405
Delta R.T. -0.00 min
Lab File: BG036874.D
Acq: 22 Sep 2018 1:14




Instrument :
BNA_G
ClientSampleId :
PL-04-092018-D

Tot Ion:188 Resp: 284101
Ion Ratio Lower Upper
188 100
94 7.7 6.7 10.1
80 8.4 8.1 12.1

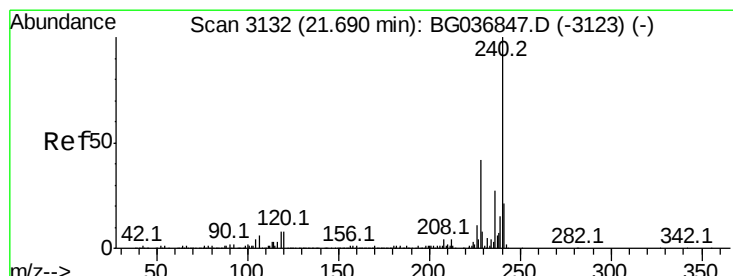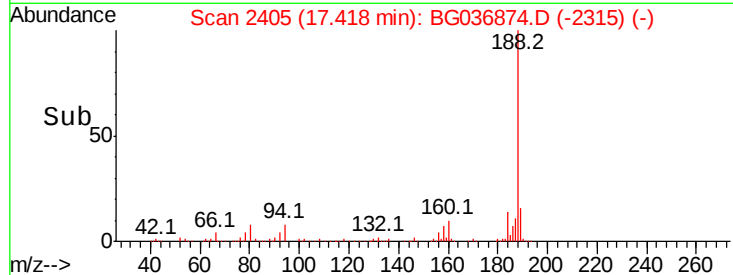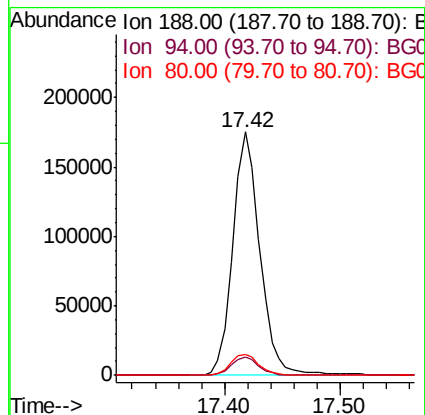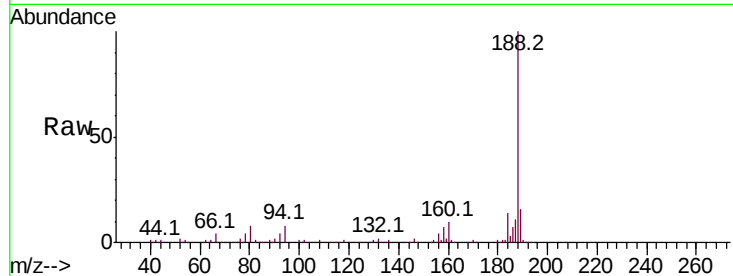

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.68 min Scan# 3131
Delta R.T. -0.01 min
Lab File: BG036874.D
Acq: 22 Sep 2018 1:14

Tgt Ion:240 Resp: 316811
Ion Ratio Lower Upper
240 100
120 8.5 6.9 10.3
236 26.3 21.2 31.8

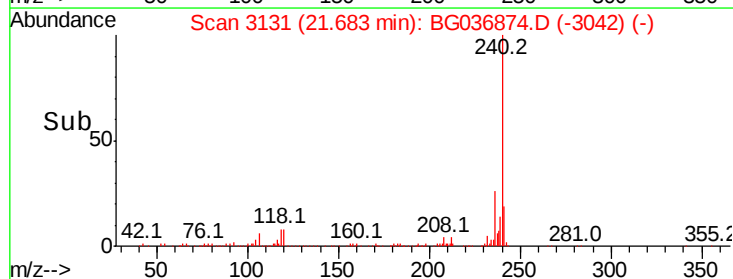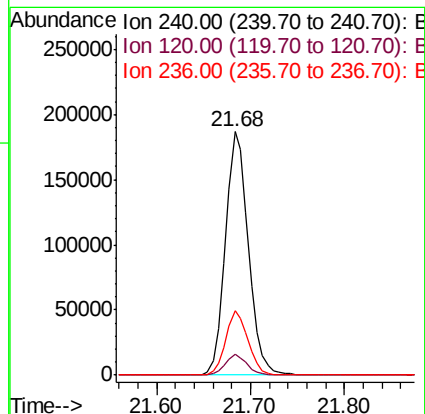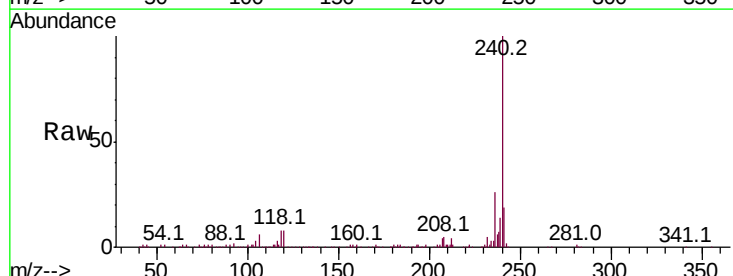







#78
 Terphenyl-d14
 Concen: 97.720 ng
 RT: 20.03 min Scan# 2849
 Delta R.T. -0.00 min
 Lab File: BG036874.D
 Acq: 22 Sep 2018 1:14

Instrument :
 BNA_G
 ClientSampleId :
 PL-04-092018-D

Tot Ion:244 Resp: 1177366

Ion	Ratio	Lower	Upper
244	100		
212	8.5	7.0	10.6
122	8.8	7.1	10.7

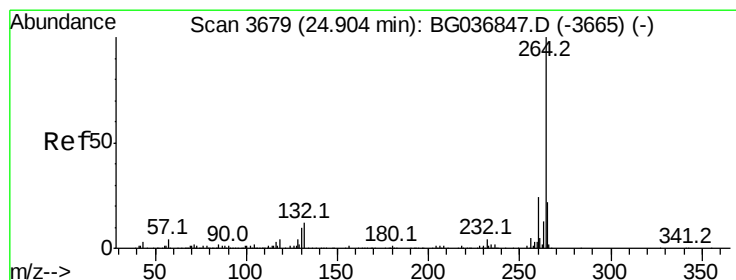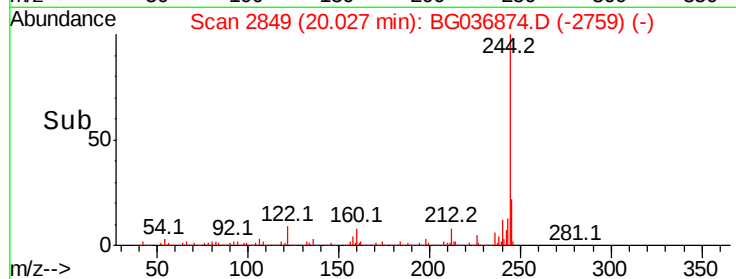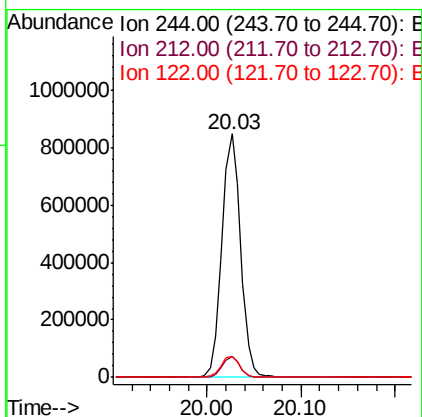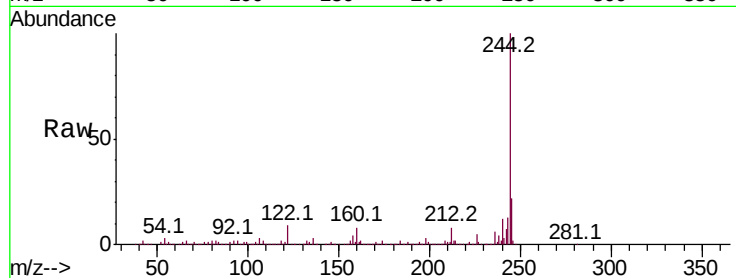

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.90 min Scan# 3678
 Delta R.T. -0.01 min
 Lab File: BG036874.D
 Acq: 22 Sep 2018 1:14

Tgt Ion:264 Resp: 312979

Ion	Ratio	Lower	Upper
264	100		
260	22.7	19.6	29.4
265	21.3	17.4	26.0

