

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092118\
 Data File : BG036854.D
 Acq On : 21 Sep 2018 11:23
 Operator : JU/SJ
 Sample : J4870-03
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PT-BN-WP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.836	88	93	110	rBV	153161	283094	3.60%	0.285%
2	5.617	390	396	414	rBV	709767	1316908	16.75%	1.324%
3	7.209	659	667	689	rBV	754591	1553020	19.76%	1.562%
4	7.579	723	730	748	rBV	734439	1410197	17.94%	1.418%
5	7.937	782	791	803	rBV	697410	1292974	16.45%	1.300%
6	8.049	804	810	823	rVB	177981	337164	4.29%	0.339%
7	8.372	857	865	868	rBV	589258	1138807	14.49%	1.145%
8	8.578	890	900	907	rBV	615523	1518709	19.32%	1.527%
9	8.854	936	947	970	rBV	915252	1673621	21.29%	1.683%
10	9.212	1000	1008	1012	rBV	491889	947417	12.05%	0.953%
11	9.253	1012	1015	1036	rVB	291577	592012	7.53%	0.595%
12	9.770	1095	1103	1122	rBV	666490	1199426	15.26%	1.206%
13	10.716	1255	1264	1276	rBV	467029	910603	11.58%	0.916%
14	10.857	1280	1288	1291	rVV	268335	505255	6.43%	0.508%
15	10.910	1291	1297	1324	rVB	1497303	2998580	38.15%	3.016%
16	12.849	1621	1627	1641	rVB	692108	1144918	14.57%	1.151%
17	13.302	1696	1704	1718	rBV	1529406	2542169	32.34%	2.557%
18	13.554	1735	1747	1763	rBV	629438	1103025	14.03%	1.109%
19	14.400	1883	1891	1906	rBV	1628014	2863796	36.43%	2.880%
20	14.676	1931	1938	1943	rBV2	471887	802935	10.21%	0.808%
21	14.741	1943	1949	1966	rVB	1795587	3052753	38.84%	3.070%
22	15.487	2069	2076	2093	rBV	1427707	2091082	26.60%	2.103%
23	15.728	2109	2117	2136	rBV2	2825542	5152966	65.55%	5.182%
24	16.163	2185	2191	2214	rBV	1172205	1886216	24.00%	1.897%
25	16.727	2281	2287	2303	rBV	861364	1391458	17.70%	1.399%
26	17.426	2396	2406	2408	rBV	626752	1019512	12.97%	1.025%
27	17.473	2408	2414	2423	rVB	3757817	6331705	80.55%	6.368%
28	18.384	2562	2569	2584	rBV	2890377	4223418	53.73%	4.247%
29	19.835	2809	2816	2827	rBV	2890768	4590719	58.40%	4.617%
30	20.029	2842	2849	2858	rBV	2971992	3980971	50.64%	4.004%
31	21.574	3105	3112	3121	rBV	2797305	3831341	48.74%	3.853%
32	21.680	3121	3130	3136	rVV2	2832535	6155305	78.31%	6.190%
33	21.751	3136	3142	3157	rVB	3416884	6486654	82.52%	6.524%
34	23.907	3495	3509	3515	rBV	2680520	7860568	100.00%	7.905%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092118\
Data File : BG036854.D
Acq On : 21 Sep 2018 11:23
Operator : JU/SJ
Sample : J4870-03
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PT-BN-WP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	23.960	3515	3518	3533	rVB	548726	1128485	14.36%	1.135%
36	24.782	3641	3658	3670	rBV	2341053	7763651	98.77%	7.808%
37	24.912	3670	3680	3694	rVB2	437794	1280495	16.29%	1.288%
38	26.046	3866	3873	3881	rVB4	28411	81302	1.03%	0.082%
39	28.637	4285	4314	4334	rVB3	791524	4990770	63.49%	5.019%


Sum of corrected areas: 99434001

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092118\
Data File : BG036854.D
Acq On : 21 Sep 2018 11:23
Operator : JU/SJ
Sample : J4870-03
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PT-BN-WP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

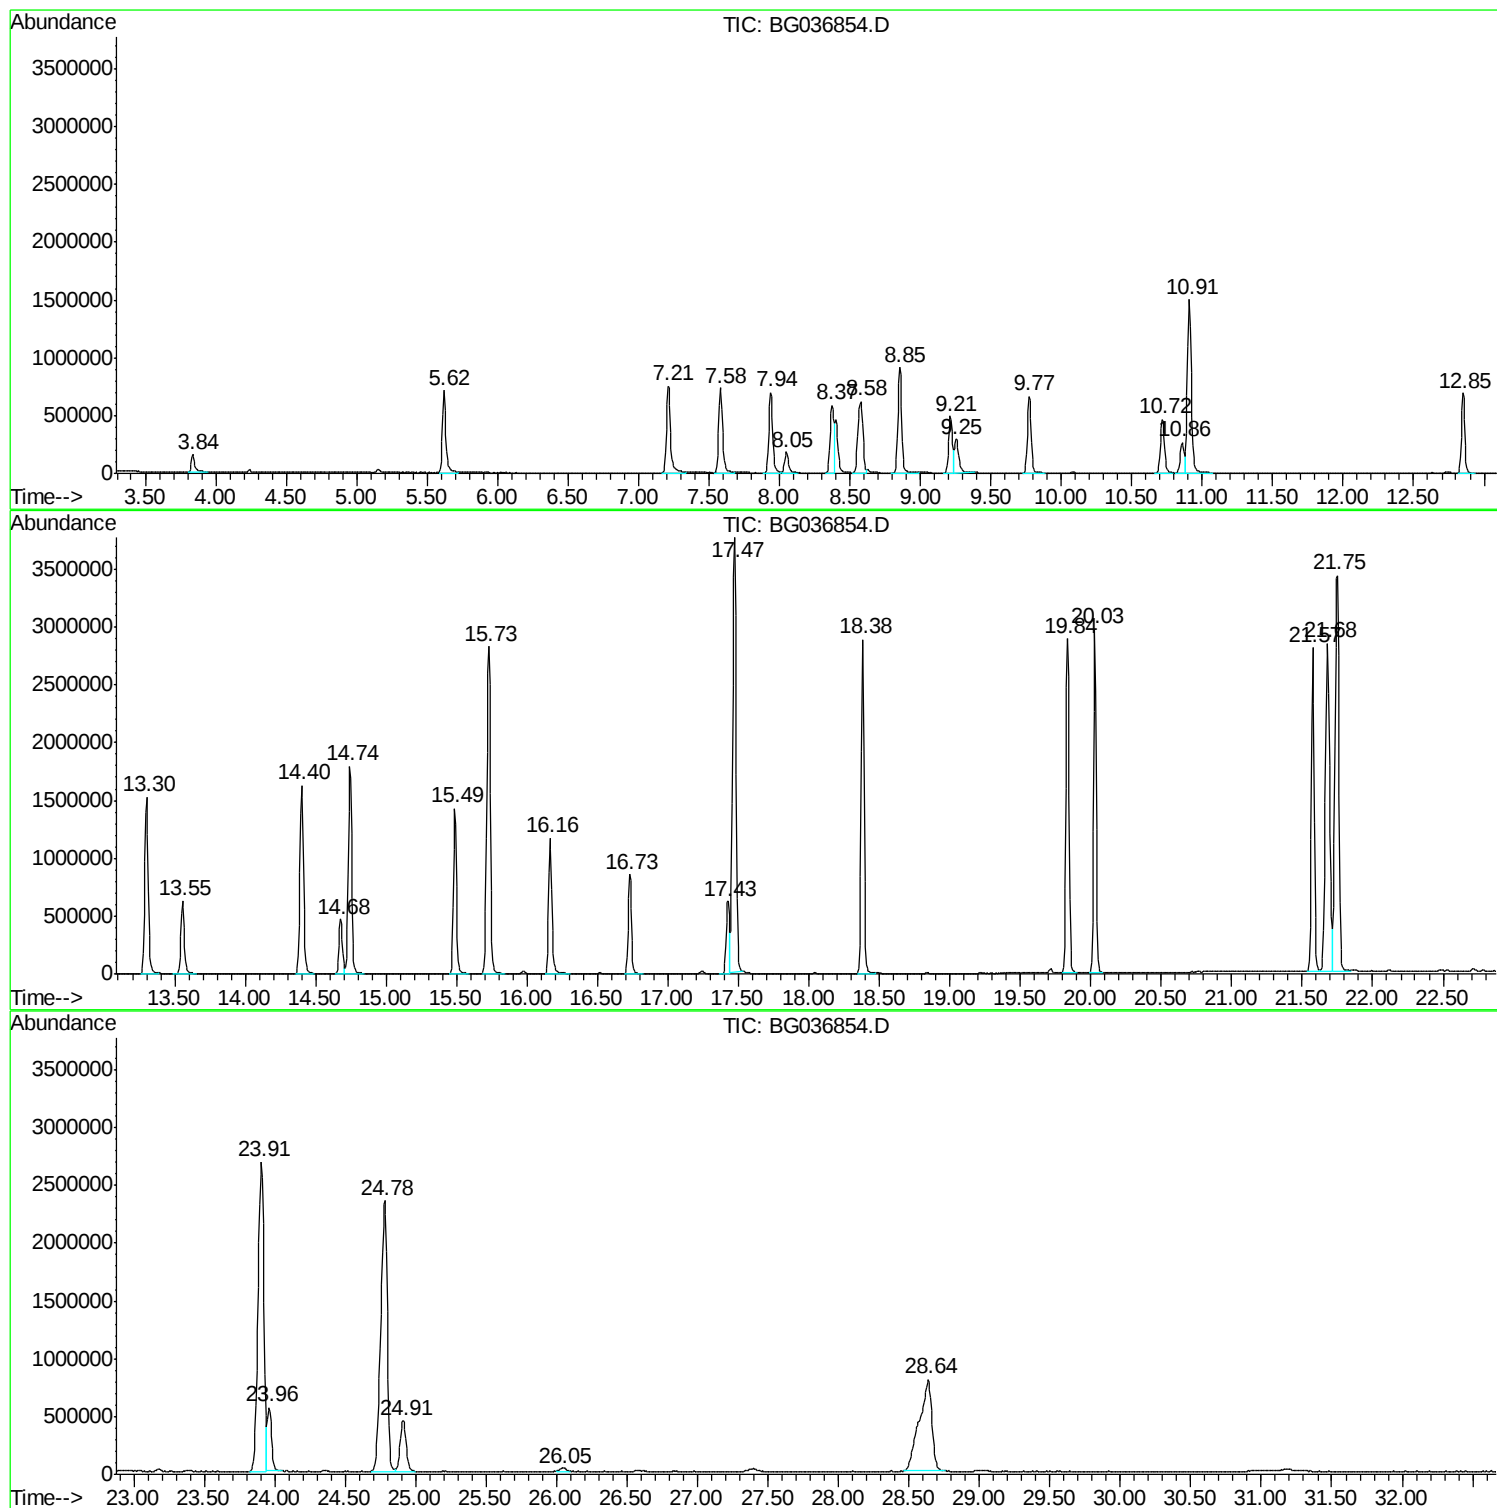

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092118\
Data File : BG036854.D
Acq On : 21 Sep 2018 11:23
Operator : JU/SJ
Sample : J4870-03
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PT-BN-WP








Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	83.65 ng	1410200	1,4-Dichlorobenzene-d4	8.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

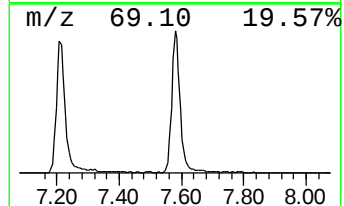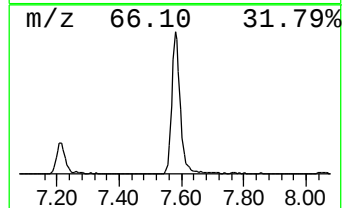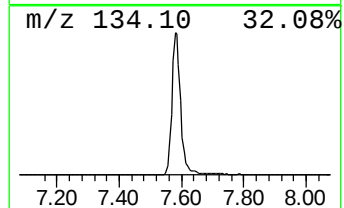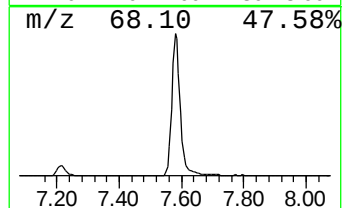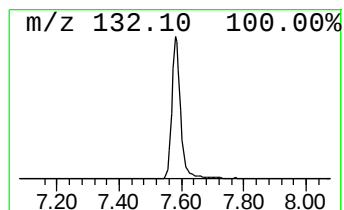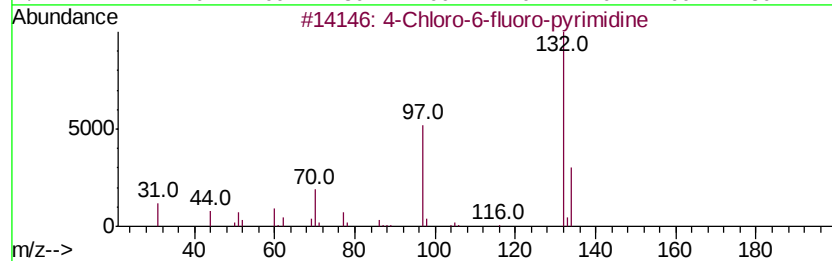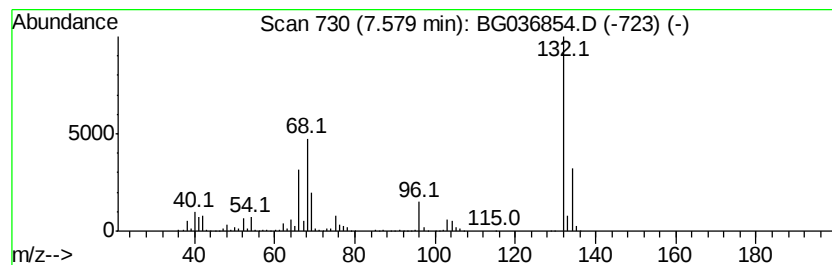

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG092118\
Data File : BG036854.D
Acq On : 21 Sep 2018 11:23
Operator : JU/SJ
Sample : J4870-03
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PT-BN-WP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.58	7.58	83.7	ng	1410200	1	8.05	337164	20.0