


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092118\
 Data File : BG036852.D
 Acq On : 21 Sep 2018 8:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 20 20:07:11 2018

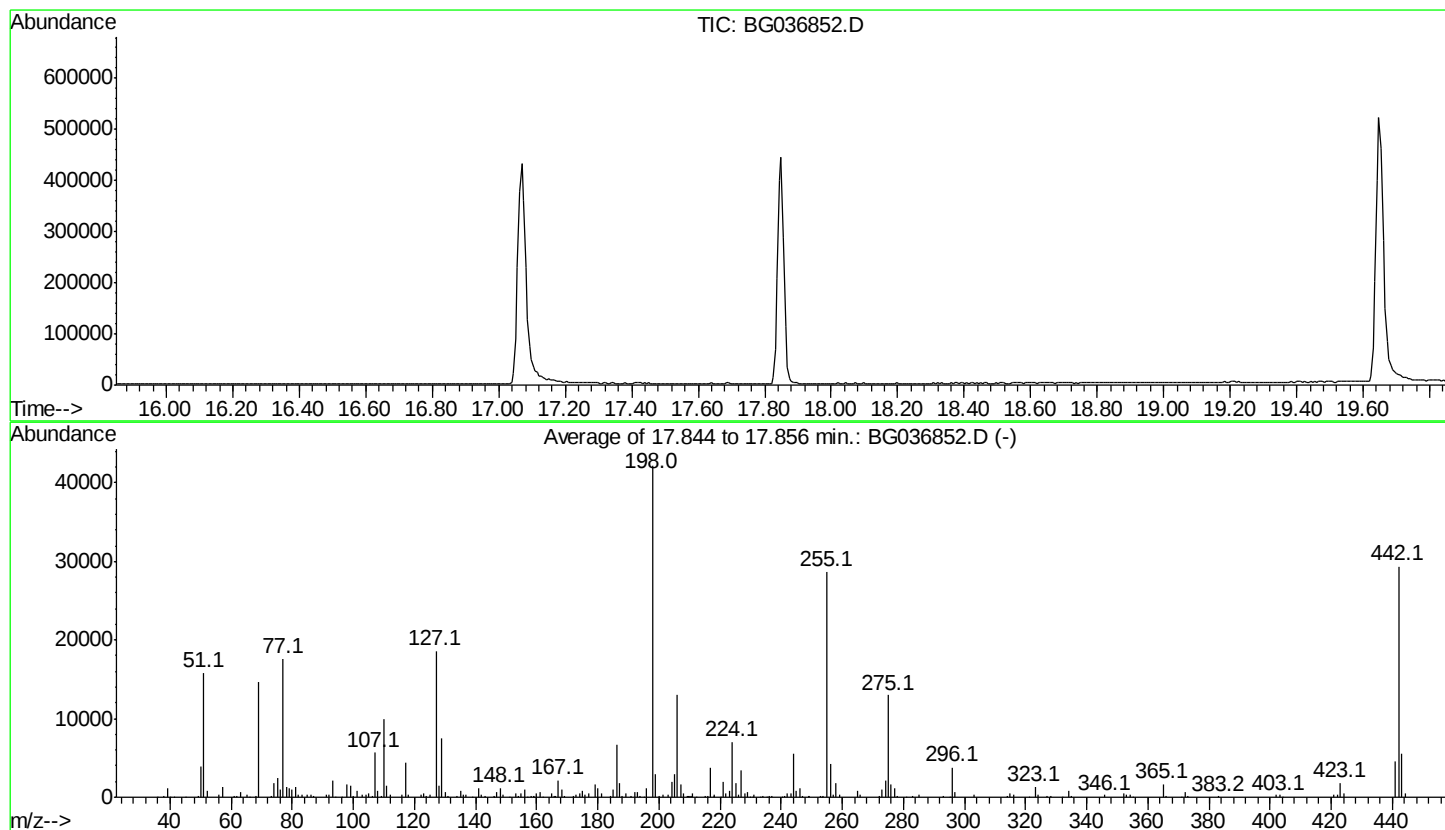

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	15876	PASS
68	69	0.00	2	0.8	119	PASS
69	198	0.00	100	34.8	14659	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.1	18606	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42184	PASS
199	198	5	9	7.0	2954	PASS
275	198	10	60	30.9	13027	PASS
365	198	1	100	3.9	1663	PASS
441	198	0.01	100	10.8	4575	PASS
442	198	50	100	69.7	29384	PASS
443	442	15	24	18.8	5525	PASS