


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092118\
 Data File : BG036881.D
 Acq On : 22 Sep 2018 6:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 20 20:07:11 2018

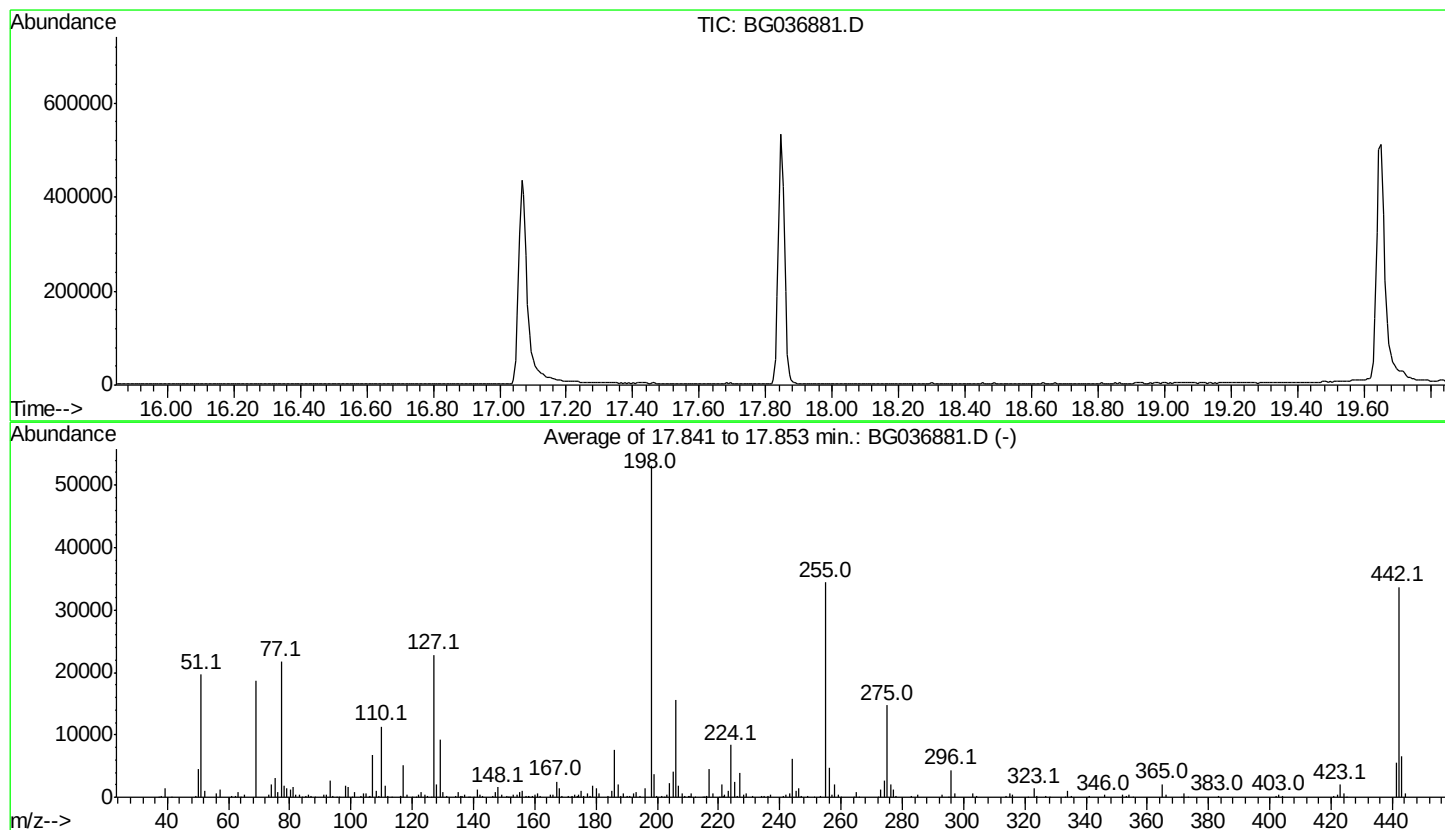

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	19623	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.3	18773	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.0	22840	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53130	PASS
199	198	5	9	7.0	3722	PASS
275	198	10	60	27.7	14735	PASS
365	198	1	100	4.0	2113	PASS
441	198	0.01	100	10.6	5614	PASS
442	198	50	100	63.4	33706	PASS
443	442	15	24	19.3	6520	PASS