
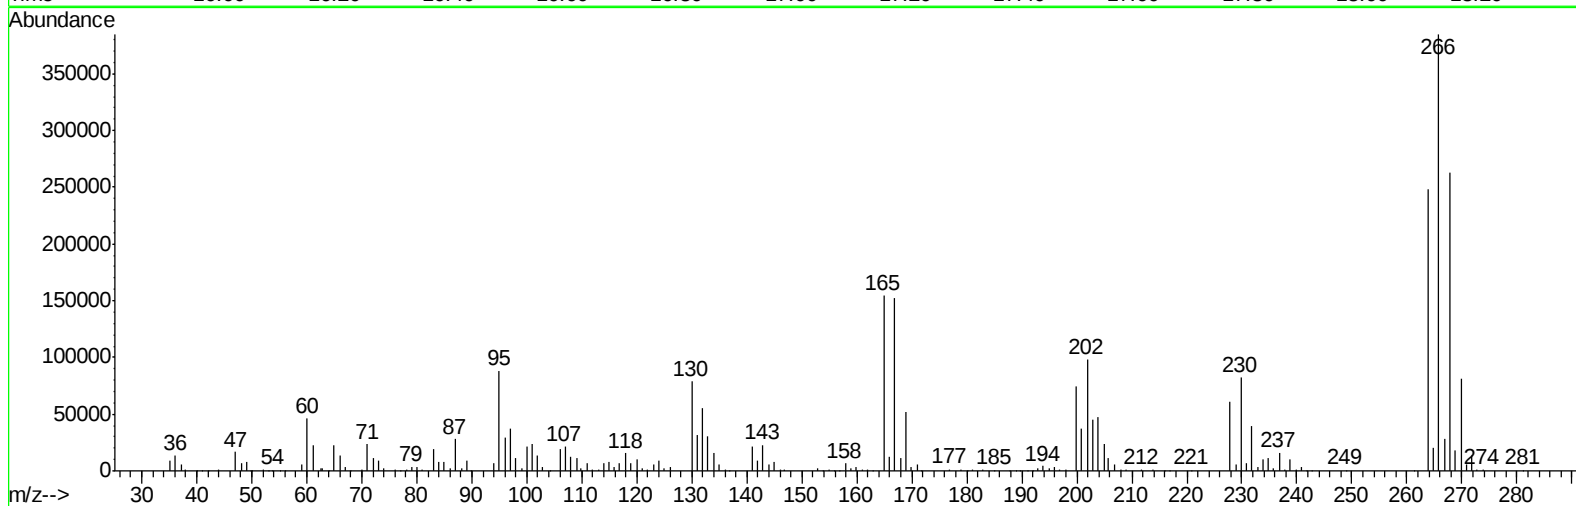


Data File : BG042904.D
Acq On : 21 Sep 2019 10:00
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 07:42:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 06:01:34 2019
Response via : Initial Calibration

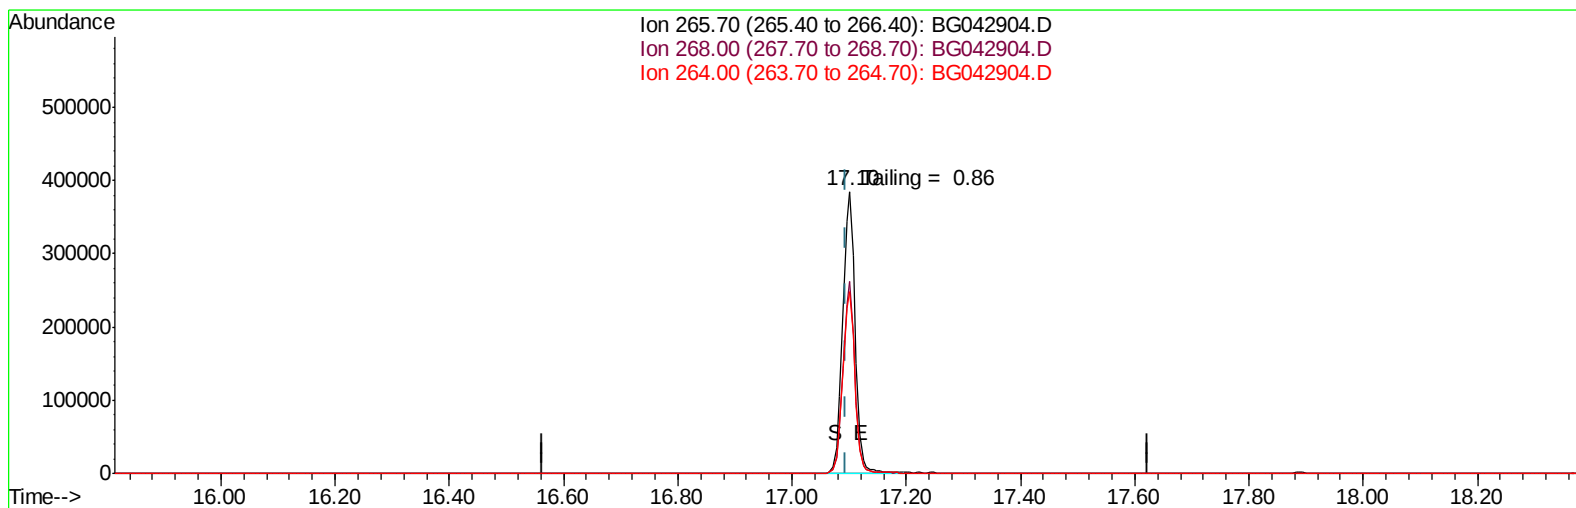

TIC: BG042904.D

(70) Pentachlorophenol (C)



17.101min (+0.006) 132421.48ng

response 586820

Ion	Exp%	Act%
265.70	100	100
268.00	67.00	68.27
264.00	64.60	64.47
0.00	0.00	0.00

Data File : BG042904.D
Acq On : 21 Sep 2019 10:00
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 07:42:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 23 06:01:34 2019
Response via : Initial Calibration

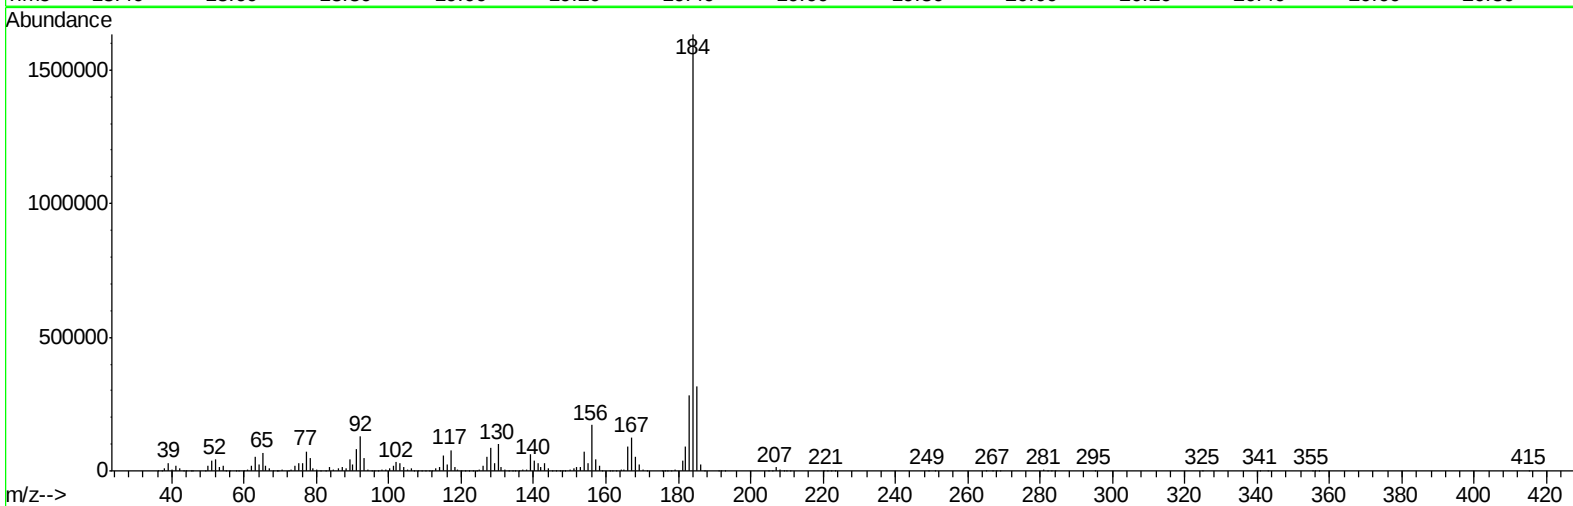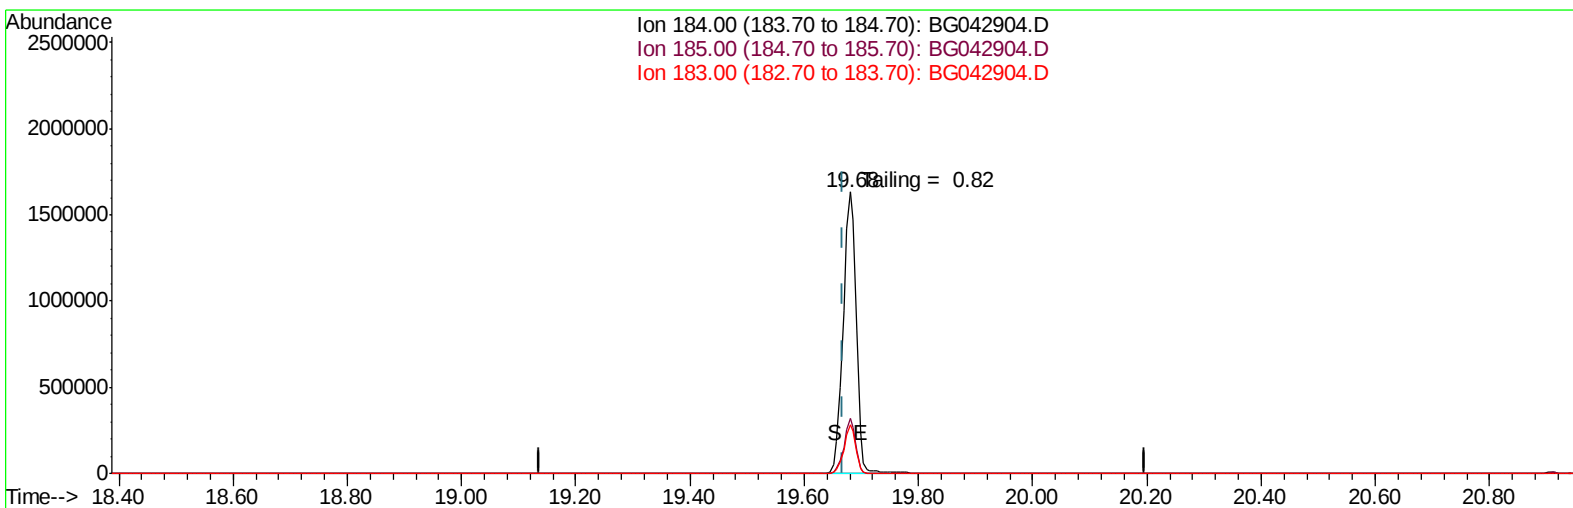

TIC: BG042904.D

(77) Benzidine

19.680min (+0.012) 76601.06ng

response 2632477

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	19.34#
183.00	13.60	17.22#
0.00	0.00	0.00