
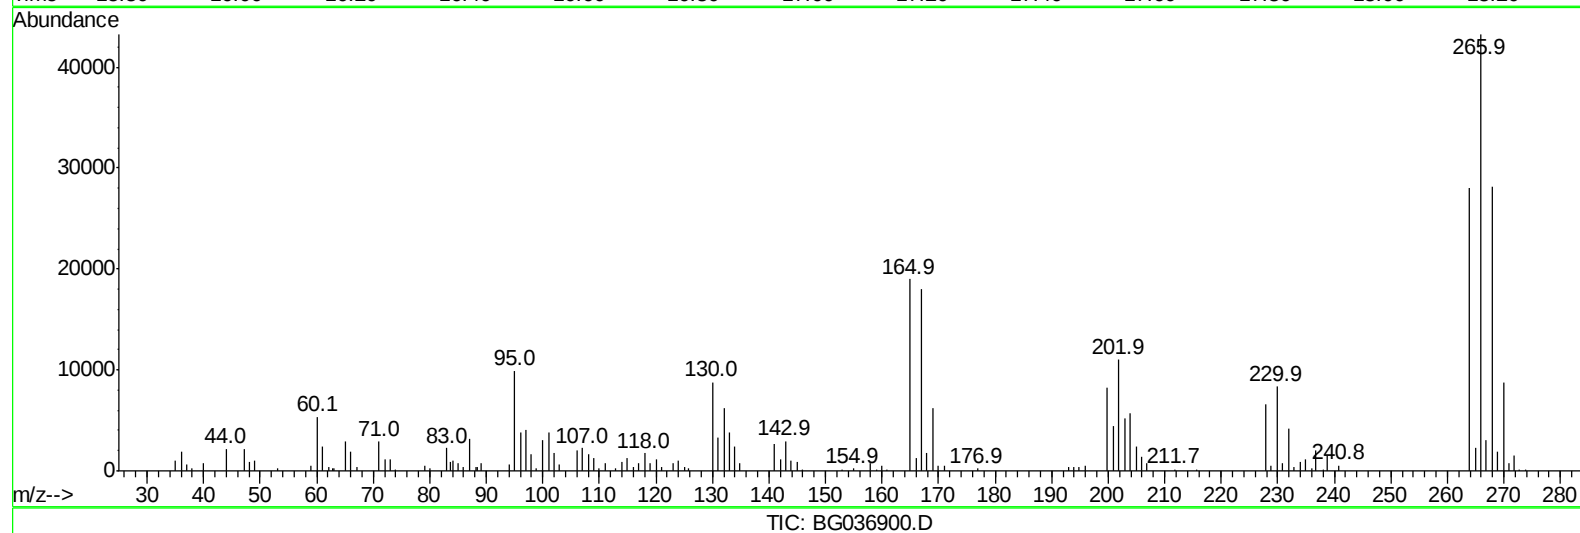


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092218\
Data File : BG036900.D
Acq On : 22 Sep 2018 20:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 05:48:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 20 20:07:11 2018
Response via : Initial Calibration

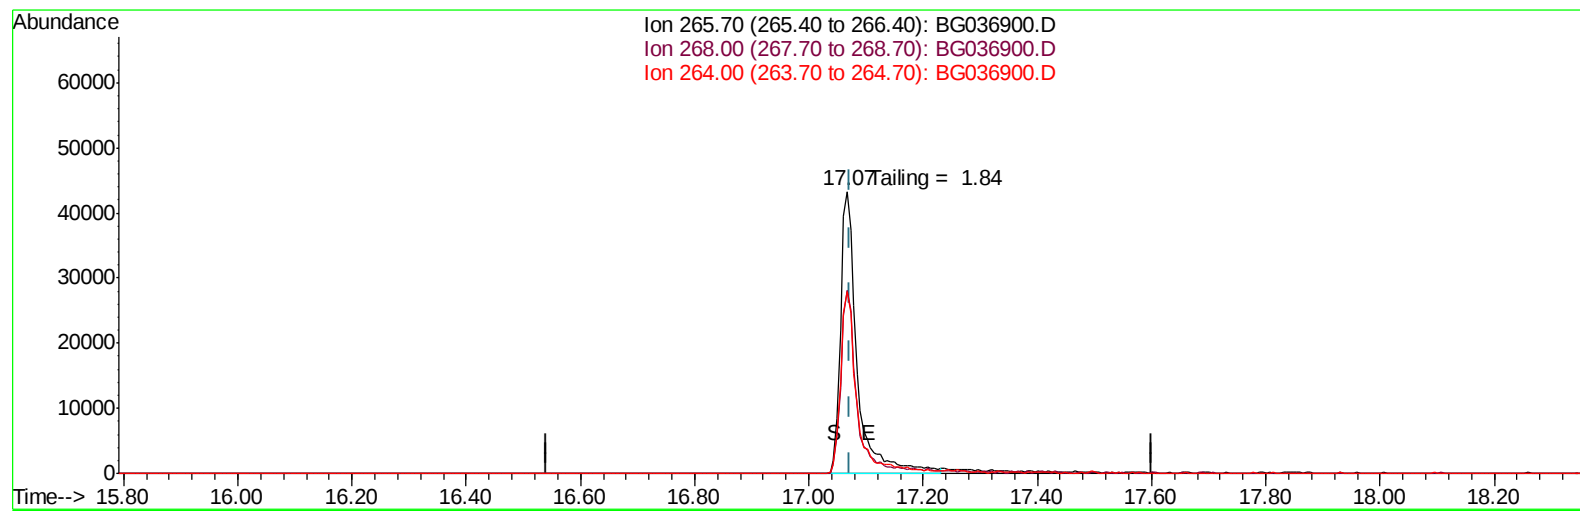

(69) Pentachlorophenol (C)



17.067min (-0.005) 14216.72ng

response 87557

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	65.13
264.00	61.10	64.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092218\
 Data File : BG036900.D
 Acq On : 22 Sep 2018 20:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 05:48:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 20 20:07:11 2018
 Response via : Initial Calibration

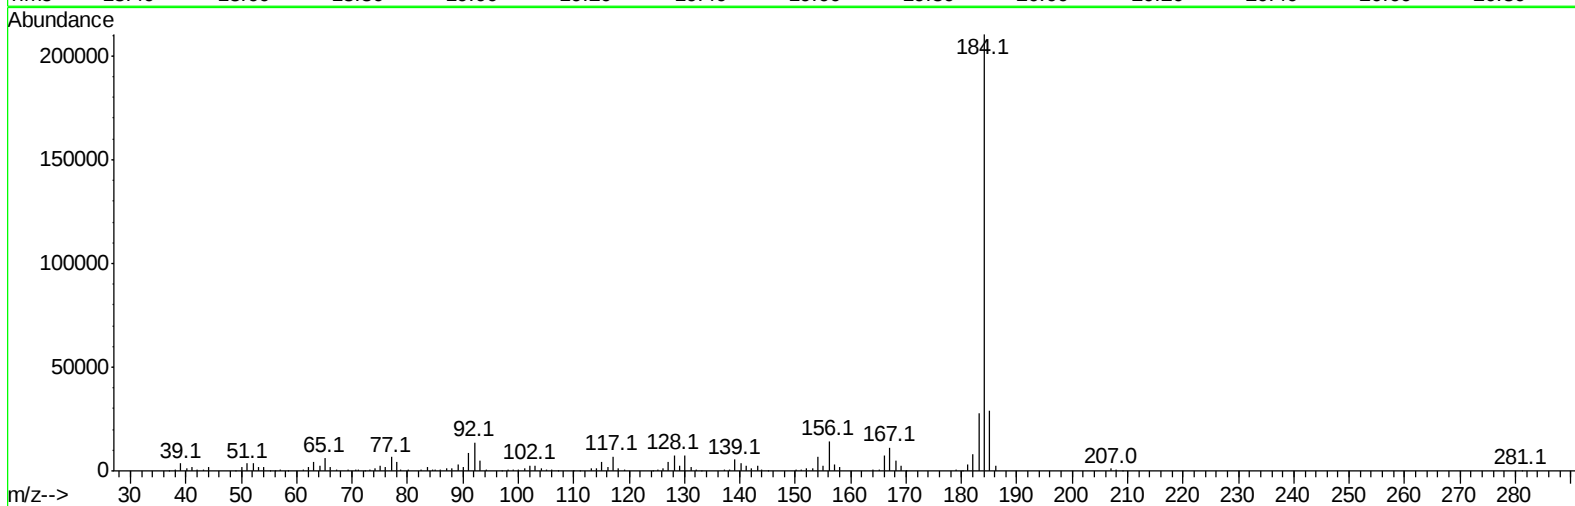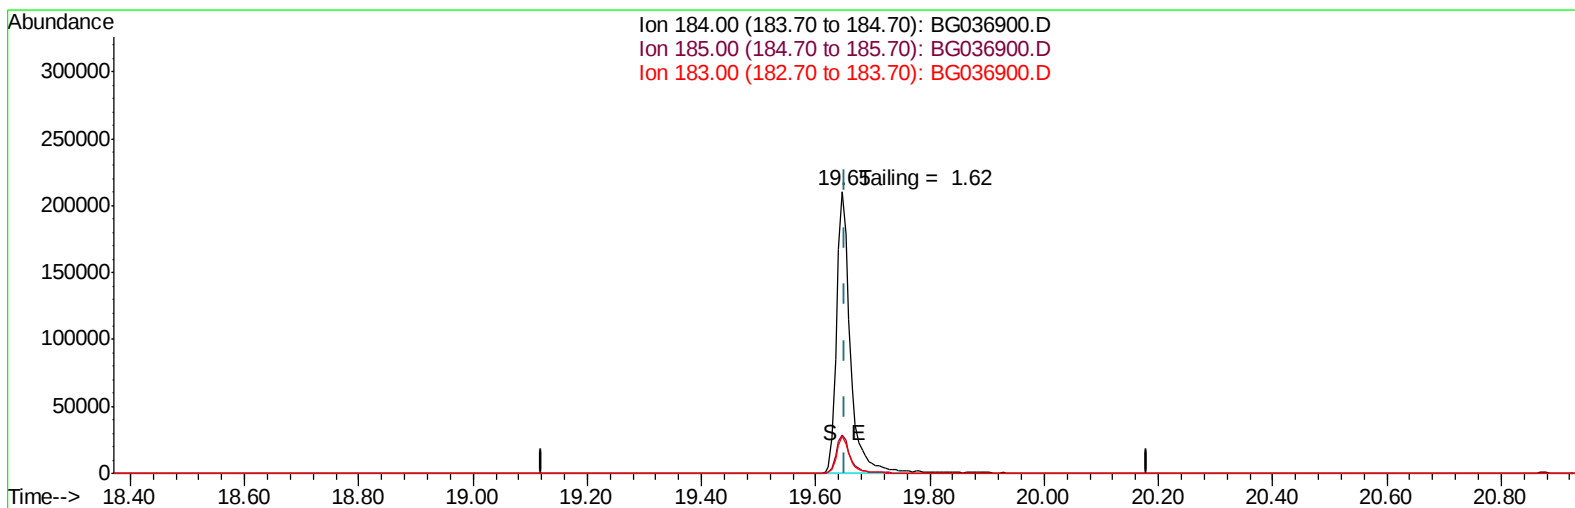

TIC: BG036900.D

(76) Benzidine

19.646min (-0.005) 10760.63ng

response 355868

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.77
183.00	13.60	13.20
0.00	0.00	0.00