

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092218\
 Data File : BG036902.D
 Acq On : 22 Sep 2018 21:24
 Operator : JU/SJ
 Sample : J5019-09
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 091918-SIDI-E-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.150	313	317	328	rBV	30237	50974	1.13%	0.303%
2	5.614	390	396	410	rBV	215997	416512	9.26%	2.479%
3	7.206	660	667	686	rBV	124590	304518	6.77%	1.812%
4	7.576	722	730	746	rBV	424648	833997	18.55%	4.964%
5	8.046	803	810	824	rBV	135182	272405	6.06%	1.621%
6	8.370	857	865	885	rBV	631013	1199851	26.68%	7.141%
7	9.210	1000	1008	1030	rBV	506644	1071284	23.82%	6.376%
8	10.849	1280	1287	1303	rBV	188004	386859	8.60%	2.302%
9	13.293	1695	1703	1724	rBV	1604858	2779978	61.83%	16.545%
10	14.668	1930	1937	1950	rBV2	346866	614950	13.68%	3.660%
11	16.160	2184	2191	2207	rBV	874725	1495132	33.25%	8.898%
12	17.418	2398	2405	2419	rBV2	482950	832121	18.51%	4.952%
13	20.021	2842	2848	2862	rBV	3154503	4496485	100.00%	26.761%
14	21.678	3124	3130	3144	rBV	522272	936211	20.82%	5.572%
15	23.164	3377	3383	3390	rBV4	22642	46096	1.03%	0.274%
16	23.963	3513	3519	3527	rVB3	22757	52709	1.17%	0.314%
17	24.891	3665	3677	3692	rBV	317784	951698	21.17%	5.664%
18	26.025	3863	3870	3884	rVB6	18512	60668	1.35%	0.361%


Sum of corrected areas: 16802448

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092218\
Data File : BG036902.D
Acq On : 22 Sep 2018 21:24
Operator : JU/SJ
Sample : J5019-09
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
091918-SIDI-E-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

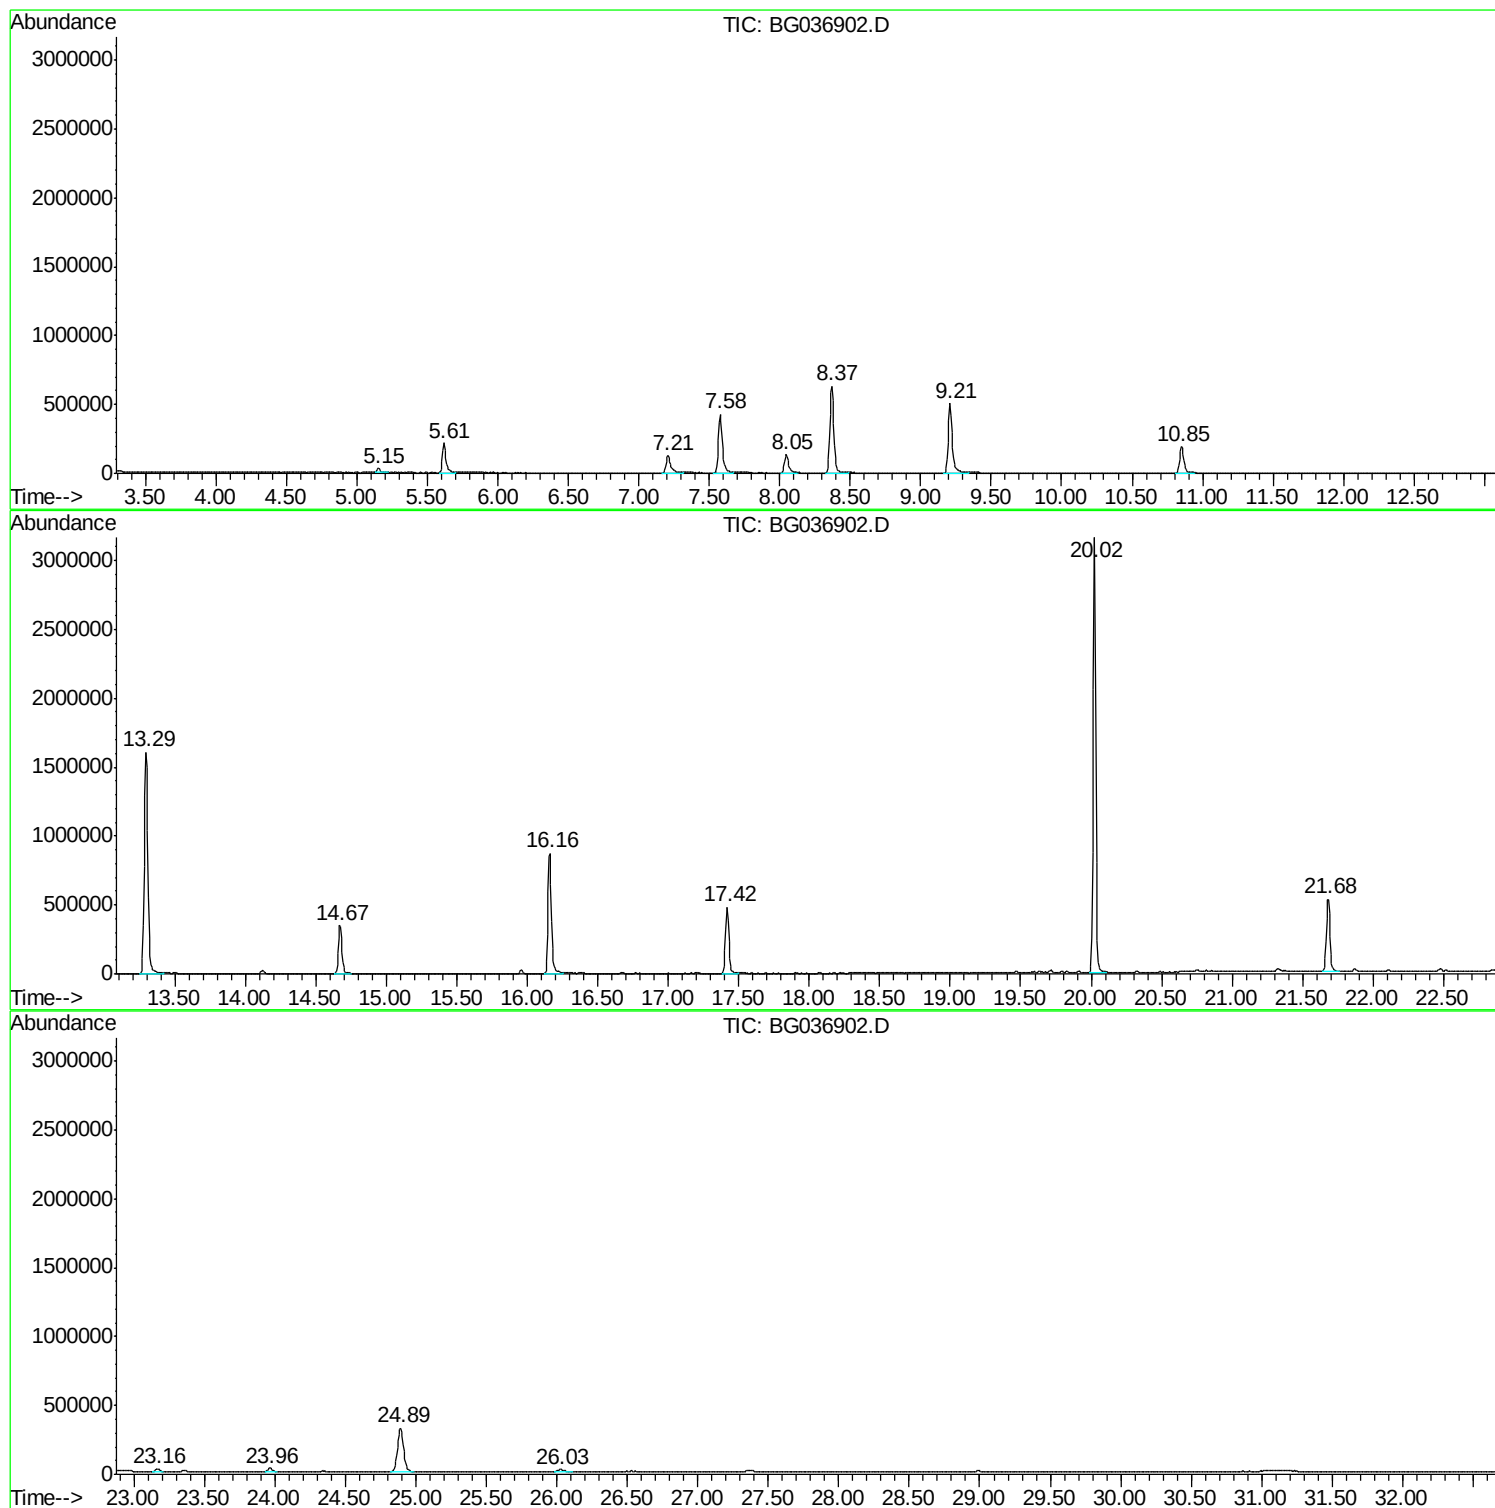

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092218\
Data File : BG036902.D
Acq On : 22 Sep 2018 21:24
Operator : JU/SJ
Sample : J5019-09
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
091918-SIDI-E-U-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.15	3.74 ng	50974	1,4-Dichlorobenzene-d4	8.05

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	40
3			2-Pentanol, 2,4-dimethyl-	116	C7H16O	000625-06-9	40
4			Oxirane, [(1-methylethoxy)methyl]-	116	C6H12O2	004016-14-2	39
5			5-Hexen-2-one	98	C6H10O	000109-49-9	9

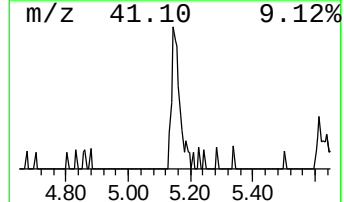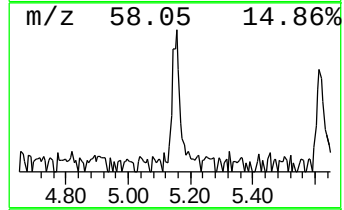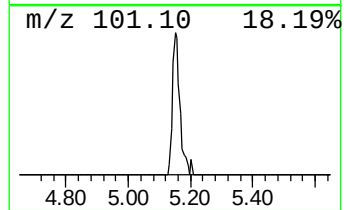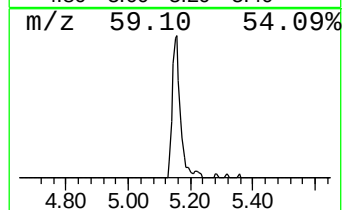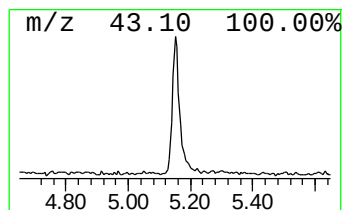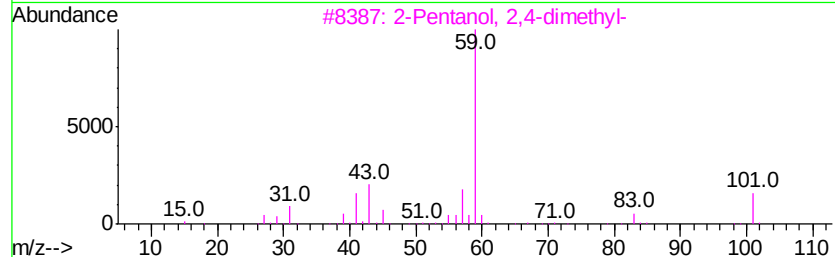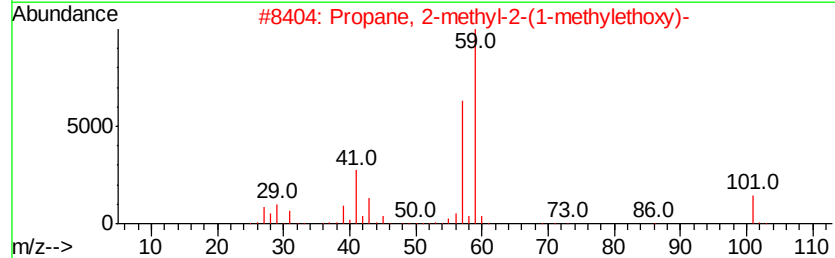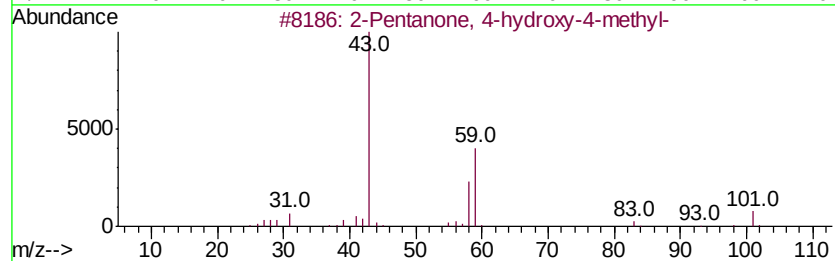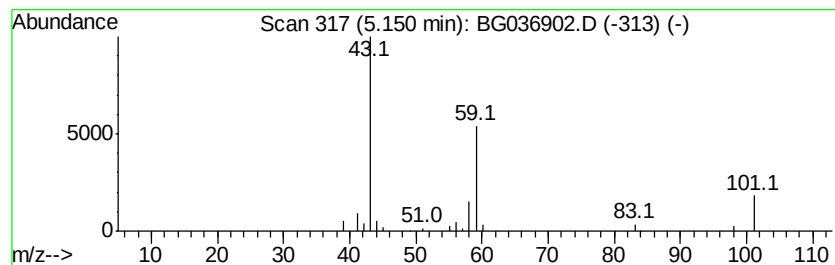

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092218\
Data File : BG036902.D
Acq On : 22 Sep 2018 21:24
Operator : JU/SJ
Sample : J5019-09
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
091918-SIDI-E-U-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.58 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	61.23 ng	833997	1,4-Dichlorobenzene-d4	8.05

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
3			5-Aminoindole	132	C8H8N2	005192-03-0	22
4			1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	17
5			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16

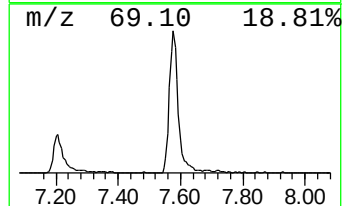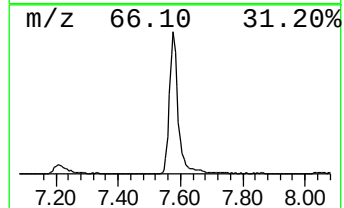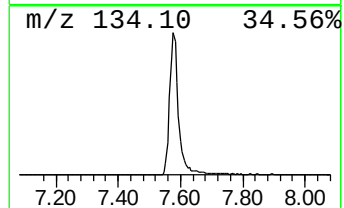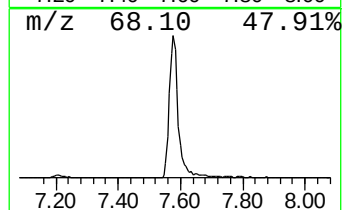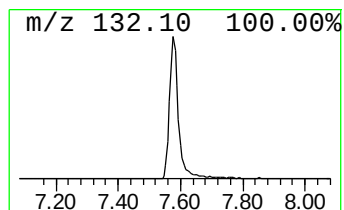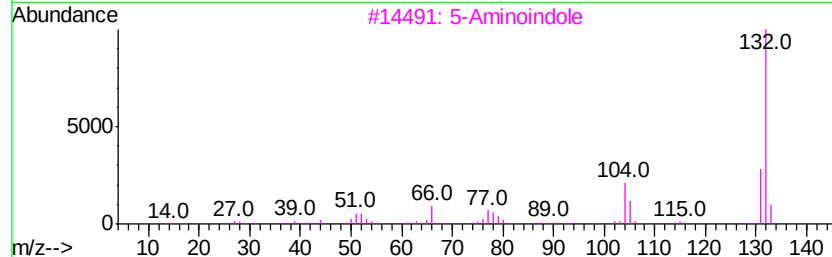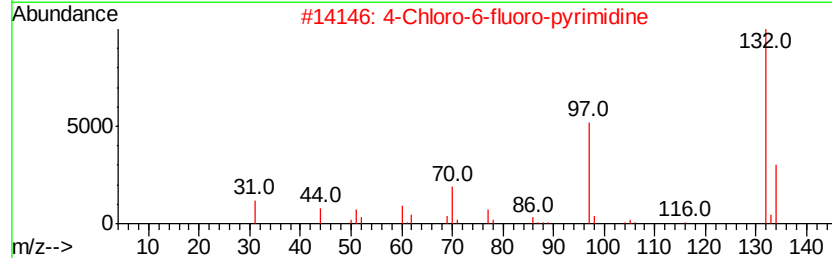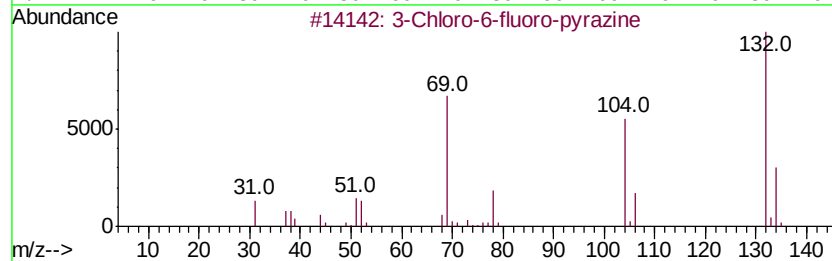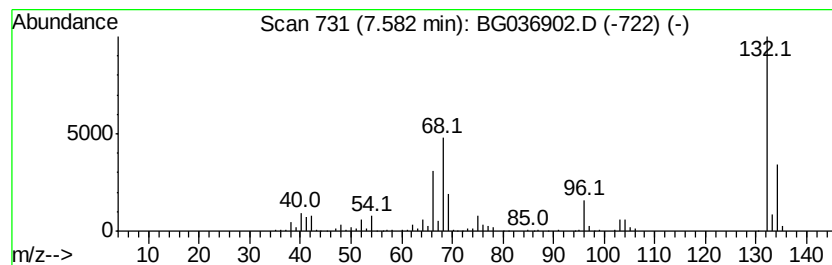

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG092218\
Data File : BG036902.D
Acq On : 22 Sep 2018 21:24
Operator : JU/SJ
Sample : J5019-09
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
091918-SIDI-E-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.15	3.7	ng	50974	1	8.05	272405	20.0
unknown7.58	7.58	61.2	ng	833997	1	8.05	272405	20.0