


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092218\
 Data File : BG036900.D
 Acq On : 22 Sep 2018 20:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

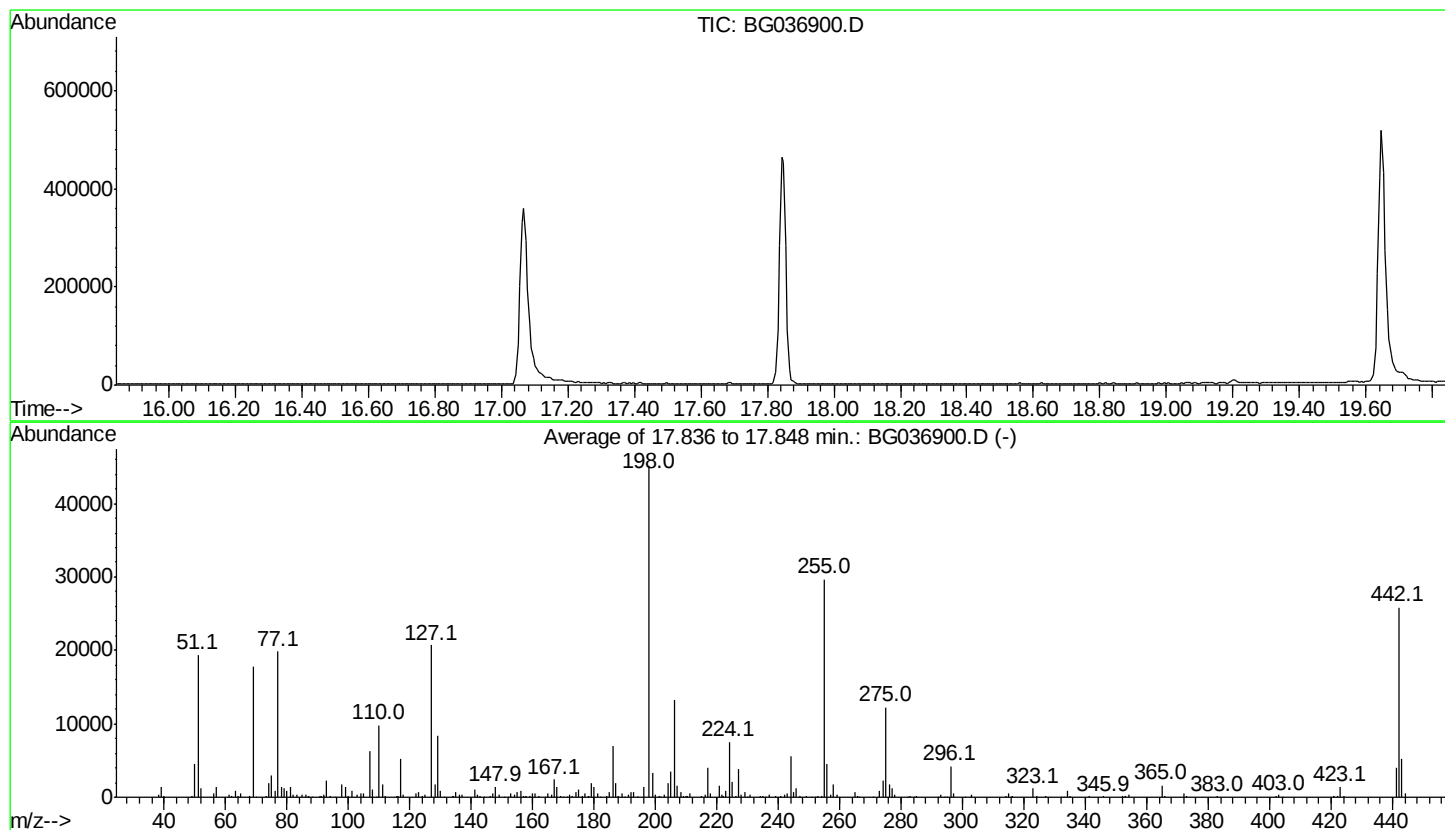

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	19391	PASS
68	69	0.00	2	0.8	137	PASS
69	198	0.00	100	39.4	17807	PASS
70	69	0.00	2	0.3	59	PASS
127	198	10	80	45.8	20701	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45157	PASS
199	198	5	9	7.4	3324	PASS
275	198	10	60	27.2	12288	PASS
365	198	1	100	3.7	1660	PASS
441	198	0.01	100	9.0	4060	PASS
442	198	50	100	57.3	25878	PASS
443	442	15	24	20.0	5182	PASS