
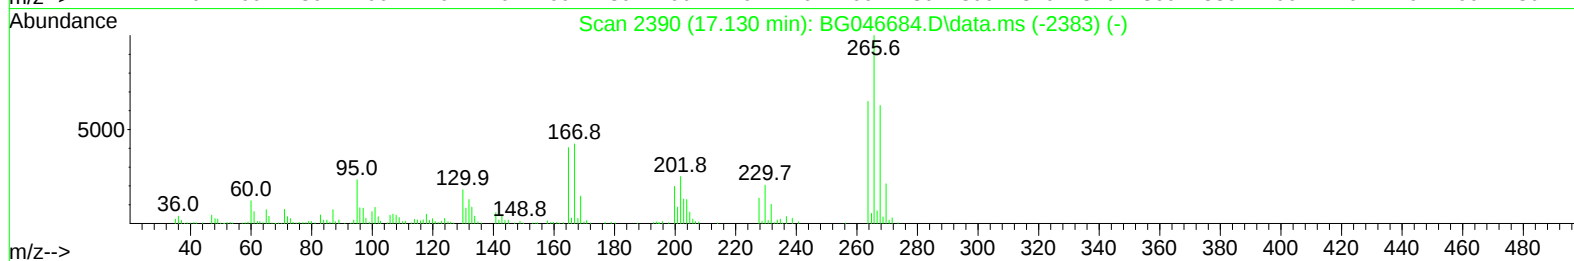
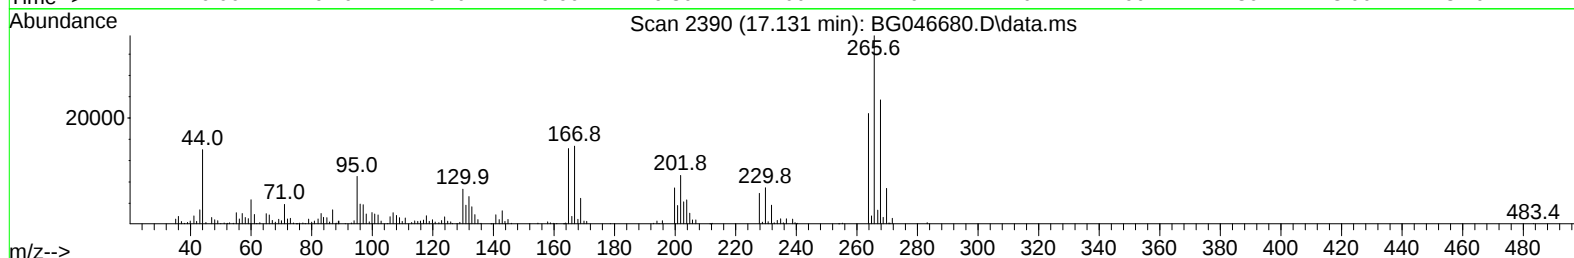


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092220\
Data File : BG046680.D
Acq On : 22 Sep 2020 16:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 15:34:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 22 21:47:28 2020
Response via : Initial Calibration

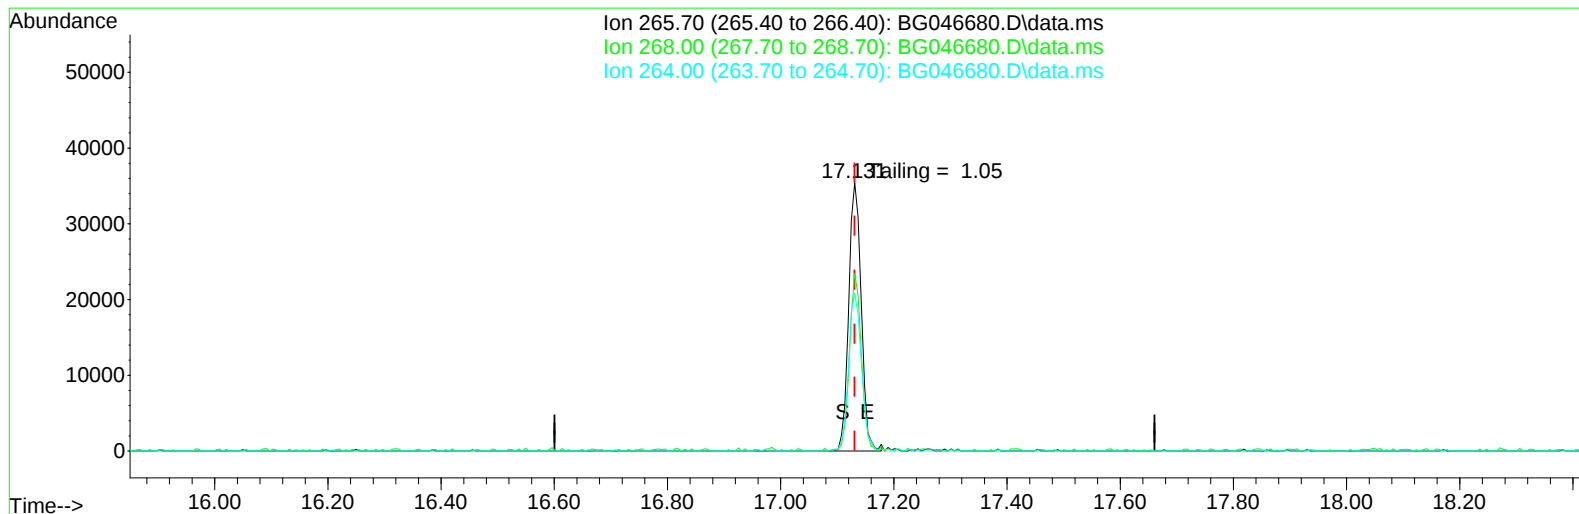

TIC: BG046680.D\data.ms

(70) Pentachlorophenol (C)




17.131min (+ 0.000) 101673.98 ng

response 54258

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.87
264.00	61.60	58.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092220\
Data File : BG046680.D
Acq On : 22 Sep 2020 16:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 15:34:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 22 21:47:28 2020
Response via : Initial Calibration

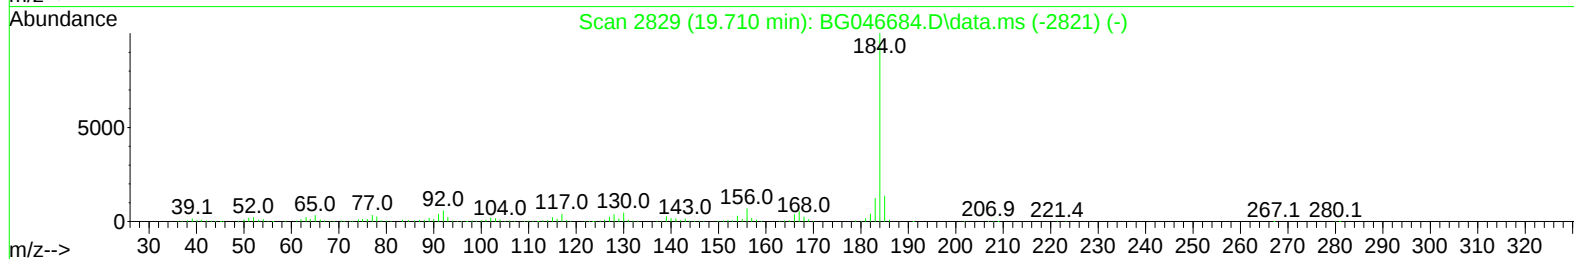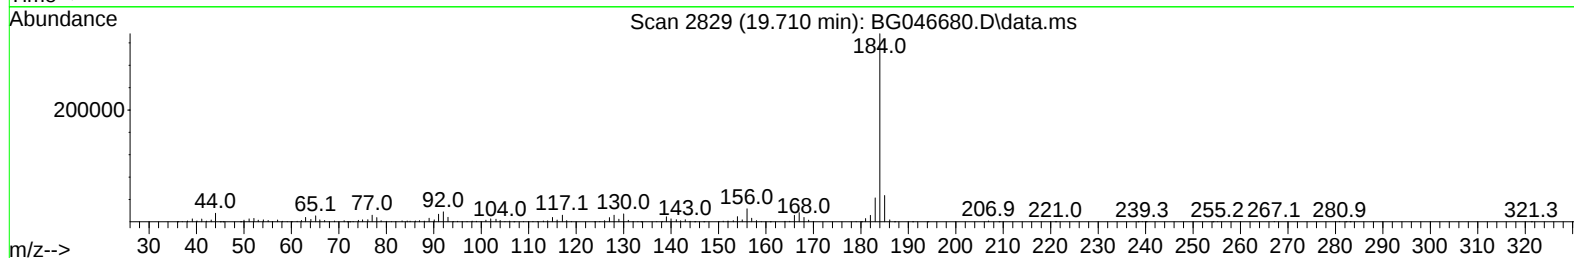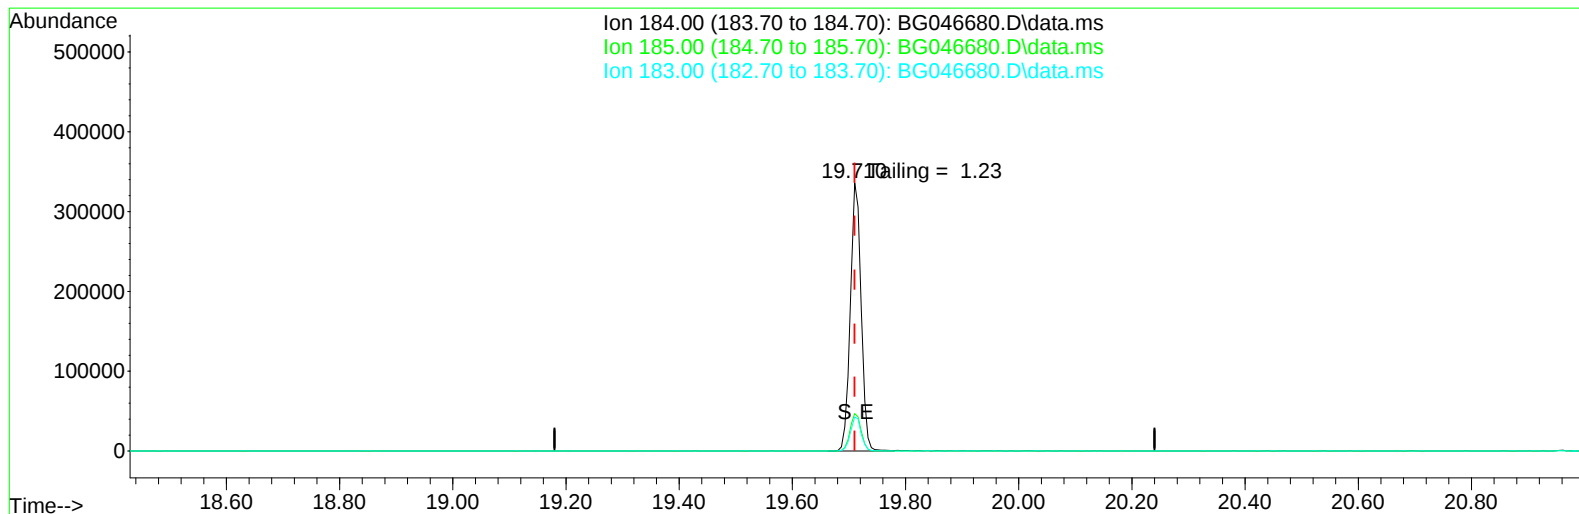

TIC: BG046680.D\data.ms

(77) Benzidine**19.710min (+ 0.000) 86983.97 ng****response 445098**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.99
183.00	13.20	12.73
0.00	0.00	0.00