
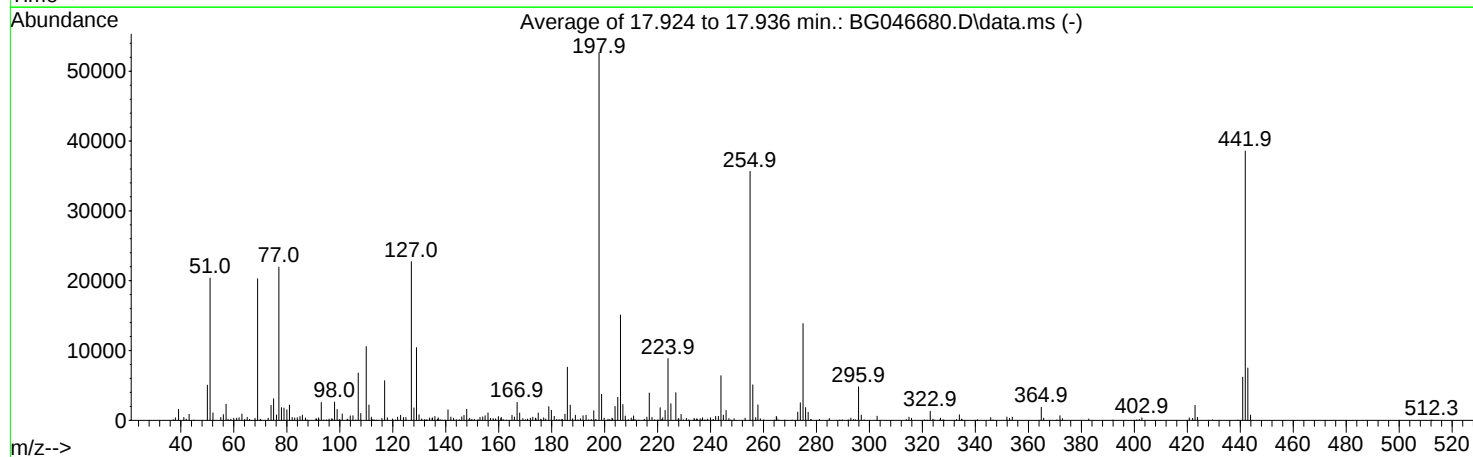


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092220\
Data File : BG046680.D
Acq On : 22 Sep 2020 16:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 22 21:47:28 2020

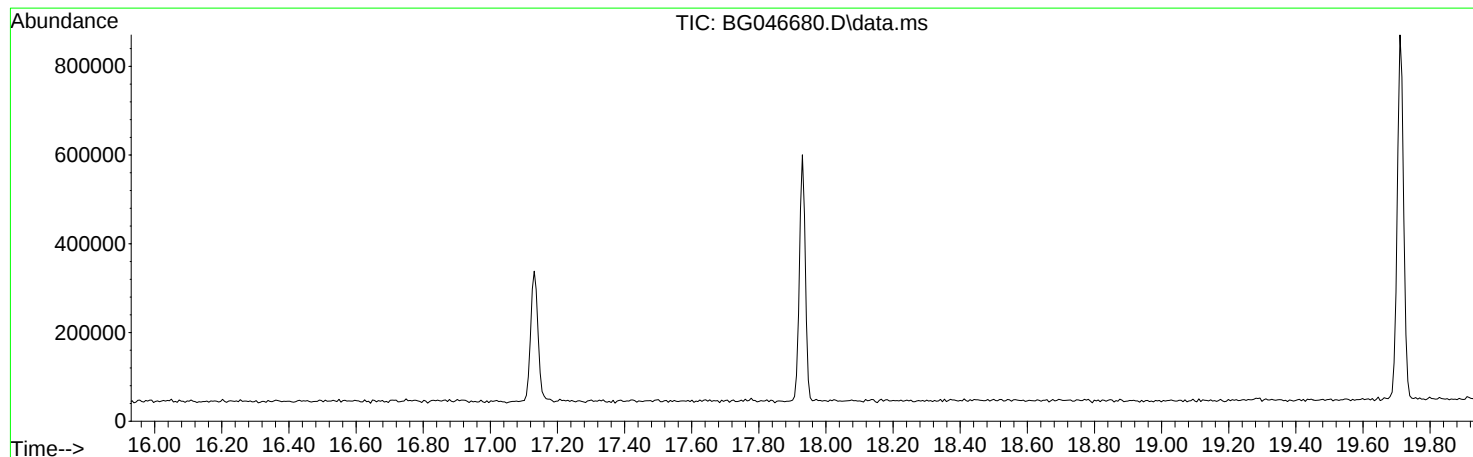

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	20361	PASS
68	69	0.00	2	1.5	307	PASS
69	198	0.00	100	38.5	20289	PASS
70	69	0.00	2	0.8	166	PASS
127	198	10	80	43.1	22724	PASS
197	198	0.00	2	0.3	159	PASS
198	198	100	100	100.0	52680	PASS
199	198	5	9	7.1	3731	PASS
275	198	10	60	26.3	13857	PASS
365	198	1	100	3.6	1877	PASS
441	198	0.01	100	11.7	6188	PASS
442	198	50	100	73.2	38573	PASS
443	442	15	24	19.4	7490	PASS