


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092319\
 Data File : BG042913.D
 Acq On : 23 Sep 2019 14:04
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 23 06:01:34 2019

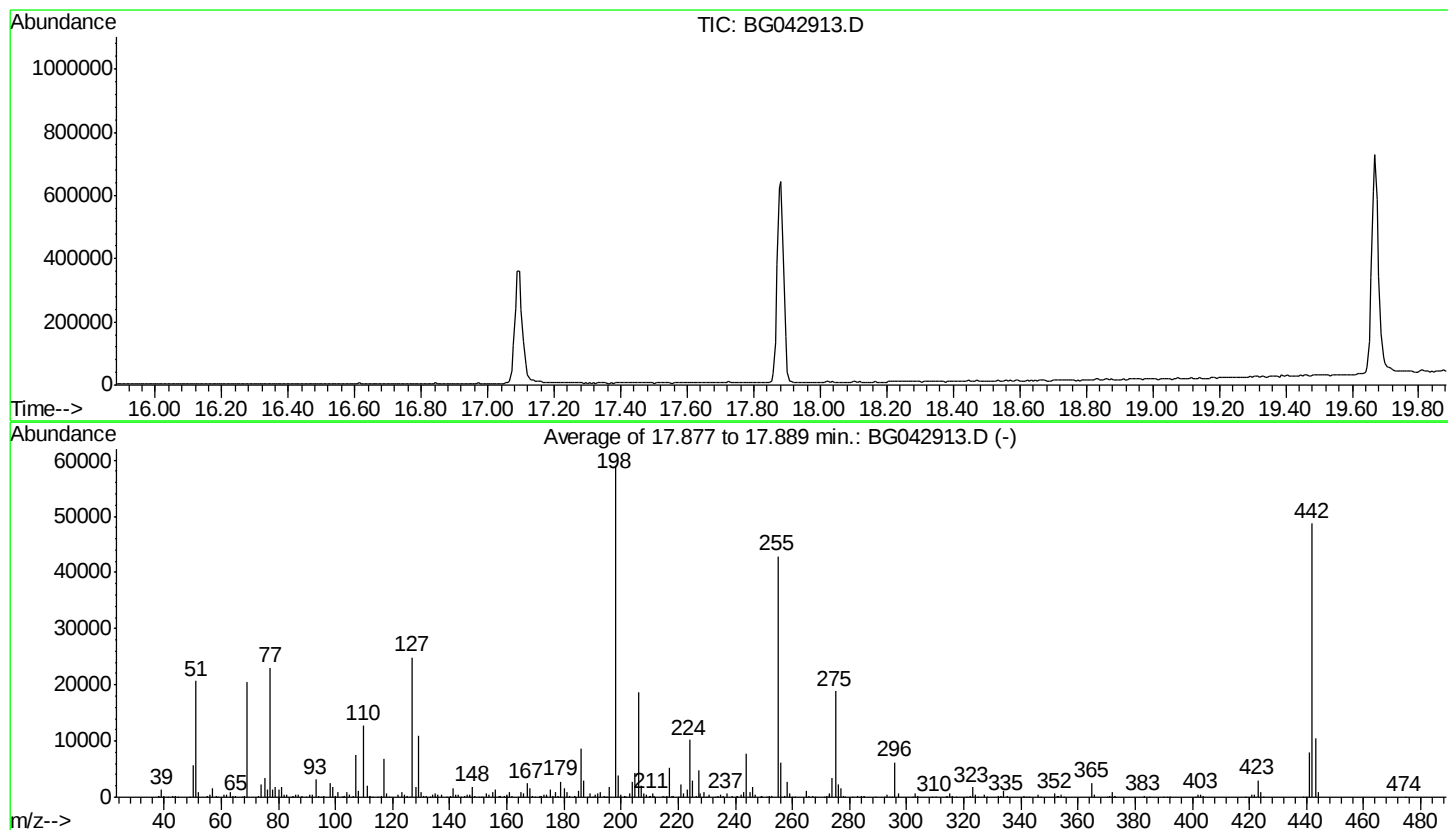

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	20695	PASS
68	69	0.00	2	1.2	236	PASS
69	198	0.00	100	34.7	20490	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.1	24874	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59021	PASS
199	198	5	9	6.6	3905	PASS
275	198	10	60	31.9	18851	PASS
365	198	1	100	4.4	2617	PASS
441	198	0.01	100	13.4	7924	PASS
442	198	50	100	82.5	48690	PASS
443	442	15	24	21.7	10561	PASS