




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:01:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

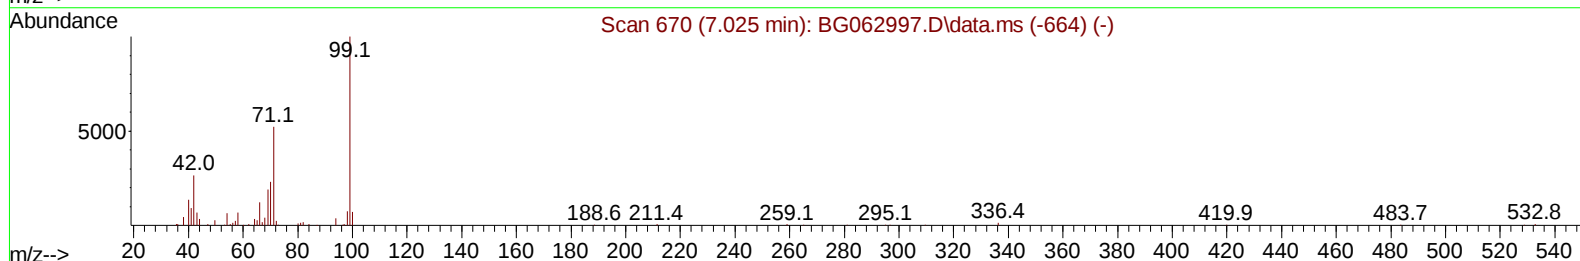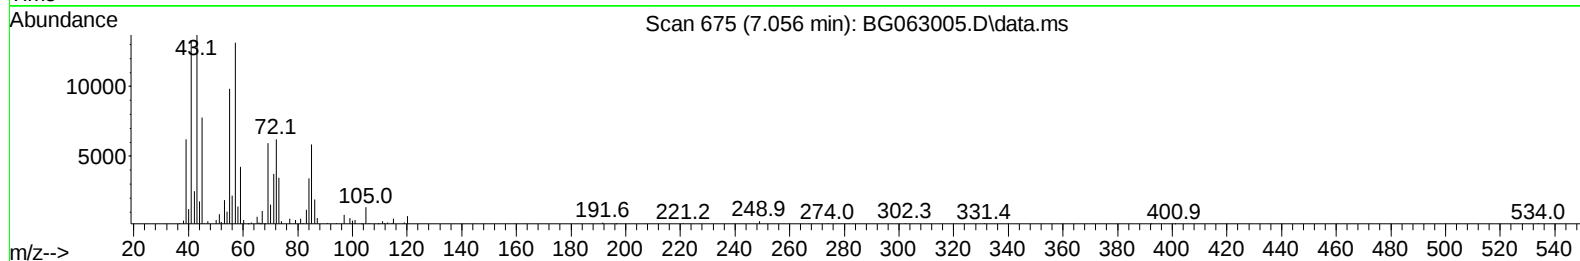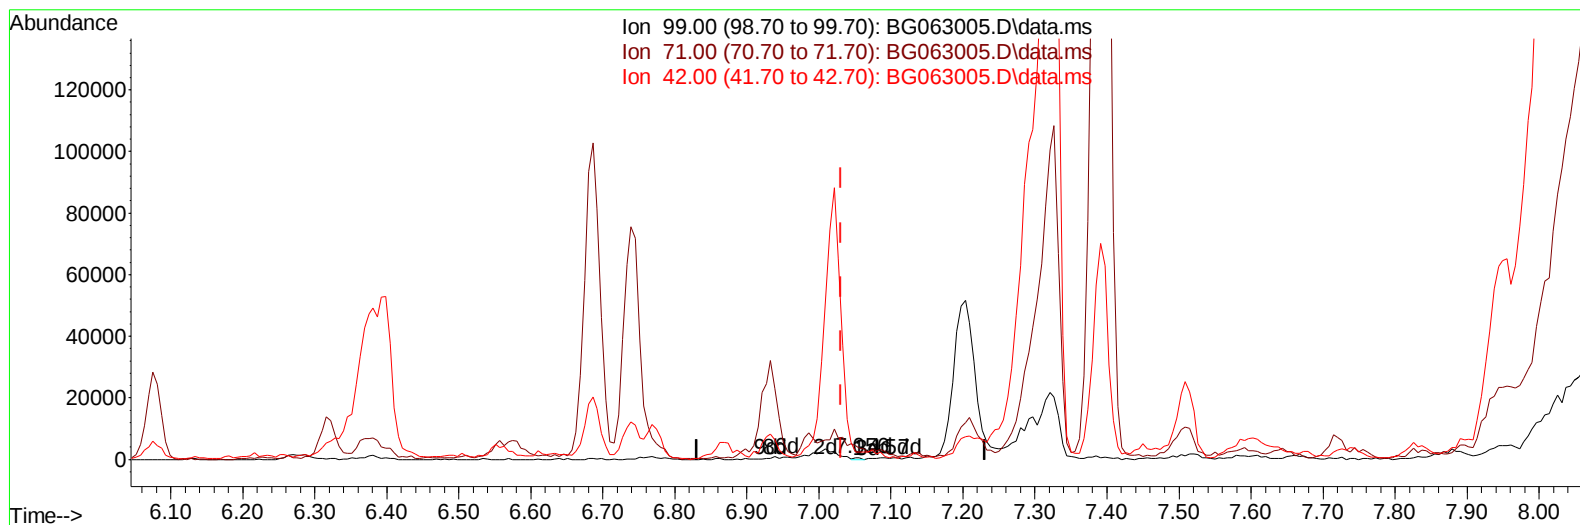

TIC: BG063005.D\data.ms

(7) Phenol-d5 (S)

7.056min (+ 0.025) 0.12 ng/u1

response 368

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	39.50	671.53#
42.00	20.50	452.97#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:01:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

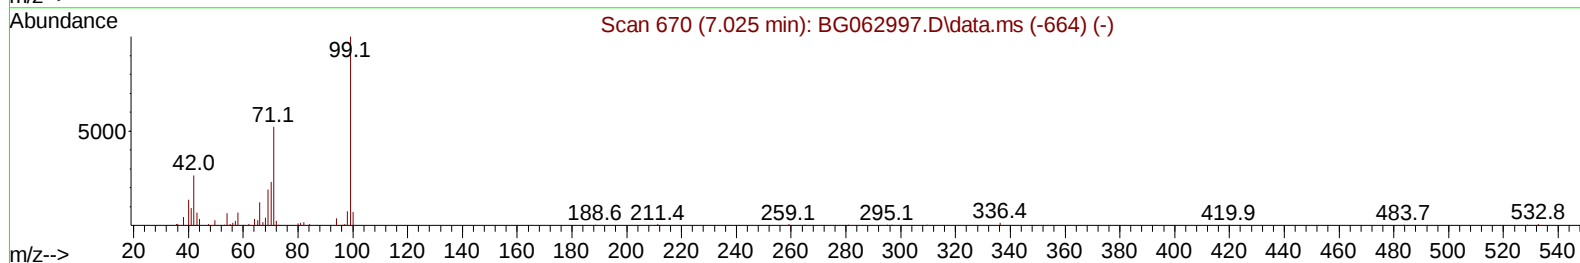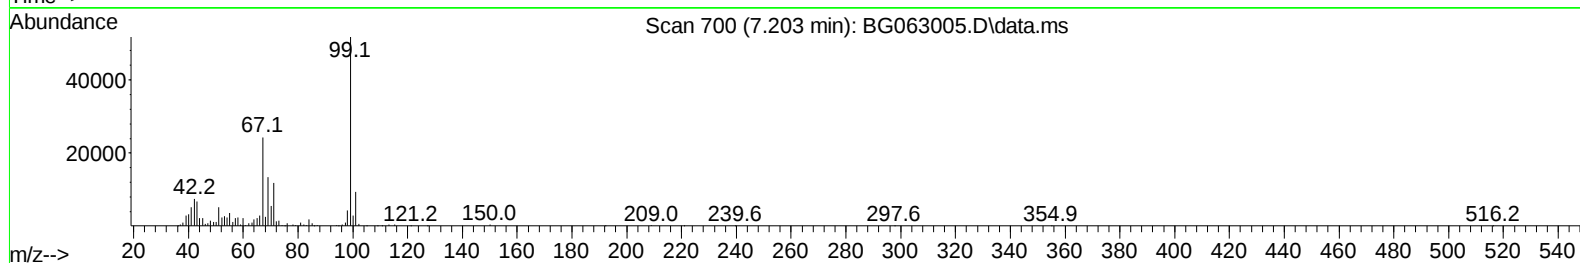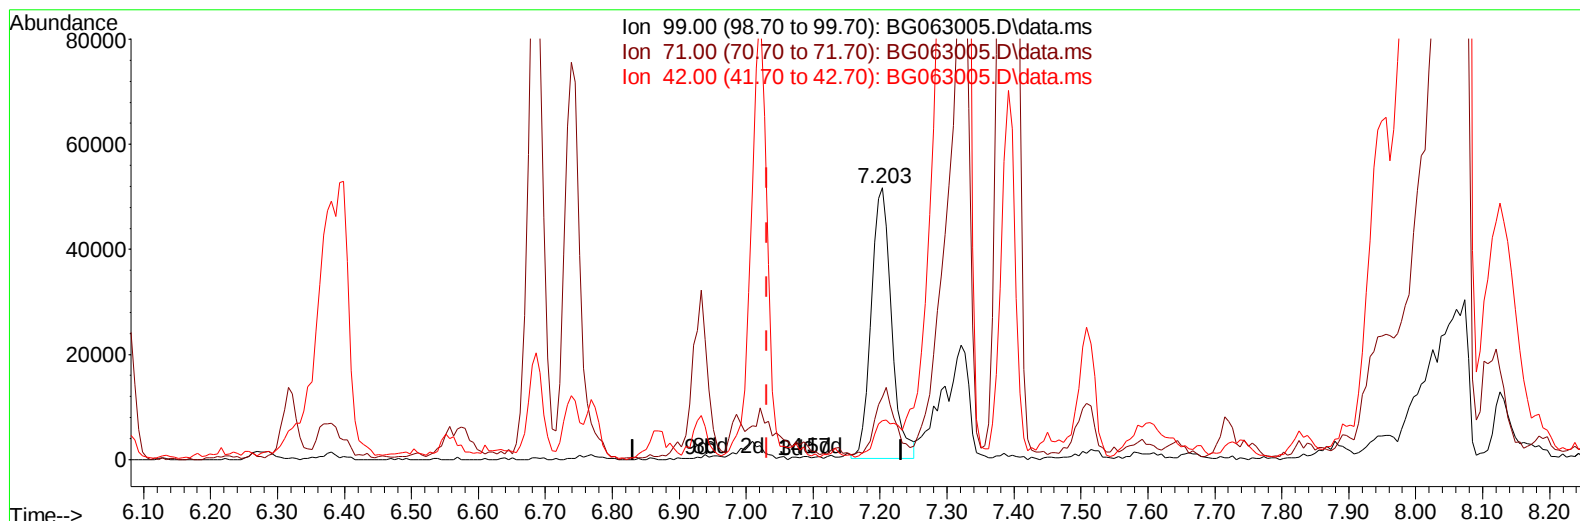

TIC: BG063005.D\data.ms

(7) Phenol-d5 (S)

7.203min (+ 0.172) 36.60 ng/u1 m

response 108152

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	39.50	23.08#
42.00	20.50	14.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:01:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

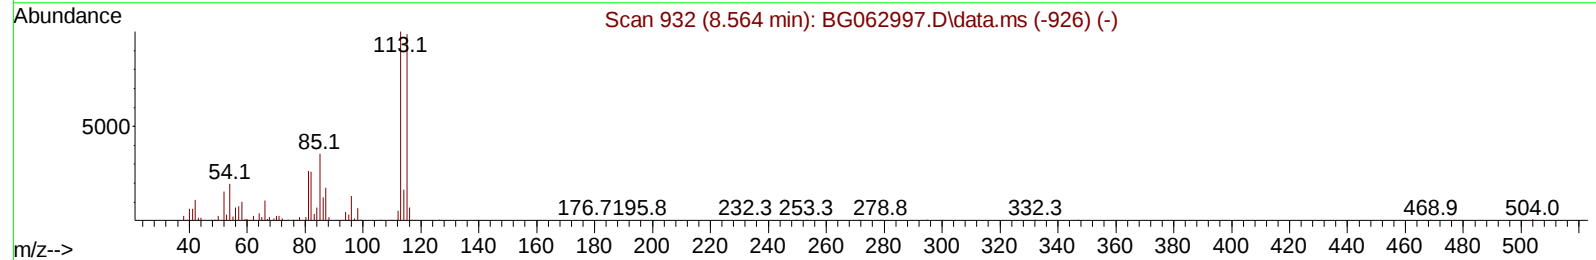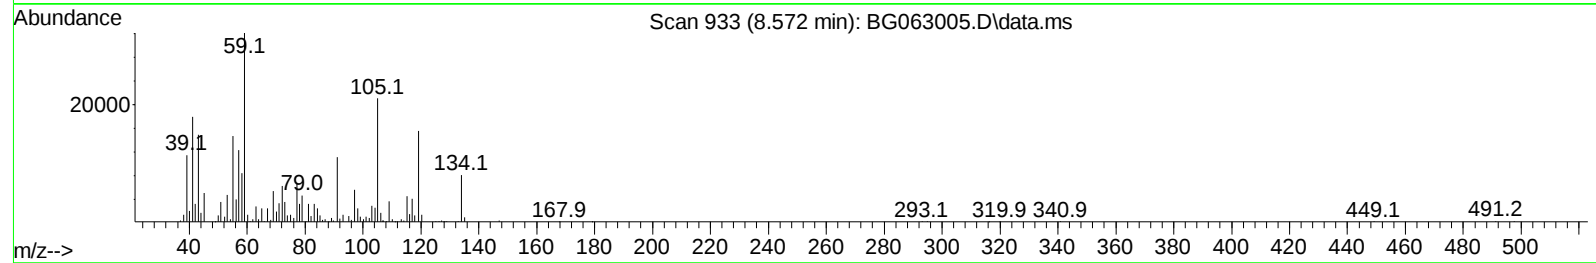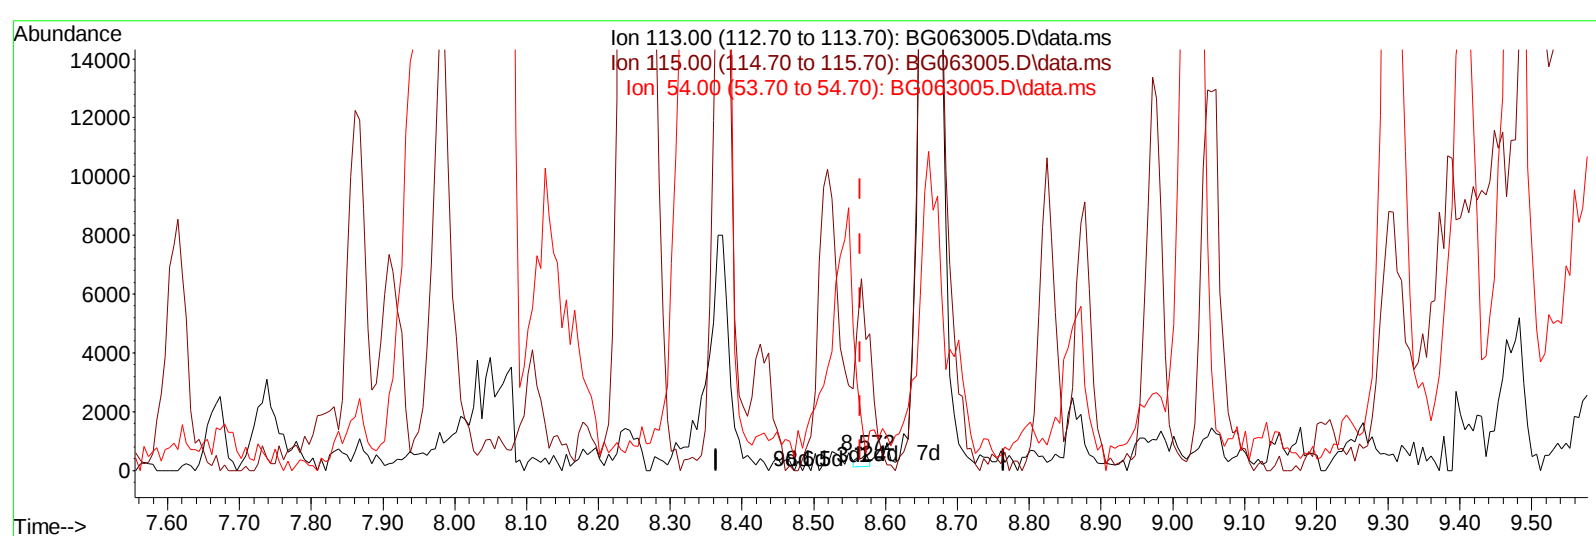

TIC: BG063005.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.572min (+ 0.008) 0.19 ng/u1

response 407

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	99.00	815.17#
54.00	17.30	106.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
 Data File : BG063005.D
 Acq On : 23 Sep 2024 23:06
 Operator : RC/JU
 Sample : P3879-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:01:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 18 00:45:18 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/26/2024

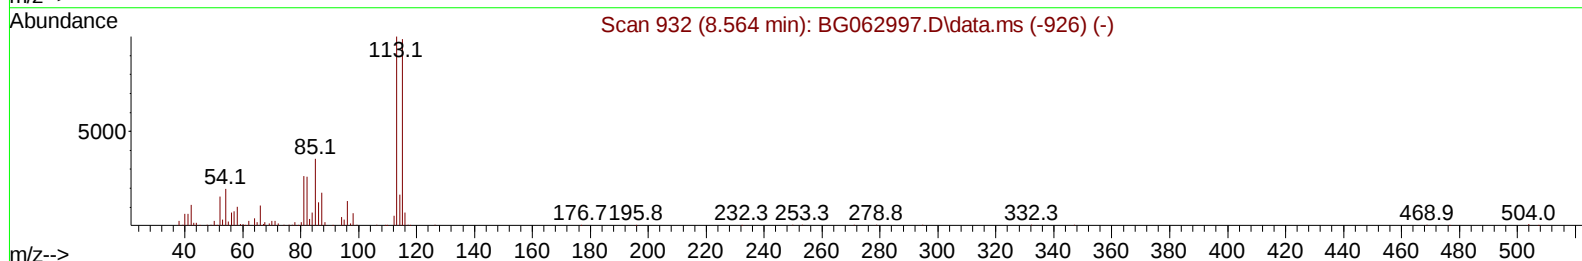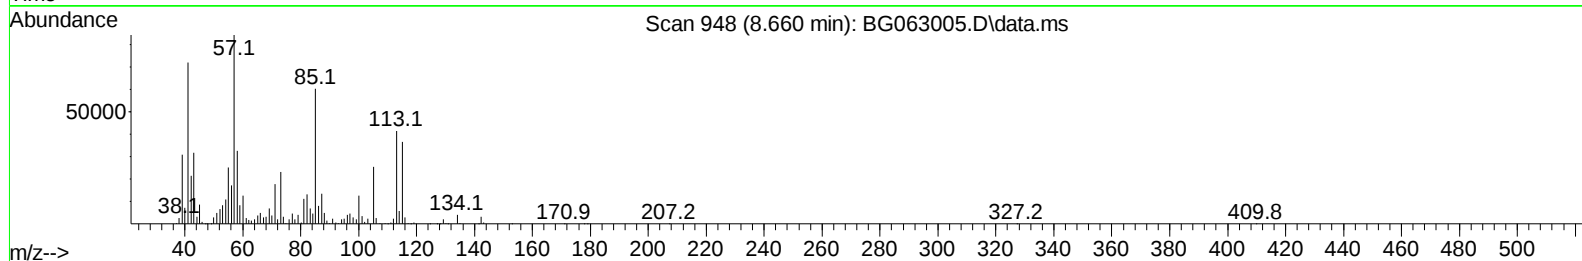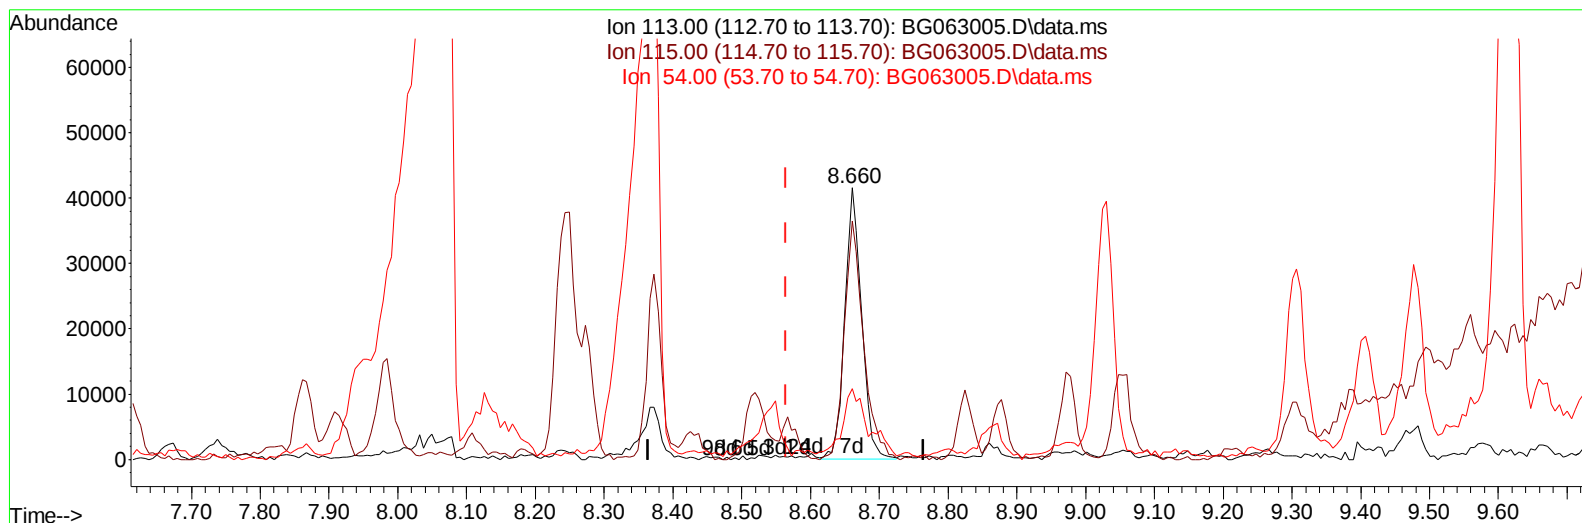

TIC: BG063005.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.660min (+ 0.096) 32.54 ng/u1 m

response 70445

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	99.00	87.87
54.00	17.30	26.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
 Data File : BG063005.D
 Acq On : 23 Sep 2024 23:06
 Operator : RC/JU
 Sample : P3879-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:08:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 18 00:45:18 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/26/2024

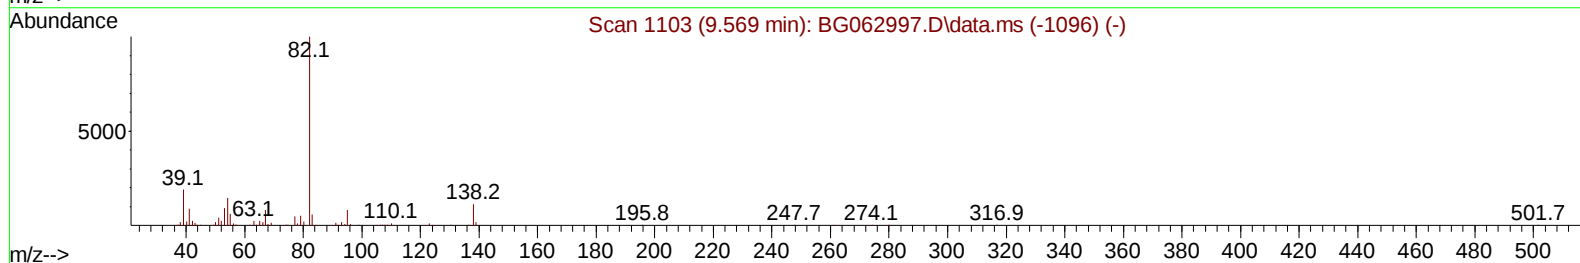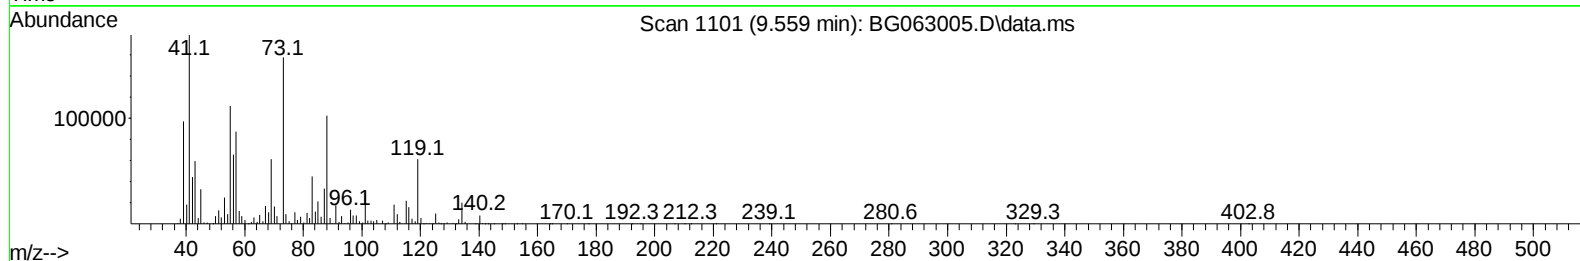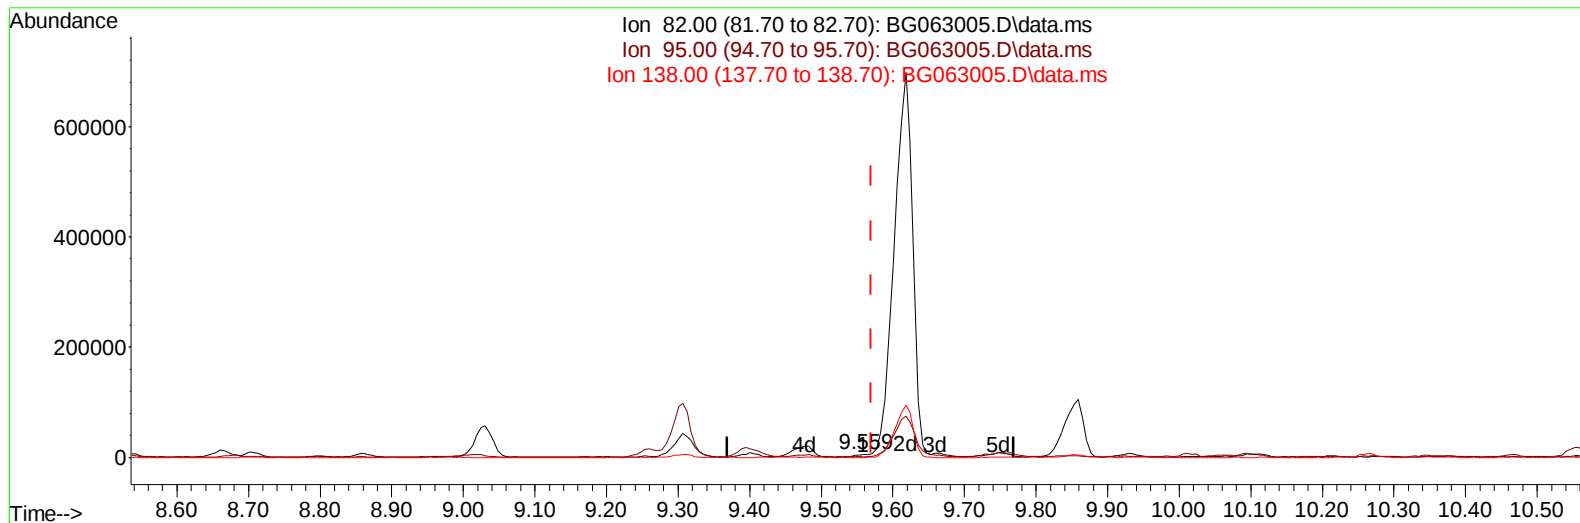

TIC: BG063005.D\data.ms

(23) Isophorone

9.559min (-0.010) 1.06 ng/u1

response 5176

Ion	Exp%	Act%
82.00	100.00	100.00
95.00	7.80	22.42#
138.00	13.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
 Data File : BG063005.D
 Acq On : 23 Sep 2024 23:06
 Operator : RC/JU
 Sample : P3879-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:08:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 18 00:45:18 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/26/2024

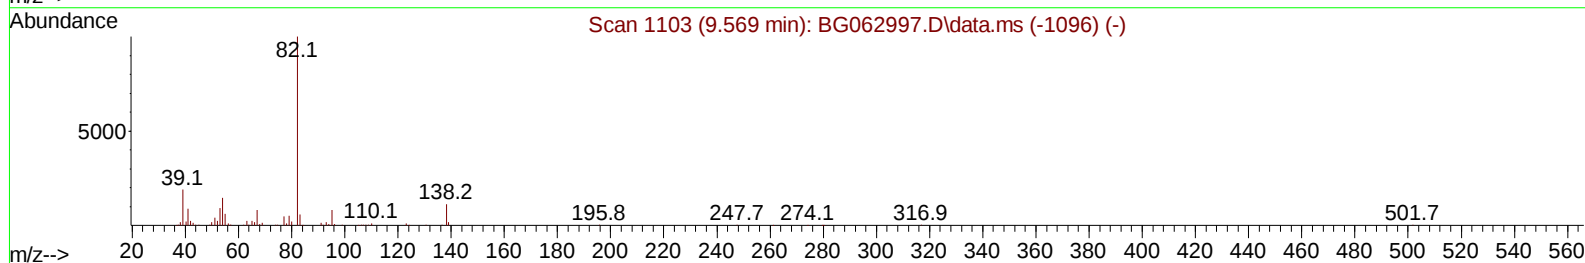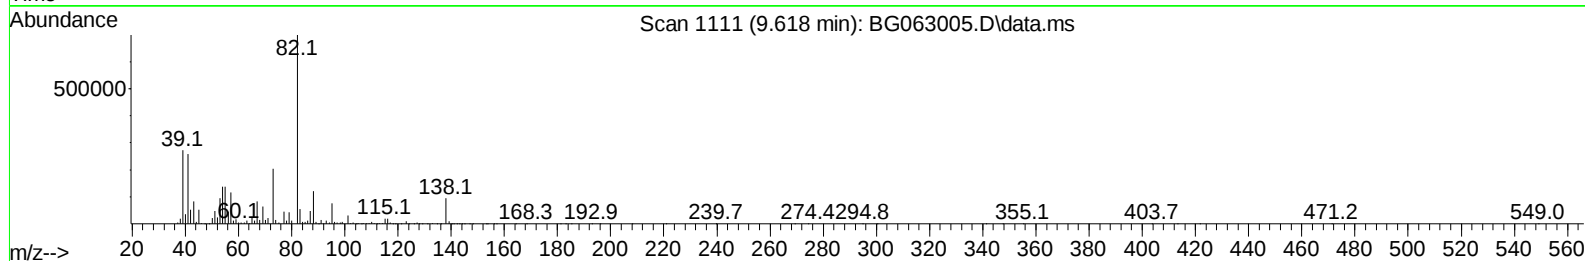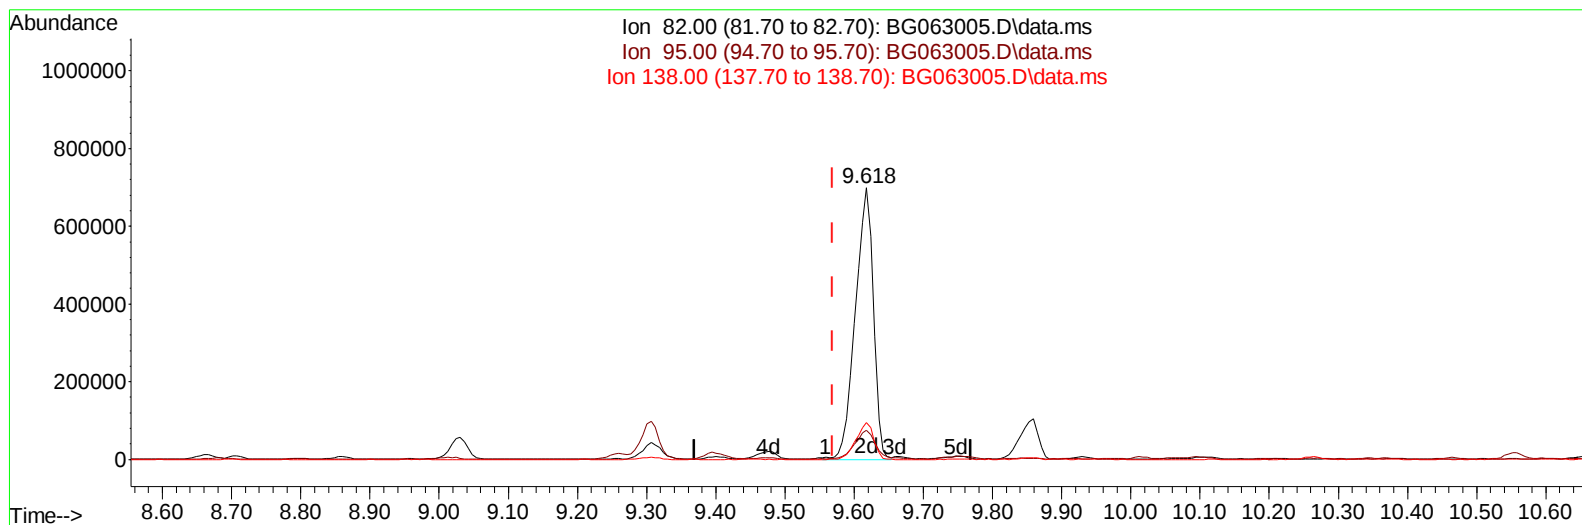

TIC: BG063005.D\data.ms

(23) Isophorone

9.618min (+ 0.049) 258.05 ng/ul m

response 1261782

Ion	Exp%	Act%
82.00	100.00	100.00
95.00	7.80	10.76#
138.00	13.60	13.56
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:08:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

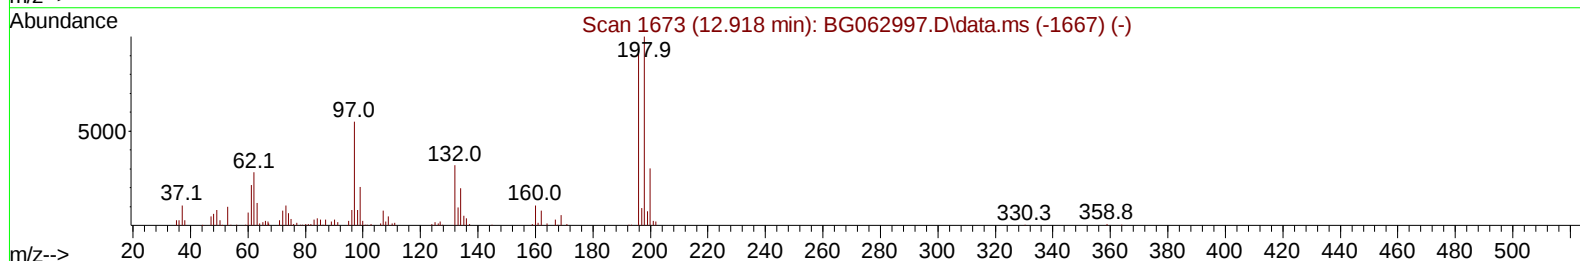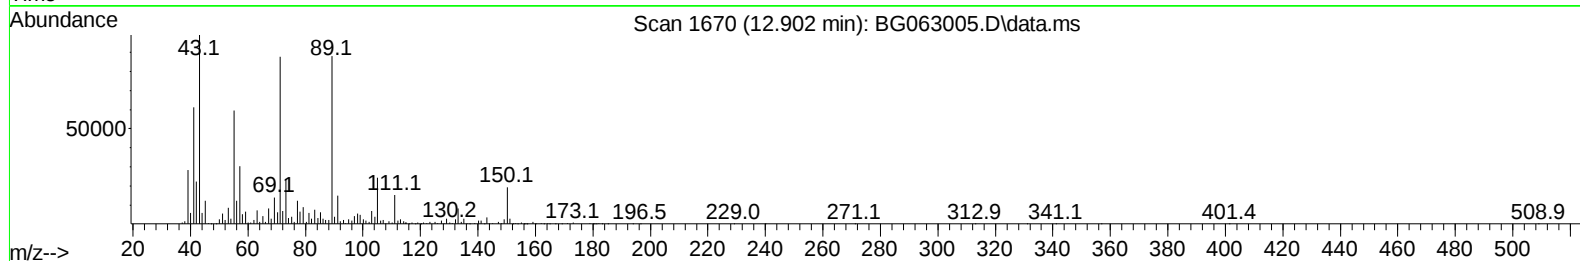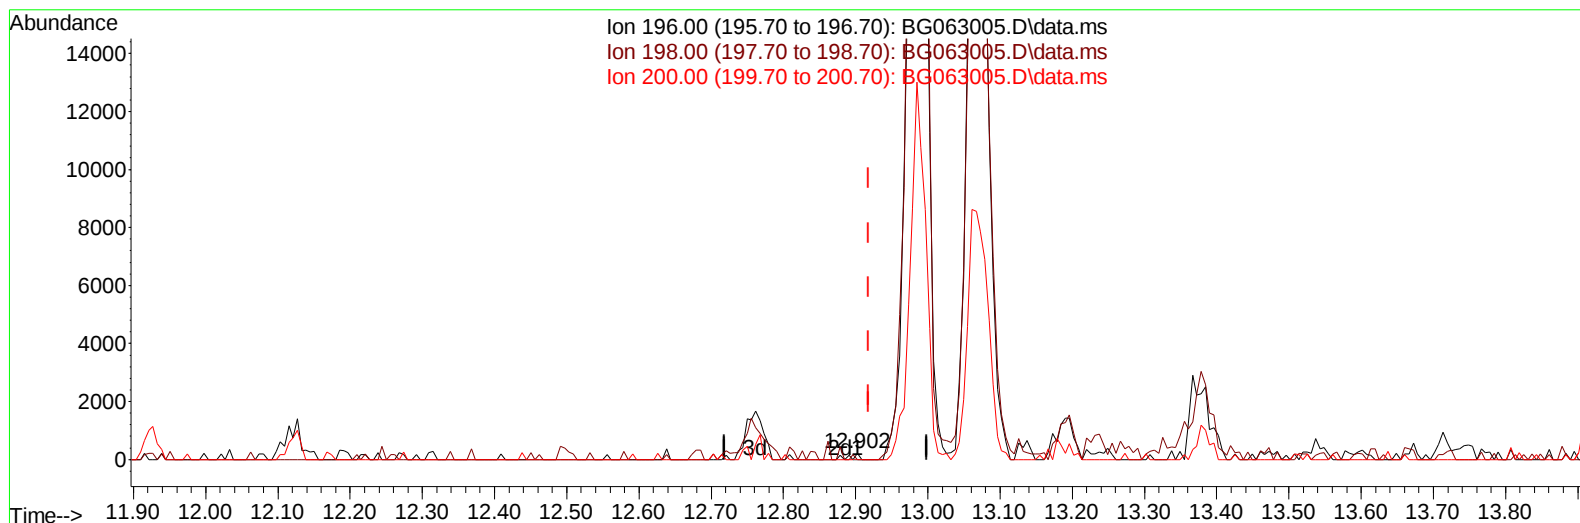

TIC: BG063005.D\data.ms

(41) 2,4,6-Trichlorophenol (C)

12.902min (-0.016) 0.05 ng/u1

response 76

Ion	Exp%	Act%
196.00	100.00	100.00
198.00	102.20	0.00#
200.00	38.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

Quant Time: Sep 24 01:08:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

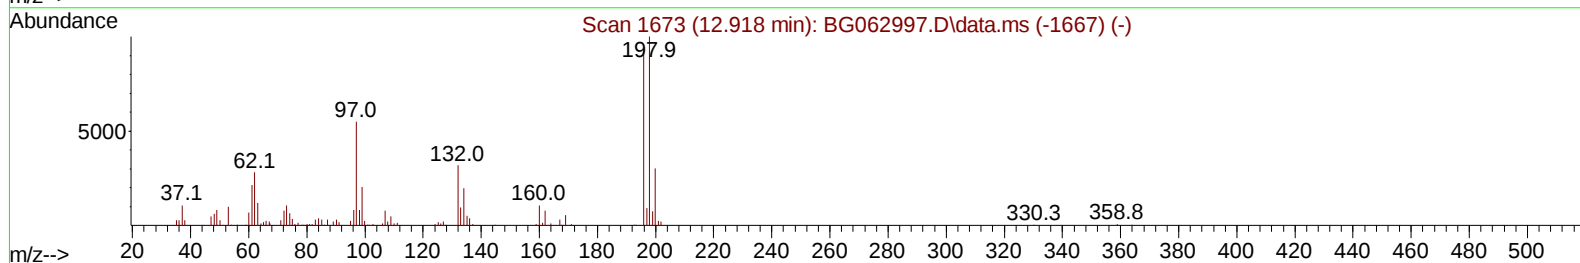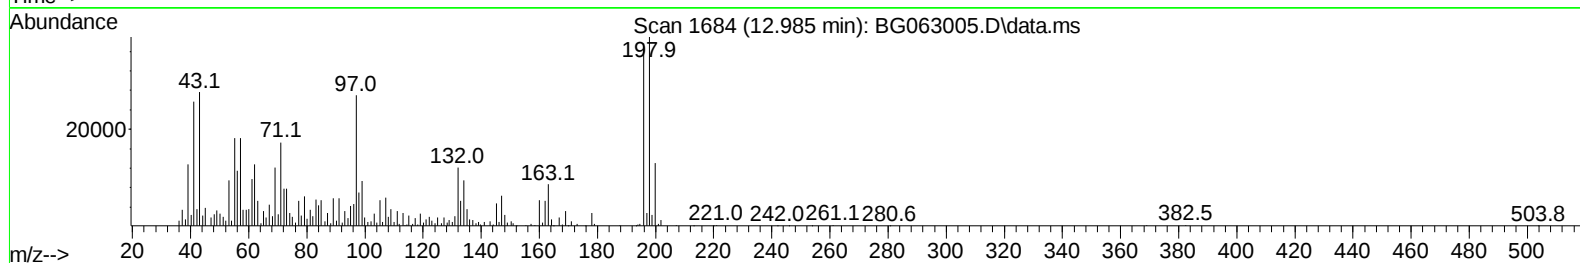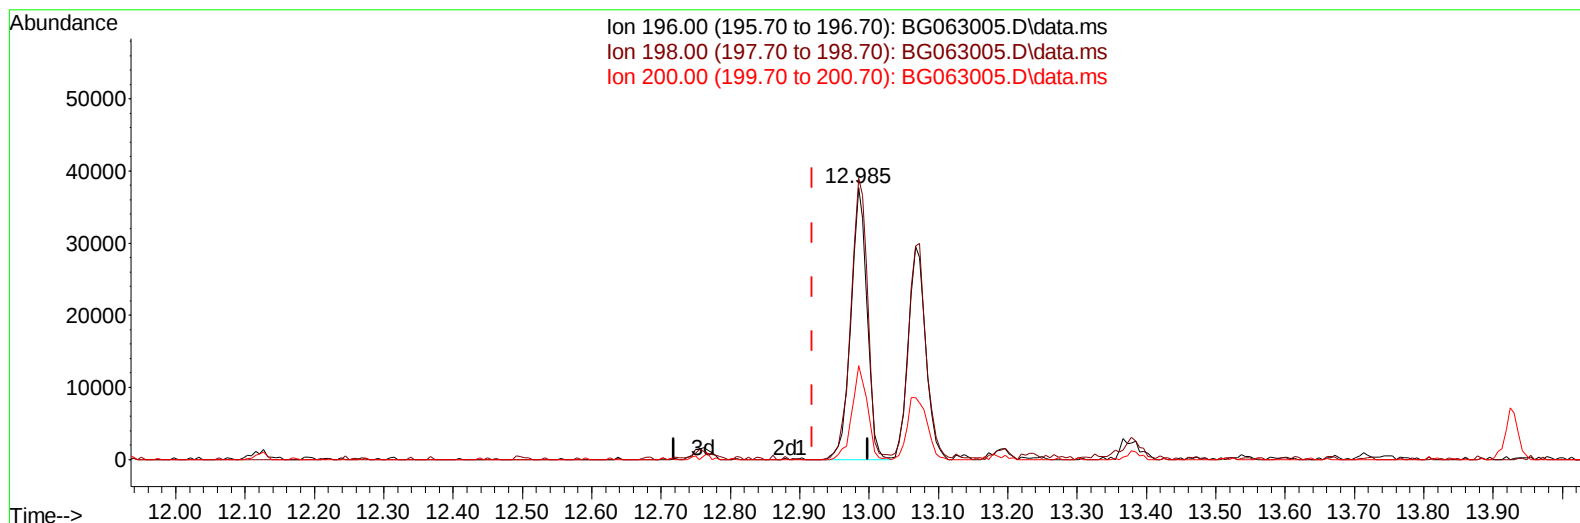

TIC: BG063005.D\data.ms

(41) 2,4,6-Trichlorophenol (C)

12.985min (+ 0.066) 38.88 ng/ul m

response 61318

Ion	Exp%	Act%
196.00	100.00	100.00
198.00	102.20	103.51
200.00	38.10	34.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
 Data File : BG063005.D
 Acq On : 23 Sep 2024 23:06
 Operator : RC/JU
 Sample : P3879-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:08:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 18 00:45:18 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/26/2024

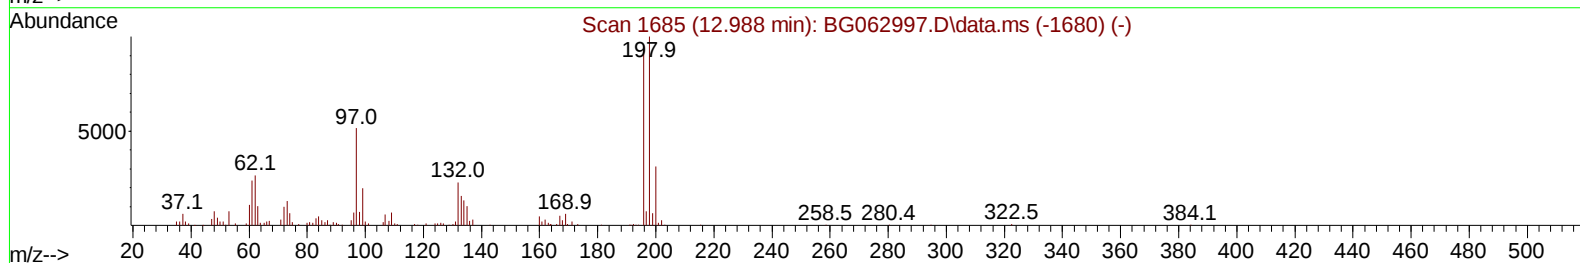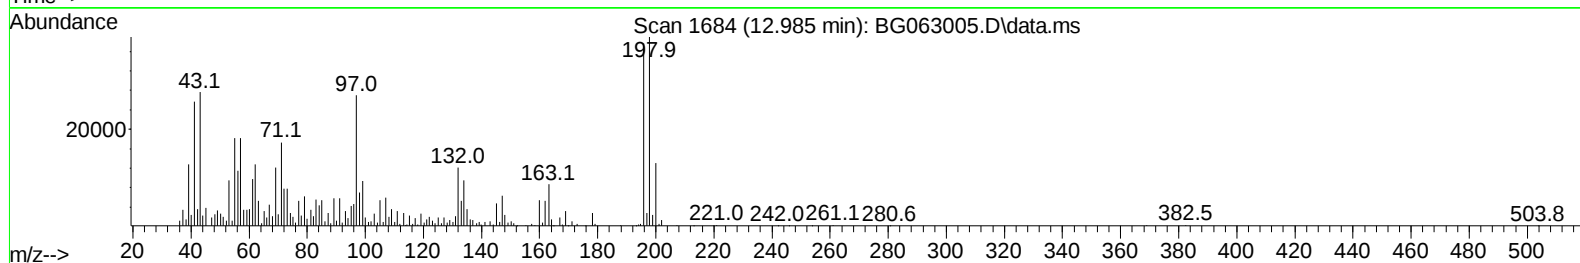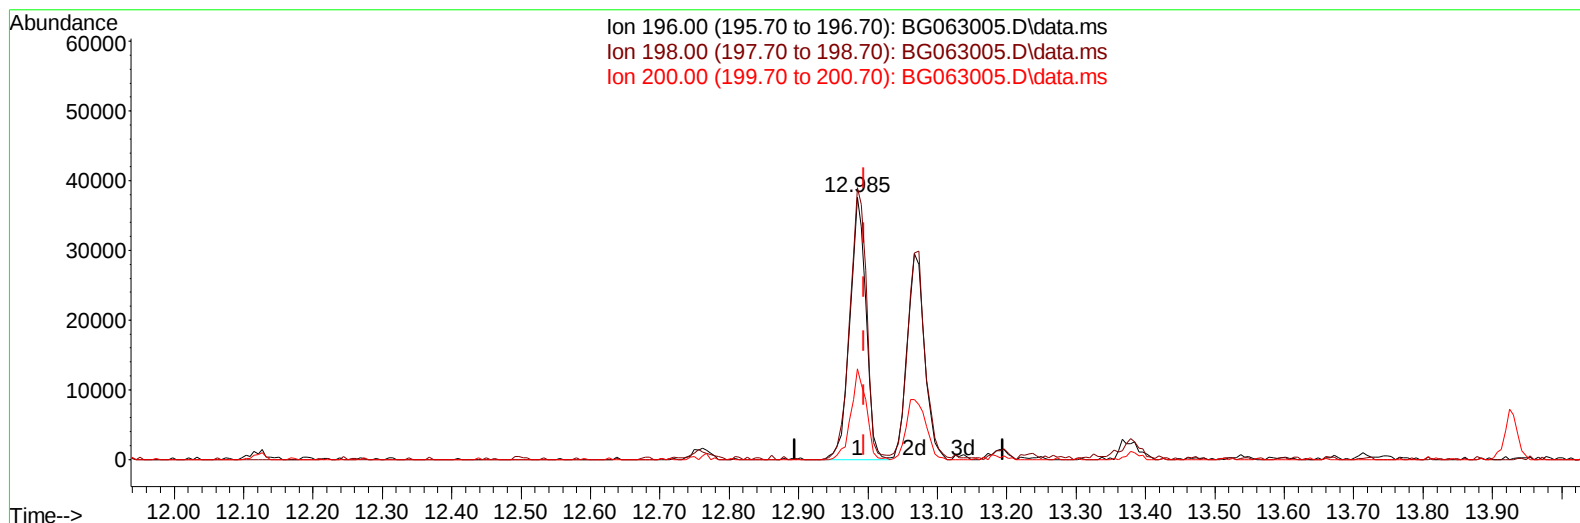

TIC: BG063005.D\data.ms

(42) 2,4,5-Trichlorophenol

12.985min (-0.010) 37.01 ng/u1

response 61318

Ion	Exp%	Act%
196.00	100.00	100.00
198.00	94.40	103.51
200.00	31.90	34.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:08:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

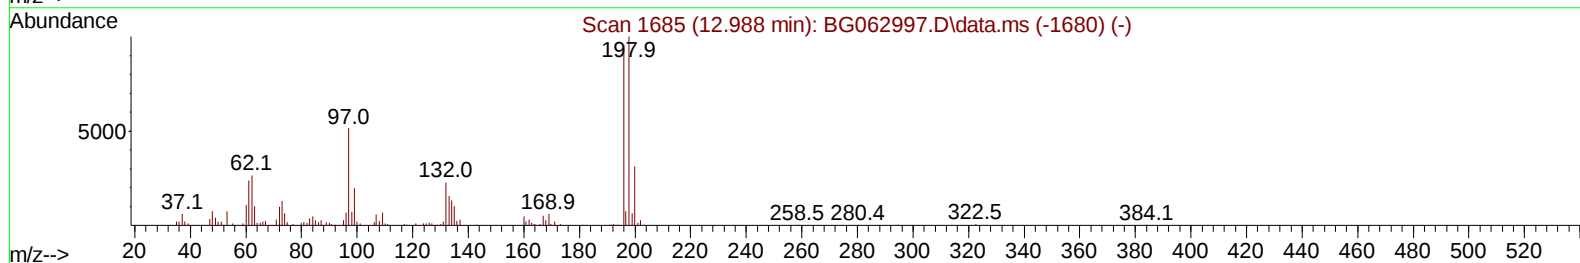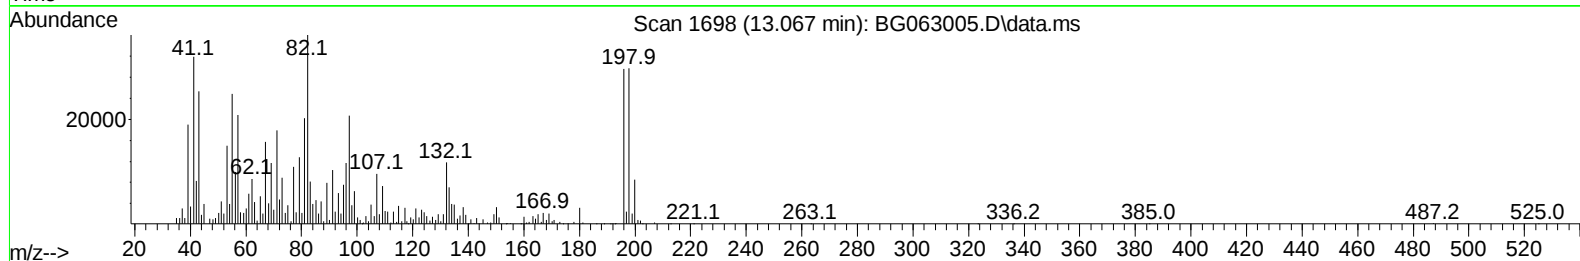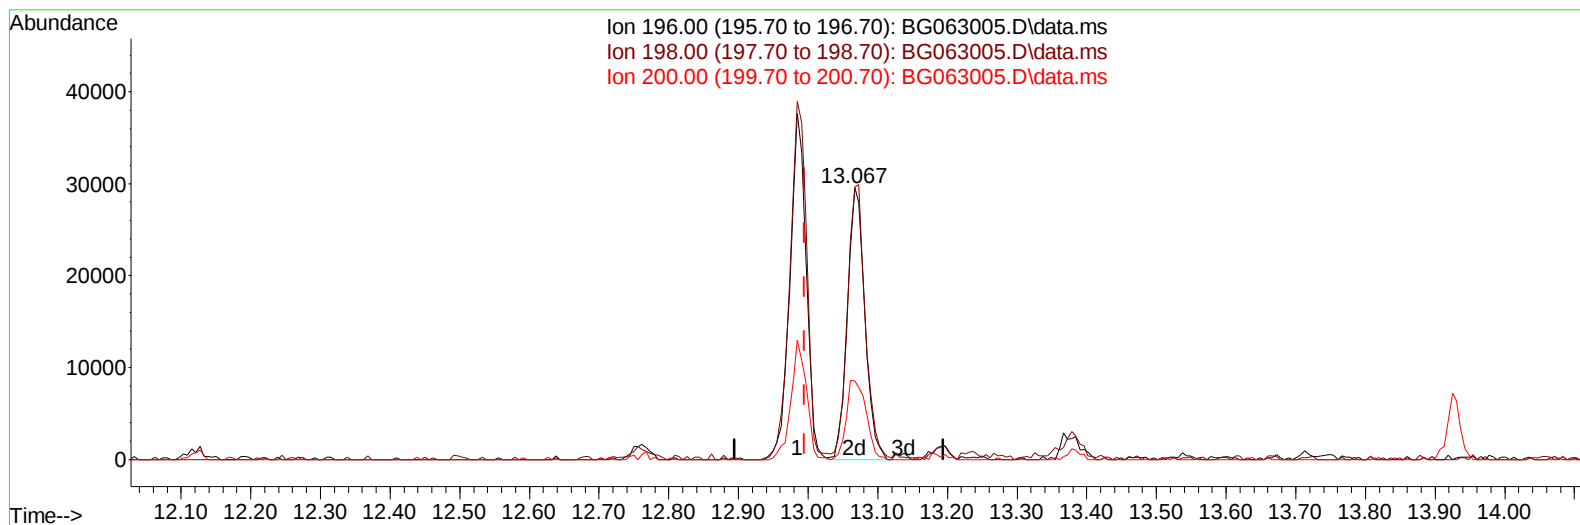

TIC: BG063005.D\data.ms

(42) 2,4,5-Trichlorophenol

13.067min (+ 0.072) 31.08 ng/ul m

response 51503

Ion	Exp%	Act%
196.00	100.00	100.00
198.00	94.40	100.24
200.00	31.90	29.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:08:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

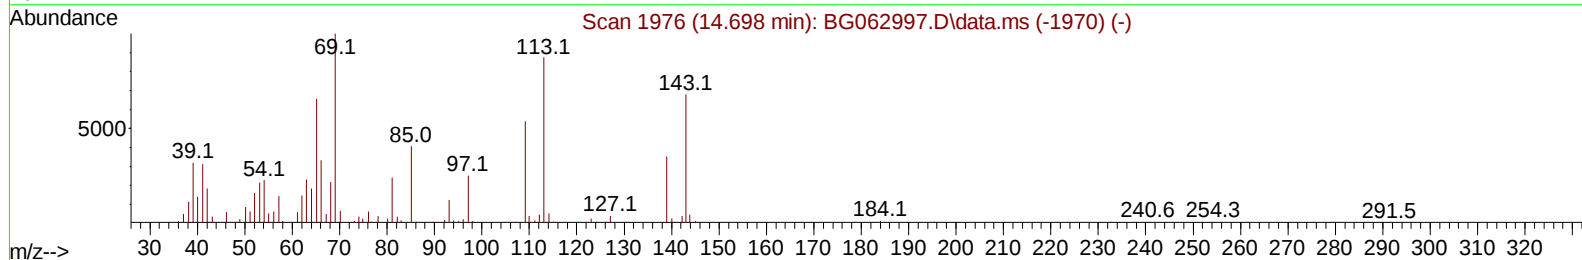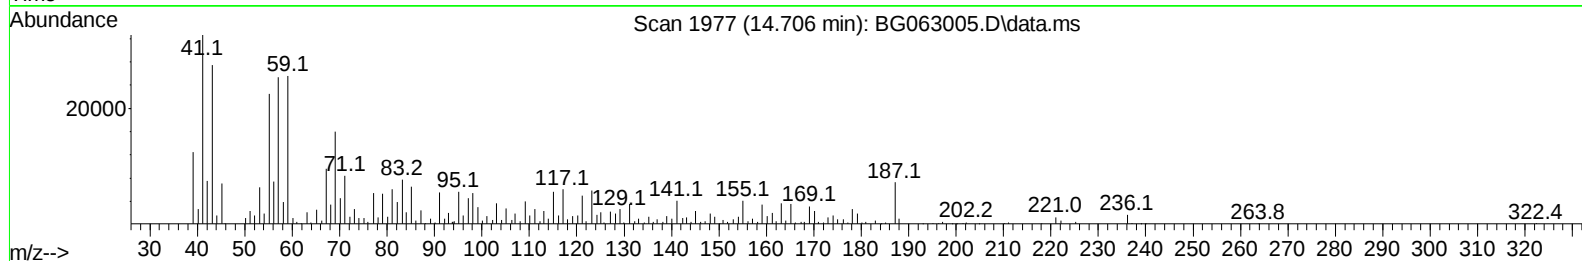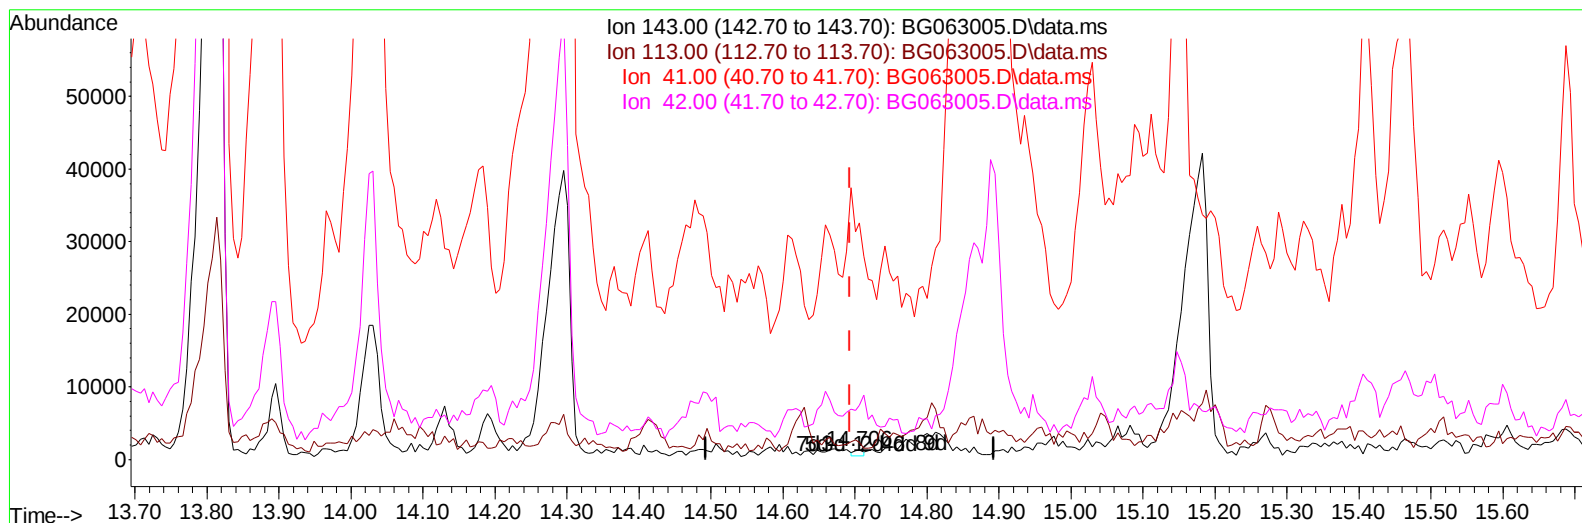

TIC: BG063005.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.706min (+ 0.013) 0.80 ng/u1

response 679

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.50	184.30#
41.00	49.70	2559.50#
42.00	34.20	587.68#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:08:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

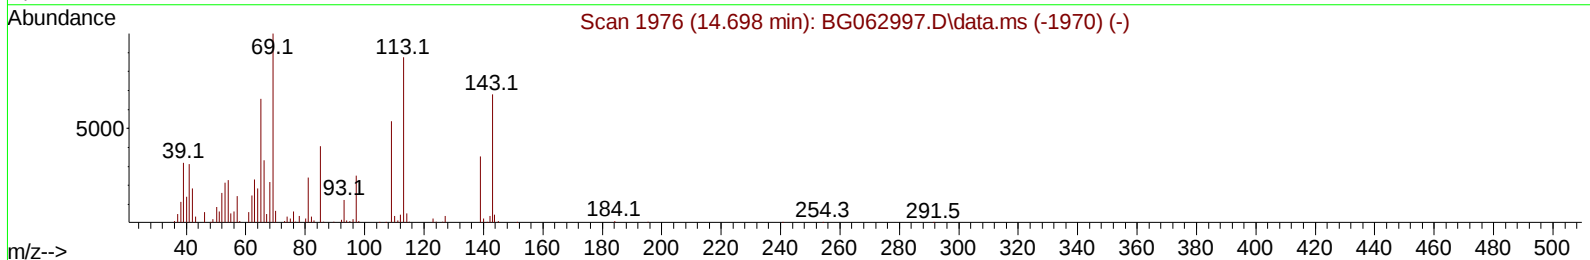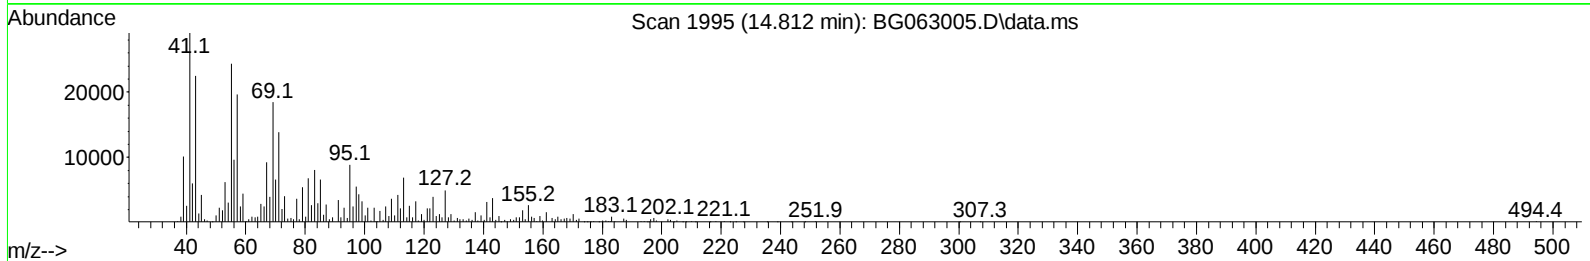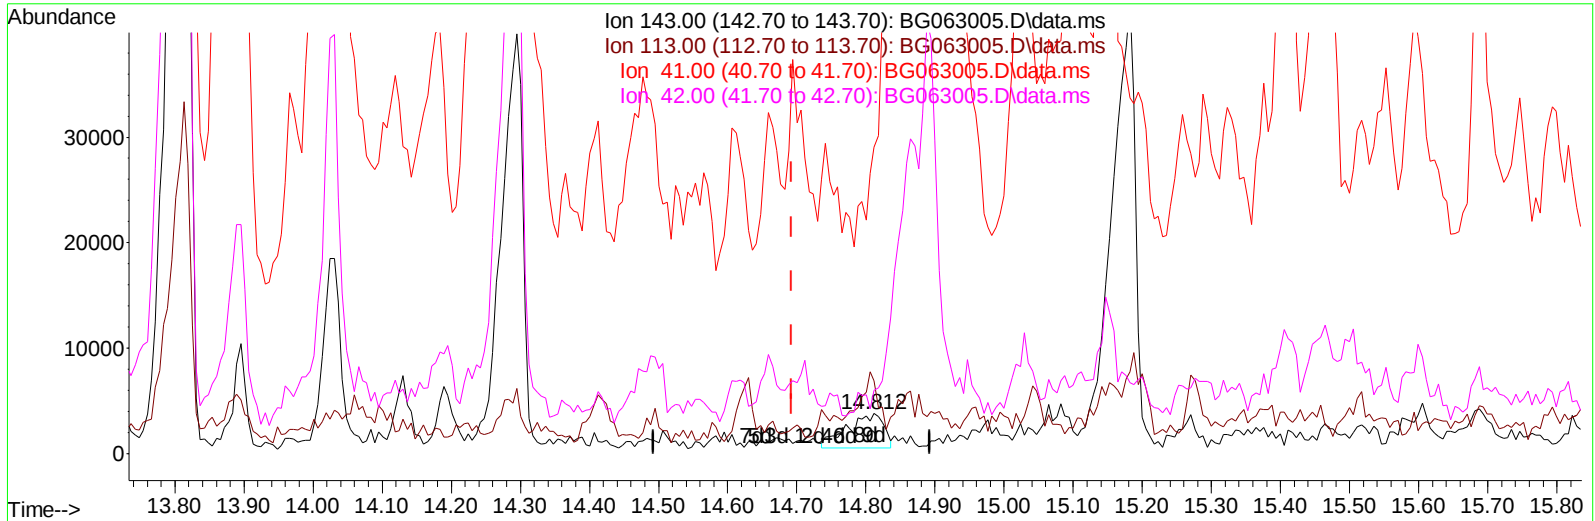

TIC: BG063005.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.812min (+ 0.119) 13.95 ng/ul m

response 11875

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.50	182.23#
41.00	49.70	764.62#
42.00	34.20	158.38#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:11:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

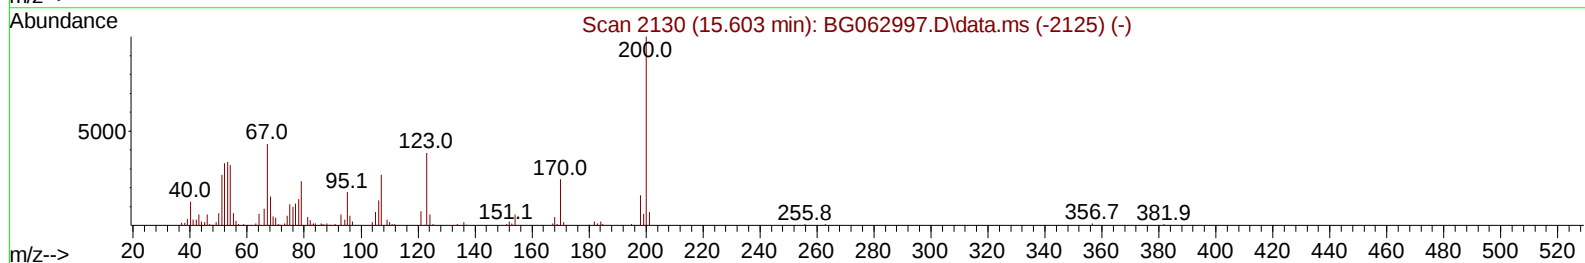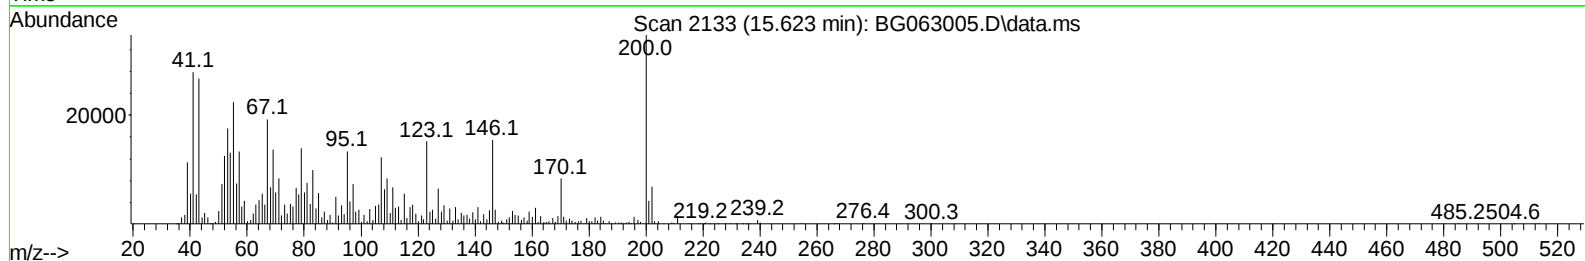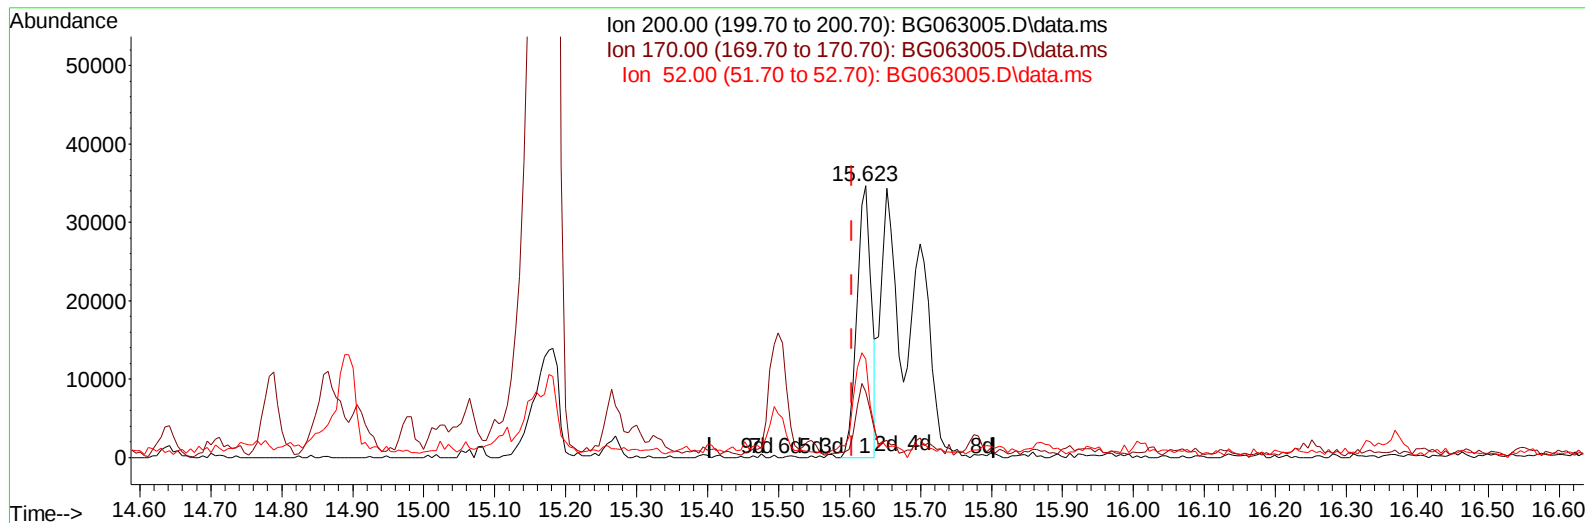

TIC: BG063005.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.623min (+ 0.019) 42.50 ng/u1

response 48925

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.60	24.28
52.00	36.60	36.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:11:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

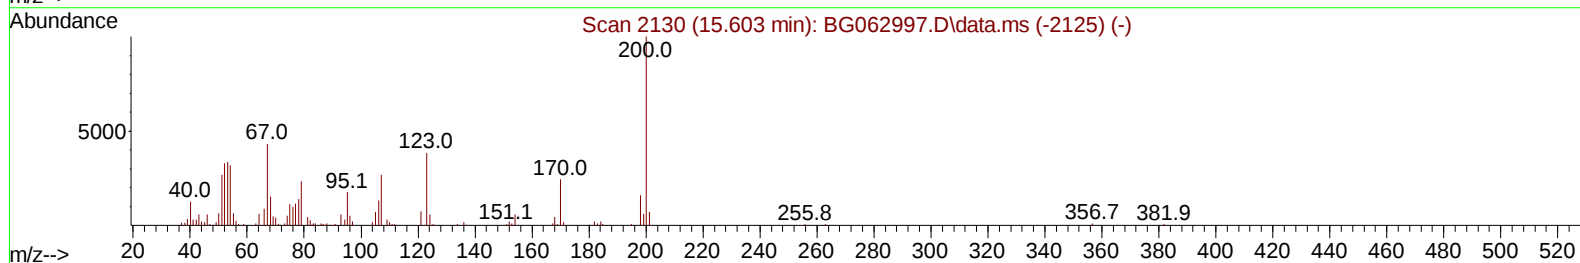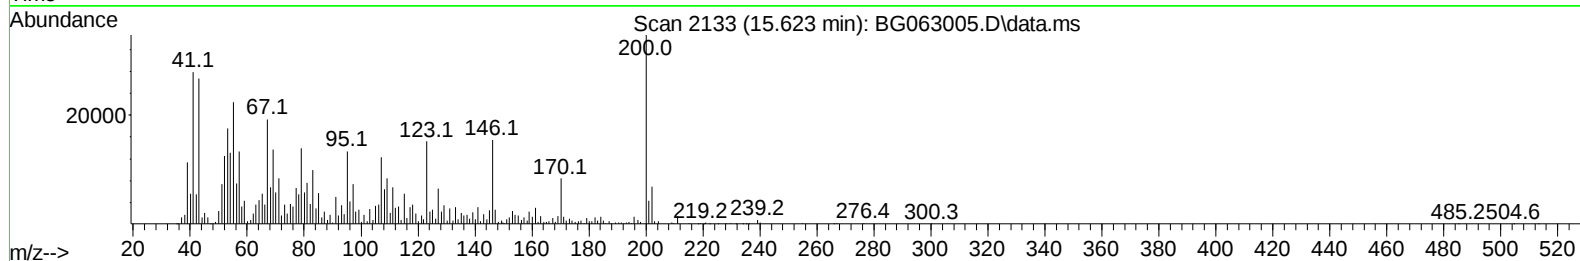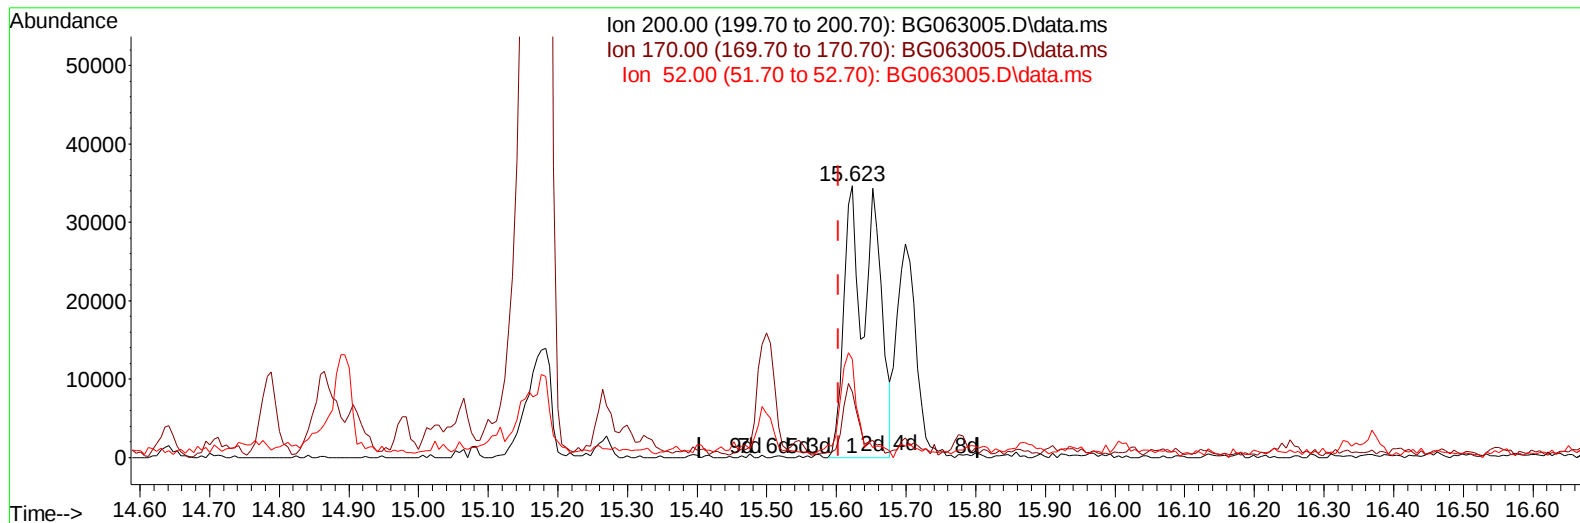

TIC: BG063005.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.623min (+ 0.019) 87.89 ng/ul m

response 101187

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.60	24.28
52.00	36.60	36.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:11:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

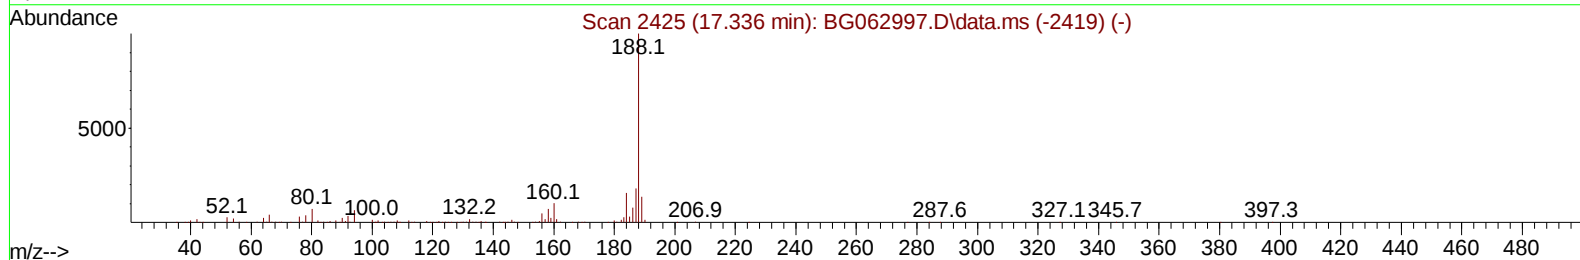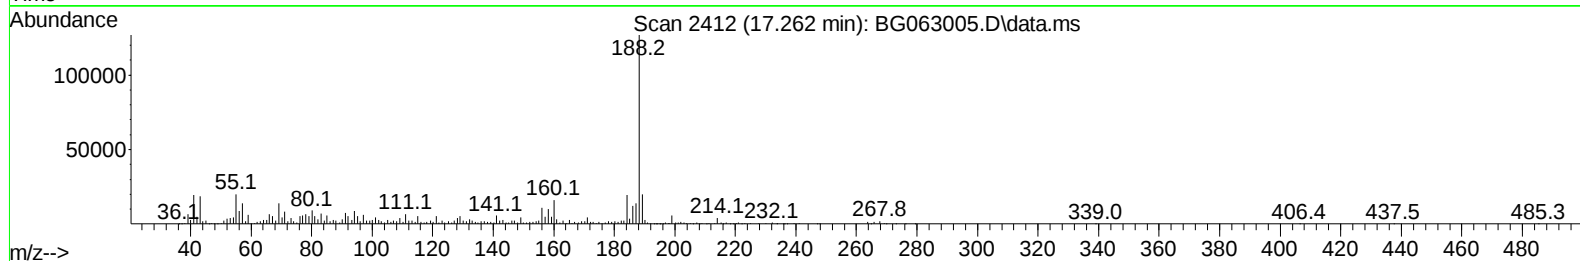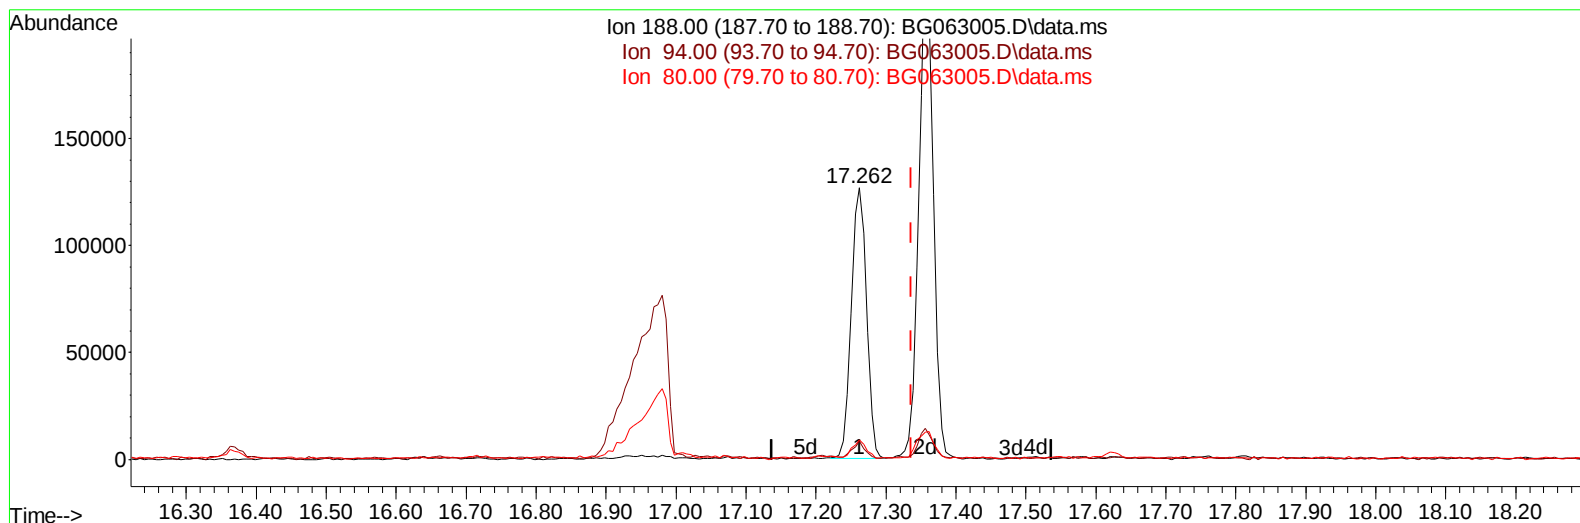

TIC: BG063005.D\data.ms

(73) Anthracene-d10 (S)

17.262min (-0.075) 21.16 ng/u1

response 190454

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.30	6.74
80.00	8.50	7.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:11:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

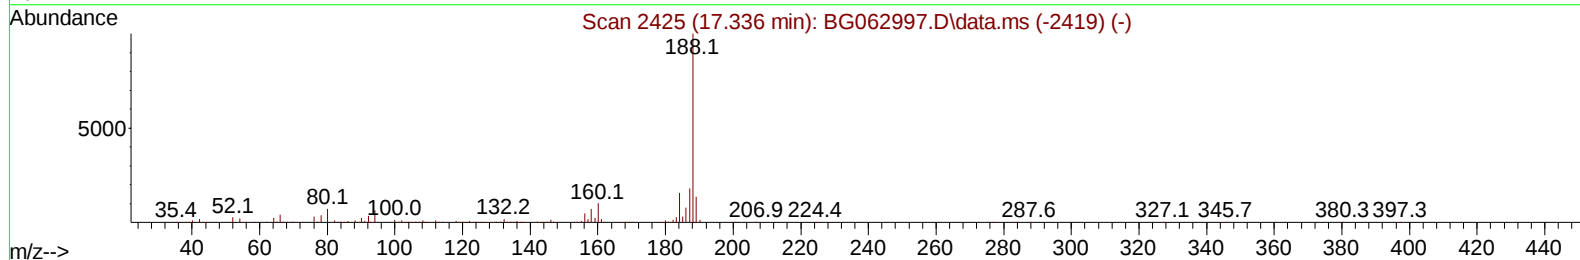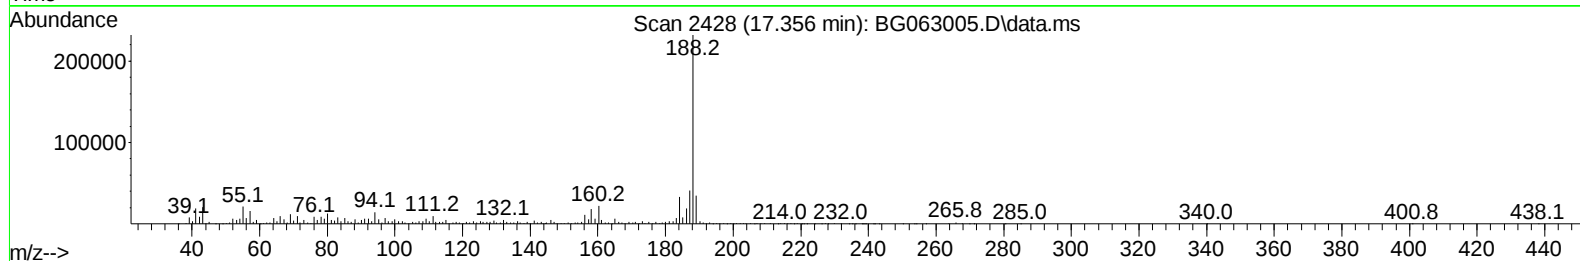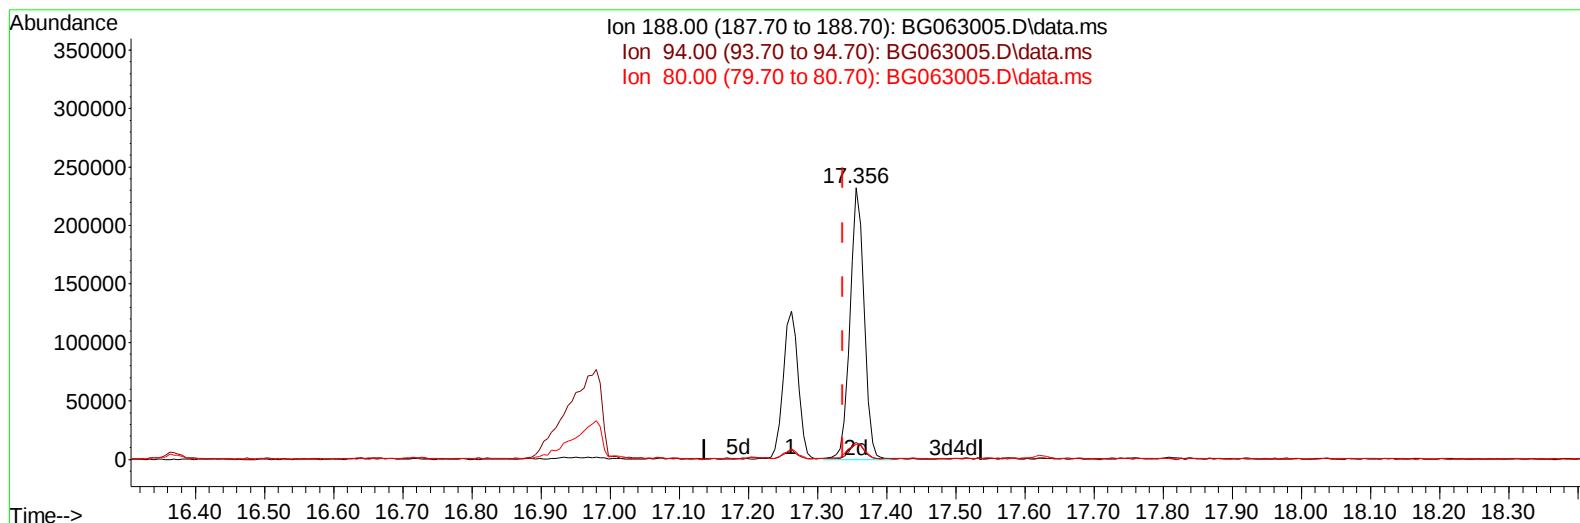

TIC: BG063005.D\data.ms

(73) Anthracene-d10 (S)

17.356min (+ 0.019) 36.72 ng/u1 m

response 330495

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	8.30	6.27#
80.00	8.50	5.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:11:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

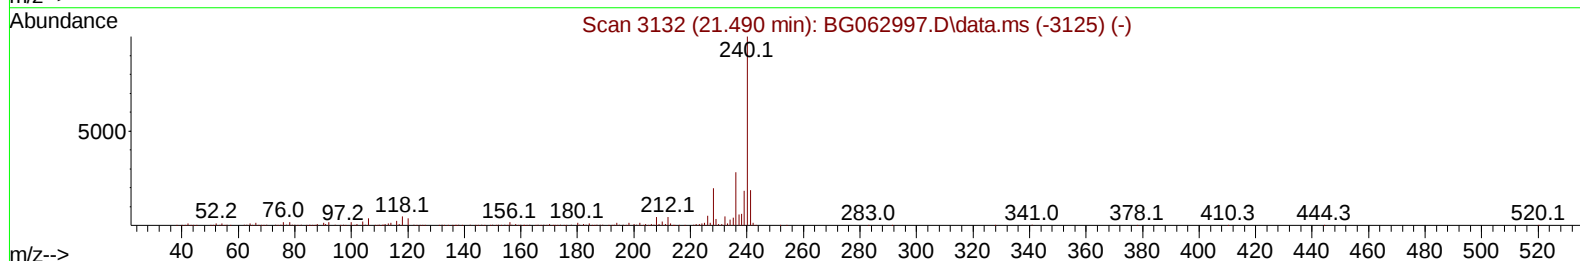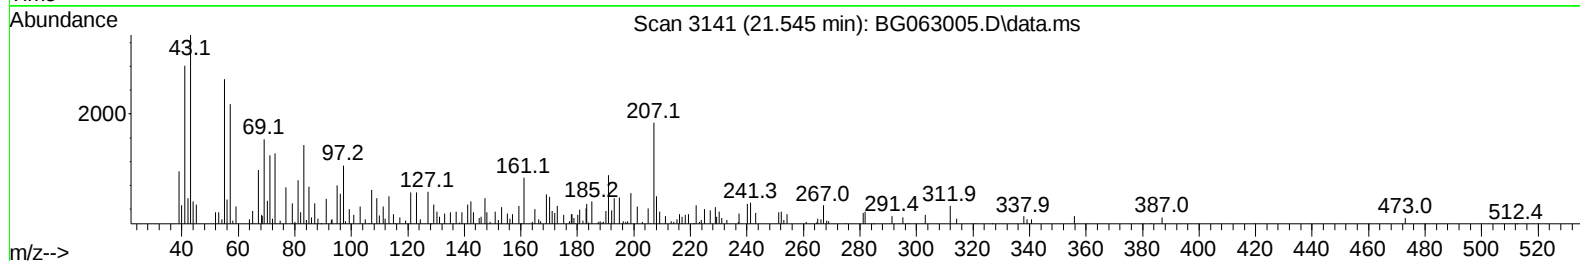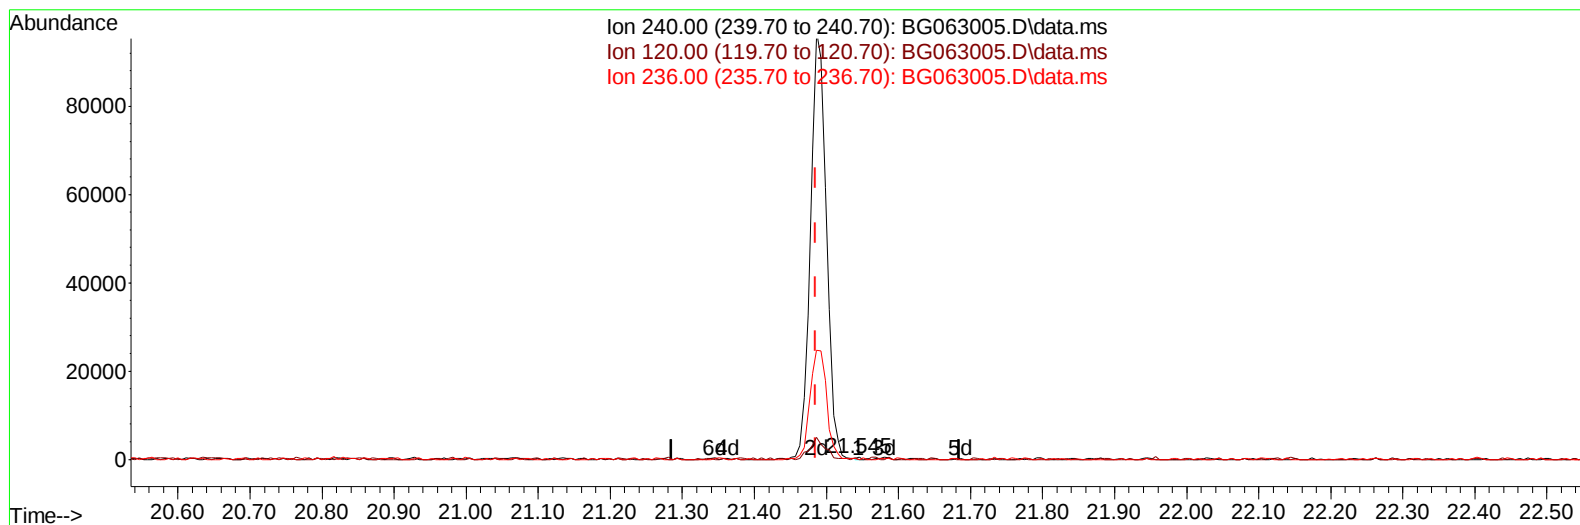

TIC: BG063005.D\data.ms

(79) Chrysene-d12 (I)

21.545min (+ 0.060) 20.00 ng/u1

response 171

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	7.60	0.00#
236.00	26.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:11:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

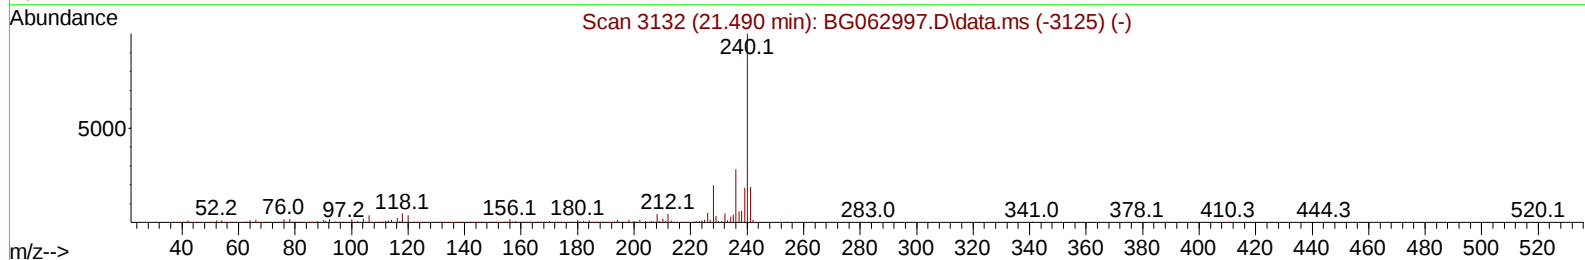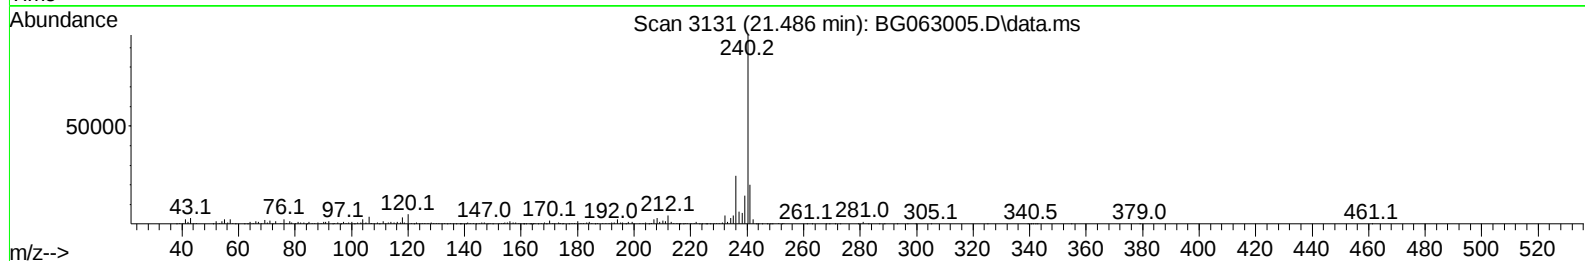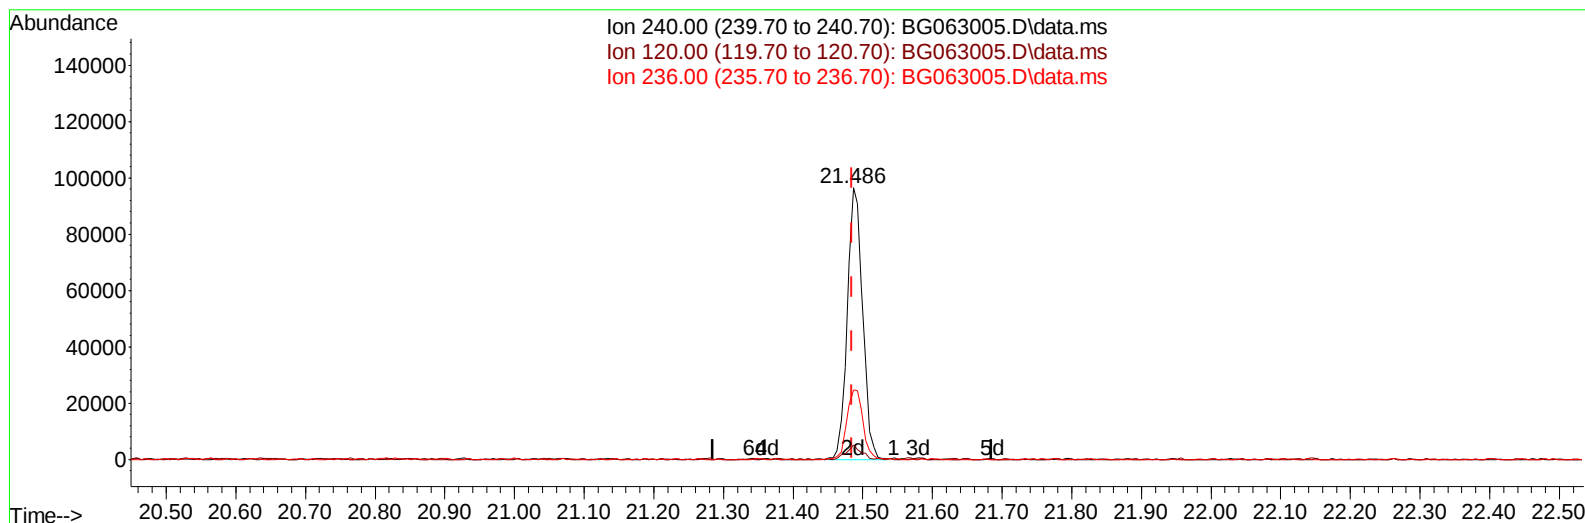

TIC: BG063005.D\data.ms

(79) Chrysene-d12 (I)

21.486min (+ 0.002) 20.00 ng/ul m

response 147626

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	7.60	5.22#
236.00	26.60	25.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
 Data File : BG063005.D
 Acq On : 23 Sep 2024 23:06
 Operator : RC/JU
 Sample : P3879-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC59

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/25/2024
 Supervised By :mohammad ahmed 09/26/2024

Quant Time: Sep 24 01:12:50 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 18 00:45:18 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.861	152		28478	20.000	ng/ul	0.00
20) Naphthalene-d8	10.664	136		103812	20.000	ng/ul	# 0.02
38) Acenaphthene-d10	14.501	164		71416	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.262	188		190454	20.000	ng/ul	0.03
79) Chrysene-d12	21.486	240		147626m	20.000	ng/ul	0.00
88) Perylene-d12	24.536	264		245974	20.000	ng/ul	0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.325	96		3988	4.102	ng/uL	0.00
4) Pyridine-d5	3.743	84		8048	3.049	ng/ul	0.00
7) Phenol-d5	7.203	99		108152m	36.599	ng/ul	0.17
9) Bis-(2-Chloroethyl)eth...	7.197	67		50237	30.379	ng/ul	0.01
11) 2-Chlorophenol-d4	7.468	132		66193	34.118	ng/ul	0.08
15) 4-Methylphenol-d8	8.660	113		70445m	32.542	ng/ul	0.10
21) Nitrobenzene-d5	9.031	128		33114	40.039	ng/ul	0.03
24) 2-Nitrophenol-d4	9.747	143		31394	33.460	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.341	165		67710	34.782	ng/ul	0.07
31) 4-Chloroaniline-d4	10.776	131		17634	7.279	ng/ul	0.00
46) Dimethylphthalate-d6	13.925	166		232050	43.695	ng/ul	0.03
49) Acenaphthylene-d8	14.195	160		240821	40.600	ng/ul	0.01
54) 4-Nitrophenol-d4	14.812	143		11875m	13.954	ng/ul	0.12
60) Fluorene-d10	15.499	176		209014	42.269	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.623	200		101187m	87.890	ng/ul	0.02
73) Anthracene-d10	17.356	188		330495m	36.717	ng/ul	0.02
81) Pyrene-d10	19.642	212		295170	33.012	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.324	264		487045	37.545	ng/ul	0.01
Target Compounds							
						Qvalue	
23) Isophorone	9.618	82		1261782m	258.049	ng/ul	
29) 2,4-Dichlorophenol	10.364	162		67886	35.227	ng/ul	90
30) Naphthalene	10.711	128		589042	102.191	ng/ul	95
36) 2-Methylnaphthalene	12.315	142		204895	49.328	ng/ul	94
37) 1-Methylnaphthalene	12.544	142		141934	33.764	ng/ul#	97
41) 2,4,6-Trichlorophenol	12.985	196		61318m	38.879	ng/ul	
42) 2,4,5-Trichlorophenol	13.067	196		51503m	31.084	ng/ul	
43) 1,1'-Biphenyl	13.331	154		26262	4.950	ng/ul#	74
52) Acenaphthene	14.565	153		6364	1.403	ng/ul	96
58) 2,3,4,6-Tetrachlorophenol	15.182	232		4021994	2697.475	ng/ul	98
61) Fluorene	15.552	166		12462	2.421	ng/ul#	89
71) Pentachlorophenol	16.980	266		9698163	6956.884	ng/ul#	77
72) Phenanthrene	17.303	178		23885	2.361	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092324\
Data File : BG063005.D
Acq On : 23 Sep 2024 23:06
Operator : RC/JU
Sample : P3879-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC59

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:12:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091724.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 18 00:45:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/25/2024
Supervised By :mohammad ahmed 09/26/2024

