
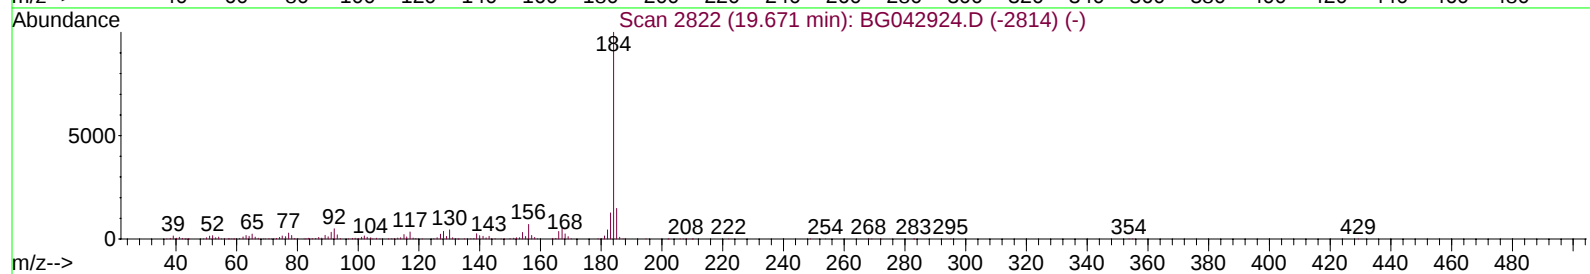
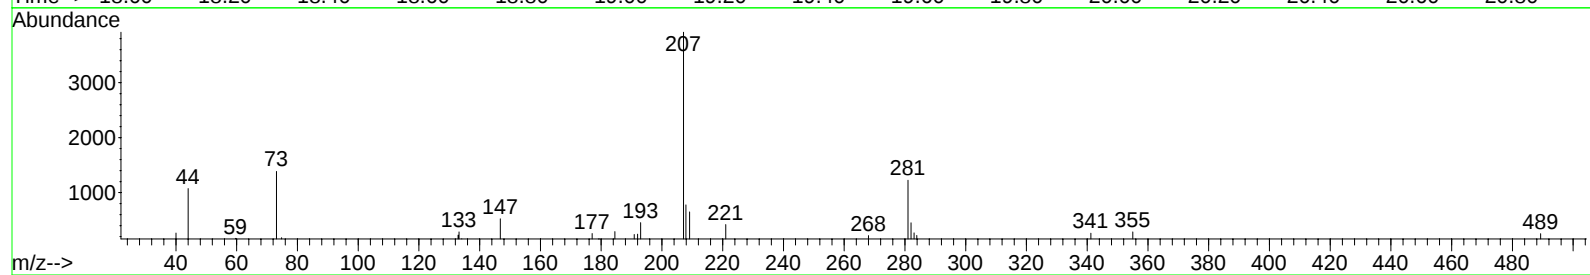


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092519\
 Data File : BG042921.D
 Acq On : 25 Sep 2019 10:14
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 18:47:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 25 15:35:52 2019
 Response via : Initial Calibration

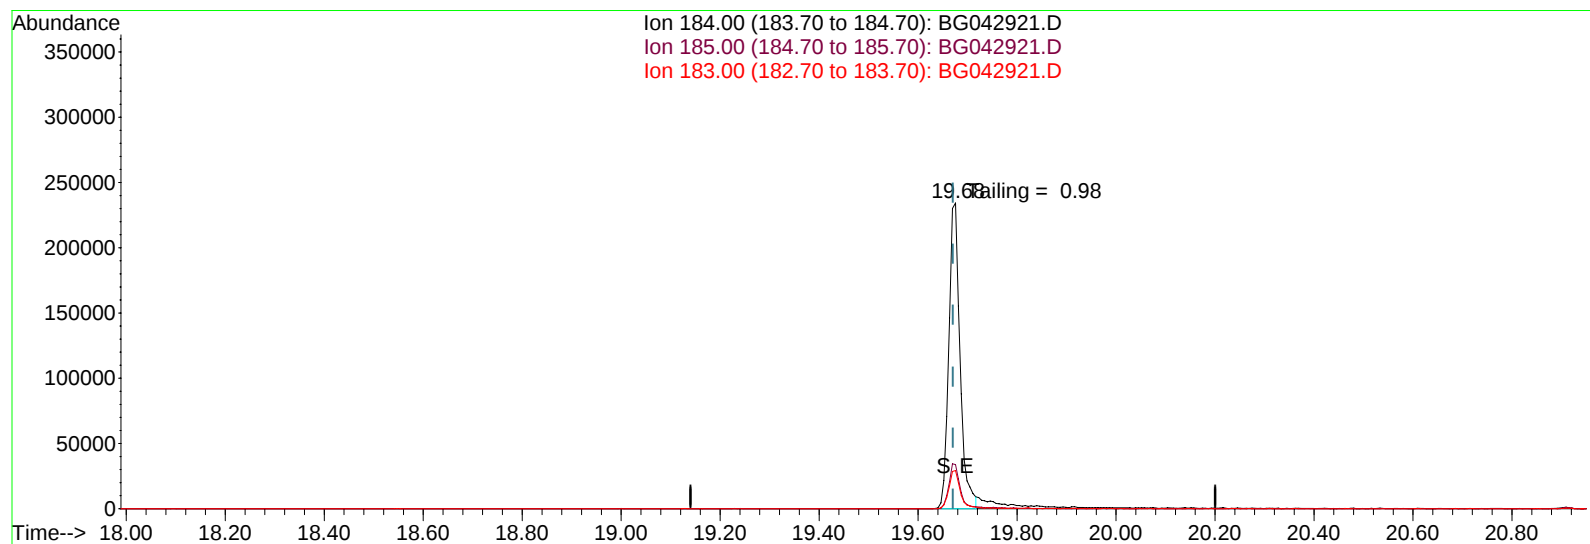

TIC: BG042921.D

(77) Benzidine




19.000min (-0.671) 0.95ng

response 103

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	0.00#
183.00	12.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092519\
Data File : BG042921.D
Acq On : 25 Sep 2019 10:14
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 18:47:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 15:35:52 2019
Response via : Initial Calibration

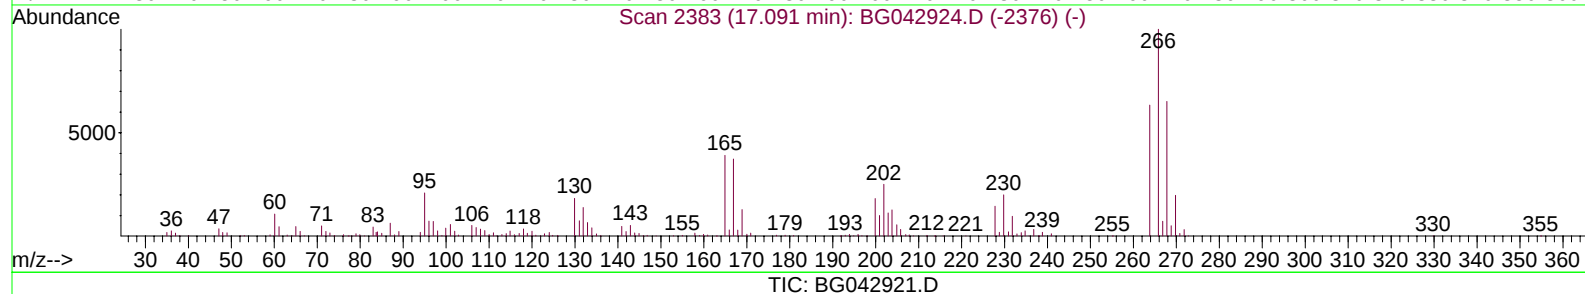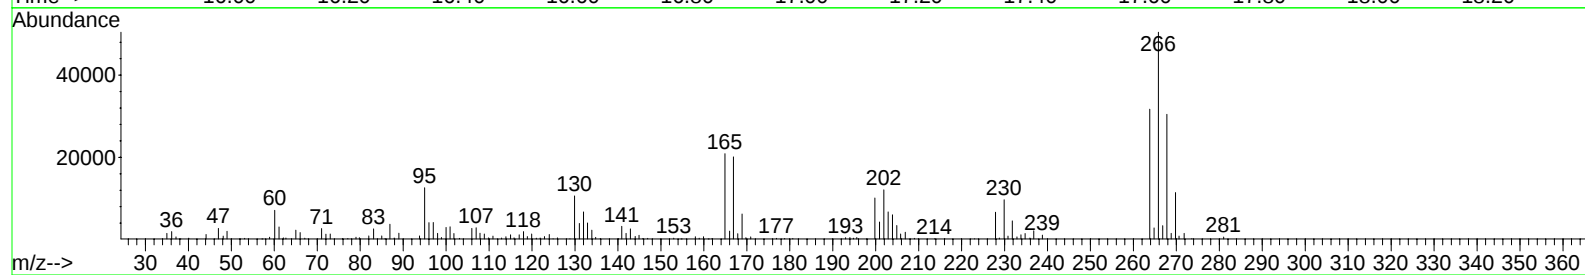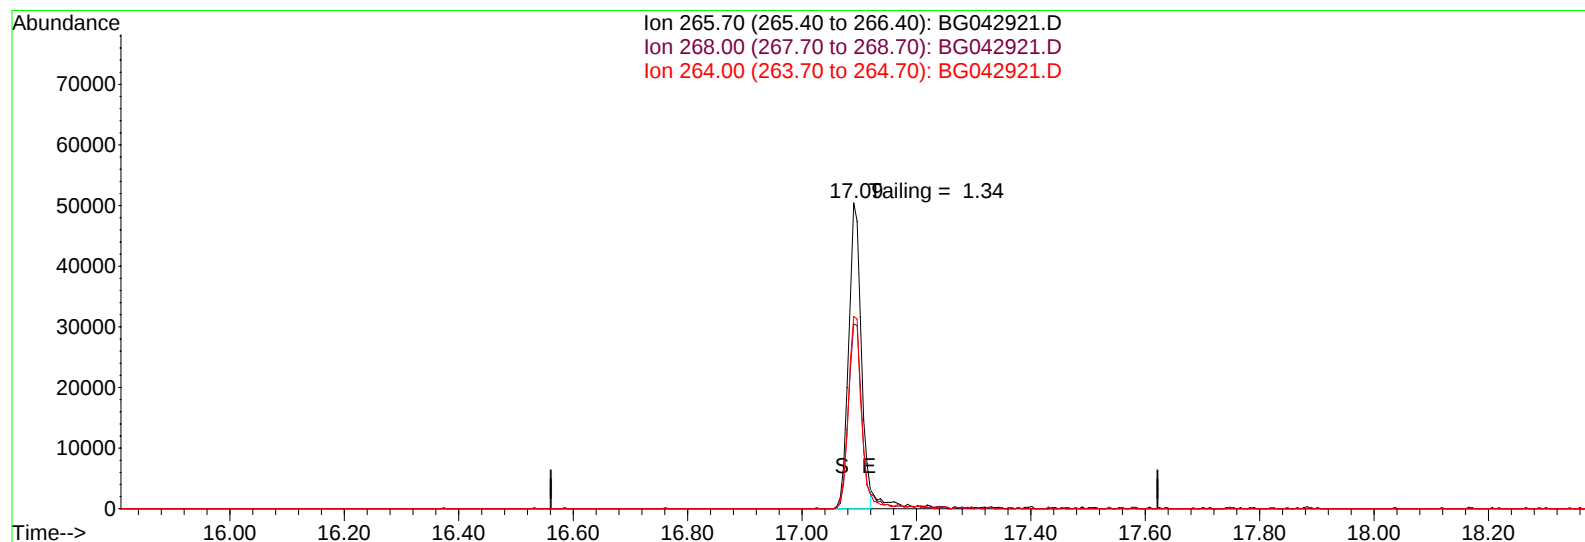

(70) Pentachlorophenol (C)

17.091min (-17.091) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	65.20	0.00#
264.00	63.40	0.00#
0.00	0.00	0.00