


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092519\
 Data File : BG042921.D
 Acq On : 25 Sep 2019 10:14
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 25 15:35:52 2019

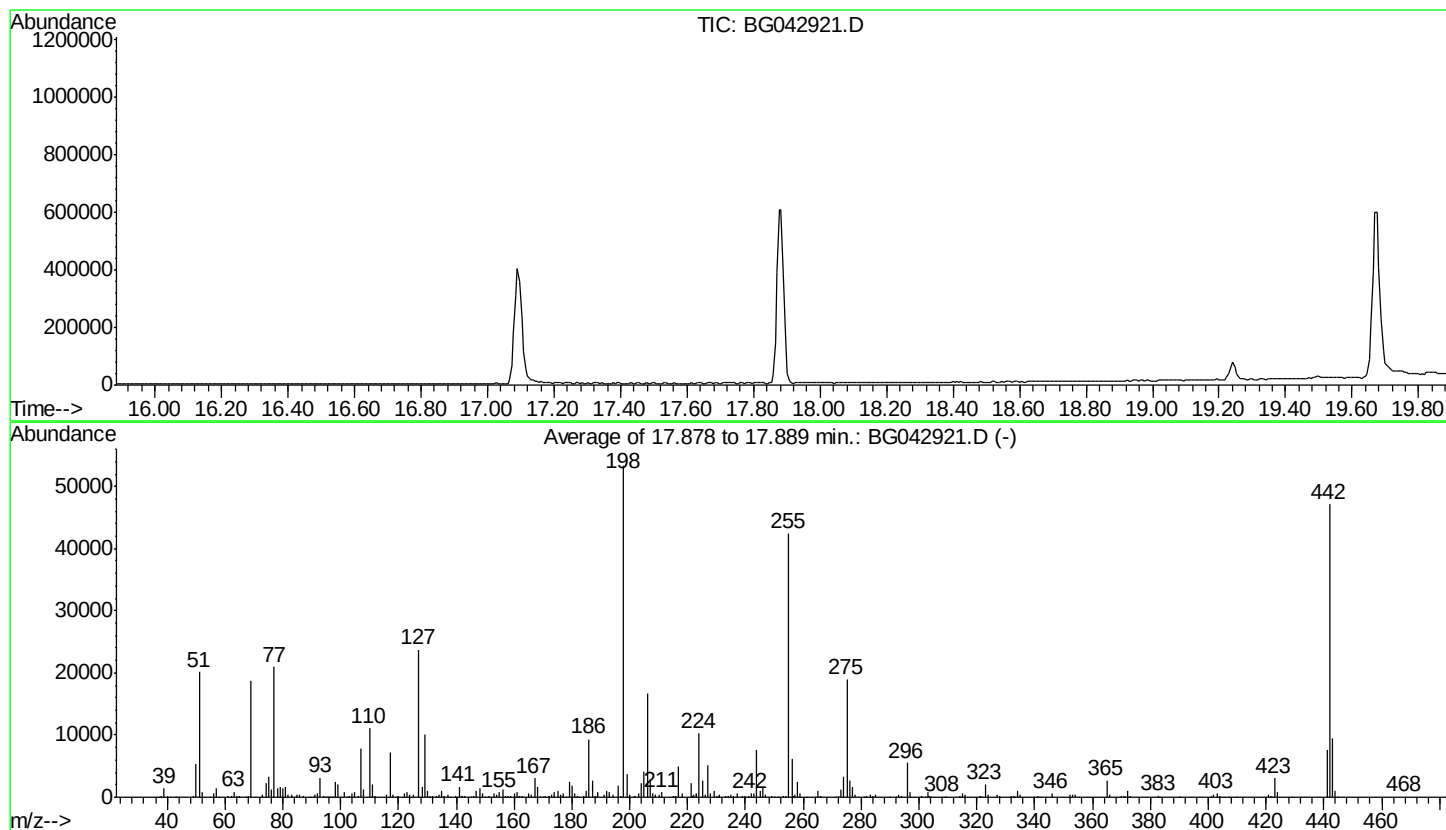

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	20146	PASS
68	69	0.00	2	0.7	136	PASS
69	198	0.00	100	35.3	18813	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.5	23717	PASS
197	198	0.00	2	0.2	122	PASS
198	198	100	100	100.0	53344	PASS
199	198	5	9	7.0	3730	PASS
275	198	10	60	35.4	18901	PASS
365	198	1	100	5.0	2673	PASS
441	198	0.01	100	14.1	7531	PASS
442	198	50	100	88.3	47109	PASS
443	442	15	24	20.0	9415	PASS