

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092521\
 Data File : BG050265.D
 Acq On : 25 Sep 2021 15:56
 Operator : CG/JU
 Sample : SST01036
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST010434

Quant Time: Sep 27 02:04:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 27 01:56:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.296	152	34186	20.000	ng/ul	0.00
20) Naphthalene-d8	11.122	136	134722	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.912	164	96960	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.655	188	225625	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.962	240	198175	20.000	ng/ul	0.00
88) Perylene-d12	25.405	264	202932	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.666	96	2913	4.394	ng/uL	0.01
4) Pyridine-d5	4.101	84	19237	9.634	ng/ul	0.00
7) Phenol-d5	7.426	99	24776	8.535	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.608	67	15455	9.583	ng/ul	0.00
11) 2-Chlorophenol-d4	7.820	132	19402	8.932	ng/ul	0.00
15) 4-Methylphenol-d8	8.983	113	20243	8.854	ng/ul	0.00
21) Nitrobenzene-d5	9.465	128	7541	7.220	ng/ul	0.00
24) 2-Nitrophenol-d4	10.188	143	8265	6.646	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.728	165	20726	9.343	ng/ul	0.00
31) 4-Chloroaniline-d4	11.245	131	27510	9.111	ng/ul	0.00
46) Dimethylphthalate-d6	14.306	166	63874	8.608	ng/ul	0.00
49) Acenaphthylene-d8	14.606	160	81164	9.329	ng/ul	0.00
54) 4-Nitrophenol-d4	15.070	143	8908	8.297	ng/ul	0.00
60) Fluorene-d10	15.899	176	59214	9.412	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.999	200	7121	4.906	ng/ul	0.00
73) Anthracene-d10	17.655	188	225625	22.269	ng/ul	-0.09
81) Pyrene-d10	20.023	212	106592	9.953	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.170	264	99132	9.208	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.701	88	3785	4.683	ng/uL#	82
5) Pyridine	4.124	79	21517	9.970	ng/ul	94
6) Benzaldehyde	7.426	77	18849	11.283	ng/ul	94
8) Phenol	7.456	94	27193	9.274	ng/ul	96
10) Bis(2-Chloroethyl)ether	7.702	93	19864	9.814	ng/ul	99
12) 2-Chlorophenol	7.855	128	20589	9.592	ng/ul#	91
13) 2-Methylphenol	8.719	108	20051	8.864	ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.819	45	26729	12.593	ng/ul#	90
16) Acetophenone	9.124	105	33083	8.873	ng/ul	97
17) N-Nitroso-di-n-propyla...	9.101	70	18301	9.775	ng/ul#	92
18) 4-Methylphenol	9.048	108	20472	8.412	ng/ul#	70
19) Hexachloroethane	9.389	117	8853	9.425	ng/ul	91
22) Nitrobenzene	9.506	77	21579	7.625	ng/ul	95
23) Isophorone	10.041	82	49121	9.741	ng/ul#	92
25) 2-Nitrophenol	10.223	139	8604	7.116	ng/ul#	78
26) 2,4-Dimethylphenol	10.264	107	26085	9.707	ng/ul	93
27) Bis(2-Chloroethoxy)met...	10.511	93	27520	10.569	ng/ul	95
29) 2,4-Dichlorophenol	10.758	162	20129	9.887	ng/ul	93
30) Naphthalene	11.169	128	68100	10.113	ng/ul	96
32) 4-Chloroaniline	11.269	127	28594	9.834	ng/ul#	86
33) Hexachlorobutadiene	11.451	225	16952	10.292	ng/ul	95
34) Caprolactam	12.062	113	5627	7.890	ng/ul	89
35) 4-Chloro-3-methylphenol	12.362	107	20956	8.612	ng/ul#	94
36) 2-Methylnaphthalene	12.755	142	47269	9.443	ng/ul	97


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092521\
 Data File : BG050265.D
 Acq On : 25 Sep 2021 15:56
 Operator : CG/JU
 Sample : SST01036
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST010434

Quant Time: Sep 27 02:04:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 27 01:56:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.973	142	46839	9.270	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	13.114	216	30880	10.843	ng/ul	96
40) Hexachlorocyclopentadiene	13.096	237	18806	14.755	ng/ul	86
41) 2,4,6-Trichlorophenol	13.349	196	17239	9.499	ng/ul	91
42) 2,4,5-Trichlorophenol	13.413	196	19045	10.013	ng/ul	97
43) 1,1'-Biphenyl	13.748	154	65907	9.729	ng/ul#	97
44) 2-Chloronaphthalene	13.795	162	52920	9.726	ng/ul	96
45) 2-Nitroaniline	13.989	65	10210	5.527	ng/ul	88
47) Dimethylphthalate	14.353	163	66026	8.991	ng/ul	98
48) 2,6-Dinitrotoluene	14.471	165	9241	6.095	ng/ul#	83
50) Acenaphthylene	14.635	152	84057	10.571	ng/ul	99
51) 3-Nitroaniline	14.806	138	10328	7.059	ng/ul#	90
52) Acenaphthene	14.970	153	53312	9.242	ng/ul	96
53) 2,4-Dinitrophenol	15.006	184	4635	5.985	ng/ul#	72
55) 4-Nitrophenol	15.082	109	8982	6.599	ng/ul#	69
56) Dibenzofuran	15.305	168	83804	10.491	ng/ul	90
57) 2,4-Dinitrotoluene	15.252	165	12925	5.926	ng/ul#	85
58) 2,3,4,6-Tetrachlorophenol	15.523	232	16320	10.354	ng/ul#	85
59) Diethylphthalate	15.711	149	66969	8.914	ng/ul#	94
61) Fluorene	15.952	166	64010	9.498	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.940	204	35505	9.957	ng/ul	89
63) 4-Nitroaniline	15.957	138	11538	7.903	ng/ul#	66
66) 4,6-Dinitro-2-methylph...	16.010	198	6895	5.241	ng/ul#	93
67) N-Nitrosodiphenylamine	16.151	169	57757	9.723	ng/ul	99
68) 4-Bromophenyl-phenylether	16.839	248	23855	9.558	ng/ul	93
69) Hexachlorobenzene	16.950	284	26139	9.069	ng/ul#	92
70) Atrazine	17.091	200	24802	9.398	ng/ul	94
71) Pentachlorophenol	17.297	266	14007	11.477	ng/ul	88
72) Phenanthrene	17.697	178	112676	10.017	ng/ul	97
74) Anthracene	17.785	178	114955	10.085	ng/ul	96
75) 1,2,3,4-Tetrachloroben...	13.719	216	32105	10.606	ng/ul#	85
76) Pentachlorobenzene	15.217	250	30841	9.615	ng/ul	98
77) Carbazole	18.049	167	99716	9.831	ng/ul	96
78) Di-n-butylphthalate	18.596	149	112734	8.691	ng/ul	99
80) Fluoranthene	19.694	202	137709	10.421	ng/ul#	94
82) Pyrene	20.053	202	137437	10.495	ng/ul#	94
83) Butylbenzylphthalate	20.934	149	42497	8.224	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.845	252	43347	9.227	ng/ul	95
85) Benzo(a)anthracene	21.939	228	116635	9.445	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.833	149	58925	8.303	ng/ul	96
87) Chrysene	22.009	228	114560	9.814	ng/ul	99
89) Di-n-octyl phthalate	23.131	149	97133	8.069	ng/ul	100
90) Benzo(b)fluoranthene	24.307	252	114615	8.830	ng/ul#	96
91) Benzo(k)fluoranthene	24.377	252	108848	8.822	ng/ul#	97
93) Benzo(a)pyrene	25.241	252	108287	9.606	ng/ul#	98
94) Indeno(1,2,3-cd)pyrene	29.354	276	49961	3.360	ng/ul#	91
95) Dibenzo(a,h)anthracene	29.436	278	50232	4.035	ng/ul#	96
96) Benzo(g,h,i)perylene	30.599	276	106566	8.524	ng/ul	97





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 4.683 ng/uL
RT: 3.701 min Scan# 113
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion: 88 Resp: 3785
Ion Ratio Lower Upper
88 100
43 28.9 21.6 32.4
58 46.5 52.0 78.0#



#5
Pyridine
Concen: 9.970 ng/uL
RT: 4.124 min Scan# 185
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion: 79 Resp: 21517
Ion Ratio Lower Upper
79 100
52 71.1 61.1 91.7
51 39.3 34.8 52.2









#6
Benzaldehyde
Concen: 11.283 ng/ul
RT: 7.426 min Scan# 747
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion: 77 Resp: 18849
Ion Ratio Lower Upper
77 100
105 94.7 72.3 108.5
106 83.7 72.3 108.5

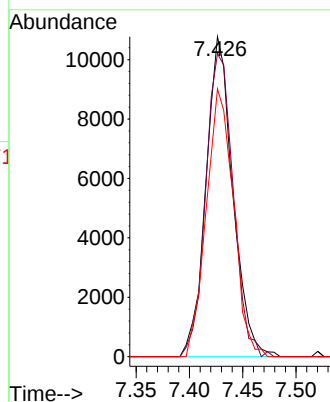

#8
Phenol
Concen: 9.274 ng/ul
RT: 7.456 min Scan# 752
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion: 94 Resp: 27193
Ion Ratio Lower Upper
94 100
65 32.9 27.7 41.5
66 45.9 39.0 58.4



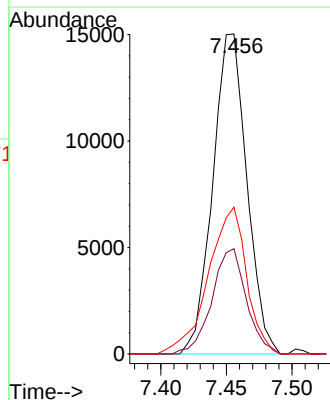





#10
Bis(2-Chloroethyl)ether
Concen: 9.814 ng/ul
RT: 7.702 min Scan# 794
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion: 93 Resp: 19864
Ion Ratio Lower Upper
93 100
63 75.0 59.9 89.9
95 32.0 27.6 41.4

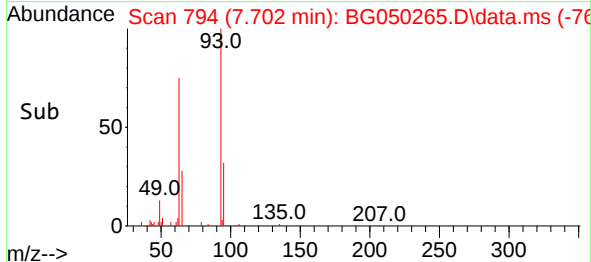

#12
2-Chlorophenol
Concen: 9.592 ng/ul
RT: 7.855 min Scan# 820
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:128 Resp: 20589
Ion Ratio Lower Upper
128 100
64 44.3 28.0 42.0#
130 29.7 24.4 36.6









#13
2-Methylphenol
Concen: 8.864 ng/ul
RT: 8.719 min Scan# 967
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:108 Resp: 20051
Ion Ratio Lower Upper
108 100
107 91.2 71.0 106.4



#14
2,2'-oxybis(1-Chloropropane)
Concen: 12.593 ng/ul
RT: 8.819 min Scan# 984
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion: 45 Resp: 26729
Ion Ratio Lower Upper
45 100
77 15.0 16.9 25.3#
79 11.1 11.0 16.4







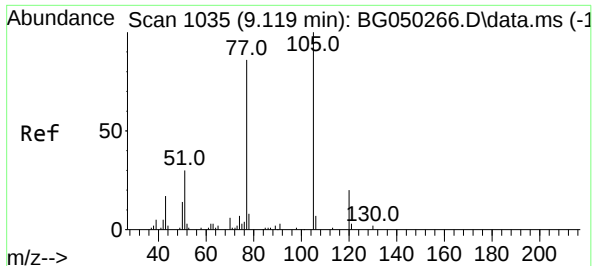

#16
Acetophenone
Concen: 8.873 ng/ul
RT: 9.124 min Scan# 1036
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:105 Resp: 33083
Ion Ratio Lower Upper
105 100
77 88.5 67.7 101.5
51 32.1 25.3 37.9

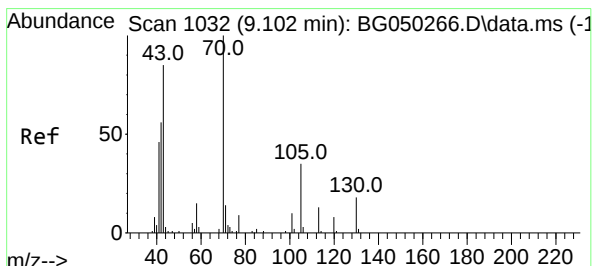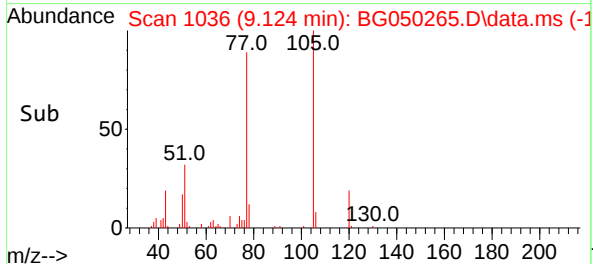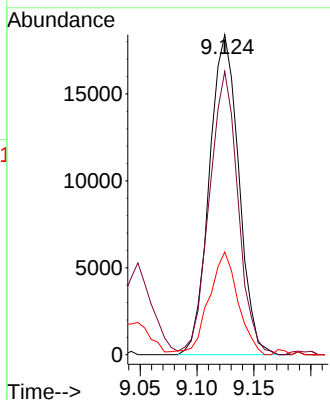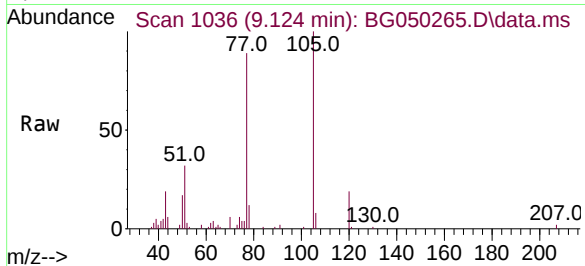

#17
N-Nitroso-di-n-propylamine
Concen: 9.775 ng/ul
RT: 9.101 min Scan# 1032
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion: 70 Resp: 18301
Ion Ratio Lower Upper
70 100
42 61.4 44.2 66.4
101 11.5 7.8 11.8
130 23.1 15.3 22.9#


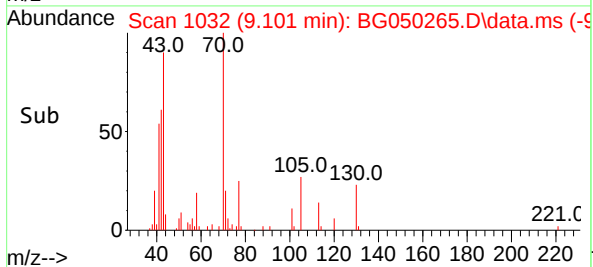
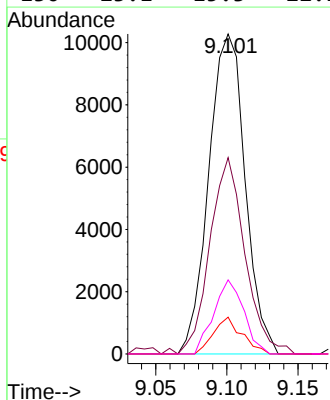
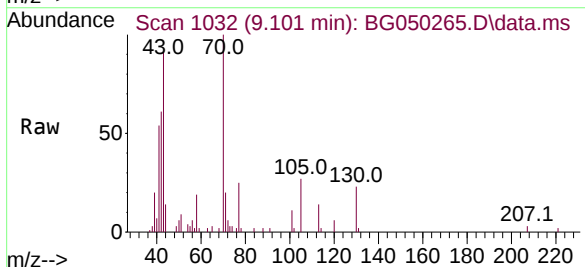




#18
4-Methylphenol
Concen: 8.412 ng/ul
RT: 9.048 min Scan# 1023
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:108 Resp: 20472
Ion Ratio Lower Upper
108 100
107 128.0 78.3 117.5#



#19
Hexachloroethane
Concen: 9.425 ng/ul
RT: 9.389 min Scan# 1081
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:117 Resp: 8853
Ion Ratio Lower Upper
117 100
201 123.7 89.3 133.9
199 65.9 50.5 75.7









#22
Nitrobenzene
Concen: 7.625 ng/ul
RT: 9.506 min Scan# 1101
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion: 77 Resp: 21579
Ion Ratio Lower Upper
77 100
123 42.0 30.4 45.6
65 14.5 11.3 16.9



#23
Isophorone
Concen: 9.741 ng/ul
RT: 10.041 min Scan# 1192
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion: 82 Resp: 49121
Ion Ratio Lower Upper
82 100
95 8.1 7.8 11.8
138 18.4 11.4 17.0#









#25
2-Nitrophenol
Concen: 7.116 ng/ul
RT: 10.223 min Scan# 1223
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion	Ratio	Lower	Upper
139	100		
65	54.1	53.1	79.7
109	32.8	44.1	66.1#



#26
2,4-Dimethylphenol
Concen: 9.707 ng/ul
RT: 10.264 min Scan# 1230
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion	Ratio	Lower	Upper
107	100		
121	42.8	32.7	49.1
122	73.5	52.6	79.0









#27
 Bis(2-Chloroethoxy)methane
 Concen: 10.569 ng/ul
 RT: 10.511 min Scan# 1272
 Delta R.T. -0.001 min
 Lab File: BG050265.D
 Acq: 25 Sep 2021 15:56




Instrument :
 BNA_G
 ClientSampleId :
 SST010434


Tgt Ion:	93	Resp:	27520
Ion	Ratio	Lower	Upper
93	100		
95	28.1	24.8	37.2
123	9.2	8.2	12.2

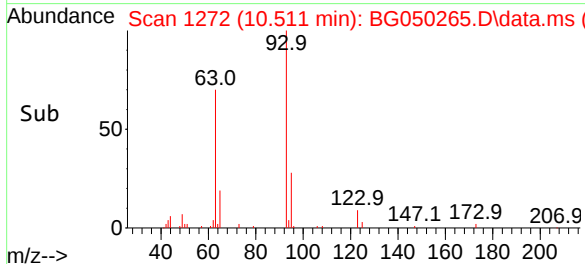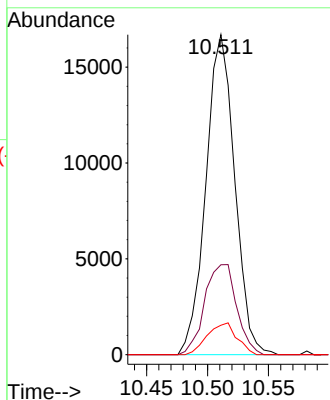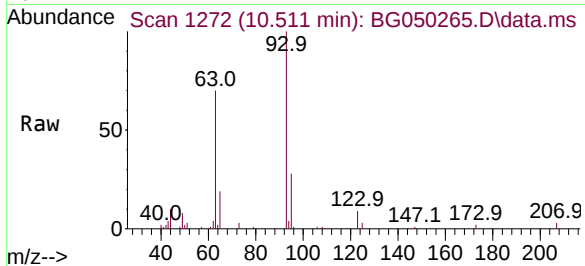

#29
 2,4-Dichlorophenol
 Concen: 9.887 ng/ul
 RT: 10.758 min Scan# 1314
 Delta R.T. 0.005 min
 Lab File: BG050265.D
 Acq: 25 Sep 2021 15:56

Tgt Ion:	162	Resp:	20129
Ion	Ratio	Lower	Upper
162	100		
164	58.8	51.0	76.6
98	30.7	27.8	41.8


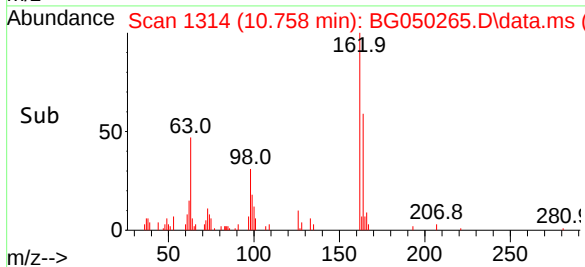
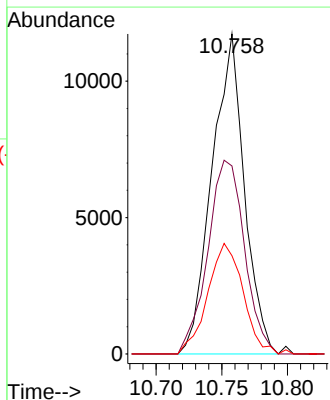
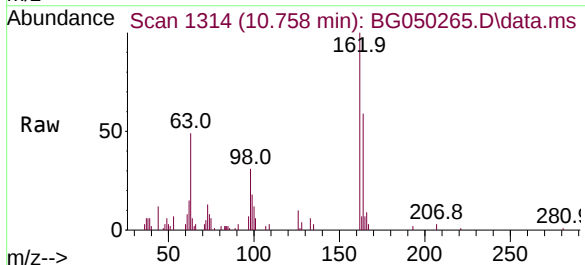




#30
Naphthalene
Concen: 10.113 ng/ul
RT: 11.169 min Scan# 1384
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion	Ratio	Lower	Upper
128	100		
129	10.1	9.3	13.9
127	13.7	9.8	14.6

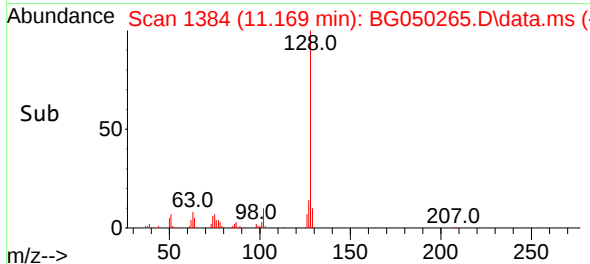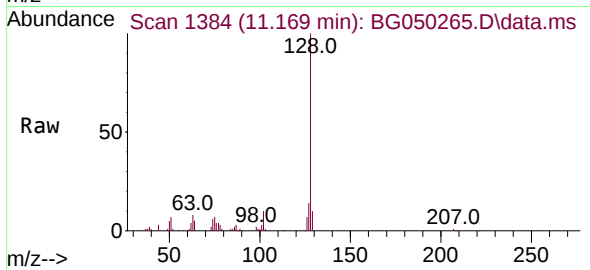

#32
4-Chloroaniline
Concen: 9.834 ng/ul
RT: 11.269 min Scan# 1401
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion	Ratio	Lower	Upper
127	100		
129	29.3	30.3	45.5#


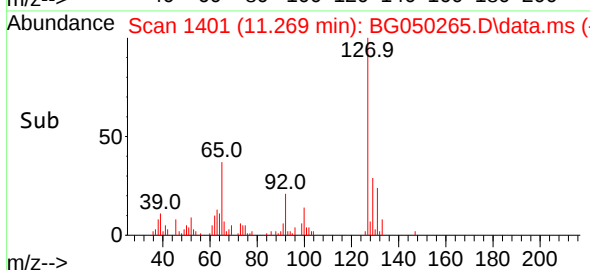

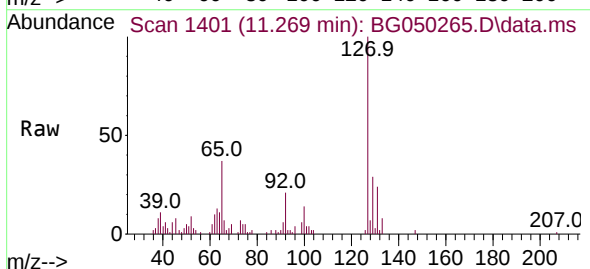




#33
Hexachlorobutadiene
Concen: 10.292 ng/ul
RT: 11.451 min Scan# 1432
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:	225	Resp:	16952
Ion Ratio	Lower	Upper	
225	100		
223	63.0	51.3	76.9
227	62.1	55.1	82.7

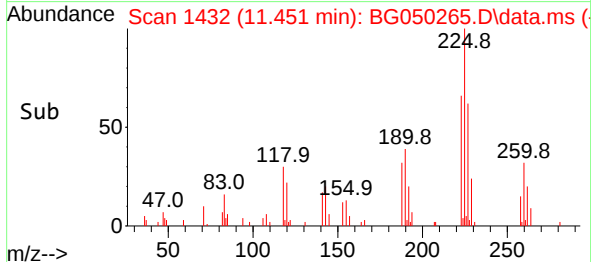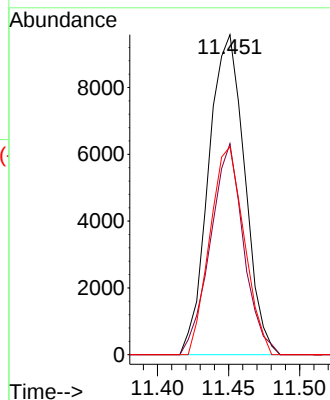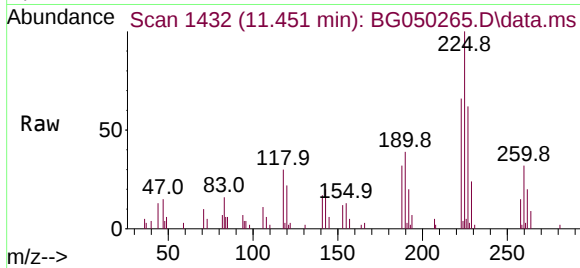

#34
Caprolactam
Concen: 7.890 ng/ul
RT: 12.062 min Scan# 1536
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:	113	Resp:	5627
Ion Ratio	Lower	Upper	
113	100		
55	143.0	114.0	171.0
56	108.4	107.4	161.0



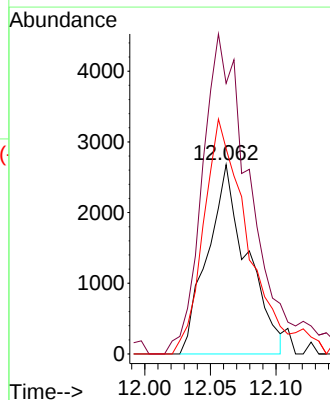
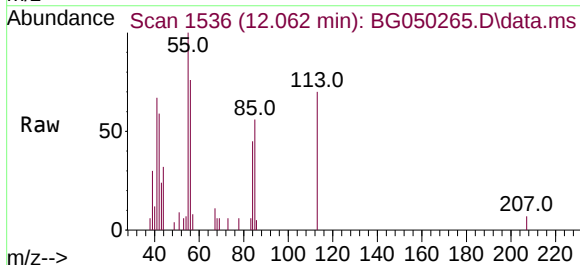




#35
4-Chloro-3-methylphenol
Concen: 8.612 ng/ul
RT: 12.362 min Scan# 1587
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:107 Resp: 20956
Ion Ratio Lower Upper
107 100
144 28.4 18.9 28.3#
142 78.4 59.2 88.8

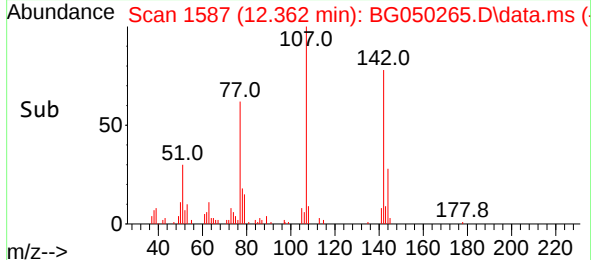

#36
2-Methylnaphthalene
Concen: 9.443 ng/ul
RT: 12.755 min Scan# 1654
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:142 Resp: 47269
Ion Ratio Lower Upper
142 100
141 85.7 70.5 105.7


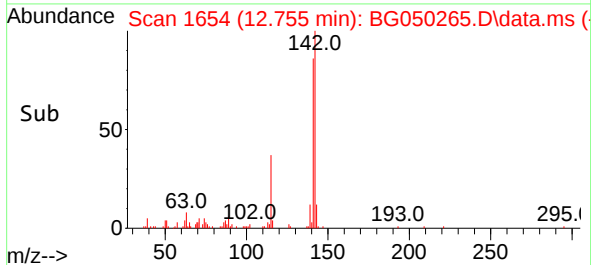




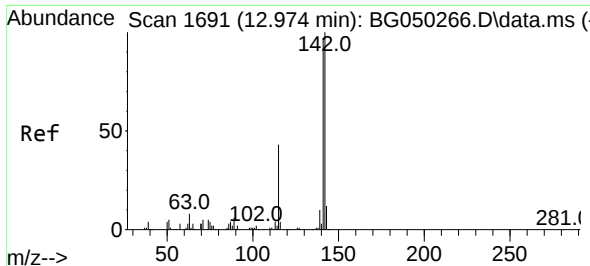

#37
1-Methylnaphthalene
Concen: 9.270 ng/ul
RT: 12.973 min Scan# 1691
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:	142	Resp:	46839
Ion Ratio	Lower	Upper	
142	100		
141	95.9	75.8	113.8
116	5.3	3.7	5.5

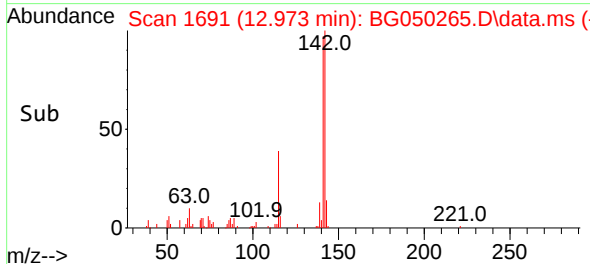

#39
1,2,4,5-Tetrachlorobenzene
Concen: 10.843 ng/ul
RT: 13.114 min Scan# 1715
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:	216	Resp:	30880
Ion Ratio	Lower	Upper	
216	100		
214	75.4	64.2	96.2
179	16.9	12.8	19.2
108	15.4	13.1	19.7


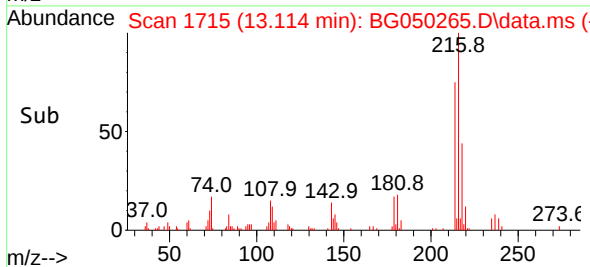

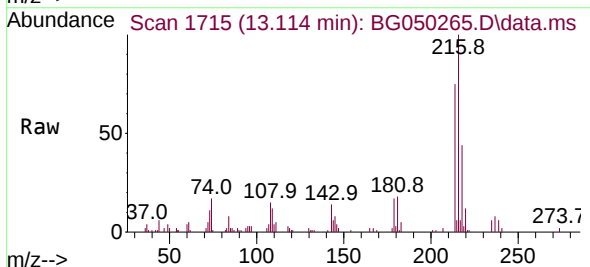




#40
Hexachlorocyclopentadiene
Concen: 14.755 ng/ul
RT: 13.096 min Scan# 1712
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:237 Resp: 18806
Ion Ratio Lower Upper
237 100
235 54.0 53.5 80.3
272 13.5 11.5 17.3

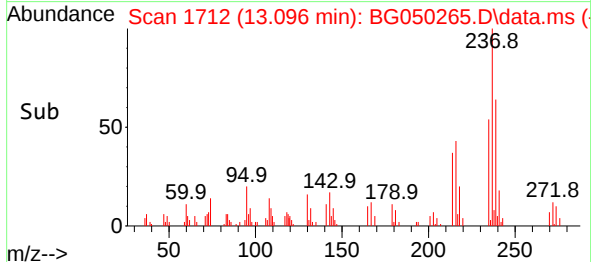

#41
2,4,6-Trichlorophenol
Concen: 9.499 ng/ul
RT: 13.349 min Scan# 1755
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:196 Resp: 17239
Ion Ratio Lower Upper
196 100
198 95.7 83.7 125.5
200 27.0 25.9 38.9









#42
2,4,5-Trichlorophenol
Concen: 10.013 ng/ul
RT: 13.413 min Scan# 1766
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:	196	Resp:	19045
Ion Ratio	Lower	Upper	
196	100		
198	87.3	70.3	105.5
200	27.6	26.6	40.0

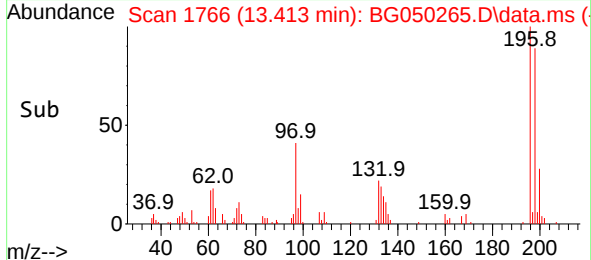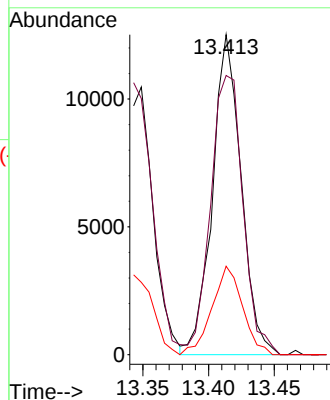

#43
1,1'-Biphenyl
Concen: 9.729 ng/ul
RT: 13.748 min Scan# 1823
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:	154	Resp:	65907
Ion Ratio	Lower	Upper	
154	100		
153	41.3	32.5	48.7
76	14.2	7.8	11.8#


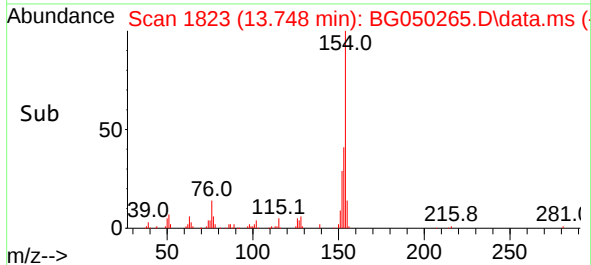
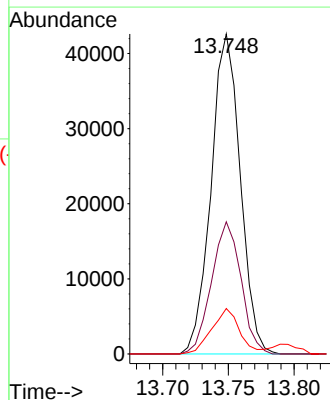



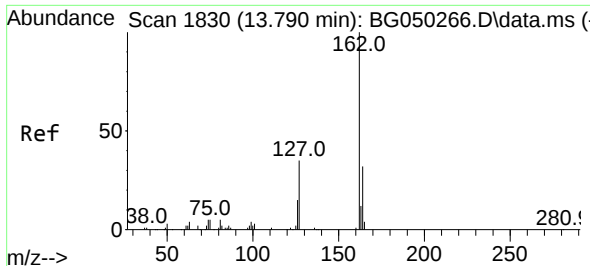

#44
2-Chloronaphthalene
Concen: 9.726 ng/ul
RT: 13.795 min Scan# 1831
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:	162	Resp:	52920
Ion Ratio	Lower	Upper	
162	100		
164	33.4	25.2	37.8
127	37.0	31.9	47.9

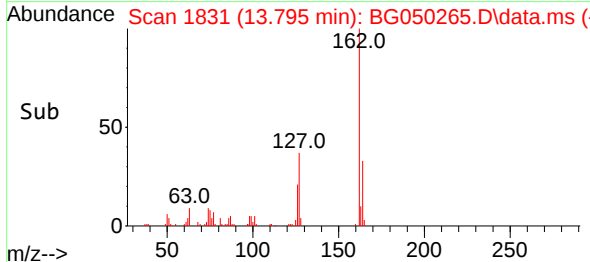

#45
2-Nitroaniline
Concen: 5.527 ng/ul
RT: 13.989 min Scan# 1864
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:	65	Resp:	10210
Ion Ratio	Lower	Upper	
65	100		
92	80.4	55.6	83.4
138	110.0	78.7	118.1


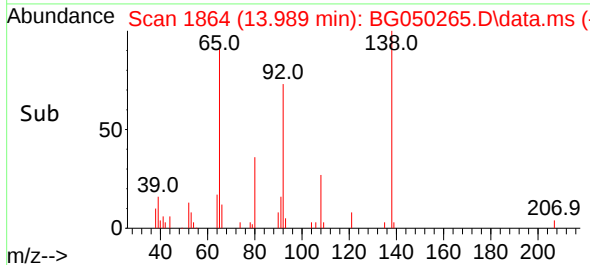

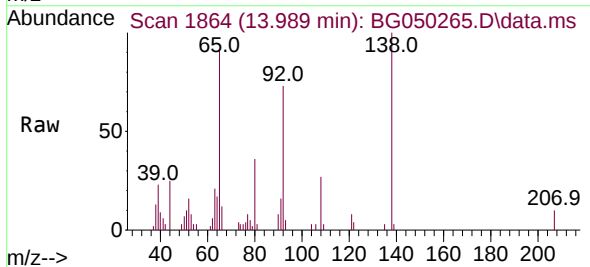




#47
Dimethylphthalate
Concen: 8.991 ng/ul
RT: 14.353 min Scan# 1926
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:163 Resp: 66026
Ion Ratio Lower Upper
163 100
194 4.9 3.4 5.0
164 11.0 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 6.095 ng/ul
RT: 14.471 min Scan# 1946
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:165 Resp: 9241
Ion Ratio Lower Upper
165 100
89 61.5 62.5 93.7#
121 21.5 22.2 33.2#




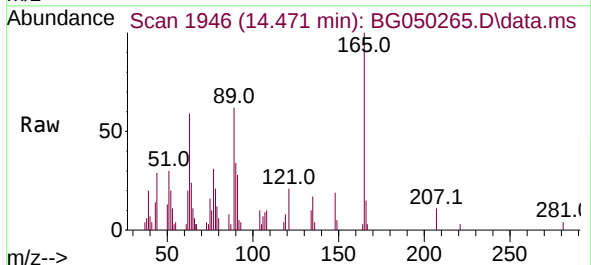




#50
Acenaphthylene
Concen: 10.571 ng/ul
RT: 14.635 min Scan# 1974
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:152 Resp: 84057
Ion Ratio Lower Upper
152 100
151 18.9 15.2 22.8
153 13.9 10.7 16.1

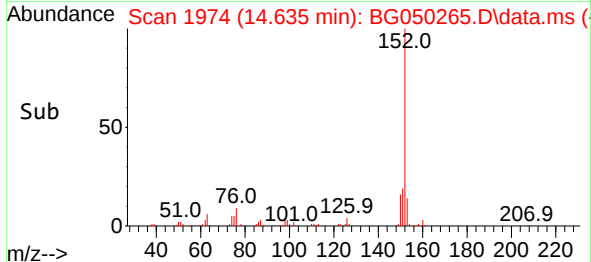

#51
3-Nitroaniline
Concen: 7.059 ng/ul
RT: 14.806 min Scan# 2003
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:138 Resp: 10328
Ion Ratio Lower Upper
138 100
108 19.4 9.0 13.4#
92 110.9 96.4 144.6




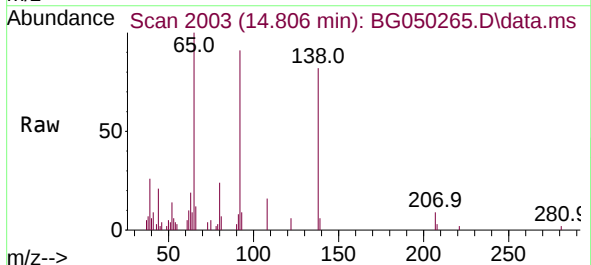




#52
Acenaphthene
Concen: 9.242 ng/ul
RT: 14.970 min Scan# 2031
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:153 Resp: 53312
Ion Ratio Lower Upper
153 100
152 47.9 37.4 56.2
154 84.0 71.5 107.3



#53
2,4-Dinitrophenol
Concen: 5.985 ng/ul
RT: 15.006 min Scan# 2037
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:184 Resp: 4635
Ion Ratio Lower Upper
184 100
63 60.0 75.8 113.8#
154 64.3 64.6 96.8#




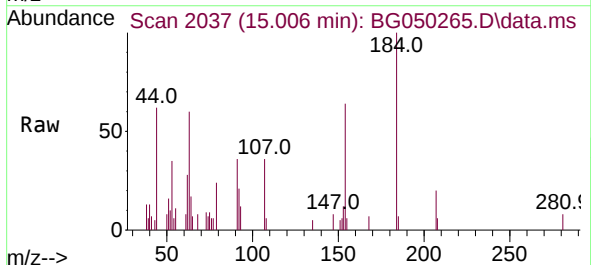


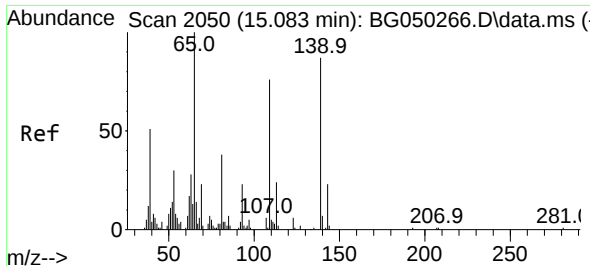

#55
4-Nitrophenol
Concen: 6.599 ng/ul
RT: 15.082 min Scan# 2050
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:109 Resp: 8982
Ion Ratio Lower Upper
109 100
139 114.4 61.4 92.0#
65 116.7 76.5 114.7#

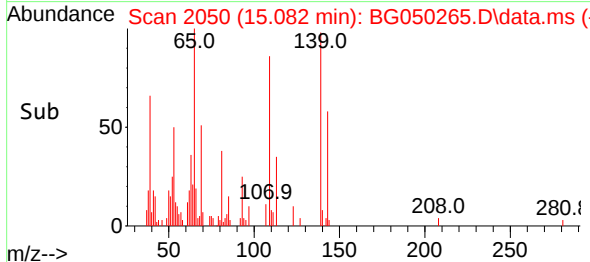

#56
Dibenzofuran
Concen: 10.491 ng/ul
RT: 15.305 min Scan# 2088
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:168 Resp: 83804
Ion Ratio Lower Upper
168 100
139 35.9 33.8 50.8


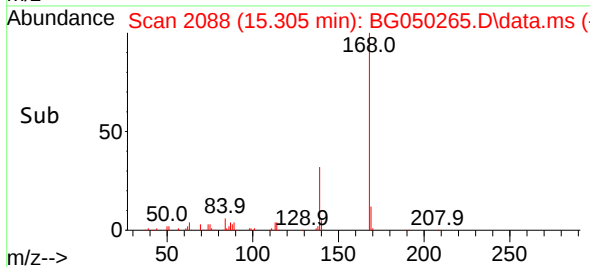

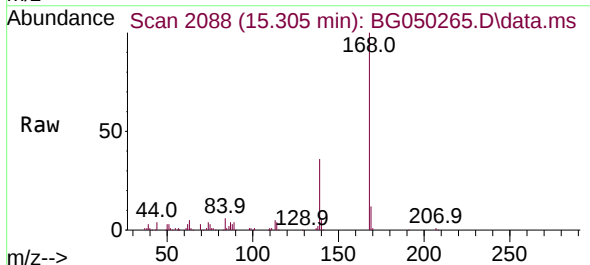




#57
2,4-Dinitrotoluene
Concen: 5.926 ng/ul
RT: 15.252 min Scan# 2079
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:165 Resp: 12925
Ion Ratio Lower Upper
165 100
63 41.8 42.3 63.5#
182 2.8 2.6 4.0

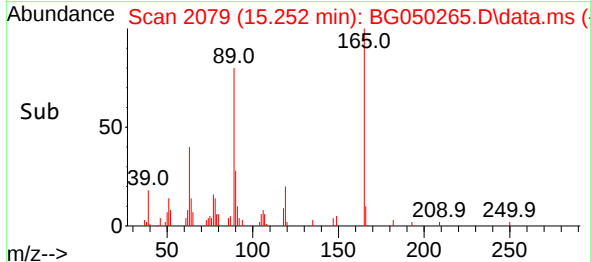

#58
2,3,4,6-Tetrachlorophenol
Concen: 10.354 ng/ul
RT: 15.523 min Scan# 2125
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:232 Resp: 16320
Ion Ratio Lower Upper
232 100
131 40.4 40.0 60.0
130 5.3 1.8 2.8#
166 21.5 24.8 37.2#


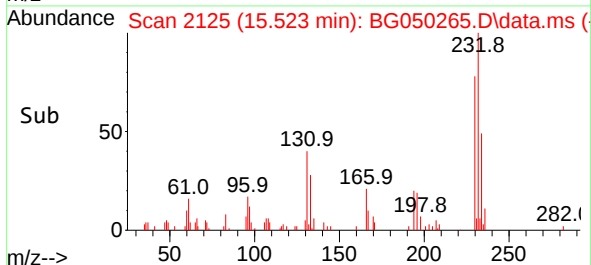
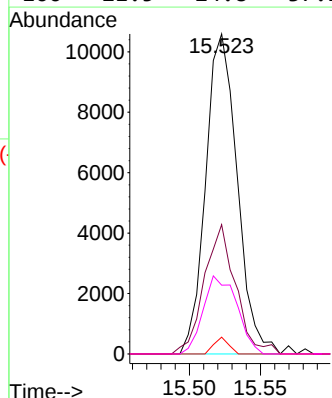
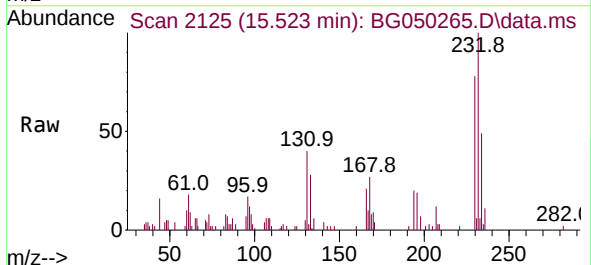




#59
Diethylphthalate
Concen: 8.914 ng/ul
RT: 15.711 min Scan# 2157
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:149 Resp: 66969
Ion Ratio Lower Upper
149 100
177 23.9 15.8 23.6#
150 12.0 9.7 14.5



#61
Fluorene
Concen: 9.498 ng/ul
RT: 15.952 min Scan# 2198
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:166 Resp: 64010
Ion Ratio Lower Upper
166 100
165 104.5 83.3 124.9
167 13.8 11.8 17.6









#62
4-Chlorophenyl-phenylether
Concen: 9.957 ng/ul
RT: 15.940 min Scan# 2196
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:204 Resp: 35505
Ion Ratio Lower Upper
204 100
206 31.2 25.4 38.2
141 52.5 51.8 77.6



#63
4-Nitroaniline
Concen: 7.903 ng/ul
RT: 15.957 min Scan# 2199
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:138 Resp: 11538
Ion Ratio Lower Upper
138 100
92 39.1 50.0 75.0#
108 86.3 101.8 152.8#









#66
 4,6-Dinitro-2-methylphenol
 Concen: 5.241 ng/ul
 RT: 16.010 min Scan# 2208
 Delta R.T. -0.001 min
 Lab File: BG050265.D
 Acq: 25 Sep 2021 15:56




Instrument :
 BNA_G
 ClientSampleId :
 SSTD010434


Tgt Ion:198 Resp: 6895
 Ion Ratio Lower Upper
 198 100
 182 0.0 3.0 4.6#
 77 26.0 23.4 35.2



#67
 N-Nitrosodiphenylamine
 Concen: 9.723 ng/ul
 RT: 16.151 min Scan# 2232
 Delta R.T. 0.005 min
 Lab File: BG050265.D
 Acq: 25 Sep 2021 15:56


Tgt Ion:169 Resp: 57757
 Ion Ratio Lower Upper
 169 100
 168 67.8 55.0 82.6
 167 35.4 29.0 43.4





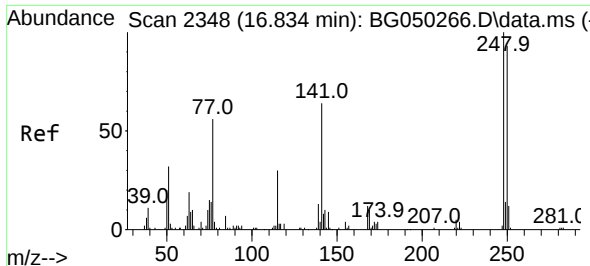


#68
4-Bromophenyl-phenylether
Concen: 9.558 ng/ul
RT: 16.839 min Scan# 2349
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56


Instrument :
BNA_G
ClientSampleId :
SSTD010434





Tgt Ion:248 Resp: 23855
Ion Ratio Lower Upper
248 100
250 98.1 80.2 120.2
141 64.1 60.6 90.8

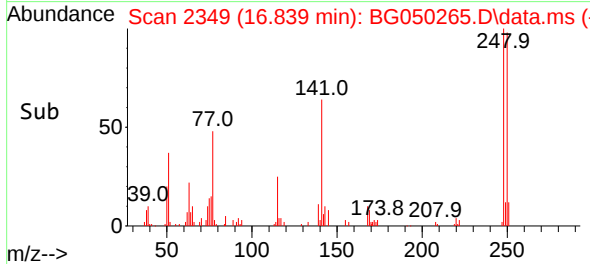


#69
Hexachlorobenzene
Concen: 9.069 ng/ul
RT: 16.950 min Scan# 2368
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

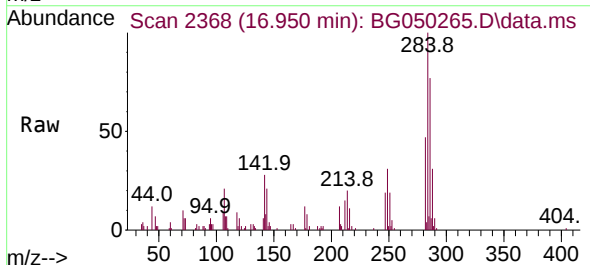

Tgt Ion:284 Resp: 26139
Ion Ratio Lower Upper
284 100
142 27.6 28.7 43.1#
249 30.8 25.5 38.3




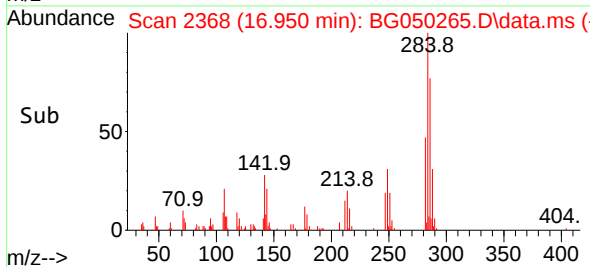




#70
Atrazine
Concen: 9.398 ng/ul
RT: 17.091 min Scan# 2392
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:200 Resp: 24802
Ion Ratio Lower Upper
200 100
173 21.2 19.3 28.9
215 47.7 34.9 52.3



#71
Pentachlorophenol
Concen: 11.477 ng/ul
RT: 17.297 min Scan# 2427
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:266 Resp: 14007
Ion Ratio Lower Upper
266 100
264 57.8 54.1 81.1
268 57.0 52.6 78.8







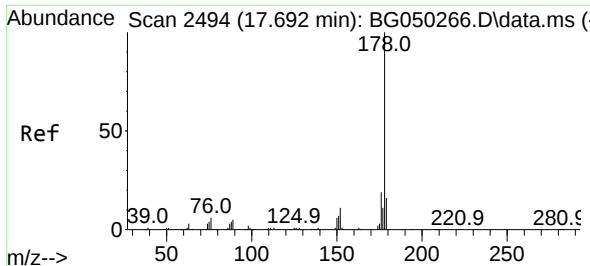

#72
Phenanthrene
Concen: 10.017 ng/ul
RT: 17.697 min Scan# 2495
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:178 Resp: 112676
Ion Ratio Lower Upper
178 100
179 14.8 11.7 17.5
176 18.3 16.2 24.2

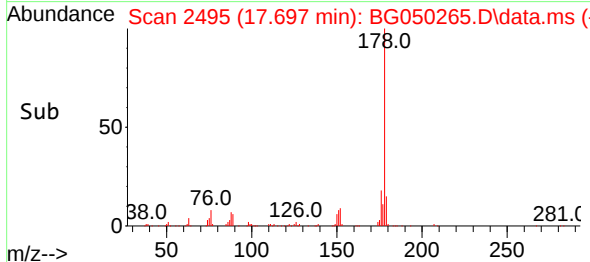

#74
Anthracene
Concen: 10.085 ng/ul
RT: 17.785 min Scan# 2510
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:178 Resp: 114955
Ion Ratio Lower Upper
178 100
179 14.5 11.4 17.0
176 18.6 12.8 19.2


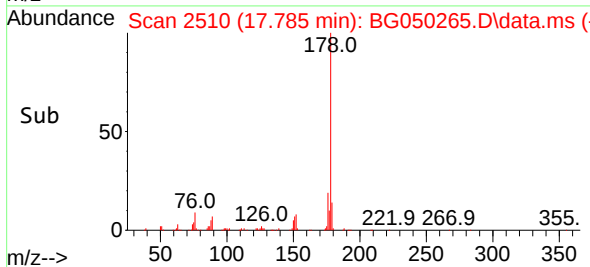

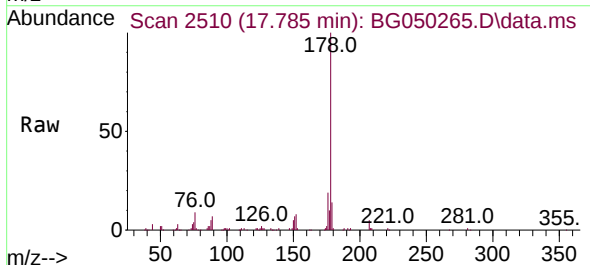




#75
1,2,3,4-Tetrachlorobenzene
Concen: 10.606 ng/uL
RT: 13.719 min Scan# 1818
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:216 Resp: 32105
Ion Ratio Lower Upper
216 100
214 74.9 70.9 106.3
218 40.7 40.9 61.3#

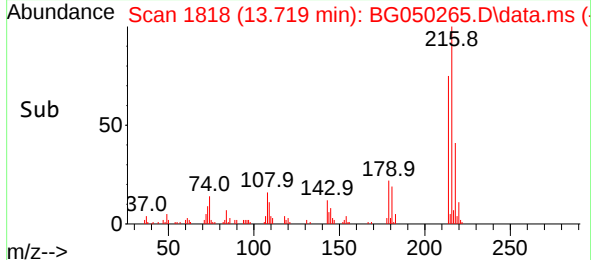

#76
Pentachlorobenzene
Concen: 9.615 ng/uL
RT: 15.217 min Scan# 2073
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:250 Resp: 30841
Ion Ratio Lower Upper
250 100
248 64.1 51.5 77.3
252 63.0 47.9 71.9


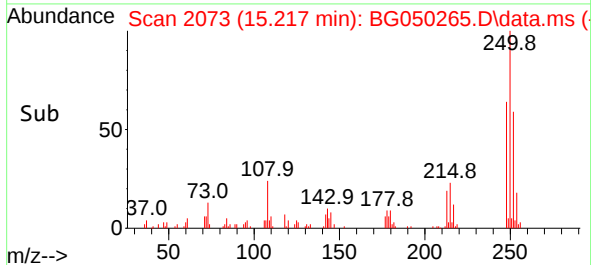






#77
 Carbazole
 Concen: 9.831 ng/ul
 RT: 18.049 min Scan# 2555
 Delta R.T. -0.001 min
 Lab File: BG050265.D
 Acq: 25 Sep 2021 15:56




Instrument :
 BNA_G
 ClientSampleId :
 SST010434


Tgt Ion:167 Resp: 99716
 Ion Ratio Lower Upper
 167 100
 166 20.3 17.8 26.8
 139 12.8 11.1 16.7



#78
 Di-n-butylphthalate
 Concen: 8.691 ng/ul
 RT: 18.596 min Scan# 2648
 Delta R.T. -0.001 min
 Lab File: BG050265.D
 Acq: 25 Sep 2021 15:56

Tgt Ion:149 Resp: 112734
 Ion Ratio Lower Upper
 149 100
 150 9.8 8.1 12.1
 104 6.5 5.3 7.9









#80
Fluoranthene
Concen: 10.421 ng/ul
RT: 19.694 min Scan# 2835
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:202 Resp: 137709
Ion Ratio Lower Upper
202 100
101 7.5 4.3 6.5#
100 6.6 3.5 5.3#



#82
Pyrene
Concen: 10.495 ng/ul
RT: 20.053 min Scan# 2896
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:202 Resp: 137437
Ion Ratio Lower Upper
202 100
101 9.1 5.4 8.0#
100 7.8 5.0 7.6#









#83
Butylbenzylphthalate
Concen: 8.224 ng/ul
RT: 20.934 min Scan# 3046
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:	149	Resp:	42497
Ion Ratio	Lower	Upper	
149	100		
91	73.5	60.6	90.8
206	25.2	16.8	25.2



#84
3,3'-Dichlorobenzidine
Concen: 9.227 ng/ul
RT: 21.845 min Scan# 3201
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:	252	Resp:	43347
Ion Ratio	Lower	Upper	
252	100		
254	63.6	54.2	81.2
126	6.9	5.4	8.0



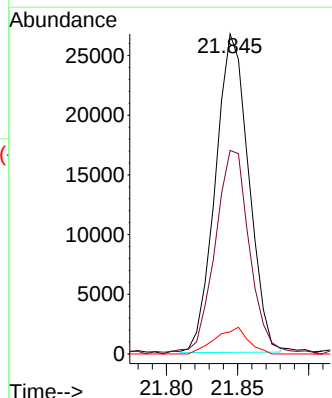





#85
Benzo(a)anthracene
Concen: 9.445 ng/ul
RT: 21.939 min Scan# 3217
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:	228	Resp:	116635
Ion Ratio	Lower	Upper	
228	100		
229	19.1	16.2	24.4
226	28.0	21.0	31.4



#86
Bis(2-ethylhexyl)phthalate
Concen: 8.303 ng/ul
RT: 21.833 min Scan# 3199
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:	149	Resp:	58925
Ion Ratio	Lower	Upper	
149	100		
167	27.7	20.4	30.6
279	5.3	3.7	5.5









#87
Chrysene
Concen: 9.814 ng/ul
RT: 22.009 min Scan# 3229
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:	228	Resp:	114560
Ion Ratio	Lower	Upper	
228	100		
226	29.3	23.0	34.4
229	21.5	17.8	26.6



#89
Di-n-octyl phthalate
Concen: 8.069 ng/ul
RT: 23.131 min Scan# 3420
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:149 Resp: 97133









#90
Benzo(b)fluoranthene
Concen: 8.830 ng/ul
RT: 24.307 min Scan# 3620
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:252 Resp: 114615
Ion Ratio Lower Upper
252 100
253 21.2 18.1 27.1
125 7.4 3.4 5.0#



#91
Benzo(k)fluoranthene
Concen: 8.822 ng/ul
RT: 24.377 min Scan# 3632
Delta R.T. 0.005 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:252 Resp: 108848
Ion Ratio Lower Upper
252 100
253 23.7 17.7 26.5
125 6.4 4.1 6.1#









#93
Benzo(a)pyrene
Concen: 9.606 ng/ul
RT: 25.241 min Scan# 3779
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56




Instrument :
BNA_G
ClientSampleId :
SSTD010434


Tgt Ion:252 Resp: 108287
Ion Ratio Lower Upper
252 100
253 21.9 17.0 25.4
125 6.9 4.4 6.6#



#94
Indeno(1,2,3-cd)pyrene
Concen: 3.360 ng/ul
RT: 29.354 min Scan# 4479
Delta R.T. -0.001 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:276 Resp: 49961
Ion Ratio Lower Upper
276 100
138 9.4 5.5 8.3#
277 28.0 18.6 27.8#









#95
Dibenzo(a,h)anthracene
Concen: 4.035 ng/ul
RT: 29.436 min Scan# 4493
Delta R.T. -0.007 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Instrument :
BNA_G
ClientSampleId :
SSTD010434

Tgt Ion:278 Resp: 50232
Ion Ratio Lower Upper
278 100
139 7.9 5.2 7.8#
279 25.8 19.0 28.4

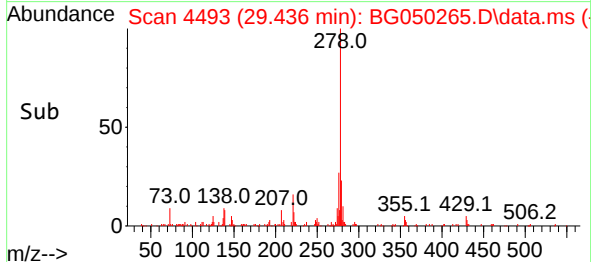

#96
Benzo(g,h,i)perylene
Concen: 8.524 ng/ul
RT: 30.599 min Scan# 4691
Delta R.T. -0.007 min
Lab File: BG050265.D
Acq: 25 Sep 2021 15:56

Tgt Ion:276 Resp: 106566
Ion Ratio Lower Upper
276 100
138 12.2 8.6 13.0
277 23.3 17.4 26.0

