

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092521\
 Data File : BG050267.D
 Acq On : 25 Sep 2021 17:19
 Operator : CG/JU
 Sample : SST04038
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST040436

Quant Time: Sep 27 02:05:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 27 01:56:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.291	152	33195	20.000	ng/u1	0.00
20) Naphthalene-d8	11.117	136	135724	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.907	164	98985	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.651	188	236869	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.958	240	223328	20.000	ng/u1	0.00
88) Perylene-d12	25.406	264	222760	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.661	96	10422	16.190	ng/uL	0.00
4) Pyridine-d5	4.096	84	85199	43.940	ng/u1	0.00
7) Phenol-d5	7.427	99	108680	38.555	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.610	67	64094	40.928	ng/u1	0.00
11) 2-Chlorophenol-d4	7.815	132	80709	38.266	ng/u1	0.00
15) 4-Methylphenol-d8	8.984	113	86043	38.759	ng/u1	0.00
21) Nitrobenzene-d5	9.466	128	35872	34.091	ng/u1	0.00
24) 2-Nitrophenol-d4	10.189	143	41343	32.997	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.729	165	90854	40.655	ng/u1	0.00
31) 4-Chloroaniline-d4	11.247	131	115547	37.987	ng/u1	0.00
46) Dimethylphthalate-d6	14.308	166	273250	36.071	ng/u1	0.00
49) Acenaphthylene-d8	14.607	160	341689	38.469	ng/u1	0.00
54) 4-Nitrophenol-d4	15.077	143	47726	43.545	ng/u1	0.00
60) Fluorene-d10	15.894	176	249307	38.815	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.000	200	40052	26.283	ng/u1	0.00
73) Anthracene-d10	17.751	188	399656	37.574	ng/u1	0.00
81) Pyrene-d10	20.019	212	477884	39.598	ng/u1	0.00
92) Benzo(a)pyrene-d12	25.166	264	463204	39.195	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.697	88	12135	15.463	ng/uL#	94
5) Pyridine	4.114	79	87484	41.746	ng/u1	97
6) Benzaldehyde	7.427	77	77831	47.982	ng/u1	96
8) Phenol	7.451	94	107575	37.783	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.704	93	83335	42.400	ng/u1	93
12) 2-Chlorophenol	7.851	128	79347	38.072	ng/u1#	77
13) 2-Methylphenol	8.720	108	86007	39.155	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.814	45	110885	53.801	ng/u1	95
16) Acetophenone	9.125	105	131039	36.195	ng/u1	98
17) N-Nitroso-di-n-propyla...	9.102	70	73484	40.423	ng/u1	96
18) 4-Methylphenol	9.049	108	87692	37.109	ng/u1#	78
19) Hexachloroethane	9.390	117	34852	38.211	ng/u1#	89
22) Nitrobenzene	9.507	77	104657	36.706	ng/u1	98
23) Isophorone	10.042	82	202093	39.782	ng/u1#	94
25) 2-Nitrophenol	10.224	139	43702	35.876	ng/u1#	78
26) 2,4-Dimethylphenol	10.265	107	104383	38.557	ng/u1#	83
27) Bis(2-Chloroethoxy)met...	10.506	93	110334	42.060	ng/u1	99
29) 2,4-Dichlorophenol	10.753	162	86714	42.276	ng/u1	95
30) Naphthalene	11.170	128	279264	41.166	ng/u1	98
32) 4-Chloroaniline	11.270	127	113449	38.728	ng/u1	91
33) Hexachlorobutadiene	11.446	225	69740	42.030	ng/u1	95
34) Caprolactam	12.063	113	16531	23.008	ng/u1	85
35) 4-Chloro-3-methylphenol	12.363	107	93619	38.190	ng/u1	97
36) 2-Methylnaphthalene	12.757	142	195450	38.758	ng/u1	95


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092521\
 Data File : BG050267.D
 Acq On : 25 Sep 2021 17:19
 Operator : CG/JU
 Sample : SST04038
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST040436

Quant Time: Sep 27 02:05:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 27 01:56:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.974	142	195183	38.345	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	13.109	216	125178	43.056	ng/ul	99
40) Hexachlorocyclopentadiene	13.091	237	87354	67.135	ng/ul	91
41) 2,4,6-Trichlorophenol	13.344	196	77484	41.821	ng/ul	91
42) 2,4,5-Trichlorophenol	13.415	196	82772	42.626	ng/ul	93
43) 1,1'-Biphenyl	13.744	154	265075	38.331	ng/ul#	95
44) 2-Chloronaphthalene	13.791	162	208921	37.612	ng/ul	97
45) 2-Nitroaniline	13.985	65	60204	31.923	ng/ul	93
47) Dimethylphthalate	14.355	163	272220	36.310	ng/ul	99
48) 2,6-Dinitrotoluene	14.472	165	47719	30.829	ng/ul	90
50) Acenaphthylene	14.637	152	340690	41.967	ng/ul	97
51) 3-Nitroaniline	14.807	138	51724	34.630	ng/ul	94
52) Acenaphthene	14.972	153	223233	37.907	ng/ul	99
53) 2,4-Dinitrophenol	15.001	184	27608	34.923	ng/ul#	68
55) 4-Nitrophenol	15.089	109	50216	36.136	ng/ul#	78
56) Dibenzofuran	15.306	168	331618	40.664	ng/ul	93
57) 2,4-Dinitrotoluene	15.254	165	69154	31.060	ng/ul#	94
58) 2,3,4,6-Tetrachlorophenol	15.518	232	76468	47.522	ng/ul#	92
59) Diethylphthalate	15.712	149	283602	36.978	ng/ul	94
61) Fluorene	15.953	166	263070	38.235	ng/ul	96
62) 4-Chlorophenyl-phenyle...	15.941	204	147762	40.589	ng/ul	88
63) 4-Nitroaniline	15.965	138	52800	35.424	ng/ul	85
66) 4,6-Dinitro-2-methylph...	16.012	198	41278	29.884	ng/ul	93
67) N-Nitrosodiphenylamine	16.147	169	237717	38.119	ng/ul	96
68) 4-Bromophenyl-phenylether	16.834	248	99567	37.998	ng/ul	93
69) Hexachlorobenzene	16.952	284	110556	36.538	ng/ul	92
70) Atrazine	17.093	200	107100	38.658	ng/ul	94
71) Pentachlorophenol	17.292	266	72576	56.645	ng/ul	93
72) Phenanthrene	17.692	178	468841	39.703	ng/ul	98
74) Anthracene	17.786	178	464551	38.821	ng/ul	95
75) 1,2,3,4-Tetrachloroben...	13.714	216	134770	42.408	ng/ul	91
76) Pentachlorobenzene	15.218	250	131421	39.027	ng/ul	96
77) Carbazole	18.050	167	432941	40.659	ng/ul	98
78) Di-n-butylphthalate	18.597	149	490985	36.053	ng/ul	99
80) Fluoranthene	19.690	202	597890	40.147	ng/ul#	92
82) Pyrene	20.054	202	593283	40.203	ng/ul#	95
83) Butylbenzylphthalate	20.929	149	207487	35.629	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.846	252	200420	37.858	ng/ul	98
85) Benzo(a)anthracene	21.940	228	541545	38.916	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.828	149	284465	35.569	ng/ul	97
87) Chrysene	22.010	228	521161	39.619	ng/ul	95
89) Di-n-octyl phthalate	23.127	149	458046	34.662	ng/ul	100
90) Benzo(b)fluoranthene	24.302	252	536178	37.629	ng/ul#	98
91) Benzo(k)fluoranthene	24.378	252	486321	35.906	ng/ul	99
93) Benzo(a)pyrene	25.248	252	505305	40.833	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	29.378	276	565508	34.643	ng/ul#	97
95) Dibenzo(a,h)anthracene	29.455	278	491294	35.952	ng/ul#	99
96) Benzo(g,h,i)perylene	30.618	276	494450	36.029	ng/ul	94





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 15.463 ng/uL
RT: 3.697 min Scan# 112
Delta R.T. -0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion: 88 Resp: 12135
Ion Ratio Lower Upper
88 100
43 33.5 21.6 32.4#
58 67.4 52.0 78.0



#5
Pyridine
Concen: 41.746 ng/uL
RT: 4.114 min Scan# 183
Delta R.T. -0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion: 79 Resp: 87484
Ion Ratio Lower Upper
79 100
52 74.3 61.1 91.7
51 40.7 34.8 52.2









#6
Benzaldehyde
Concen: 47.982 ng/ul
RT: 7.427 min Scan# 747
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion: 77 Resp: 77831
Ion Ratio Lower Upper
77 100
105 92.7 72.3 108.5
106 85.0 72.3 108.5



#8
Phenol
Concen: 37.783 ng/ul
RT: 7.451 min Scan# 751
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion: 94 Resp: 107575
Ion Ratio Lower Upper
94 100
65 34.2 27.7 41.5
66 46.8 39.0 58.4









#10
Bis(2-Chloroethyl)ether
Concen: 42.400 ng/ul
RT: 7.704 min Scan# 794
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:	93	Resp:	83335
Ion	Ratio	Lower	Upper
93	100		
63	82.8	59.9	89.9
95	32.4	27.6	41.4



#12
2-Chlorophenol
Concen: 38.072 ng/ul
RT: 7.851 min Scan# 819
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:	128	Resp:	79347
Ion	Ratio	Lower	Upper
128	100		
64	56.8	28.0	42.0#
130	33.6	24.4	36.6









#13
2-Methylphenol
Concen: 39.155 ng/ul
RT: 8.720 min Scan# 967
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:108 Resp: 86007
Ion Ratio Lower Upper
108 100
107 91.1 71.0 106.4



#14
2,2'-oxybis(1-Chloropropane)
Concen: 53.801 ng/ul
RT: 8.814 min Scan# 983
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion: 45 Resp: 110885
Ion Ratio Lower Upper
45 100
77 17.8 16.9 25.3
79 12.6 11.0 16.4









#16
Acetophenone
Concen: 36.195 ng/ul
RT: 9.125 min Scan# 1036
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:105 Resp: 131039
Ion Ratio Lower Upper
105 100
77 83.7 67.7 101.5
51 29.7 25.3 37.9



#17
N-Nitroso-di-n-propylamine
Concen: 40.423 ng/ul
RT: 9.102 min Scan# 1032
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion: 70 Resp: 73484
Ion Ratio Lower Upper
70 100
42 58.6 44.2 66.4
101 9.0 7.8 11.8
130 16.7 15.3 22.9









#18
4-Methylphenol
Concen: 37.109 ng/ul
RT: 9.049 min Scan# 1023
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:108 Resp: 87692
Ion Ratio Lower Upper
108 100
107 119.4 78.3 117.5#



#19
Hexachloroethane
Concen: 38.211 ng/ul
RT: 9.390 min Scan# 1081
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:117 Resp: 34852
Ion Ratio Lower Upper
117 100
201 119.1 89.3 133.9
199 76.4 50.5 75.7#









#22
Nitrobenzene
Concen: 36.706 ng/ul
RT: 9.507 min Scan# 1101
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion: 77 Resp: 104657
Ion Ratio Lower Upper
77 100
123 39.6 30.4 45.6
65 13.5 11.3 16.9



#23
Isophorone
Concen: 39.782 ng/ul
RT: 10.042 min Scan# 1192
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion: 82 Resp: 202093
Ion Ratio Lower Upper
82 100
95 8.3 7.8 11.8
138 17.1 11.4 17.0#









#25
2-Nitrophenol
Concen: 35.876 ng/ul
RT: 10.224 min Scan# 1223
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:139 Resp: 43702
Ion Ratio Lower Upper
139 100
65 54.9 53.1 79.7
109 32.0 44.1 66.1#



#26
2,4-Dimethylphenol
Concen: 38.557 ng/ul
RT: 10.265 min Scan# 1230
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:107 Resp: 104383
Ion Ratio Lower Upper
107 100
121 48.1 32.7 49.1
122 82.2 52.6 79.0#









#27
 Bis(2-Chloroethoxy)methane
 Concen: 42.060 ng/ul
 RT: 10.506 min Scan# 1271
 Delta R.T. -0.006 min
 Lab File: BG050267.D
 Acq: 25 Sep 2021 17:19




Instrument :
 BNA_G
 ClientSampleId :
 SSTD040436


Tgt Ion: 93 Resp: 110334
 Ion Ratio Lower Upper
 93 100
 95 31.3 24.8 37.2
 123 10.5 8.2 12.2



#29
 2,4-Dichlorophenol
 Concen: 42.276 ng/ul
 RT: 10.753 min Scan# 1313
 Delta R.T. 0.000 min
 Lab File: BG050267.D
 Acq: 25 Sep 2021 17:19


Tgt Ion:162 Resp: 86714
 Ion Ratio Lower Upper
 162 100
 164 69.2 51.0 76.6
 98 35.9 27.8 41.8








#30
Naphthalene
Concen: 41.166 ng/ul
RT: 11.170 min Scan# 1384
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19


Instrument :
BNA_G
ClientSampleId :
SSTD040436





Tgt Ion	Ratio	Lower	Upper
128	100		
129	10.7	9.3	13.9
127	13.2	9.8	14.6




#32
4-Chloroaniline
Concen: 38.728 ng/ul
RT: 11.270 min Scan# 1401
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19



Tgt Ion	Ratio	Lower	Upper
127	100		
129	32.5	30.3	45.5









#33
Hexachlorobutadiene
Concen: 42.030 ng/ul
RT: 11.446 min Scan# 1431
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:225 Resp: 69740
Ion Ratio Lower Upper
225 100
223 61.0 51.3 76.9
227 63.8 55.1 82.7



#34
Caprolactam
Concen: 23.008 ng/ul
RT: 12.063 min Scan# 1536
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:113 Resp: 16531
Ion Ratio Lower Upper
113 100
55 165.1 114.0 171.0
56 120.0 107.4 161.0









#35
4-Chloro-3-methylphenol
Concen: 38.190 ng/ul
RT: 12.363 min Scan# 1587
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:107 Resp: 93619
Ion Ratio Lower Upper
107 100
144 27.2 18.9 28.3
142 72.7 59.2 88.8



#36
2-Methylnaphthalene
Concen: 38.758 ng/ul
RT: 12.757 min Scan# 1654
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:142 Resp: 195450
Ion Ratio Lower Upper
142 100
141 92.9 70.5 105.7









#37
1-Methylnaphthalene
Concen: 38.345 ng/ul
RT: 12.974 min Scan# 1691
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:142 Resp: 195183
Ion Ratio Lower Upper
142 100
141 93.9 75.8 113.8
116 4.4 3.7 5.5



#39
1,2,4,5-Tetrachlorobenzene
Concen: 43.056 ng/ul
RT: 13.109 min Scan# 1714
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:216 Resp: 125178
Ion Ratio Lower Upper
216 100
214 80.0 64.2 96.2
179 17.7 12.8 19.2
108 16.3 13.1 19.7









#40
Hexachlorocyclopentadiene
Concen: 67.135 ng/ul
RT: 13.091 min Scan# 1711
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:	237	Resp:	87354
Ion Ratio	Lower	Upper	
237	100		
235	58.9	53.5	80.3
272	12.1	11.5	17.3



#41
2,4,6-Trichlorophenol
Concen: 41.821 ng/ul
RT: 13.344 min Scan# 1754
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:	196	Resp:	77484
Ion Ratio	Lower	Upper	
196	100		
198	94.3	83.7	125.5
200	28.9	25.9	38.9









#42
2,4,5-Trichlorophenol
Concen: 42.626 ng/ul
RT: 13.415 min Scan# 1766
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:196 Resp: 82772
Ion Ratio Lower Upper
196 100
198 94.8 70.3 105.5
200 30.2 26.6 40.0



#43
1,1'-Biphenyl
Concen: 38.331 ng/ul
RT: 13.744 min Scan# 1822
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:154 Resp: 265075
Ion Ratio Lower Upper
154 100
153 43.0 32.5 48.7
76 13.3 7.8 11.8#









#44
2-Chloronaphthalene
Concen: 37.612 ng/ul
RT: 13.791 min Scan# 1830
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:162 Resp: 208921
Ion Ratio Lower Upper
162 100
164 34.4 25.2 37.8
127 39.6 31.9 47.9



#45
2-Nitroaniline
Concen: 31.923 ng/ul
RT: 13.985 min Scan# 1863
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion: 65 Resp: 60204
Ion Ratio Lower Upper
65 100
92 65.3 55.6 83.4
138 90.4 78.7 118.1









#47
Dimethylphthalate
Concen: 36.310 ng/ul
RT: 14.355 min Scan# 1926
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:163 Resp: 272220
Ion Ratio Lower Upper
163 100
194 3.8 3.4 5.0
164 10.4 8.2 12.4



#48
2,6-Dinitrotoluene
Concen: 30.829 ng/ul
RT: 14.472 min Scan# 1946
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:165 Resp: 47719
Ion Ratio Lower Upper
165 100
89 69.0 62.5 93.7
121 23.9 22.2 33.2









#50
Acenaphthylene
Concen: 41.967 ng/ul
RT: 14.637 min Scan# 1974
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:152 Resp: 340690
Ion Ratio Lower Upper
152 100
151 20.6 15.2 22.8
153 12.6 10.7 16.1



#51
3-Nitroaniline
Concen: 34.630 ng/ul
RT: 14.807 min Scan# 2003
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:138 Resp: 51724
Ion Ratio Lower Upper
138 100
108 13.4 9.0 13.4
92 126.7 96.4 144.6









#52
Acenaphthene
Concen: 37.907 ng/ul
RT: 14.972 min Scan# 2031
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:153 Resp: 223233
Ion Ratio Lower Upper
153 100
152 47.0 37.4 56.2
154 87.6 71.5 107.3



#53
2,4-Dinitrophenol
Concen: 34.923 ng/ul
RT: 15.001 min Scan# 2036
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:184 Resp: 27608
Ion Ratio Lower Upper
184 100
63 52.6 75.8 113.8#
154 64.9 64.6 96.8









#55
4-Nitrophenol
Concen: 36.136 ng/ul
RT: 15.089 min Scan# 2051
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:109 Resp: 50216
Ion Ratio Lower Upper
109 100
139 94.8 61.4 92.0#
65 118.3 76.5 114.7#



#56
Dibenzofuran
Concen: 40.664 ng/ul
RT: 15.306 min Scan# 2088
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:168 Resp: 331618
Ion Ratio Lower Upper
168 100
139 37.7 33.8 50.8









#57
2,4-Dinitrotoluene
Concen: 31.060 ng/ul
RT: 15.254 min Scan# 2079
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:165 Resp: 69154
Ion Ratio Lower Upper
165 100
63 48.1 42.3 63.5
182 2.5 2.6 4.0#



#58
2,3,4,6-Tetrachlorophenol
Concen: 47.522 ng/ul
RT: 15.518 min Scan# 2124
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:232 Resp: 76468
Ion Ratio Lower Upper
232 100
131 44.4 40.0 60.0
130 2.9 1.8 2.8#
166 26.6 24.8 37.2









#59
Diethylphthalate
Concen: 36.978 ng/ul
RT: 15.712 min Scan# 2157
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:149 Resp: 283602
Ion Ratio Lower Upper
149 100
177 23.5 15.8 23.6
150 13.0 9.7 14.5



#61
Fluorene
Concen: 38.235 ng/ul
RT: 15.953 min Scan# 2198
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:166 Resp: 263070
Ion Ratio Lower Upper
166 100
165 99.9 83.3 124.9
167 13.5 11.8 17.6









#62
4-Chlorophenyl-phenylether
Concen: 40.589 ng/ul
RT: 15.941 min Scan# 2196
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:204 Resp: 147762
Ion Ratio Lower Upper
204 100
206 33.8 25.4 38.2
141 52.3 51.8 77.6



#63
4-Nitroaniline
Concen: 35.424 ng/ul
RT: 15.965 min Scan# 2200
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:138 Resp: 52800
Ion Ratio Lower Upper
138 100
92 59.1 50.0 75.0
108 104.5 101.8 152.8









#66
4,6-Dinitro-2-methylphenol
Concen: 29.884 ng/ul
RT: 16.012 min Scan# 2208
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:198 Resp: 41278
Ion Ratio Lower Upper
198 100
182 3.9 3.0 4.6
77 25.0 23.4 35.2



#67
N-Nitrosodiphenylamine
Concen: 38.119 ng/ul
RT: 16.147 min Scan# 2231
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:169 Resp: 237717
Ion Ratio Lower Upper
169 100
168 72.2 55.0 82.6
167 38.9 29.0 43.4







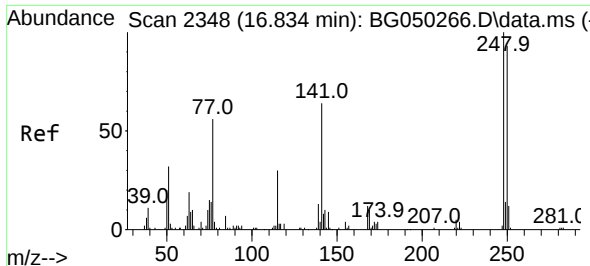

#68
4-Bromophenyl-phenylether
Concen: 37.998 ng/ul
RT: 16.834 min Scan# 2348
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:	248	Resp:	99567
Ion Ratio	Lower	Upper	
248	100		
250	96.0	80.2	120.2
141	66.3	60.6	90.8



#69
Hexachlorobenzene
Concen: 36.538 ng/ul
RT: 16.952 min Scan# 2368
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:	284	Resp:	110556
Ion Ratio	Lower	Upper	
284	100		
142	29.9	28.7	43.1
249	34.7	25.5	38.3









#70
Atrazine
Concen: 38.658 ng/ul
RT: 17.093 min Scan# 2392
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:200 Resp: 107100
Ion Ratio Lower Upper
200 100
173 25.7 19.3 28.9
215 48.5 34.9 52.3



#71
Pentachlorophenol
Concen: 56.645 ng/ul
RT: 17.292 min Scan# 2426
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:266 Resp: 72576
Ion Ratio Lower Upper
266 100
264 59.0 54.1 81.1
268 63.2 52.6 78.8









#72
Phenanthrene
Concen: 39.703 ng/ul
RT: 17.692 min Scan# 2494
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:178 Resp: 468841
Ion Ratio Lower Upper
178 100
179 15.9 11.7 17.5
176 19.8 16.2 24.2



#74
Anthracene
Concen: 38.821 ng/ul
RT: 17.786 min Scan# 2510
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:178 Resp: 464551
Ion Ratio Lower Upper
178 100
179 15.9 11.4 17.0
176 18.4 12.8 19.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 42.408 ng/uL
RT: 13.714 min Scan# 1817
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:216 Resp: 134770
Ion Ratio Lower Upper
216 100
214 78.9 70.9 106.3
218 46.2 40.9 61.3



#76
Pentachlorobenzene
Concen: 39.027 ng/uL
RT: 15.218 min Scan# 2073
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:250 Resp: 131421
Ion Ratio Lower Upper
250 100
248 64.4 51.5 77.3
252 65.6 47.9 71.9









#77
 Carbazole
 Concen: 40.659 ng/ul
 RT: 18.050 min Scan# 2555
 Delta R.T. 0.000 min
 Lab File: BG050267.D
 Acq: 25 Sep 2021 17:19




Instrument :
 BNA_G
 ClientSampleId :
 SSTD040436


Tgt Ion:167 Resp: 432941
 Ion Ratio Lower Upper
 167 100
 166 21.5 17.8 26.8
 139 12.9 11.1 16.7



#78
 Di-n-butylphthalate
 Concen: 36.053 ng/ul
 RT: 18.597 min Scan# 2648
 Delta R.T. 0.000 min
 Lab File: BG050267.D
 Acq: 25 Sep 2021 17:19

Tgt Ion:149 Resp: 490985
 Ion Ratio Lower Upper
 149 100
 150 9.6 8.1 12.1
 104 6.3 5.3 7.9









#80
Fluoranthene
Concen: 40.147 ng/ul
RT: 19.690 min Scan# 2834
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:202 Resp: 597890
Ion Ratio Lower Upper
202 100
101 8.2 4.3 6.5#
100 6.8 3.5 5.3#



#82
Pyrene
Concen: 40.203 ng/ul
RT: 20.054 min Scan# 2896
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:202 Resp: 593283
Ion Ratio Lower Upper
202 100
101 9.1 5.4 8.0#
100 7.6 5.0 7.6#









#83
Butylbenzylphthalate
Concen: 35.629 ng/ul
RT: 20.929 min Scan# 3045
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:149	Resp:	207487
Ion Ratio	Lower	Upper
149	100	
91	75.9	60.6 90.8
206	23.8	16.8 25.2



#84
3,3'-Dichlorobenzidine
Concen: 37.858 ng/ul
RT: 21.846 min Scan# 3201
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:252	Resp:	200420
Ion Ratio	Lower	Upper
252	100	
254	66.4	54.2 81.2
126	7.8	5.4 8.0









#85
Benzo(a)anthracene
Concen: 38.916 ng/ul
RT: 21.940 min Scan# 3217
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:	228	Resp:	541545
Ion Ratio	Lower	Upper	
228	100		
229	20.5	16.2	24.4
226	28.3	21.0	31.4



#86
Bis(2-ethylhexyl)phthalate
Concen: 35.569 ng/ul
RT: 21.828 min Scan# 3198
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:	149	Resp:	284465
Ion Ratio	Lower	Upper	
149	100		
167	26.9	20.4	30.6
279	5.0	3.7	5.5









#87
Chrysene
Concen: 39.619 ng/ul
RT: 22.010 min Scan# 3229
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:	228	Resp:	521161
Ion Ratio	Lower	Upper	
228	100		
226	31.1	23.0	34.4
229	20.0	17.8	26.6



#89
Di-n-octyl phthalate
Concen: 34.662 ng/ul
RT: 23.127 min Scan# 3419
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:149 Resp: 458046









#90
Benzo(b)fluoranthene
Concen: 37.629 ng/ul
RT: 24.302 min Scan# 3619
Delta R.T. 0.000 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:252 Resp: 536178
Ion Ratio Lower Upper
252 100
253 22.2 18.1 27.1
125 6.4 3.4 5.0#



#91
Benzo(k)fluoranthene
Concen: 35.906 ng/ul
RT: 24.378 min Scan# 3632
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:252 Resp: 486321
Ion Ratio Lower Upper
252 100
253 22.4 17.7 26.5
125 6.0 4.1 6.1









#93
Benzo(a)pyrene
Concen: 40.833 ng/ul
RT: 25.248 min Scan# 3780
Delta R.T. 0.006 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19




Instrument :
BNA_G
ClientSampleId :
SSTD040436


Tgt Ion:252 Resp: 505305
Ion Ratio Lower Upper
252 100
253 21.6 17.0 25.4
125 5.9 4.4 6.6



#94
Indeno(1,2,3-cd)pyrene
Concen: 34.643 ng/ul
RT: 29.378 min Scan# 4483
Delta R.T. 0.024 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:276 Resp: 565508
Ion Ratio Lower Upper
276 100
138 10.8 5.5 8.3#
277 23.6 18.6 27.8









#95
Dibenzo(a,h)anthracene
Concen: 35.952 ng/ul
RT: 29.455 min Scan# 4496
Delta R.T. 0.012 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Instrument :
BNA_G
ClientSampleId :
SSTD040436

Tgt Ion:278 Resp: 491294
Ion Ratio Lower Upper
278 100
139 8.3 5.2 7.8#
279 23.9 19.0 28.4



#96
Benzo(g,h,i)perylene
Concen: 36.029 ng/ul
RT: 30.618 min Scan# 4694
Delta R.T. 0.012 min
Lab File: BG050267.D
Acq: 25 Sep 2021 17:19

Tgt Ion:276 Resp: 494450
Ion Ratio Lower Upper
276 100
138 11.0 8.6 13.0
277 25.7 17.4 26.0

