

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092523\
 Data File : BG059177.D
 Acq On : 25 Sep 2023 10:21
 Operator : MA/JU
 Sample : PB155606BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK606

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.057	109	114	124	rBV	272469	469490	23.31%	2.501%
2	5.890	425	426	428	rBV2	3859	3139	0.16%	0.017%
3	6.301	494	496	499	rBV3	3549	5070	0.25%	0.027%
4	6.595	544	546	547	rBV	3282	3120	0.15%	0.017%
5	7.224	648	653	656	rBV5	3152	6193	0.31%	0.033%
6	7.435	682	689	697	rBV	302147	522876	25.96%	2.785%
7	7.629	715	722	730	rBV	247029	413883	20.55%	2.205%
8	7.829	749	756	765	rVB	286113	503021	24.97%	2.680%
9	7.964	776	779	780	rBV2	3363	2806	0.14%	0.015%
10	8.311	831	838	847	rVB	187572	335849	16.67%	1.789%
11	8.998	947	955	963	rBV	365335	621665	30.86%	3.312%
12	9.380	1018	1020	1024	rVB2	3382	3161	0.16%	0.017%
13	9.509	1034	1042	1048	rBV	275913	494308	24.54%	2.633%
14	9.627	1059	1062	1064	rBV4	3093	3363	0.17%	0.018%
15	9.897	1107	1108	1111	rBV2	2502	2998	0.15%	0.016%
16	10.226	1155	1164	1173	rBV	229195	419414	20.82%	2.234%
17	10.355	1185	1186	1190	rVB2	2898	2578	0.13%	0.014%
18	10.667	1237	1239	1243	rBV3	1962	3141	0.16%	0.017%
19	10.755	1247	1254	1264	rVV	345440	598081	29.69%	3.186%
20	11.154	1314	1322	1329	rVB	284596	506606	25.15%	2.699%
21	11.219	1331	1333	1338	rVB5	2614	4237	0.21%	0.023%
22	11.296	1338	1346	1357	rBV2	329498	644457	32.00%	3.433%
23	11.660	1404	1408	1411	rVB4	1741	2703	0.13%	0.014%
24	11.865	1440	1443	1445	rBV3	3567	3291	0.16%	0.018%
25	12.136	1484	1489	1492	rBV4	2212	3245	0.16%	0.017%
26	12.529	1553	1556	1559	rVB2	2952	3817	0.19%	0.020%
27	12.576	1559	1564	1566	rBV4	2499	4124	0.20%	0.022%
28	12.617	1569	1571	1575	rBV2	2075	3100	0.15%	0.017%
29	12.717	1583	1588	1592	rVB3	7586	11639	0.58%	0.062%
30	12.935	1622	1625	1628	rBV4	1902	2624	0.13%	0.014%
31	12.988	1631	1634	1637	rBV4	1709	2657	0.13%	0.014%
32	13.258	1676	1680	1683	rVB4	2373	3526	0.18%	0.019%
33	13.769	1761	1767	1772	rVB5	11383	20308	1.01%	0.108%
34	13.904	1787	1790	1793	rBV4	2349	3163	0.16%	0.017%
35	14.333	1856	1863	1868	rBV	707447	997868	49.54%	5.316%
36	14.639	1908	1915	1923	rBV	720923	1192231	59.19%	6.351%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092523\
 Data File : BG059177.D
 Acq On : 25 Sep 2023 10:21
 Operator : MA/JU
 Sample : PB155606BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK606

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

37	14.815	1944	1945	1949	rBV3	2388	3231	0.16%	0.017%
38	14.885	1952	1957	1959	rVV3	2069	2970	0.15%	0.016%
39	14.938	1959	1966	1973	rVV	468468	714546	35.48%	3.806%
40	15.120	1989	1997	2005	rBV2	148294	288917	14.34%	1.539%
41	15.596	2076	2078	2081	rVB2	3946	3642	0.18%	0.019%
42	15.925	2126	2134	2143	rBV	984132	1480998	73.53%	7.889%
43	16.031	2146	2152	2165	rBV	283949	467741	23.22%	2.492%
44	16.160	2171	2174	2178	rVB6	7342	11284	0.56%	0.060%
45	16.542	2236	2239	2240	rBV2	4525	3233	0.16%	0.017%
46	16.642	2254	2256	2258	rVB3	3353	2653	0.13%	0.014%
47	16.777	2276	2279	2282	rVB2	2358	2597	0.13%	0.014%
48	16.948	2306	2308	2310	rBV3	2146	2642	0.13%	0.014%
49	17.253	2358	2360	2364	rBV4	1974	2561	0.13%	0.014%
50	17.347	2372	2376	2379	rBV3	3323	5493	0.27%	0.029%
51	17.547	2407	2410	2412	rBV4	3780	4637	0.23%	0.025%
52	17.688	2427	2434	2441	rBV	622877	930479	46.20%	4.957%
53	17.788	2444	2451	2463	rBV2	1082822	1651605	82.00%	8.798%
54	18.135	2507	2510	2511	rBV3	3564	3759	0.19%	0.020%
55	18.152	2511	2513	2515	rVV2	4368	4764	0.24%	0.025%
56	18.193	2518	2520	2522	rBV3	3191	3287	0.16%	0.018%
57	18.246	2527	2529	2531	rBV3	3038	2870	0.14%	0.015%
58	18.264	2531	2532	2534	rVB2	6243	3150	0.16%	0.017%
59	18.299	2536	2538	2541	rBV4	4730	6105	0.30%	0.033%
60	18.605	2587	2590	2591	rBV2	3480	3684	0.18%	0.020%
61	18.693	2602	2605	2606	rBV3	4228	3847	0.19%	0.020%
62	19.145	2680	2682	2683	rBV2	3630	3203	0.16%	0.017%
63	19.468	2735	2737	2740	rVB4	5659	4305	0.21%	0.023%
64	19.621	2760	2763	2768	rVB4	18666	24573	1.22%	0.131%
65	20.062	2832	2838	2847	rBV2	1299674	2014213	100.00%	10.730%
66	22.012	3164	3170	3180	rBV	457586	822131	40.82%	4.379%
67	25.326	3724	3734	3749	rBV3	507551	1620400	80.45%	8.632%
68	25.573	3768	3776	3788	rVB2	270573	849067	42.15%	4.523%




Sum of corrected areas: 18772339

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092523\
Data File : BG059177.D
Acq On : 25 Sep 2023 10:21
Operator : MA/JU
Sample : PB155606BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK606

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

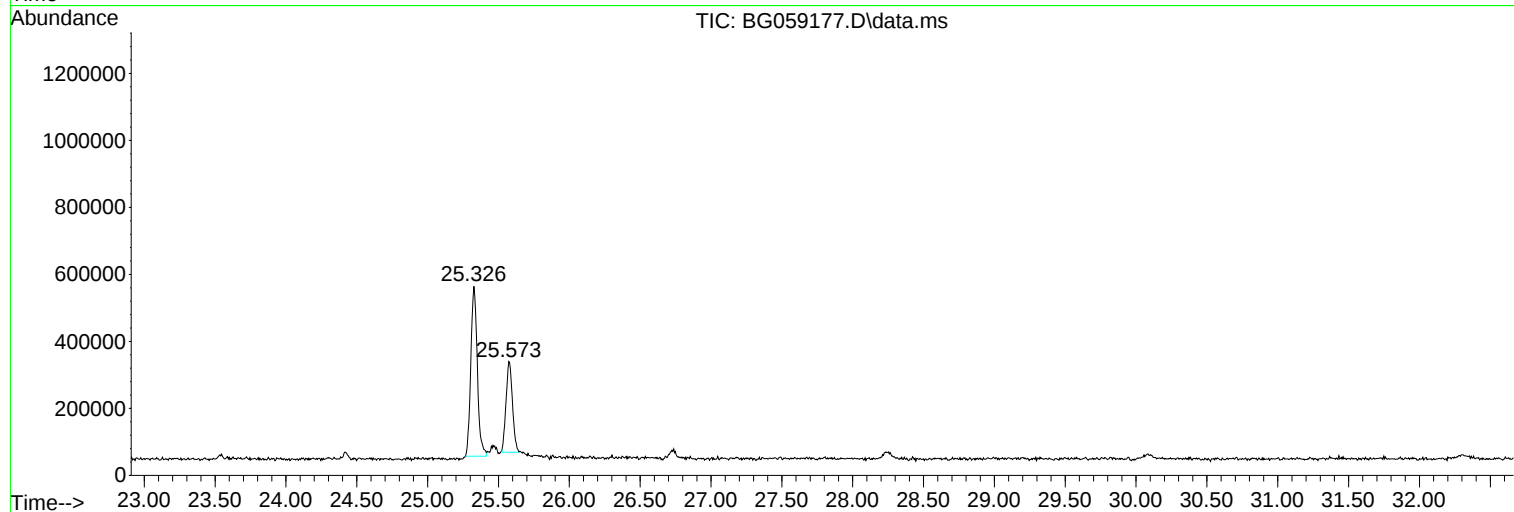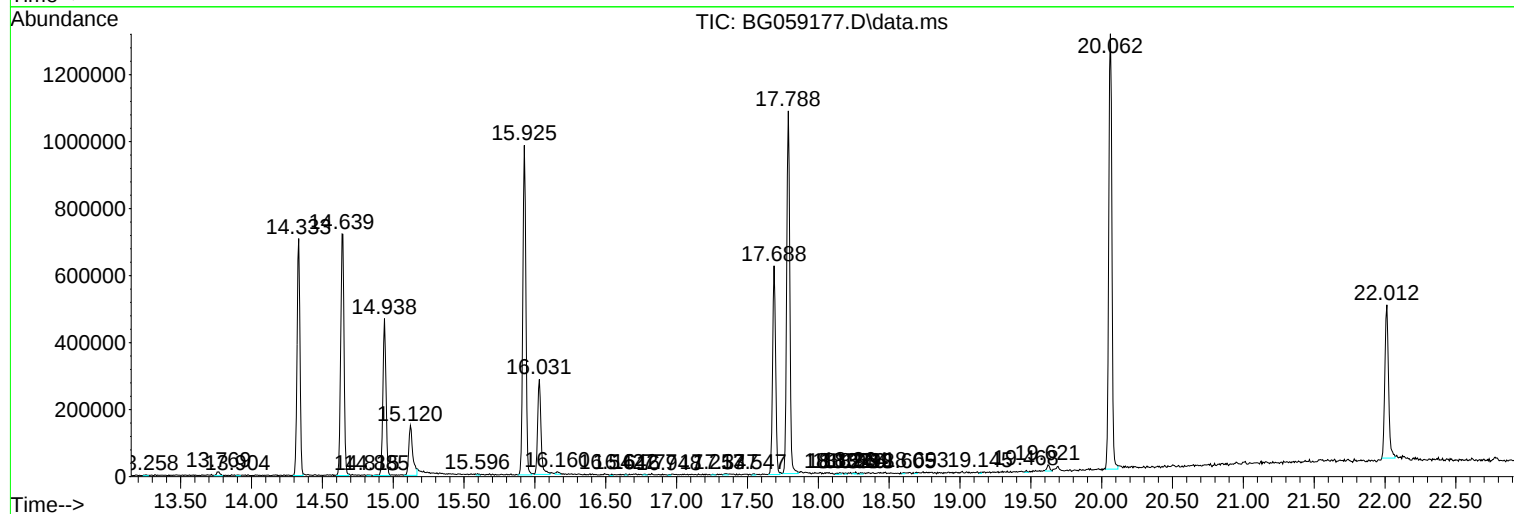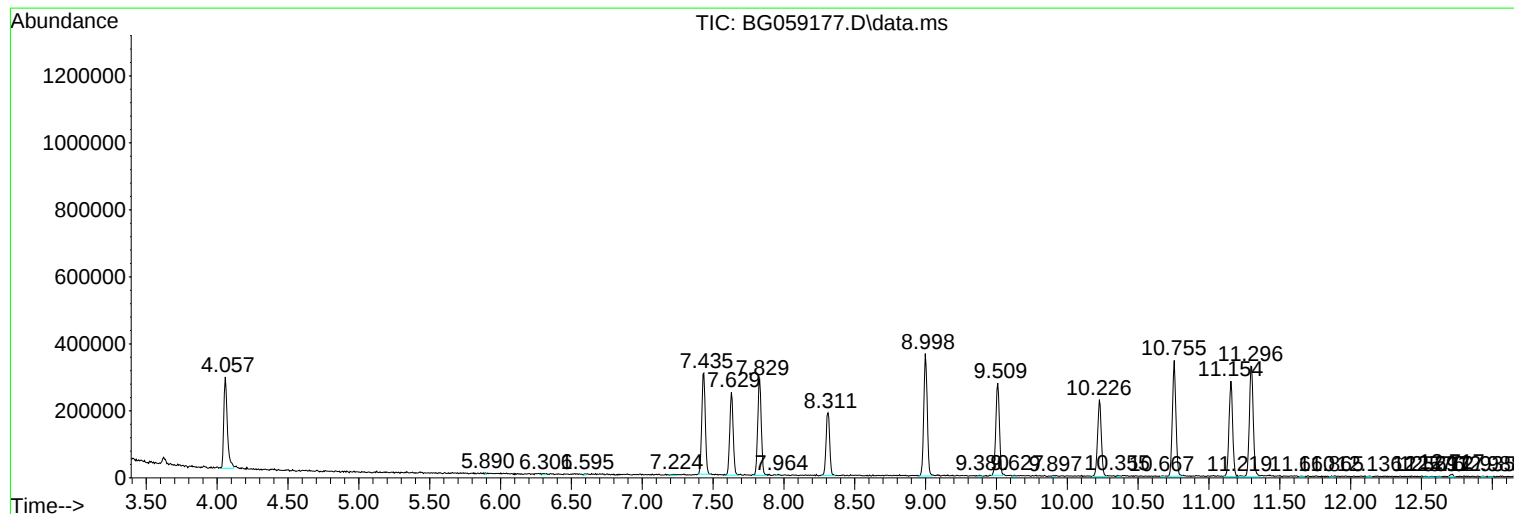

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092523\
Data File : BG059177.D
Acq On : 25 Sep 2023 10:21
Operator : MA/JU
Sample : PB155606BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK606

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092523\
Data File : BG059177.D
Acq On : 25 Sep 2023 10:21
Operator : MA/JU
Sample : PB155606BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK606

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc