




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
Data File : BG063063.D
Acq On : 26 Sep 2024 13:46
Operator : RC/JU
Sample : P3879-11DL2 50X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ9DL2

Manual IntegrationsAPPROVED

Quant Time: Sep 26 15:00:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 25 13:16:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2024
Supervised By :mohammad ahmed 09/27/2024

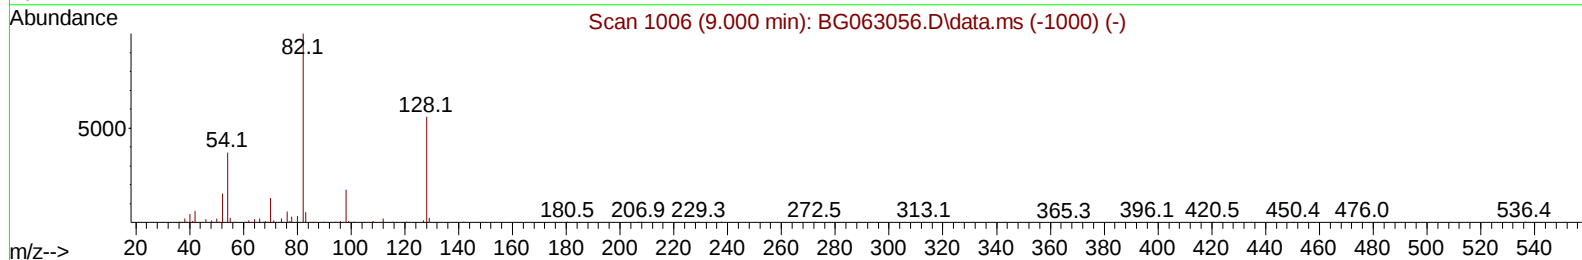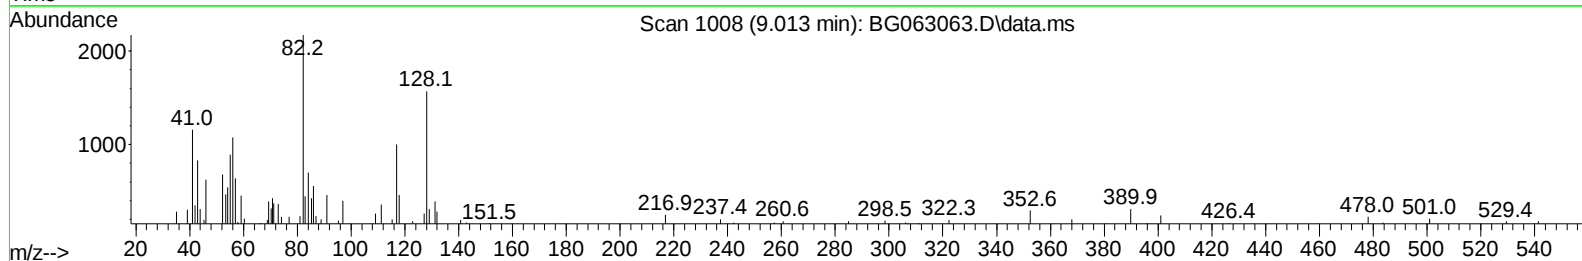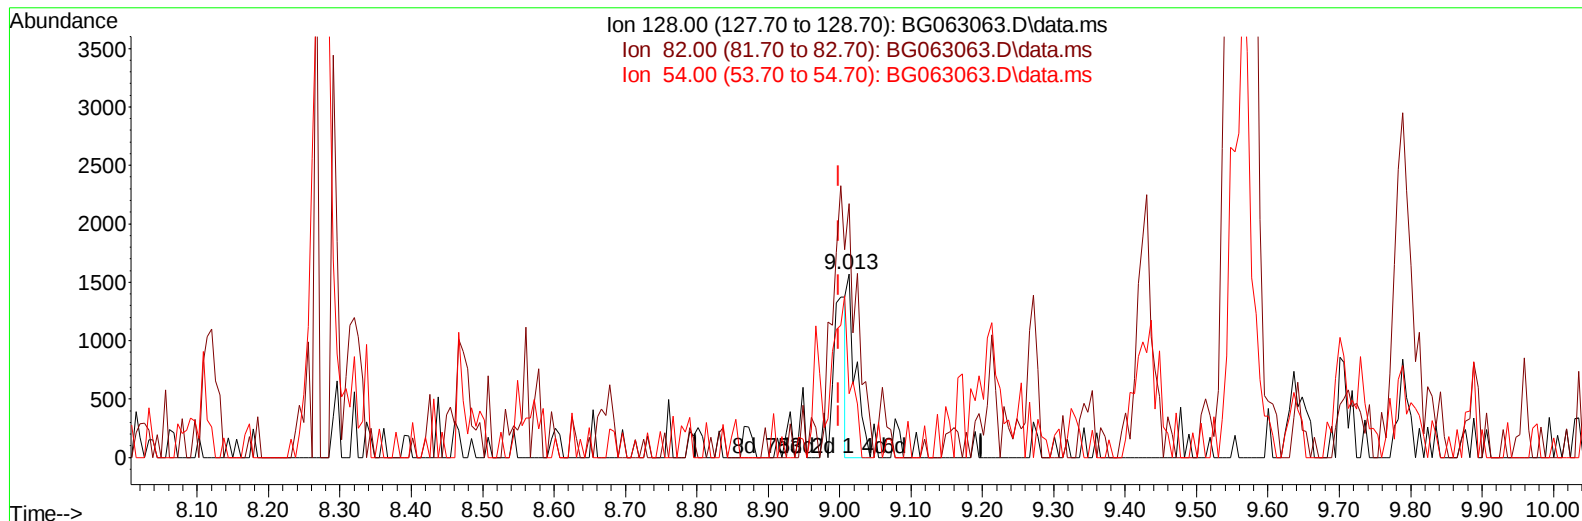

TIC: BG063063.D\data.ms

(21) Nitrobenzene-d5 (S)

9.013min (+ 0.014) 0.49 ng/u1

response 1259

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	197.00	138.28#
54.00	88.90	34.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
Data File : BG063063.D
Acq On : 26 Sep 2024 13:46
Operator : RC/JU
Sample : P3879-11DL2 50X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ9DL2

Manual IntegrationsAPPROVED

Quant Time: Sep 26 15:00:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 25 13:16:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2024
Supervised By :mohammad ahmed 09/27/2024

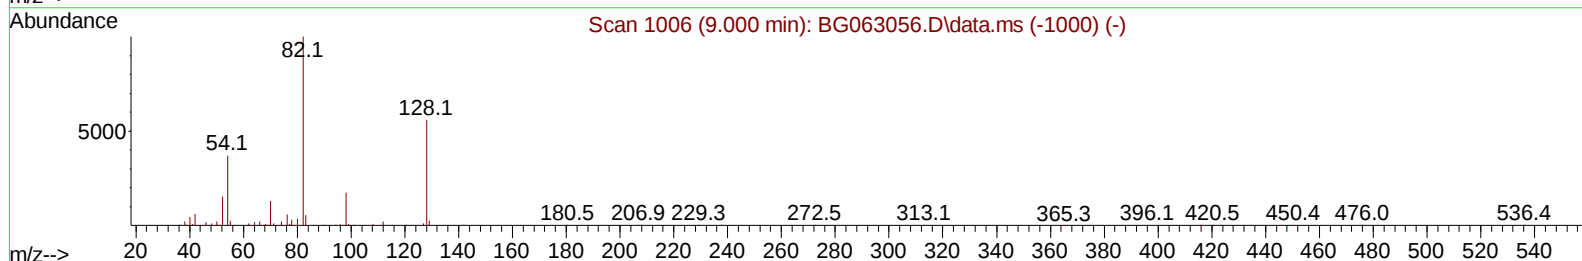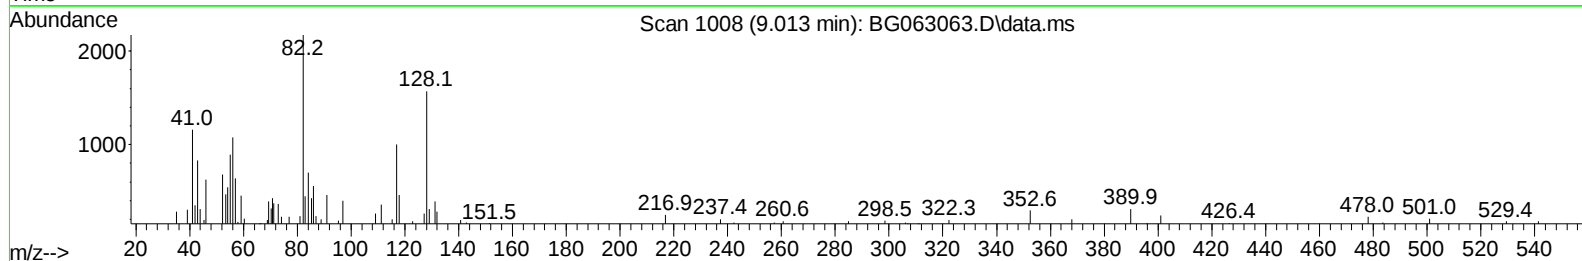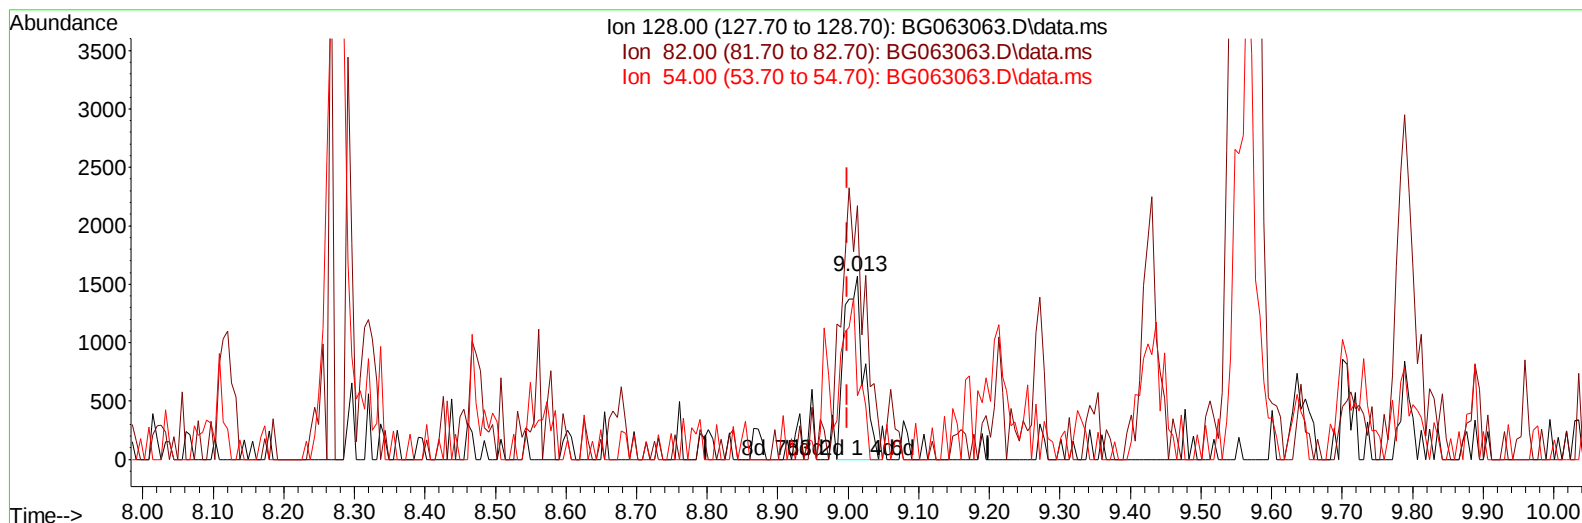

TIC: BG063063.D\data.ms

(21) Nitrobenzene-d5 (S)

9.013min (+ 0.014) 1.13 ng/ul m

response 2914

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	197.00	138.28#
54.00	88.90	34.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
Data File : BG063063.D
Acq On : 26 Sep 2024 13:46
Operator : RC/JU
Sample : P3879-11DL2 50X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ9DL2

Manual IntegrationsAPPROVED

Quant Time: Sep 26 15:00:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 25 13:16:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2024
Supervised By :mohammad ahmed 09/27/2024

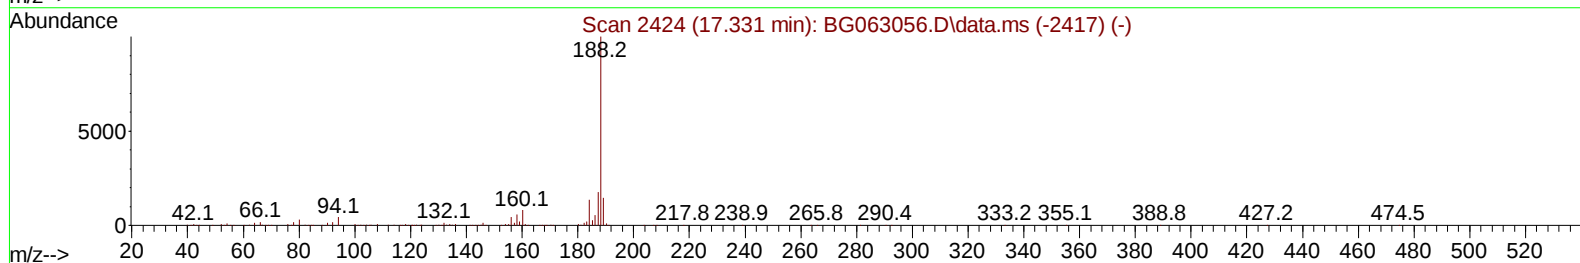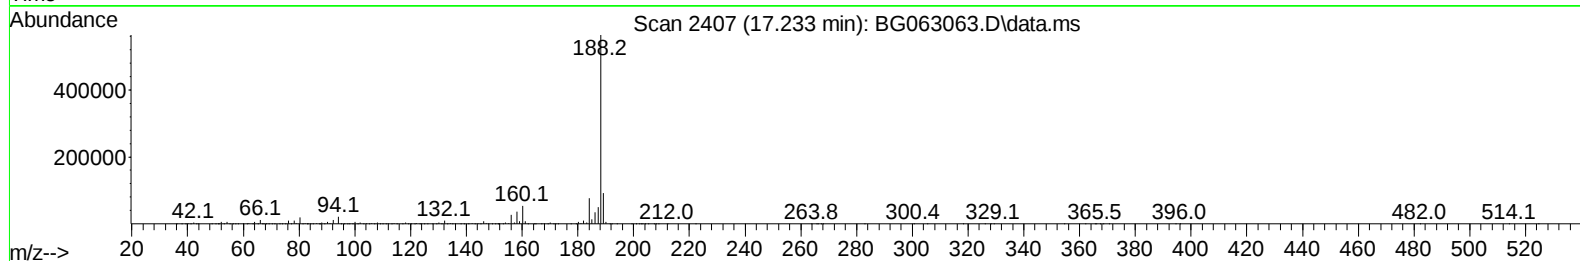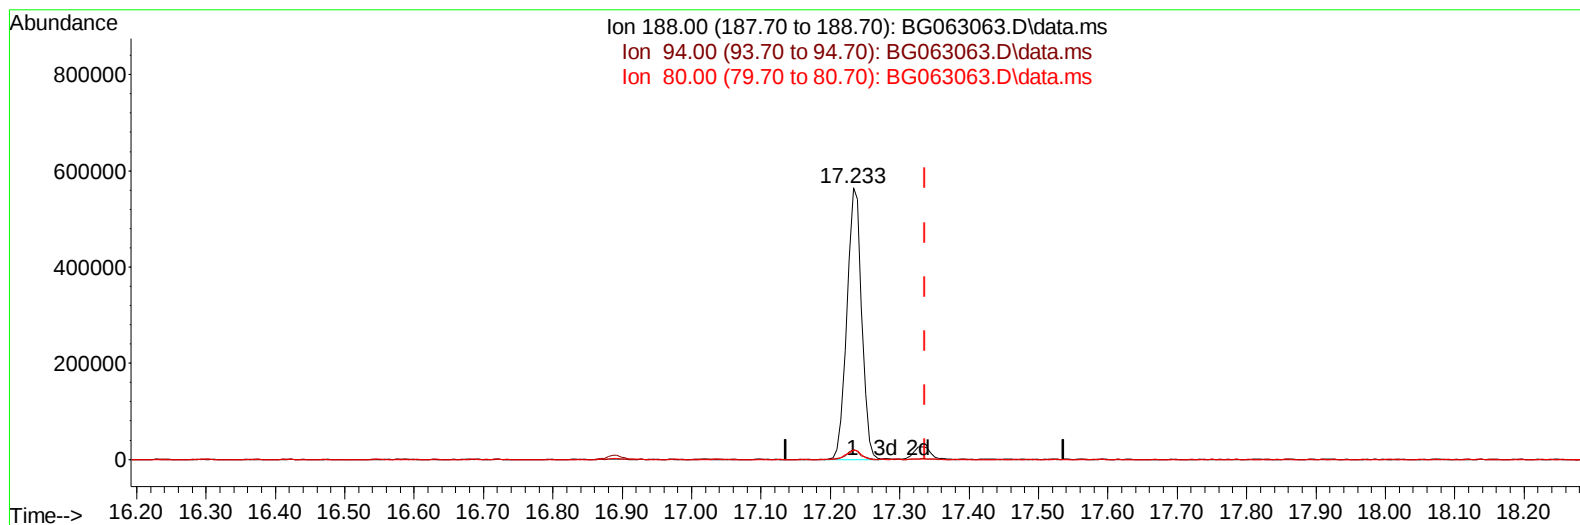

TIC: BG063063.D\data.ms

(73) Anthracene-d10 (S)

17.233min (-0.103) 20.84 ng/u1

response 830505

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	3.30	3.64
80.00	3.00	3.35
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
Data File : BG063063.D
Acq On : 26 Sep 2024 13:46
Operator : RC/JU
Sample : P3879-11DL2 50X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ9DL2

Manual IntegrationsAPPROVED

Quant Time: Sep 26 15:00:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 25 13:16:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2024
Supervised By :mohammad ahmed 09/27/2024

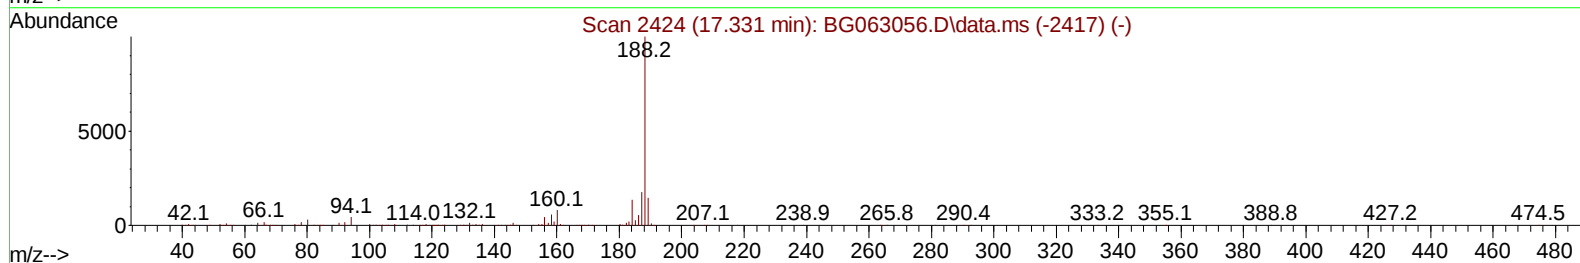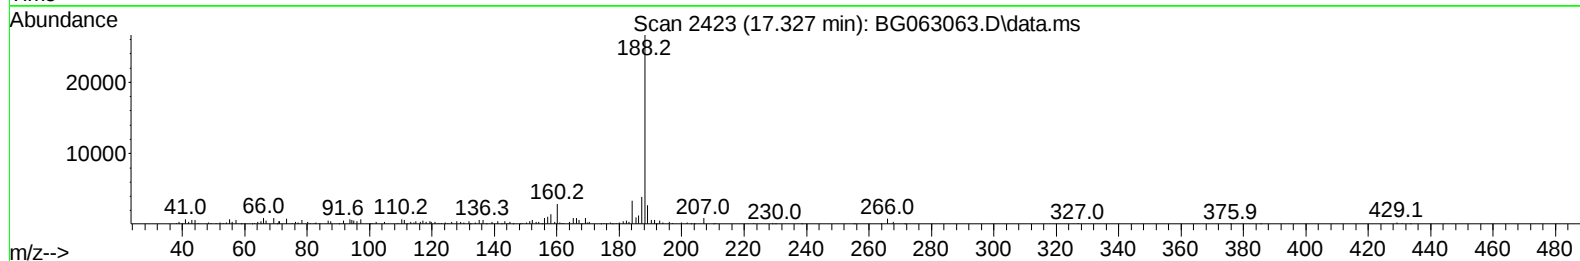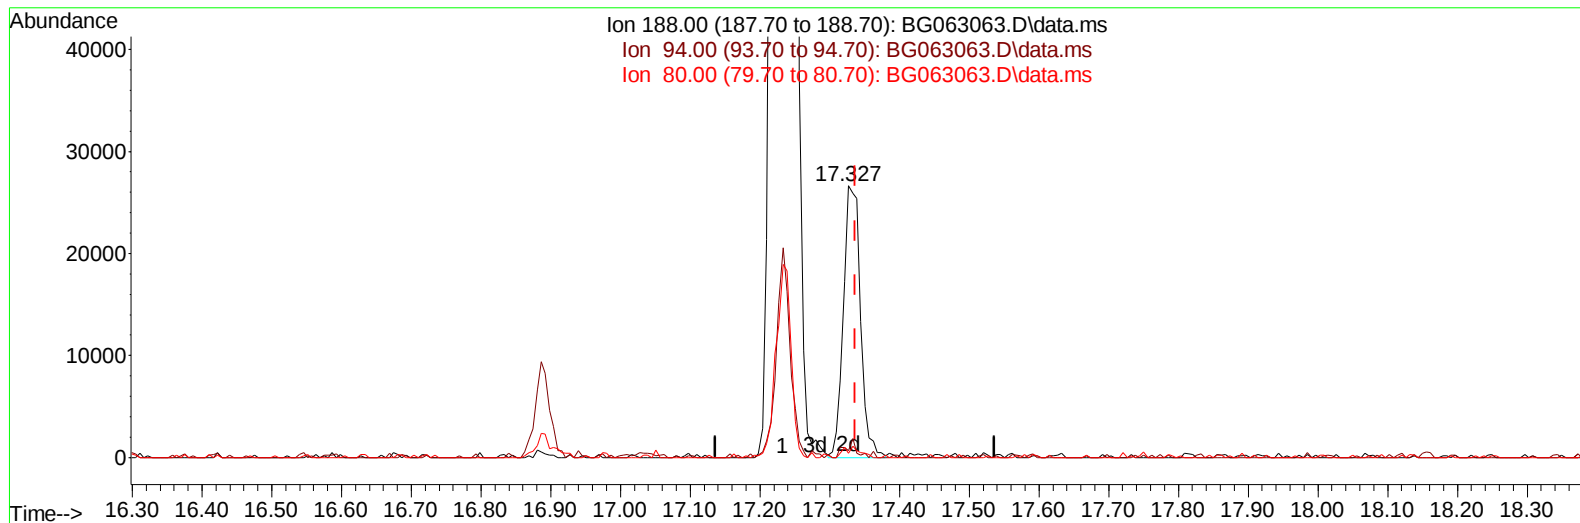

TIC: BG063063.D\data.ms

(73) Anthracene-d10 (S)

17.327min (-0.009) 1.14 ng/u1 m

response 45373

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	3.30	2.51#
80.00	3.00	1.54#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
 Data File : BG063063.D
 Acq On : 26 Sep 2024 13:46
 Operator : RC/JU
 Sample : P3879-11DL2 50X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCVZ9DL2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/27/2024
 Supervised By :mohammad ahmed 09/27/2024

Quant Time: Sep 26 15:03:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 25 13:16:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.844	152	86958	20.000	ng/ul	0.00
20) Naphthalene-d8	10.641	136	349582	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.483	164	313759	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	830505	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.487	240	1045310	20.000	ng/ul	# 0.00
88) Perylene-d12	24.524	264	1165473	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	0.000	99	0d	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0d	0.000	ng/ul	
11) 2-Chlorophenol-d4	7.380	132	4657	0.882	ng/ul	0.00
15) 4-Methylphenol-d8	8.555	113	3789	0.781	ng/ul	0.00
21) Nitrobenzene-d5	9.013	128	2914m	1.134	ng/ul	0.01
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	10.271	165	7422	1.083	ng/ul	0.00
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	13.884	166	23700	0.950	ng/ul	0.00
49) Acenaphthylene-d8	14.178	160	24934	0.943	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.476	176	21954	0.960	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.327	188	45373m	1.139	ng/ul	0.00
81) Pyrene-d10	19.624	212	60792	1.033	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.313	264	67735	1.085	ng/ul	0.00
Target Compounds						
					Qvalue	
23) Isophorone	9.566	82	54897	5.858	ng/ul	94
30) Naphthalene	10.688	128	51864	2.919	ng/ul#	95
36) 2-Methylnaphthalene	12.298	142	30756	2.134	ng/ul	87
37) 1-Methylnaphthalene	12.521	142	19337	1.327	ng/ul#	96
58) 2,3,4,6-Tetrachlorophenol	15.112	232	393332	47.772	ng/ul	96
71) Pentachlorophenol	16.892	266	993835	140.642	ng/ul	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
Data File : BG063063.D
Acq On : 26 Sep 2024 13:46
Operator : RC/JU
Sample : P3879-11DL2 50X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCVZ9DL2

Manual IntegrationsAPPROVED

Quant Time: Sep 26 15:03:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 25 13:16:45 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2024
Supervised By :mohammad ahmed 09/27/2024

