

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
 Data File : BG063036.D
 Acq On : 25 Sep 2024 16:44
 Operator : RC/JU
 Sample : PB163543BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK543

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.718	104	107	116	rBV	178456	260188	4.95%	0.733%
2	4.529	243	245	251	rBV4	5183	9666	0.18%	0.027%
3	5.346	380	384	387	rVB4	5118	6923	0.13%	0.019%
4	5.463	402	404	407	rBV3	5030	6497	0.12%	0.018%
5	5.540	414	417	420	rBV4	5171	8734	0.17%	0.025%
6	5.828	463	466	469	rBV3	5588	6387	0.12%	0.018%
7	6.609	595	599	602	rVB4	4372	6011	0.11%	0.017%
8	7.020	662	669	679	rBV	242548	403278	7.68%	1.136%
9	7.179	690	696	706	rVB	160287	267739	5.10%	0.754%
10	7.385	723	731	741	rBV	269394	441887	8.41%	1.245%
11	7.849	802	810	820	rVB	233201	406615	7.74%	1.145%
12	8.407	902	905	907	rBV	4706	6198	0.12%	0.017%
13	8.554	924	930	943	rBV	336581	574924	10.94%	1.619%
14	9.001	999	1006	1016	rBV	258852	444708	8.46%	1.253%
15	9.171	1031	1035	1037	rBV3	6274	8361	0.16%	0.024%
16	9.189	1037	1038	1042	rVV	6342	6672	0.13%	0.019%
17	9.523	1092	1095	1098	rVB	6539	8224	0.16%	0.023%
18	9.723	1122	1129	1138	rBV	264950	471403	8.97%	1.328%
19	9.911	1160	1161	1166	rVB4	6309	7838	0.15%	0.022%
20	10.264	1212	1221	1231	rBV	432149	785710	14.95%	2.213%
21	10.640	1278	1285	1292	rBV	380311	673740	12.82%	1.898%
22	10.775	1300	1308	1320	rBV	375303	728002	13.86%	2.050%
23	10.963	1338	1340	1343	rBV2	5863	9091	0.17%	0.026%
24	11.392	1410	1413	1417	rBV2	5305	7979	0.15%	0.022%
25	11.503	1428	1432	1434	rBV3	6432	7593	0.14%	0.021%
26	12.244	1554	1558	1559	rBV3	7824	8596	0.16%	0.024%
27	12.702	1629	1636	1637	rBV4	6408	10388	0.20%	0.029%
28	12.831	1656	1658	1661	rBV	8046	7111	0.14%	0.020%
29	13.290	1730	1736	1737	rBV3	3655	6691	0.13%	0.019%
30	13.554	1775	1781	1784	rBV3	3817	7951	0.15%	0.022%
31	13.889	1832	1838	1850	rVB	1209538	1701860	32.39%	4.793%
32	14.177	1878	1887	1896	rBV	1124193	1835754	34.94%	5.171%
33	14.482	1932	1939	1946	rBV	835066	1282268	24.41%	3.612%
34	14.688	1967	1974	1983	rBV	405907	680273	12.95%	1.916%
35	15.117	2046	2047	2052	rBV2	8163	10955	0.21%	0.031%
36	15.422	2096	2099	2101	rBV2	5517	6684	0.13%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
 Data File : BG063036.D
 Acq On : 25 Sep 2024 16:44
 Operator : RC/JU
 Sample : PB163543BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK543

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Title : SVOA CALIBRATION

37	15.481	2101	2109	2115	rBV	1686823	2512554	47.82%	7.077%
38	15.599	2123	2129	2137	rBV	530526	804476	15.31%	2.266%
39	15.722	2146	2150	2154	rVB6	6954	9621	0.18%	0.027%
40	16.045	2203	2205	2208	rVB2	5598	6646	0.13%	0.019%
41	16.421	2267	2269	2274	rBV4	4577	8110	0.15%	0.023%
42	16.927	2348	2355	2358	rBV5	6735	15520	0.30%	0.044%
43	17.232	2401	2407	2416	rBV	1354461	2065414	39.31%	5.817%
44	17.332	2418	2424	2434	rVB2	2090428	3176539	60.46%	8.947%
45	17.896	2518	2520	2521	rBV2	8906	8857	0.17%	0.025%
46	18.178	2564	2568	2569	rBV4	4605	6058	0.12%	0.017%
47	18.442	2608	2613	2616	rBV3	7040	10635	0.20%	0.030%
48	19.089	2722	2723	2726	rBV3	7387	6405	0.12%	0.018%
49	19.194	2735	2741	2746	rBV3	41386	63532	1.21%	0.179%
50	19.265	2749	2753	2756	rBV	38077	54753	1.04%	0.154%
51	19.559	2802	2803	2806	rVB3	12522	6469	0.12%	0.018%
52	19.629	2809	2815	2825	rVV	3132978	4354342	82.88%	12.264%
53	21.392	3112	3115	3117	rBV4	23726	23878	0.45%	0.067%
54	21.486	3124	3131	3138	rBV2	1852490	2985756	56.83%	8.410%
55	24.312	3603	3612	3629	rVB2	2034075	5253974	100.00%	14.798%
56	24.523	3638	3648	3660	rBV	1134640	3007520	57.24%	8.471%




Sum of corrected areas: 35503958

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
Data File : BG063036.D
Acq On : 25 Sep 2024 16:44
Operator : RC/JU
Sample : PB163543BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

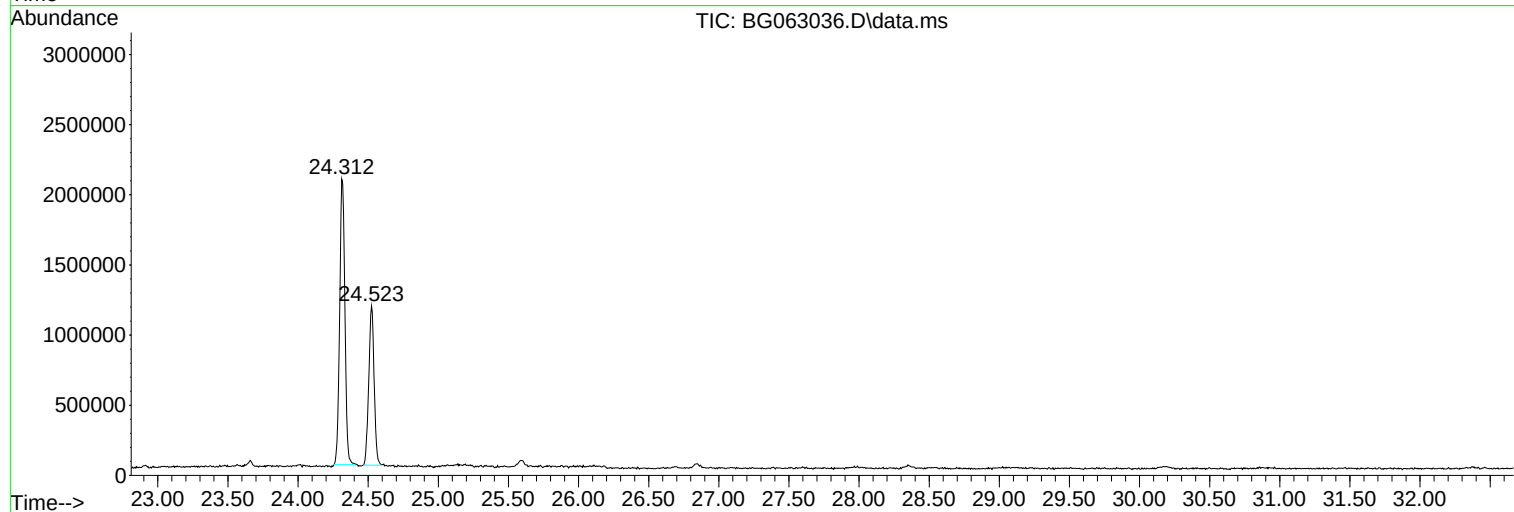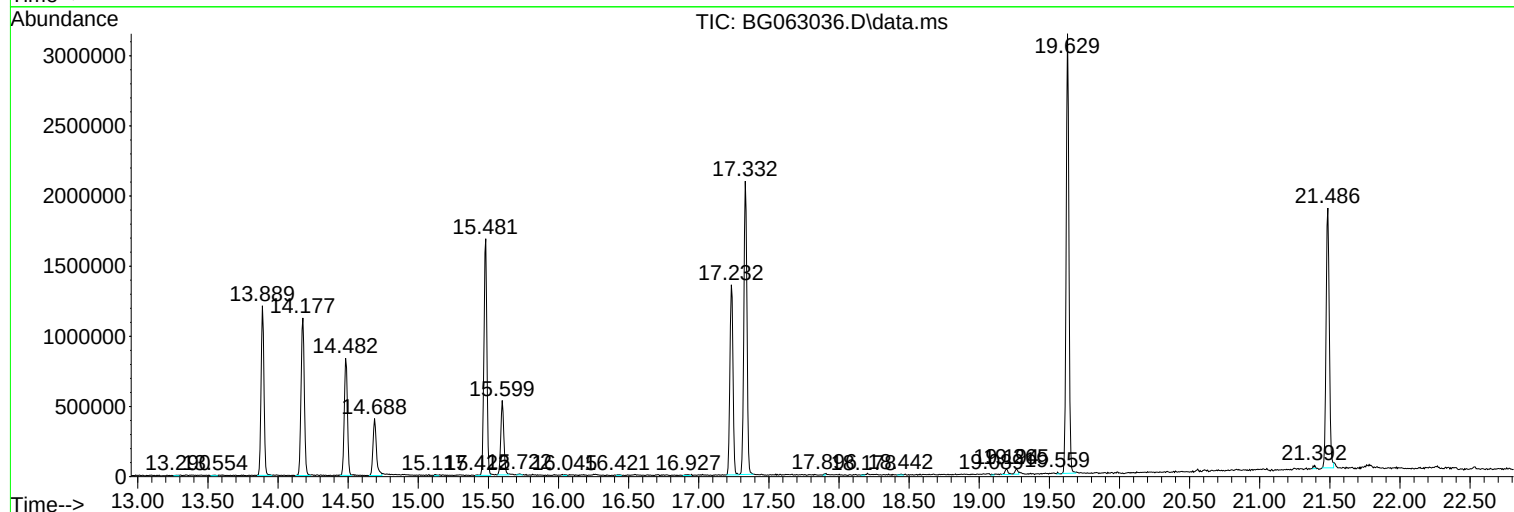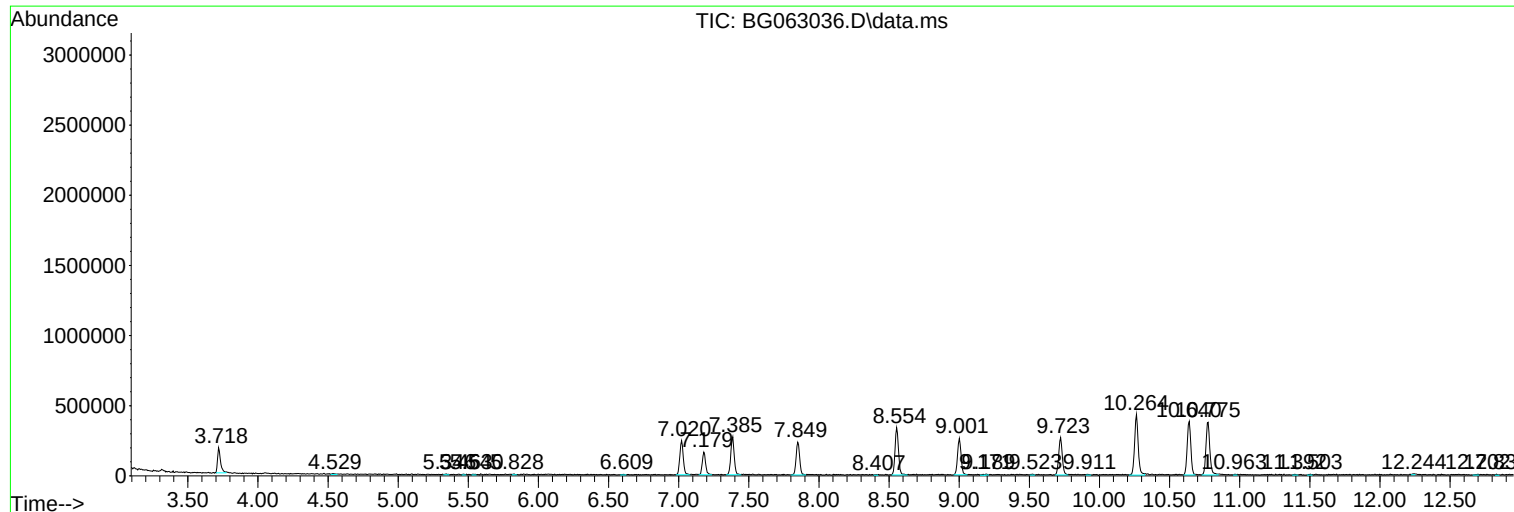

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
Data File : BG063036.D
Acq On : 25 Sep 2024 16:44
Operator : RC/JU
Sample : PB163543BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092524\
Data File : BG063036.D
Acq On : 25 Sep 2024 16:44
Operator : RC/JU
Sample : PB163543BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK543

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------