

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092525\
 Data File : BG064453.D
 Acq On : 25 Sep 2025 21:30
 Operator : RC/JU
 Sample : PB169726BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB169726BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG064453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.961	312	319	326	rBV2	51248	76508	3.31%	0.906%
2	5.431	392	399	407	rBV	394600	618143	26.72%	7.324%
3	7.012	661	668	680	rBV	411619	701006	30.30%	8.305%
4	7.834	802	808	815	rBV	77389	129534	5.60%	1.535%
5	8.992	997	1005	1012	rBV	264127	470538	20.34%	5.575%
6	10.625	1276	1283	1293	rBV	96424	170700	7.38%	2.022%
7	13.087	1695	1702	1709	rBV	750051	1148846	49.66%	13.611%
8	14.462	1930	1936	1944	rBV	168938	257603	11.14%	3.052%
9	15.954	2183	2190	2207	rBV	759591	1148569	49.65%	13.608%
10	17.206	2397	2403	2414	rVB2	255766	373859	16.16%	4.429%
11	19.826	2843	2849	2858	rBV	1814152	2313394	100.00%	27.408%
12	21.430	3116	3122	3138	rVB2	277094	467120	20.19%	5.534%
13	24.432	3623	3633	3643	rBV2	169119	473919	20.49%	5.615%
14	25.490	3806	3813	3821	rVB7	15277	38303	1.66%	0.454%
15	26.718	4015	4022	4024	rBV5	13953	24968	1.08%	0.296%
16	28.210	4267	4276	4279	rBV9	10667	27444	1.19%	0.325%




Sum of corrected areas: 8440454

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092525\
Data File : BG064453.D
Acq On : 25 Sep 2025 21:30
Operator : RC/JU
Sample : PB169726BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB169726BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

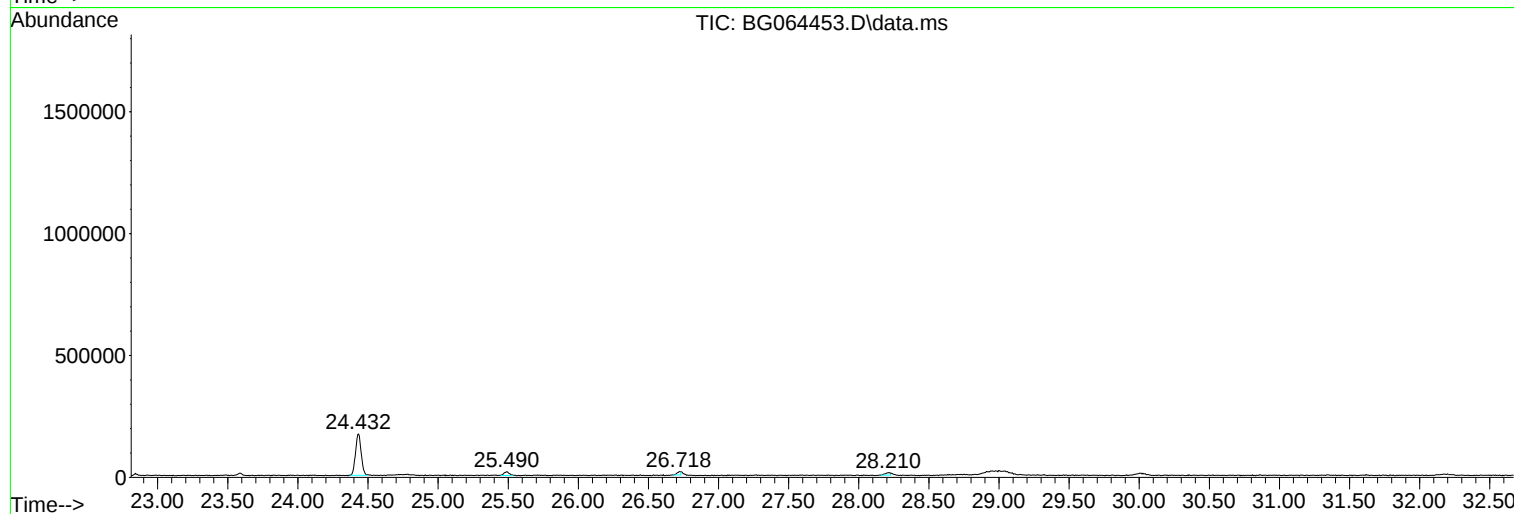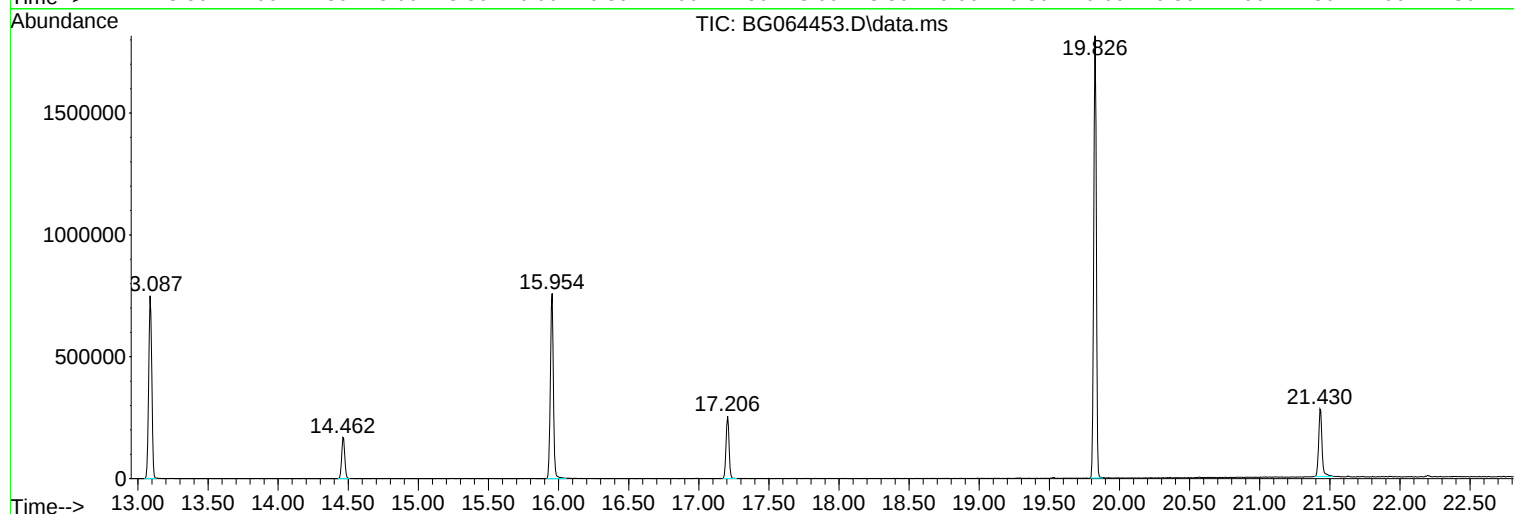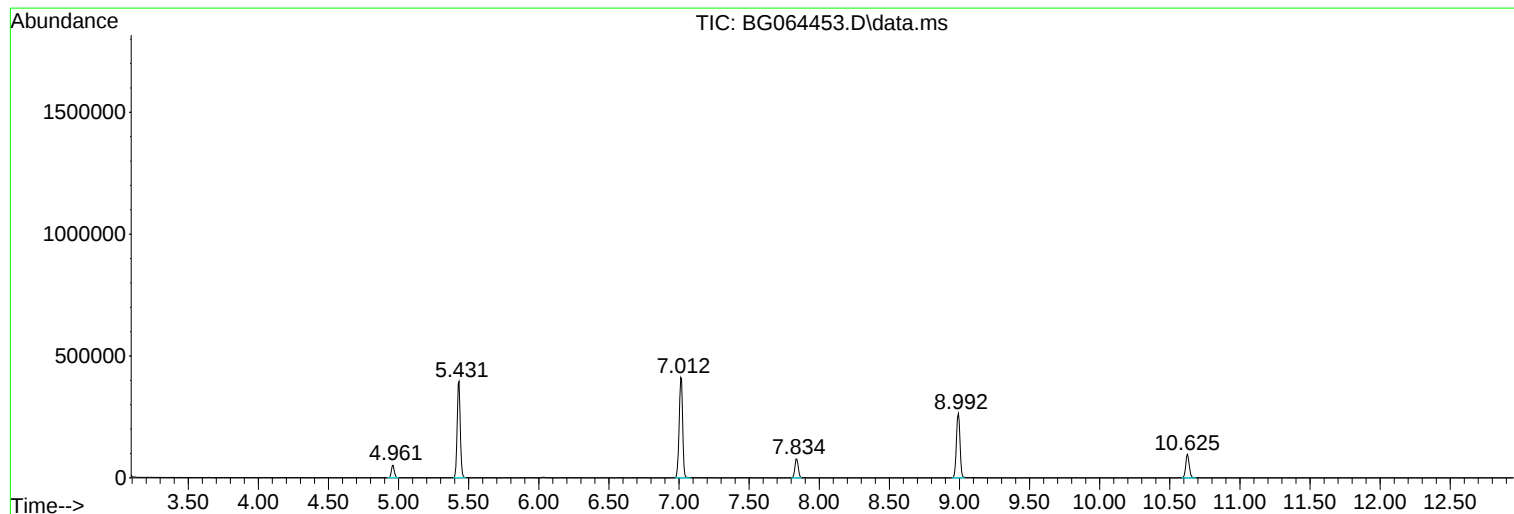

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092525\
Data File : BG064453.D
Acq On : 25 Sep 2025 21:30
Operator : RC/JU
Sample : PB169726BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB169726BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092525\
Data File : BG064453.D
Acq On : 25 Sep 2025 21:30
Operator : RC/JU
Sample : PB169726BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB169726BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------