
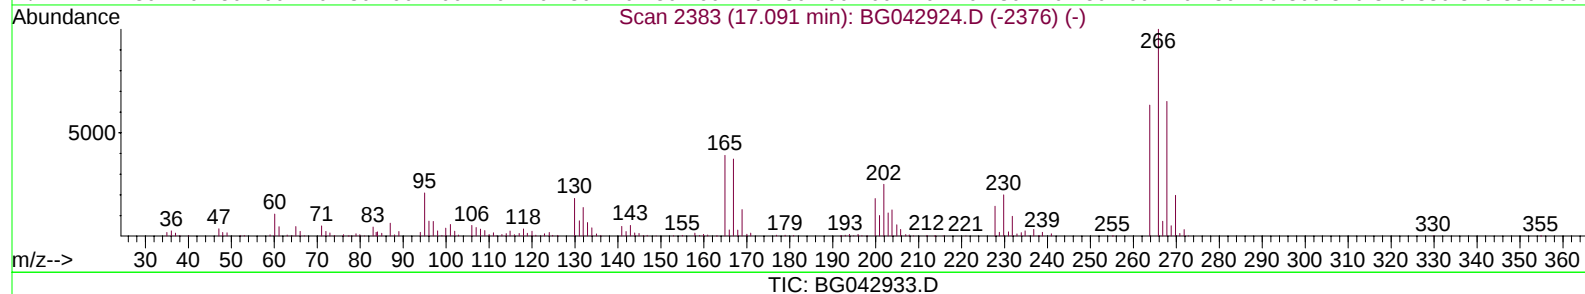
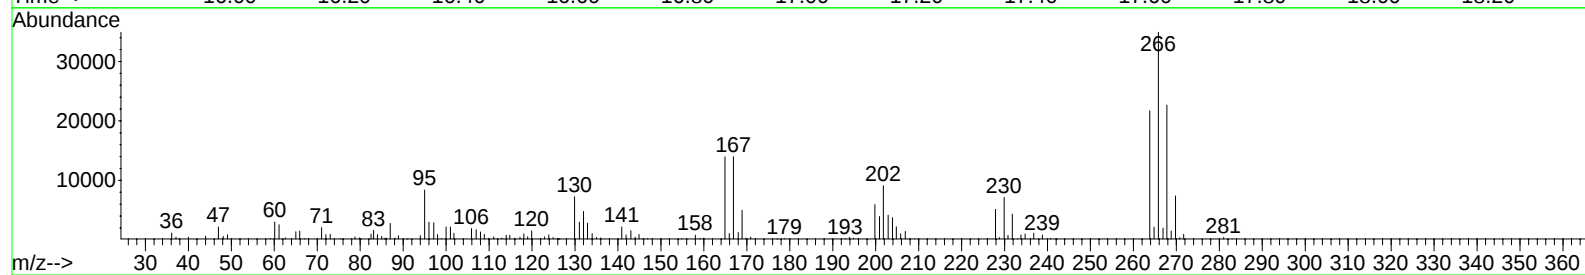


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092619\
Data File : BG042933.D
Acq On : 26 Sep 2019 10:00
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 18:51:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 15:35:52 2019
Response via : Initial Calibration

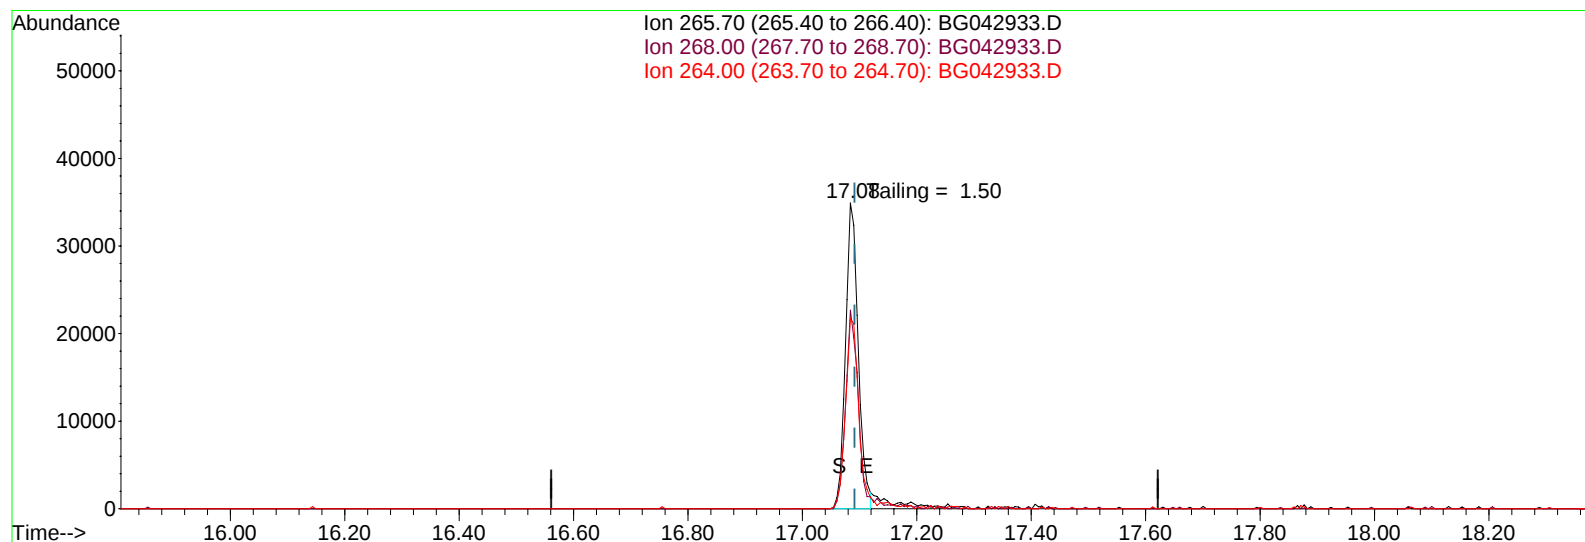

TIC: BG042933.D

(70) Pentachlorophenol (C)




17.084min (-0.008) 0.00ng

response 56660

Ion	Exp%	Act%
265.70	100	100
268.00	65.20	64.92
264.00	63.40	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG092619\
Data File : BG042933.D
Acq On : 26 Sep 2019 10:00
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 18:51:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 15:35:52 2019
Response via : Initial Calibration

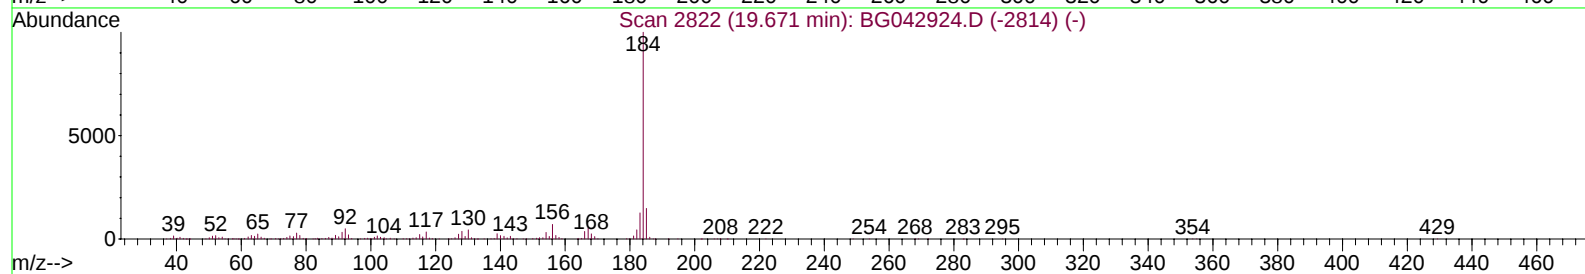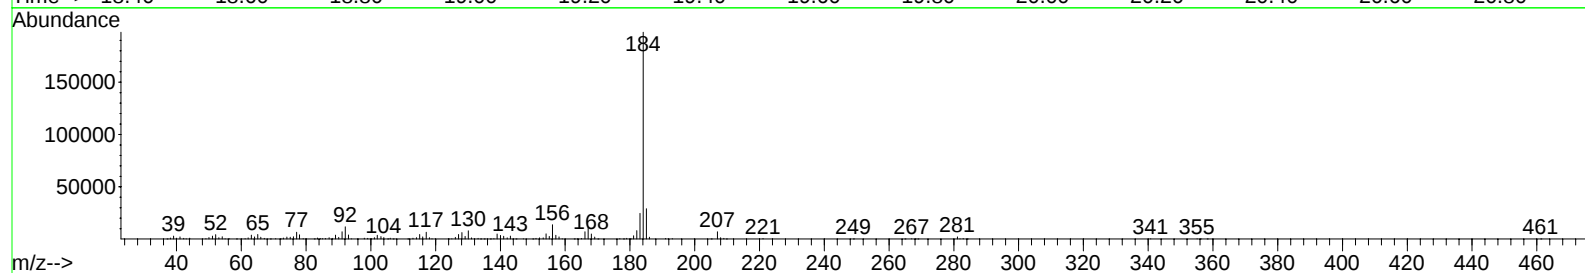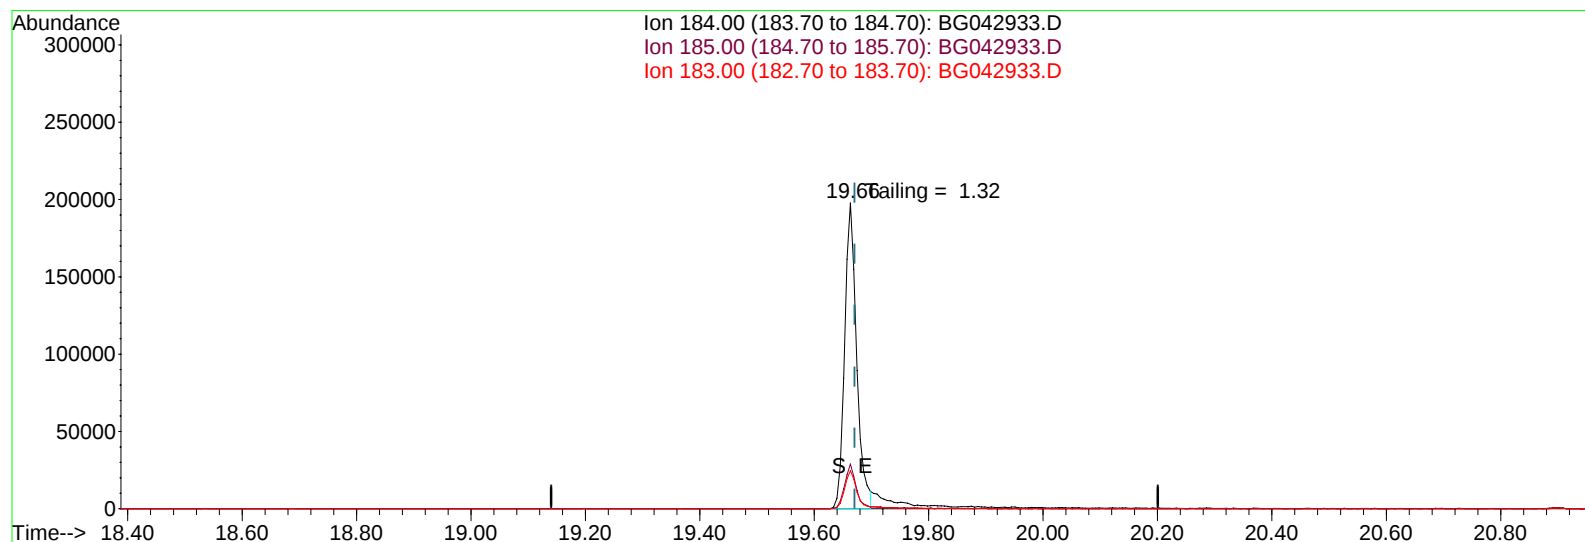

(77) Benzidine

19.663min (-0.008) 0.00ng

response 306873

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.66
183.00	12.60	12.44
0.00	0.00	0.00