


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG092619\
 Data File : BG042933.D
 Acq On : 26 Sep 2019 10:00
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 25 15:35:52 2019

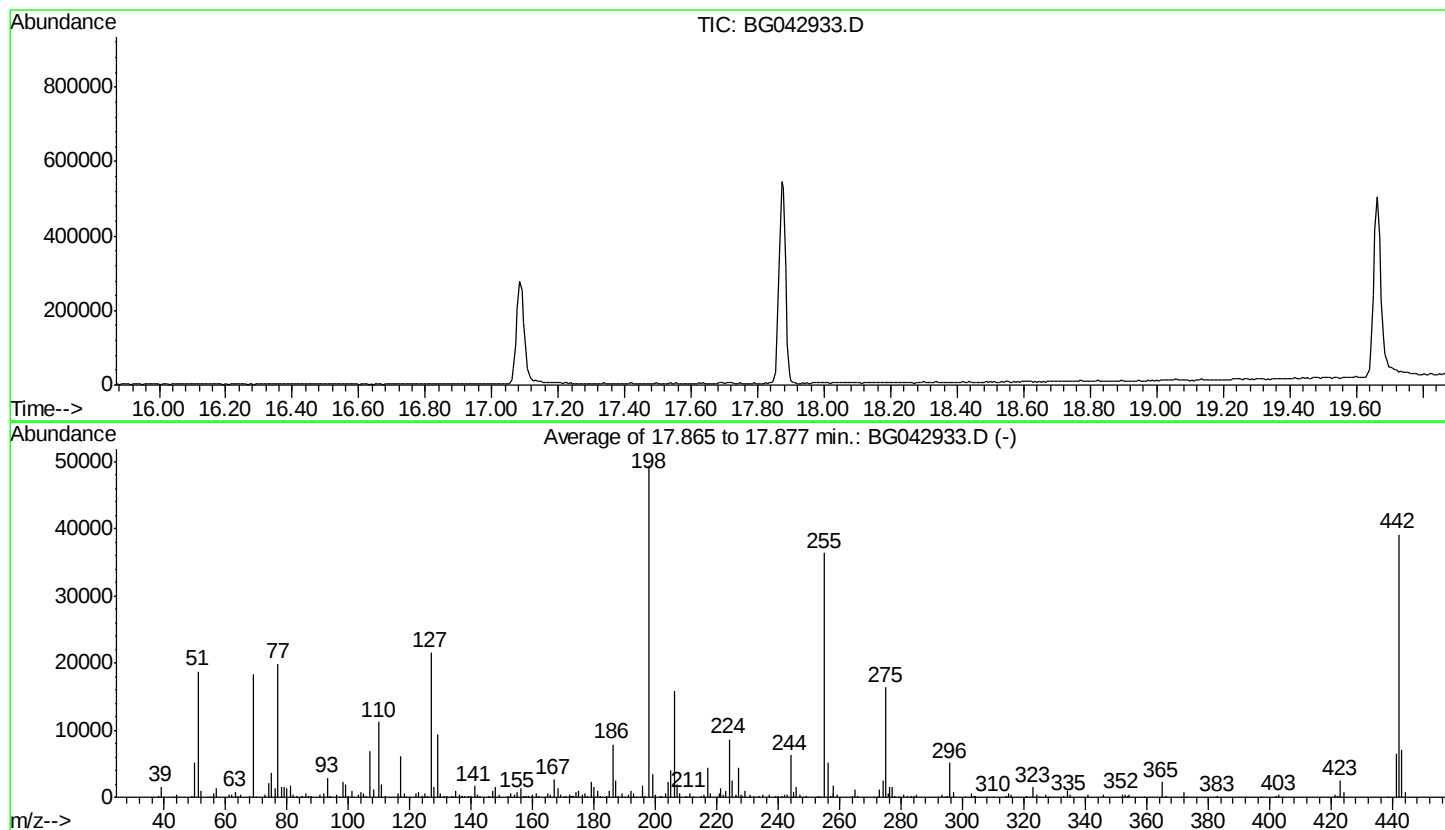

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	18772	PASS
68	69	0.00	2	0.7	136	PASS
69	198	0.00	100	37.2	18353	PASS
70	69	0.00	2	0.4	65	PASS
127	198	10	80	43.5	21472	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49365	PASS
199	198	5	9	7.1	3488	PASS
275	198	10	60	33.2	16369	PASS
365	198	1	100	4.5	2219	PASS
441	198	0.01	100	13.1	6464	PASS
442	198	50	100	79.3	39152	PASS
443	442	15	24	17.9	6989	PASS