


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092622\
Data File : BG055022.D
Acq On : 26 Sep 2022 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 19 17:41:40 2022

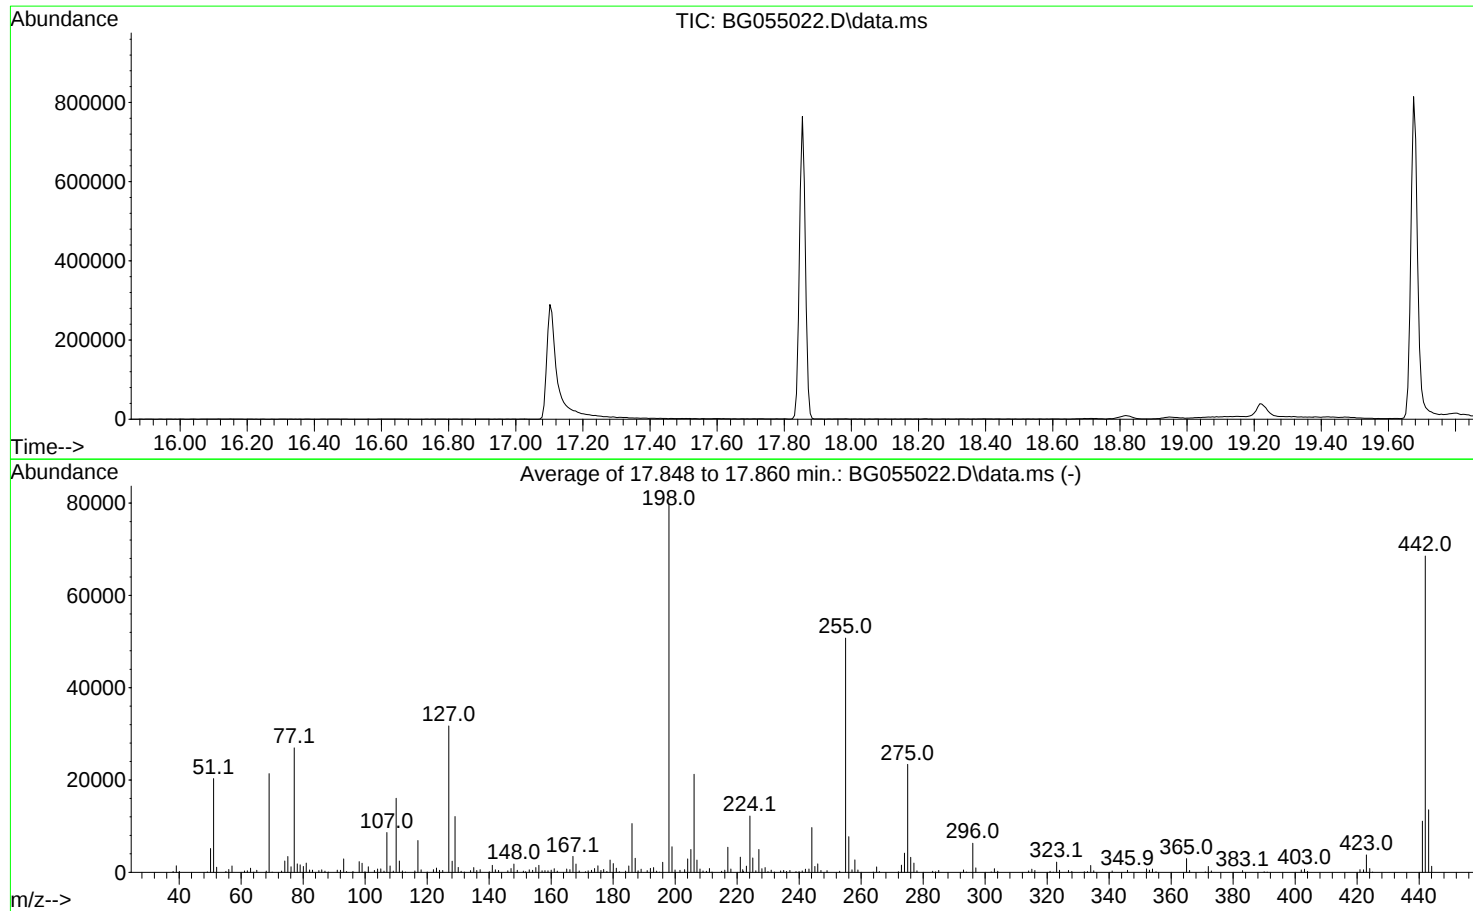




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	20296	PASS
68	69	0.00	2	1.3	275	PASS
69	198	0.00	100	26.8	21371	PASS
70	69	0.00	2	0.2	51	PASS
127	198	10	80	39.8	31725	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	79720	PASS
199	198	5	9	6.9	5522	PASS
275	198	10	60	29.3	23381	PASS
365	198	1	100	3.7	2980	PASS
441	198	0.01	100	13.9	11092	PASS
442	442	50	100	100.0	68536	PASS
443	442	15	24	19.8	13539	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092622\
Data File : BG055022.D
Acq On : 26 Sep 2022 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 27 06:38:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

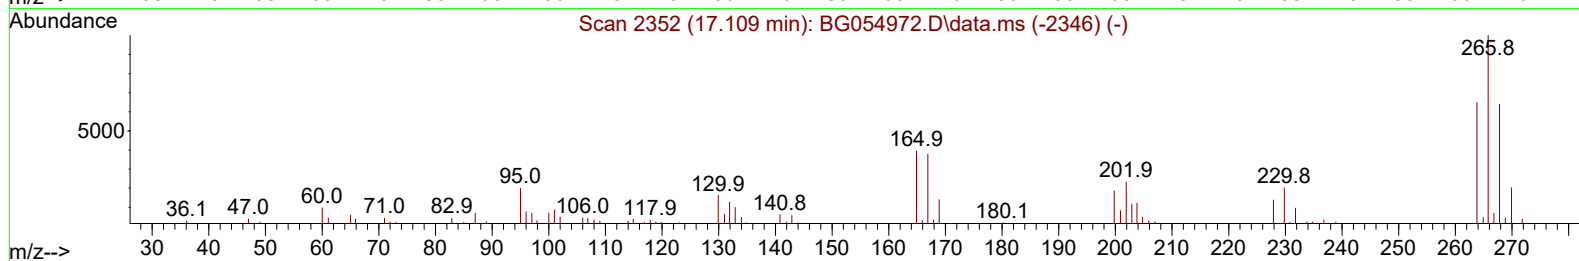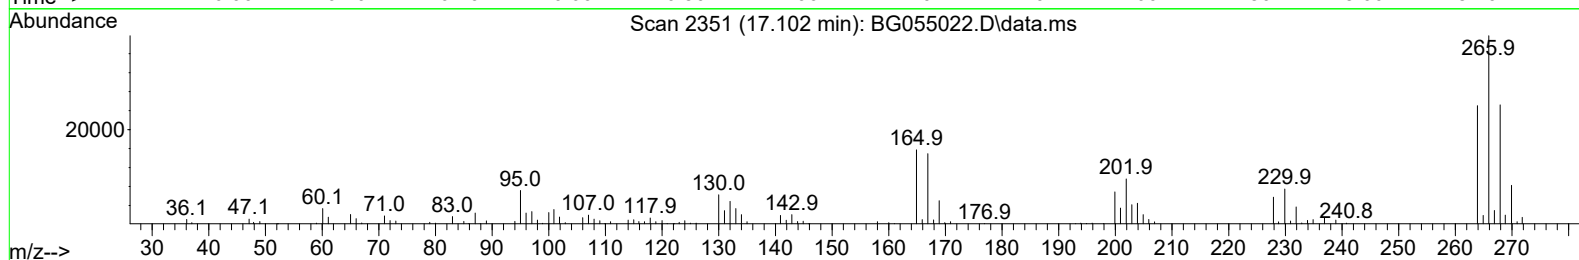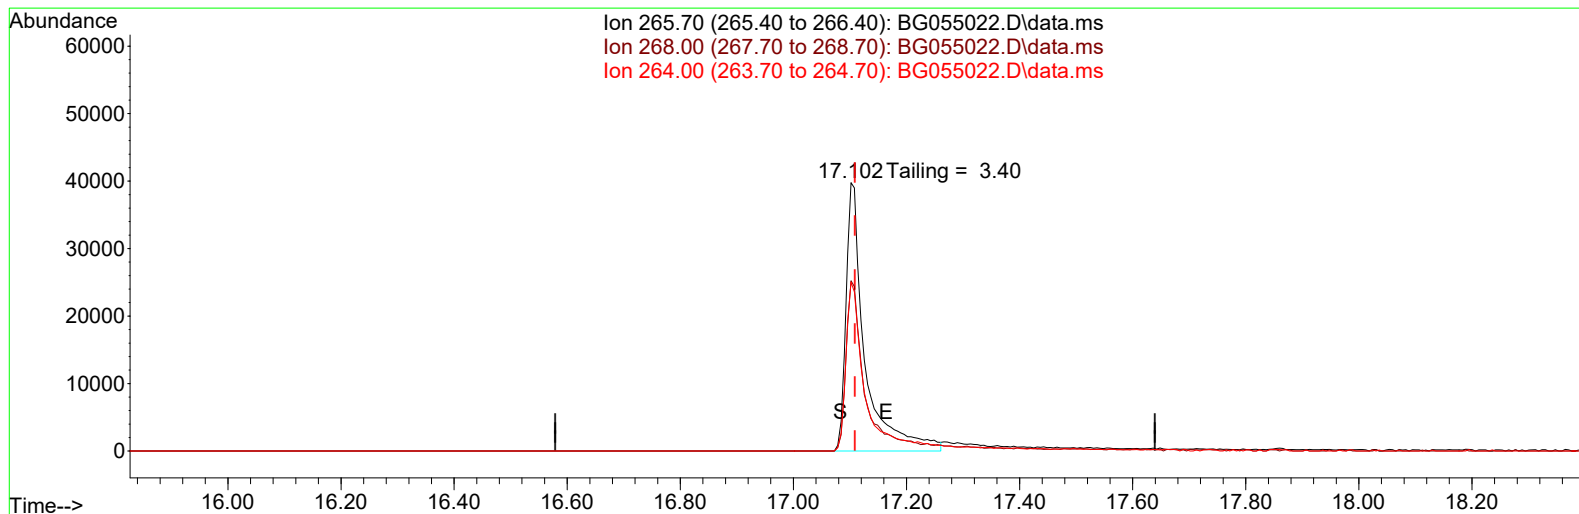

TIC: BG055022.D\data.ms

(70) Pentachlorophenol (C)

17.102min (-0.007) 3592.01 ng




response 93230

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.42
264.00	61.70	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092622\
Data File : BG055022.D
Acq On : 26 Sep 2022 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 27 06:38:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

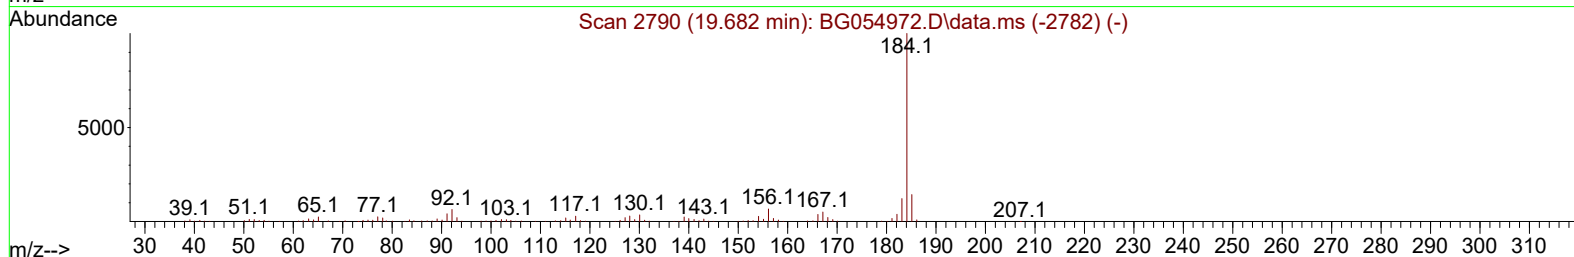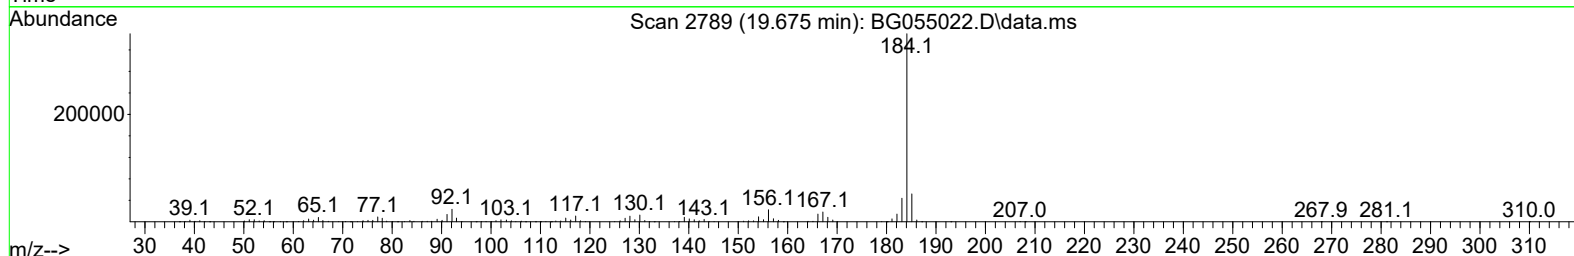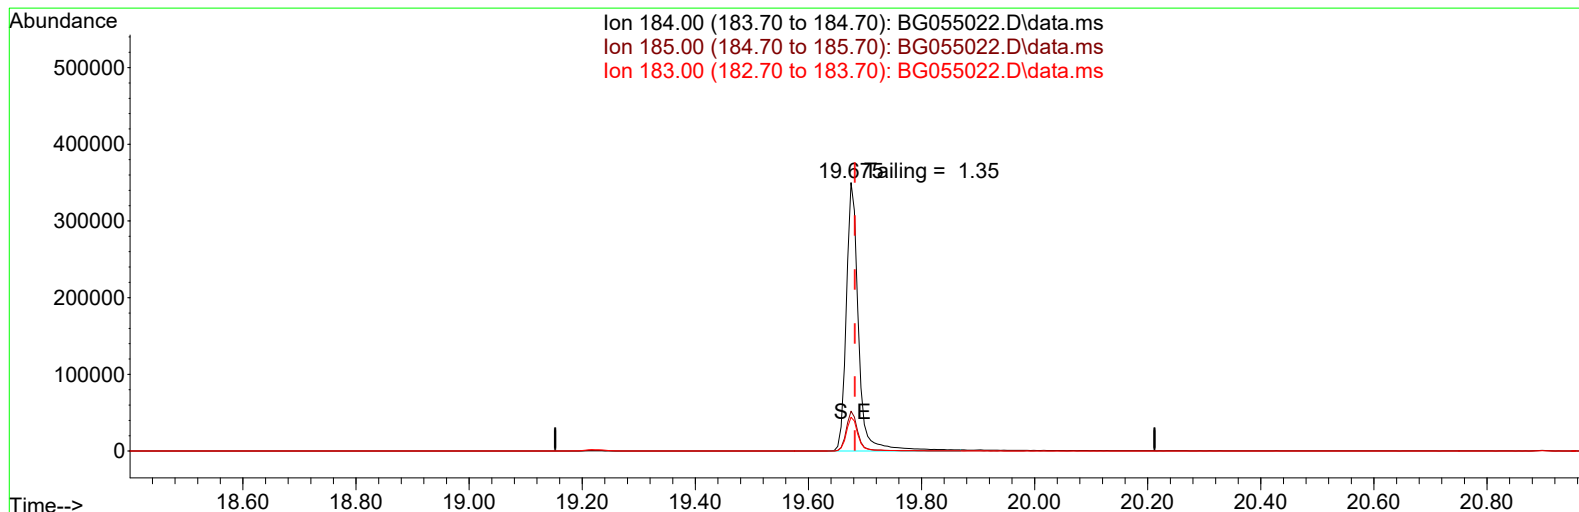

TIC: BG055022.D\data.ms

(77) Benzidine

19.675min (-0.007) 0.00 ng

response 529045

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.84
183.00	12.30	12.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/26/2022	BNA_G	BG055022.D
Compound Name	Response	Retention Time
DDT	261438	20.897
DDD	9691	20.457
DDE	111	19.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9802	271240	3.61

Instrument :
BNA_G
ClientSampleId :
DFTPP