




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
 Data File : BG059203.D
 Acq On : 26 Sep 2023 19:46
 Operator : MA/JU
 Sample : PB155788BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK788

Manual IntegrationsAPPROVED

Quant Time: Sep 26 23:50:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 23:48:55 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :mohammad ahmed 09/29/2023

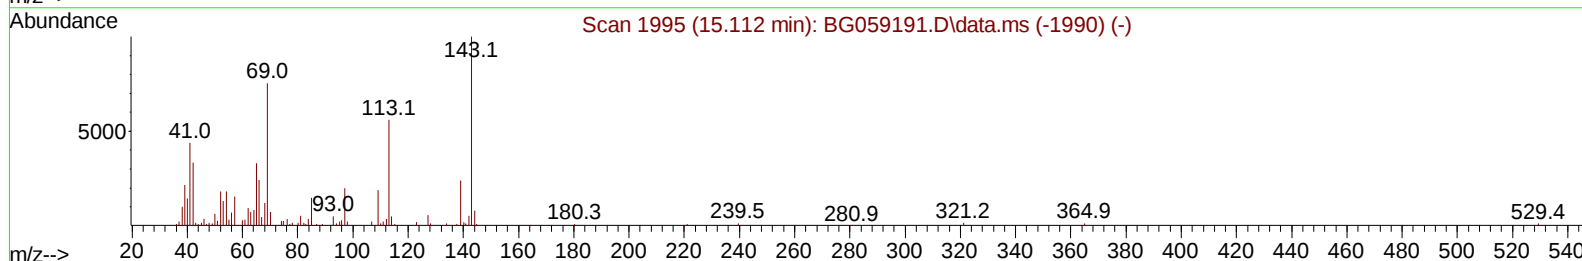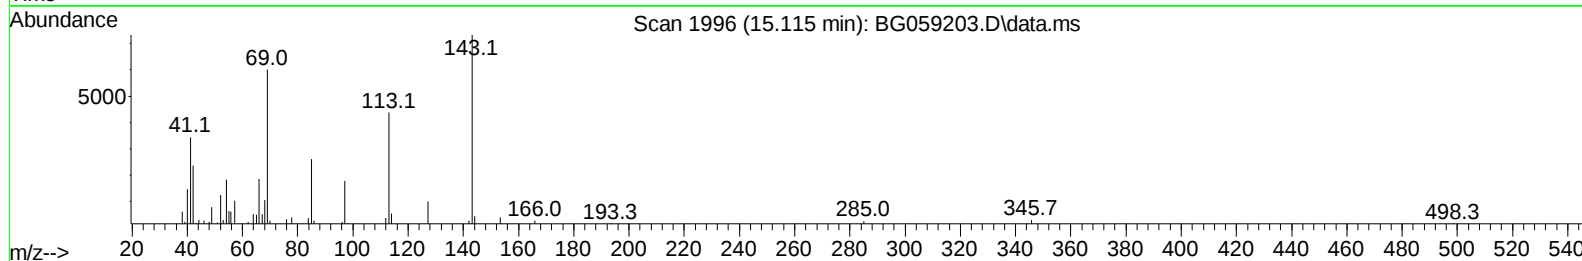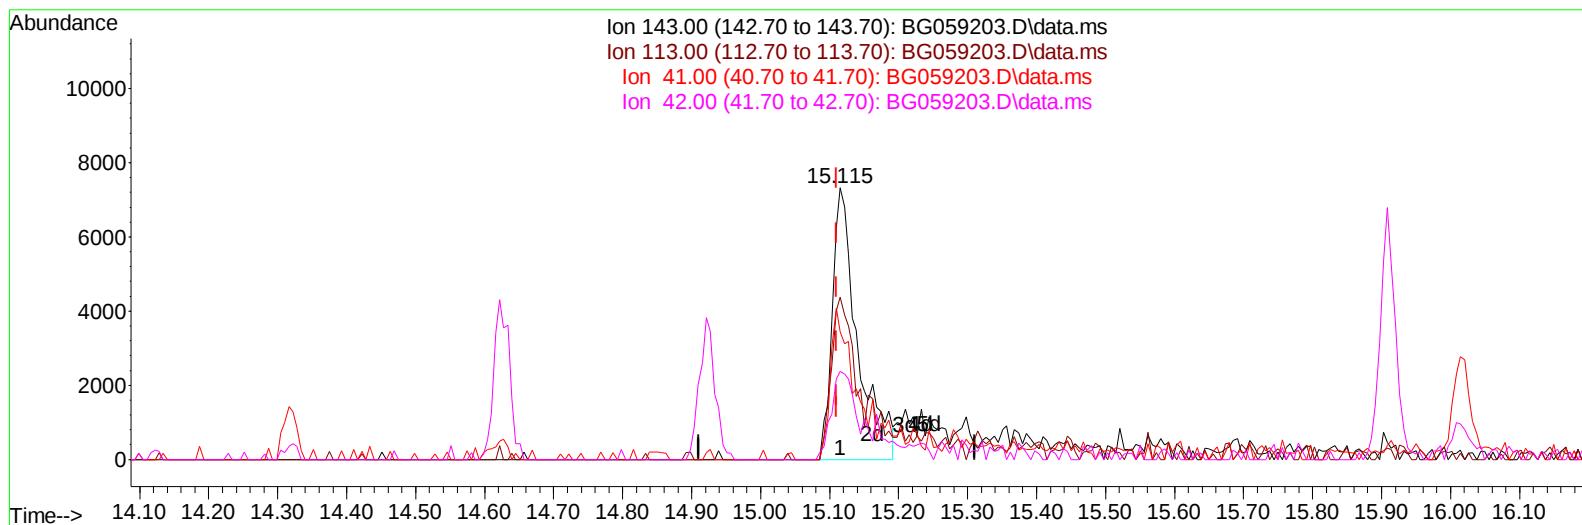

TIC: BG059203.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.115min (+ 0.005) 9.18 ng/ul m

response 18670

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	69.10	59.80
41.00	52.00	47.06
42.00	40.70	32.47#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
 Data File : BG059203.D
 Acq On : 26 Sep 2023 19:46
 Operator : MA/JU
 Sample : PB155788BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK788

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :mohammad ahmed 09/29/2023

Quant Time: Sep 26 23:57:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 23:48:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.300	152	36113	20.000	ng/ul	0.00
20) Naphthalene-d8	11.138	136	195654	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.921	164	144974	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.677	188	346639	20.000	ng/ul	0.00
79) Chrysene-d12	21.990	240	259332	20.000	ng/ul	0.00
88) Perylene-d12	25.538	264	295116	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.605	96	6650	7.208	ng/uL	0.00
4) Pyridine-d5	4.040	84	98640	36.443	ng/ul	0.00
7) Phenol-d5	7.418	99	126084	35.507	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.612	67	81303	37.310	ng/ul	0.00
11) 2-Chlorophenol-d4	7.812	132	89384	34.110	ng/ul	0.00
15) 4-Methylphenol-d8	8.987	113	95133	33.639	ng/ul	0.00
21) Nitrobenzene-d5	9.487	128	49957	33.089	ng/ul	0.00
24) 2-Nitrophenol-d4	10.209	143	54646	35.830	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.738	165	95422	32.956	ng/ul	0.00
31) 4-Chloroaniline-d4	11.284	131	145516	32.200	ng/ul	0.00
46) Dimethylphthalate-d6	14.316	166	396297	35.544	ng/ul	0.00
49) Acenaphthylene-d8	14.628	160	425299	31.328	ng/ul	0.00
54) 4-Nitrophenol-d4	15.115	143	18670m	9.178	ng/ul	0.00
60) Fluorene-d10	15.908	176	344134	33.719	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.020	200	42618	21.625	ng/ul	0.00
73) Anthracene-d10	17.771	188	532862	33.785	ng/ul	0.00
81) Pyrene-d10	20.045	212	615703	40.619	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.292	264	470705	32.665	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
Data File : BG059203.D
Acq On : 26 Sep 2023 19:46
Operator : MA/JU
Sample : PB155788BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK788

Manual IntegrationsAPPROVED

Quant Time: Sep 26 23:57:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 26 23:48:55 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :mohammad ahmed 09/29/2023

