




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
 Data File : BG059208.D
 Acq On : 26 Sep 2023 23:10
 Operator : MA/JU
 Sample : 04450-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBBN0

Manual IntegrationsAPPROVED

Quant Time: Sep 26 23:51:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 23:48:55 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :mohammad ahmed 09/29/2023

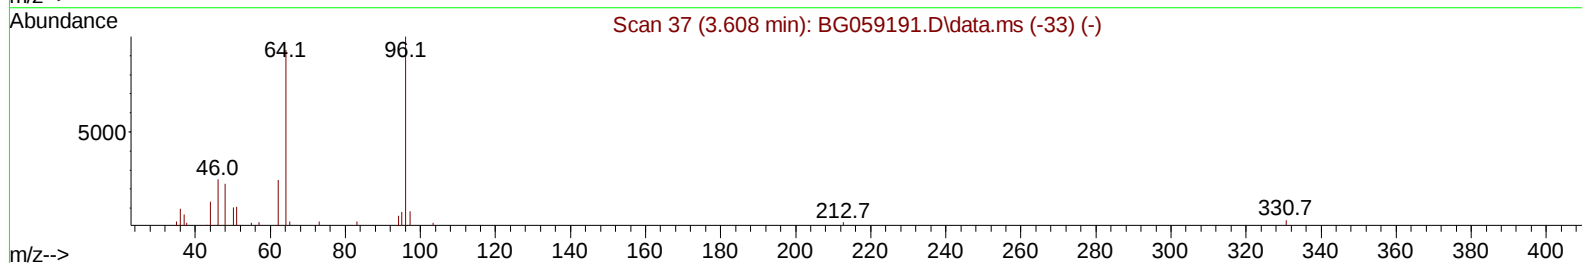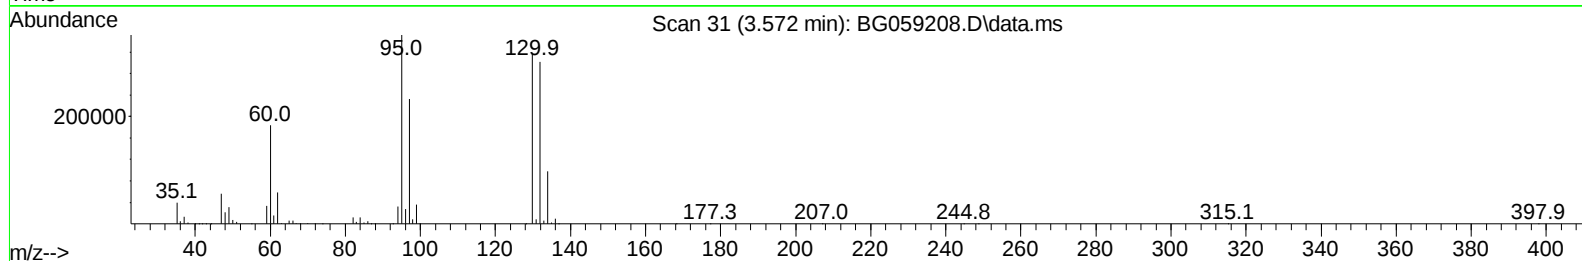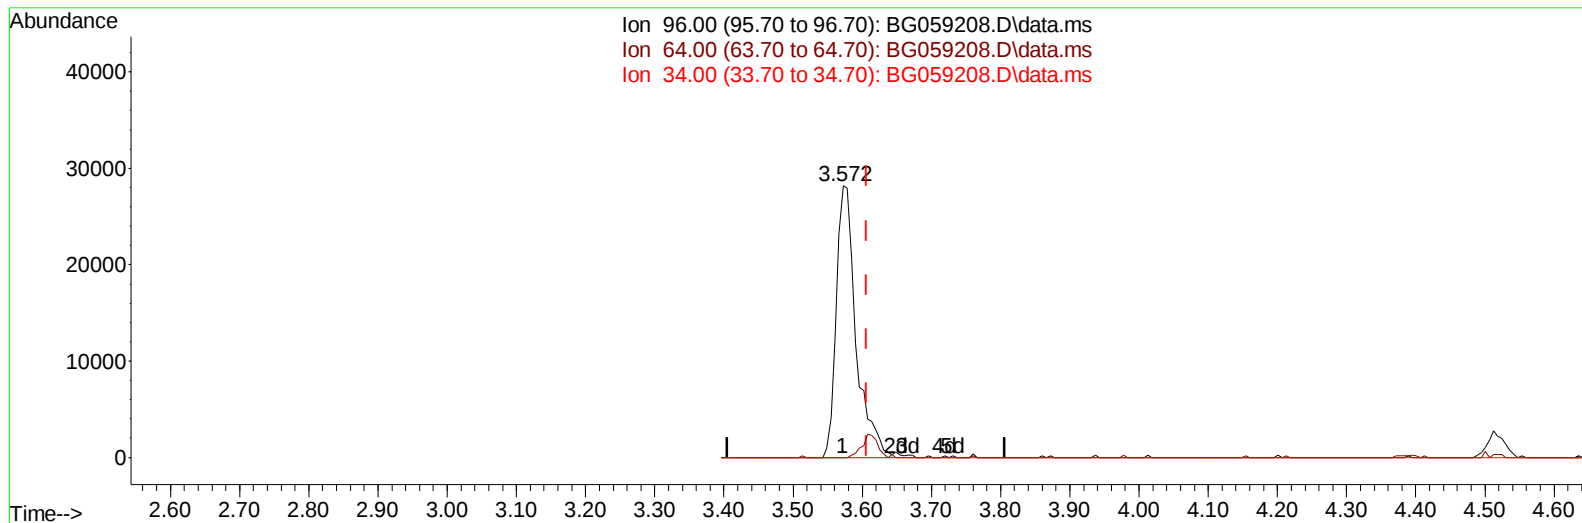

TIC: BG059208.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.572min (-0.034) 68.92 ng/uL

response 55476

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	88.00	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
 Data File : BG059208.D
 Acq On : 26 Sep 2023 23:10
 Operator : MA/JU
 Sample : 04450-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBBN0

Manual IntegrationsAPPROVED

Quant Time: Sep 26 23:51:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 23:48:55 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :mohammad ahmed 09/29/2023

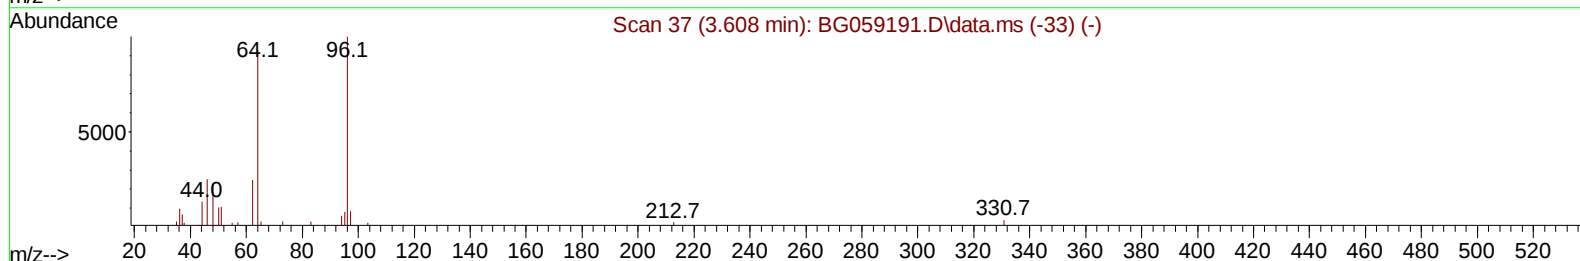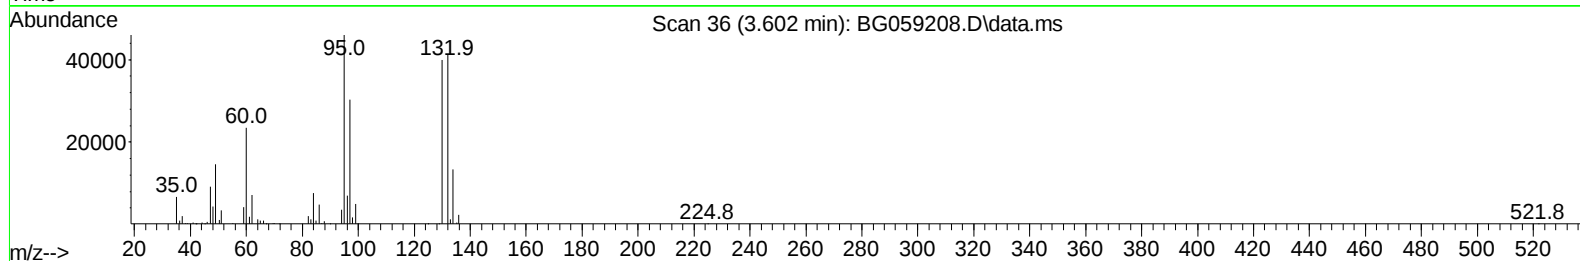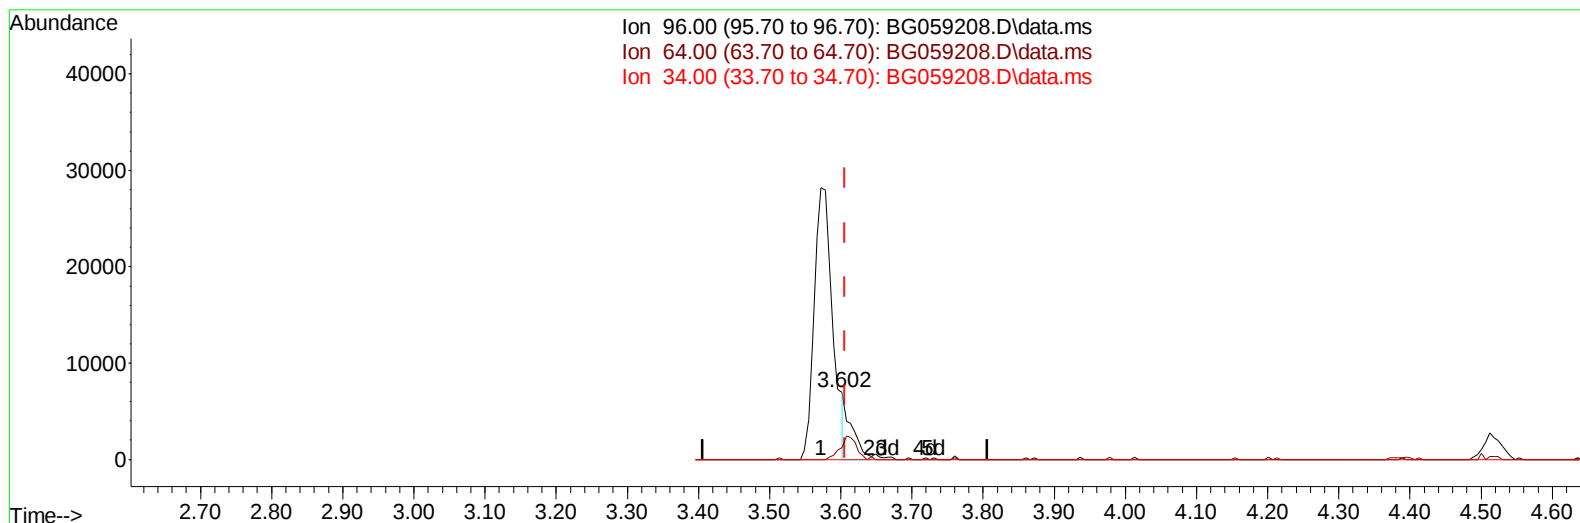

TIC: BG059208.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.602min (-0.004) 6.14 ng/uL m

response 4939

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	88.00	17.93#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
Data File : BG059208.D
Acq On : 26 Sep 2023 23:10
Operator : MA/JU
Sample : 04450-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBBN0

Manual IntegrationsAPPROVED

Quant Time: Sep 27 02:30:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 26 23:48:55 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :mohammad ahmed 09/29/2023

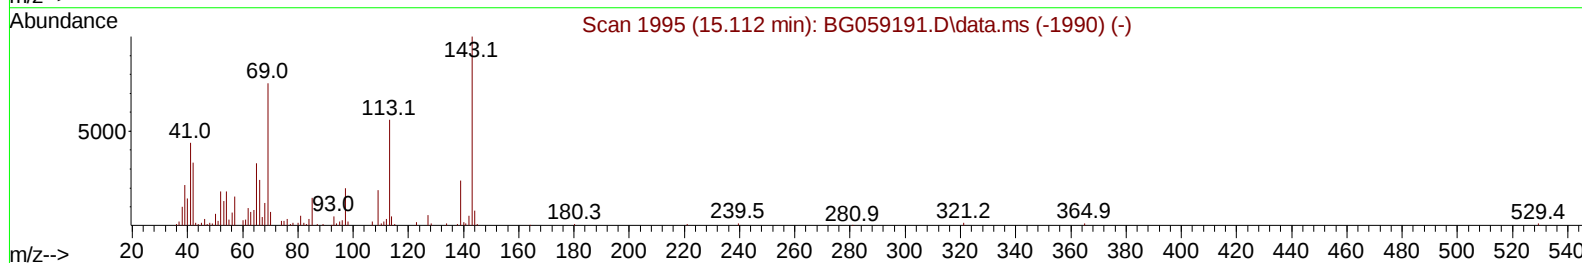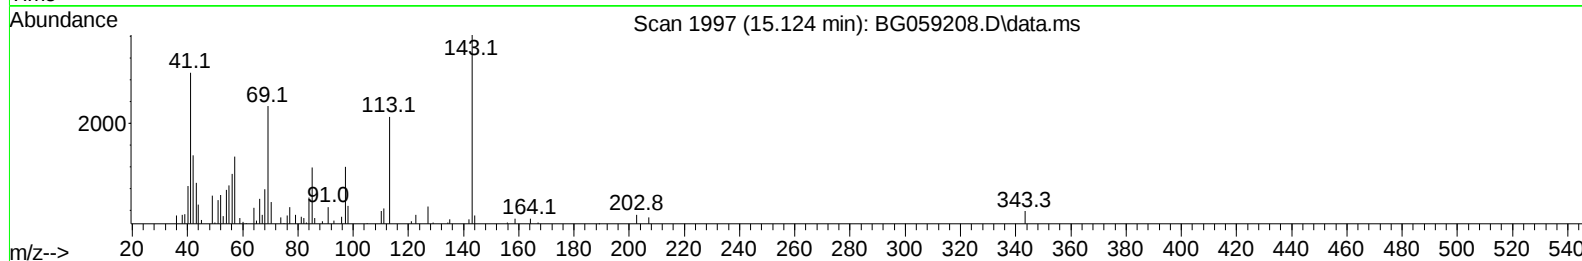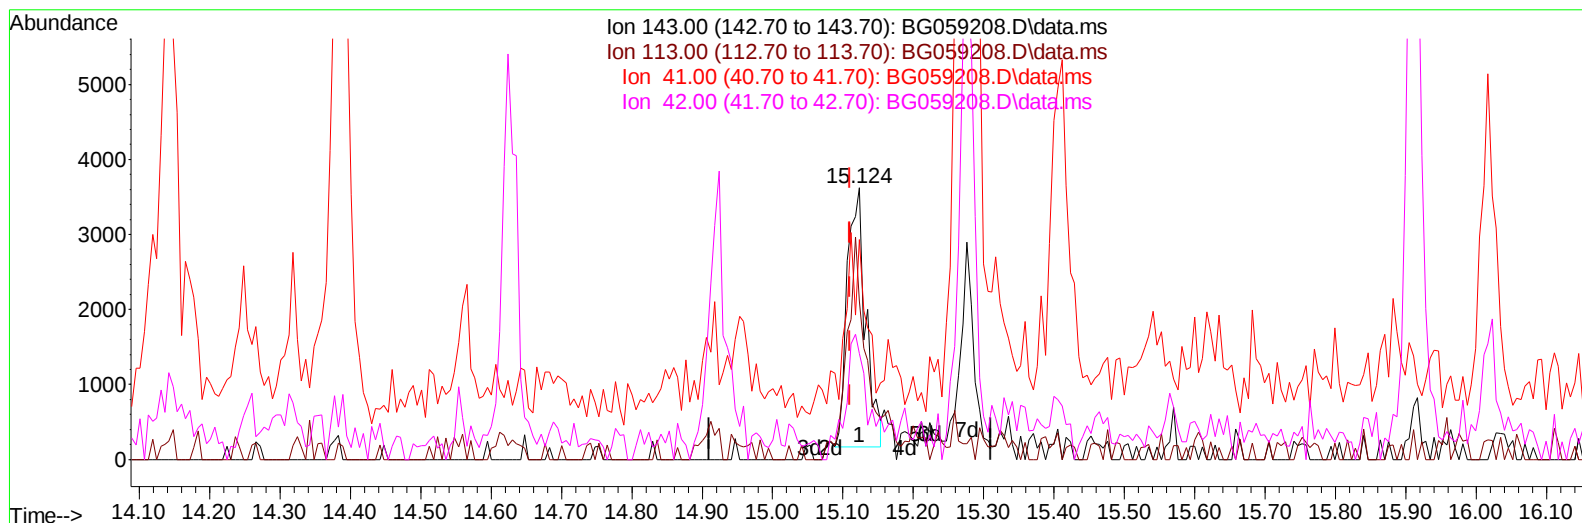

TIC: BG059208.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.124min (+ 0.013) 3.78 ng/u1

response 6214

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	69.10	58.31
41.00	52.00	80.99#
42.00	40.70	38.92




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
 Data File : BG059208.D
 Acq On : 26 Sep 2023 23:10
 Operator : MA/JU
 Sample : 04450-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBBN0

Manual IntegrationsAPPROVED

Quant Time: Sep 27 02:30:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 23:48:55 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :mohammad ahmed 09/29/2023

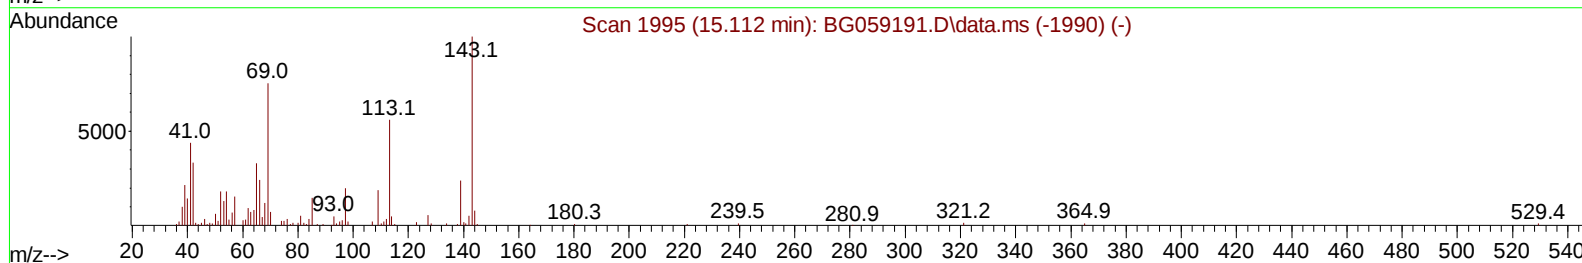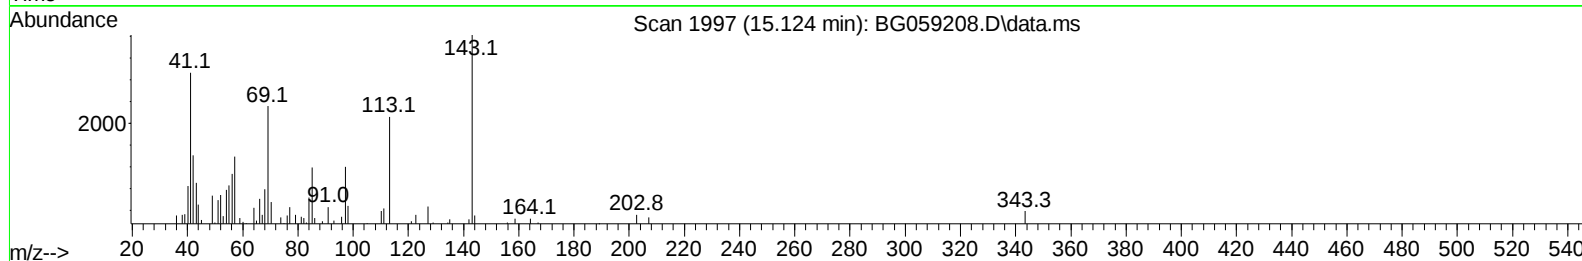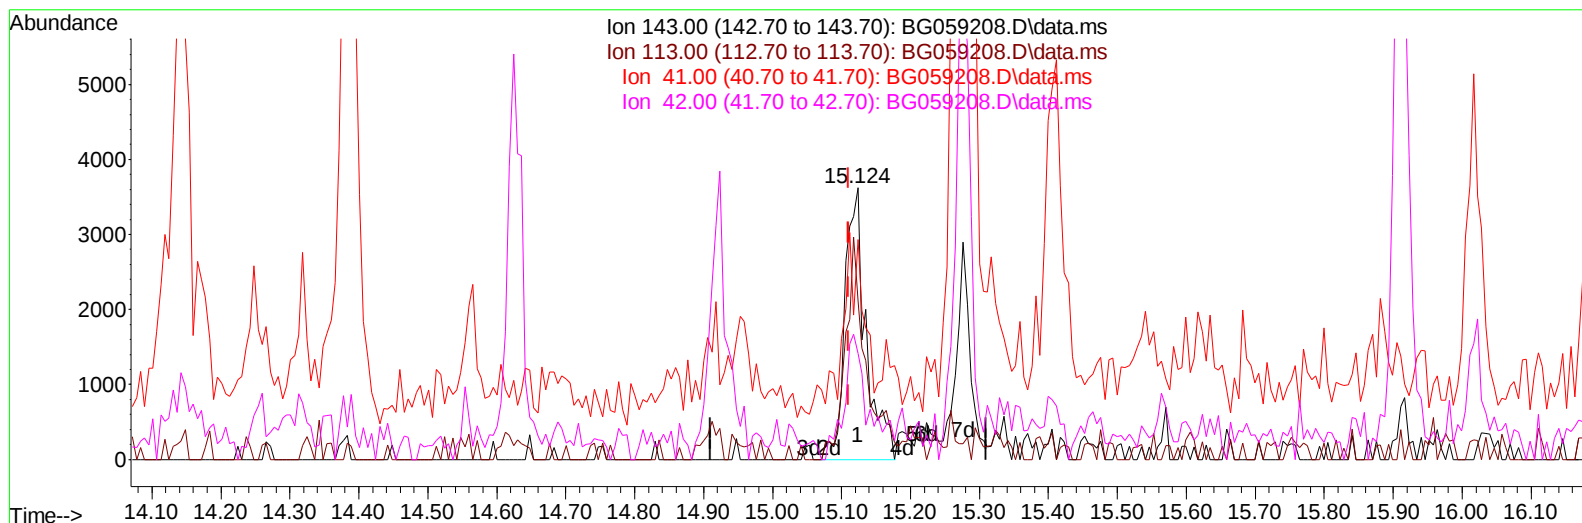

TIC: BG059208.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.124min (+ 0.013) 4.65 ng/ul m

response 7647

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	69.10	58.31
41.00	52.00	80.99#
42.00	40.70	38.92

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
 Data File : BG059208.D
 Acq On : 26 Sep 2023 23:10
 Operator : MA/JU
 Sample : 04450-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBBN0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/27/2023
 Supervised By :mohammad ahmed 09/29/2023

Quant Time: Sep 27 02:31:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 26 23:48:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.296	152	31508	20.000	ng/ul	0.00
20) Naphthalene-d8	11.140	136	161899	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.924	164	117096	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.673	188	265096	20.000	ng/ul	0.00
79) Chrysene-d12	21.992	240	216858	20.000	ng/ul	0.00
88) Perylene-d12	25.547	264	266826	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.602	96	4939m	6.136	ng/uL	0.00
4) Pyridine-d5	4.048	84	42037	17.801	ng/ul	0.00
7) Phenol-d5	7.421	99	37741	12.182	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.615	67	85555	45.000	ng/ul	0.00
11) 2-Chlorophenol-d4	7.814	132	83691	36.605	ng/ul	0.00
15) 4-Methylphenol-d8	8.984	113	49072	19.888	ng/ul	0.00
21) Nitrobenzene-d5	9.495	128	52811	42.273	ng/ul	0.00
24) 2-Nitrophenol-d4	10.212	143	51027	40.433	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.740	165	107826	45.004	ng/ul	0.00
31) 4-Chloroaniline-d4	11.287	131	109882	29.384	ng/ul	0.00
46) Dimethylphthalate-d6	14.319	166	428782	47.613	ng/ul	0.00
49) Acenaphthylene-d8	14.630	160	476560	43.461	ng/ul	0.00
54) 4-Nitrophenol-d4	15.124	143	7647m	4.654	ng/ul	0.01
60) Fluorene-d10	15.911	176	376558	45.681	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.017	200	52343	34.730	ng/ul	0.00
73) Anthracene-d10	17.773	188	558955	46.340	ng/ul	0.00
81) Pyrene-d10	20.047	212	682443	53.840	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.294	264	597492	45.859	ng/ul	0.00
Target Compounds						
						Qvalue
43) 1,1'-Biphenyl	13.760	154	10425	1.115	ng/ul#	97
59) Diethylphthalate	15.711	149	14904	1.644	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
Data File : BG059208.D
Acq On : 26 Sep 2023 23:10
Operator : MA/JU
Sample : 04450-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBBN0

Manual IntegrationsAPPROVED

Quant Time: Sep 27 02:31:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 26 23:48:55 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/27/2023
Supervised By :mohammad ahmed 09/29/2023

