

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
 Data File : BG059204.D
 Acq On : 26 Sep 2023 20:27
 Operator : MA/JU
 Sample : PB155793BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK793

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG059204.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.043	106	111	124	rBV	181751	315983	19.82%	2.355%
2	6.387	508	510	512	rBV2	2793	2460	0.15%	0.018%
3	6.546	535	537	540	rVB3	2755	2961	0.19%	0.022%
4	6.704	561	564	565	rBV3	5343	4490	0.28%	0.033%
5	6.910	597	599	601	rBV3	4170	4182	0.26%	0.031%
6	7.068	623	626	627	rBV3	4535	4004	0.25%	0.030%
7	7.245	655	656	661	rBV4	2924	2345	0.15%	0.017%
8	7.415	679	685	693	rBV	186487	331848	20.82%	2.473%
9	7.615	713	719	727	rVB	155678	260130	16.32%	1.939%
10	7.815	746	753	763	rVB	181016	308595	19.36%	2.300%
11	8.138	805	808	810	rBV3	2967	3339	0.21%	0.025%
12	8.296	828	835	844	rVB	110178	189265	11.87%	1.410%
13	8.420	854	856	859	rBV3	2060	2184	0.14%	0.016%
14	8.590	883	885	889	rBV3	2375	3774	0.24%	0.028%
15	8.714	904	906	909	rVB4	2760	2434	0.15%	0.018%
16	8.743	909	911	912	rBV2	2592	2277	0.14%	0.017%
17	8.984	944	952	965	rBV	228777	404254	25.36%	3.013%
18	9.101	970	972	975	rVB3	3209	3056	0.19%	0.023%
19	9.231	993	994	998	rBV3	2615	2581	0.16%	0.019%
20	9.360	1014	1016	1018	rVB2	2754	2182	0.14%	0.016%
21	9.489	1030	1038	1045	rBV	178522	330169	20.71%	2.461%
22	9.712	1075	1076	1079	rVB2	3328	2392	0.15%	0.018%
23	9.812	1090	1093	1095	rBV3	2346	2576	0.16%	0.019%
24	9.895	1103	1107	1111	rBV3	2416	4092	0.26%	0.030%
25	10.059	1133	1135	1139	rVB2	2968	2852	0.18%	0.021%
26	10.212	1154	1161	1168	rVB	155516	269864	16.93%	2.011%
27	10.335	1179	1182	1184	rBV2	2884	2828	0.18%	0.021%
28	10.353	1184	1185	1187	rVB	4211	2302	0.14%	0.017%
29	10.376	1187	1189	1192	rBV3	2442	3603	0.23%	0.027%
30	10.605	1226	1228	1232	rVB3	2391	2206	0.14%	0.016%
31	10.647	1232	1235	1237	rBV3	2868	2554	0.16%	0.019%
32	10.741	1244	1251	1258	rBV	213739	389661	24.45%	2.904%
33	11.140	1312	1319	1325	rVB	172280	312013	19.57%	2.325%
34	11.281	1337	1343	1355	rBV2	231958	441141	27.68%	3.288%
35	11.640	1403	1404	1408	rVV3	2329	2553	0.16%	0.019%
36	11.681	1408	1411	1416	rVB2	2718	3796	0.24%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
 Data File : BG059204.D
 Acq On : 26 Sep 2023 20:27
 Operator : MA/JU
 Sample : PB155793BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK793

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

37	11.845	1435	1439	1441	rVB3	2682	3221	0.20%	0.024%
38	12.104	1481	1483	1486	rBV3	2370	2489	0.16%	0.019%
39	12.274	1510	1512	1517	rVB2	2516	3779	0.24%	0.028%
40	12.309	1517	1518	1521	rBV2	2141	2659	0.17%	0.020%

41	12.697	1580	1584	1589	rBV4	4259	8941	0.56%	0.067%
42	12.774	1594	1597	1600	rBV	2188	3101	0.19%	0.023%
43	12.926	1621	1623	1625	rBV	2980	2465	0.15%	0.018%
44	12.967	1627	1630	1633	rVV3	2486	3524	0.22%	0.026%
45	13.003	1633	1636	1639	rVB2	2017	2256	0.14%	0.017%

46	13.097	1648	1652	1655	rBV2	2323	3512	0.22%	0.026%
47	13.749	1760	1763	1766	rBV3	7669	8562	0.54%	0.064%
48	13.925	1790	1793	1795	rVB3	2576	2901	0.18%	0.022%
49	14.125	1824	1827	1828	rBV	3431	2738	0.17%	0.020%
50	14.272	1850	1852	1854	rBV2	2406	2375	0.15%	0.018%

51	14.319	1854	1860	1867	rVV	544035	783129	49.13%	5.836%
52	14.624	1906	1912	1921	rBV2	551071	889778	55.82%	6.631%
53	14.924	1956	1963	1970	rBV	337111	502419	31.52%	3.744%
54	15.118	1990	1996	2001	rBV4	45028	99091	6.22%	0.738%
55	15.600	2074	2078	2079	rBV2	3097	2650	0.17%	0.020%

56	15.641	2083	2085	2089	rVB3	2291	2339	0.15%	0.017%
57	15.752	2102	2104	2106	rBV3	2900	3186	0.20%	0.024%
58	15.911	2124	2131	2140	rBV	794806	1154426	72.43%	8.603%
59	16.017	2144	2149	2157	rBV2	172470	282779	17.74%	2.107%
60	16.152	2170	2172	2175	rVB3	6660	6527	0.41%	0.049%

61	16.240	2183	2187	2189	rVB3	2295	3483	0.22%	0.026%
62	16.516	2232	2234	2236	rBV	4194	4450	0.28%	0.033%
63	16.563	2239	2242	2245	rBV2	2316	3521	0.22%	0.026%
64	16.657	2257	2258	2260	rBV2	2453	2185	0.14%	0.016%
65	16.863	2290	2293	2295	rVB3	3322	2807	0.18%	0.021%

66	17.022	2317	2320	2323	rBV2	2687	3388	0.21%	0.025%
67	17.139	2338	2340	2343	rBV3	2416	2399	0.15%	0.018%
68	17.227	2353	2355	2358	rBV2	2581	2318	0.15%	0.017%
69	17.286	2363	2365	2368	rBV2	2579	2602	0.16%	0.019%
70	17.333	2370	2373	2378	rBV5	3111	4893	0.31%	0.036%

71	17.562	2410	2412	2415	rBV4	2288	2223	0.14%	0.017%
72	17.603	2418	2419	2422	rVB3	4360	2249	0.14%	0.017%
73	17.674	2424	2431	2438	rBV	438106	668002	41.91%	4.978%
74	17.774	2441	2448	2459	rBV2	824539	1328267	83.33%	9.899%
75	18.191	2517	2519	2521	rVB2	4181	2761	0.17%	0.021%

76	18.355	2545	2547	2548	rVB2	3266	2196	0.14%	0.016%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
 Data File : BG059204.D
 Acq On : 26 Sep 2023 20:27
 Operator : MA/JU
 Sample : PB155793BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK793

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
 Title : SVOA CALIBRATION

77	18.367	2548	2549	2551	rBV2	3967	2791	0.18%	0.021%
78	18.432	2558	2560	2562	rVB3	3211	2727	0.17%	0.020%
79	18.467	2564	2566	2569	rVV3	2483	2505	0.16%	0.019%
80	18.602	2585	2589	2591	rBV3	2287	2402	0.15%	0.018%
81	18.720	2607	2609	2611	rVB3	2720	2410	0.15%	0.018%
82	18.743	2611	2613	2616	rBV4	2256	2665	0.17%	0.020%
83	18.808	2620	2624	2627	rBV6	3457	4916	0.31%	0.037%
84	18.843	2629	2630	2634	rVB3	3351	3519	0.22%	0.026%
85	19.049	2662	2665	2667	rBV2	3518	3360	0.21%	0.025%
86	19.101	2672	2674	2675	rBV2	3572	2350	0.15%	0.018%
87	19.143	2680	2681	2685	rBV3	5068	4415	0.28%	0.033%
88	19.219	2692	2694	2696	rBV2	2927	3169	0.20%	0.024%
89	19.284	2702	2705	2706	rBV3	2673	2967	0.19%	0.022%
90	19.395	2722	2724	2725	rBV2	5483	3275	0.21%	0.024%
91	19.607	2755	2760	2764	rBV6	14569	25012	1.57%	0.186%
92	19.683	2769	2773	2779	rVB4	10444	18436	1.16%	0.137%
93	19.824	2796	2797	2800	rVB3	4968	4007	0.25%	0.030%
94	19.994	2824	2826	2827	rVB2	5826	3596	0.23%	0.027%
95	20.047	2827	2835	2846	rBV	1086877	1593959	100.00%	11.879%
96	20.412	2895	2897	2898	rVB2	7547	3710	0.23%	0.028%
97	20.429	2898	2900	2904	rBV5	6733	9533	0.60%	0.071%
98	21.992	3160	3166	3177	rBV2	295414	554184	34.77%	4.130%
99	25.294	3718	3728	3741	rBV2	355795	1152052	72.28%	8.586%
100	25.547	3763	3771	3783	rVB2	171552	566924	35.57%	4.225%




Sum of corrected areas: 13418421

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
Data File : BG059204.D
Acq On : 26 Sep 2023 20:27
Operator : MA/JU
Sample : PB155793BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK793

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

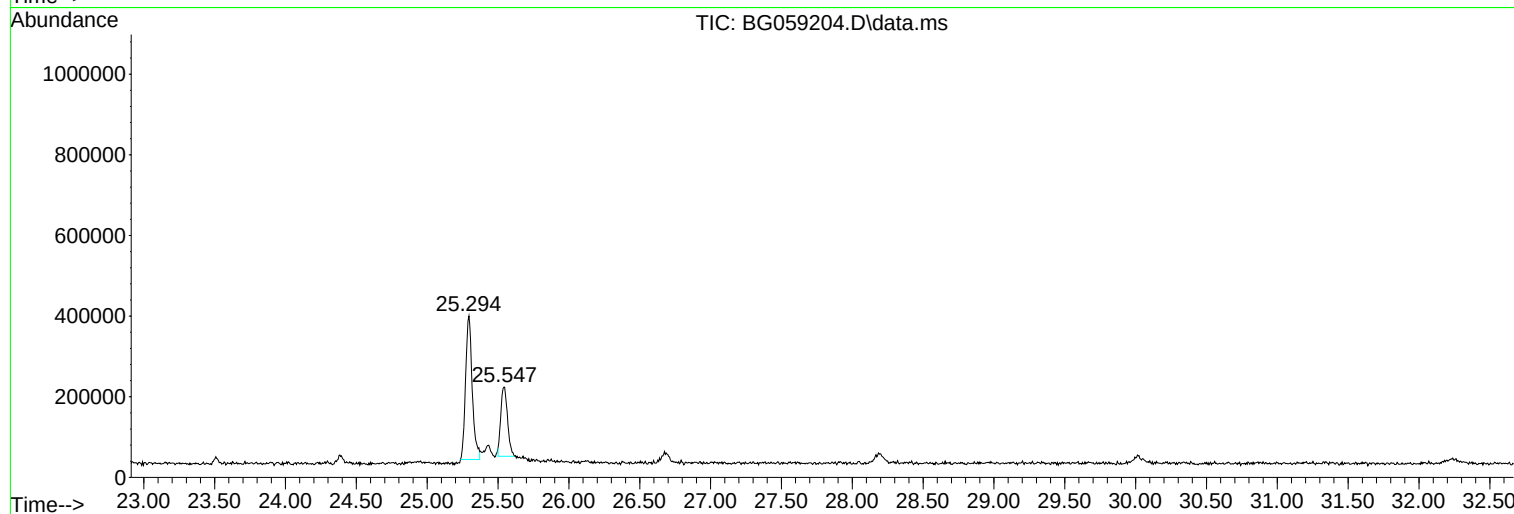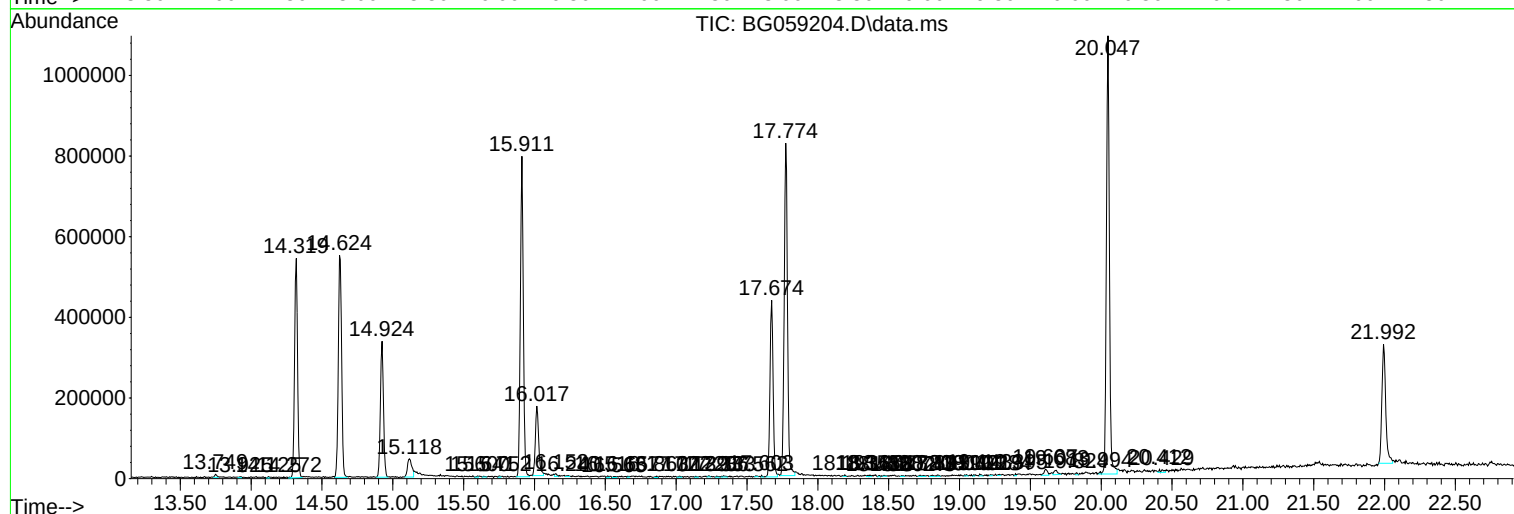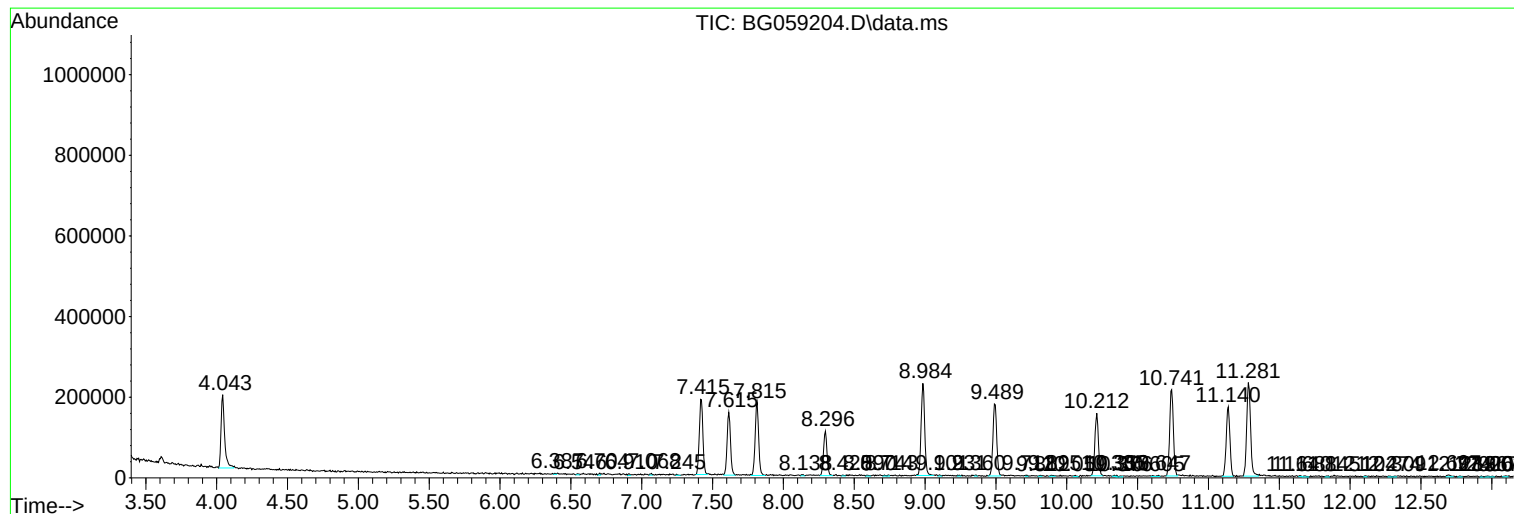

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
Data File : BG059204.D
Acq On : 26 Sep 2023 20:27
Operator : MA/JU
Sample : PB155793BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK793

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092623\
Data File : BG059204.D
Acq On : 26 Sep 2023 20:27
Operator : MA/JU
Sample : PB155793BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK793

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG091923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc