


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092625\
Data File : BG064455.D
Acq On : 26 Sep 2025 15:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 26 06:30:03 2025

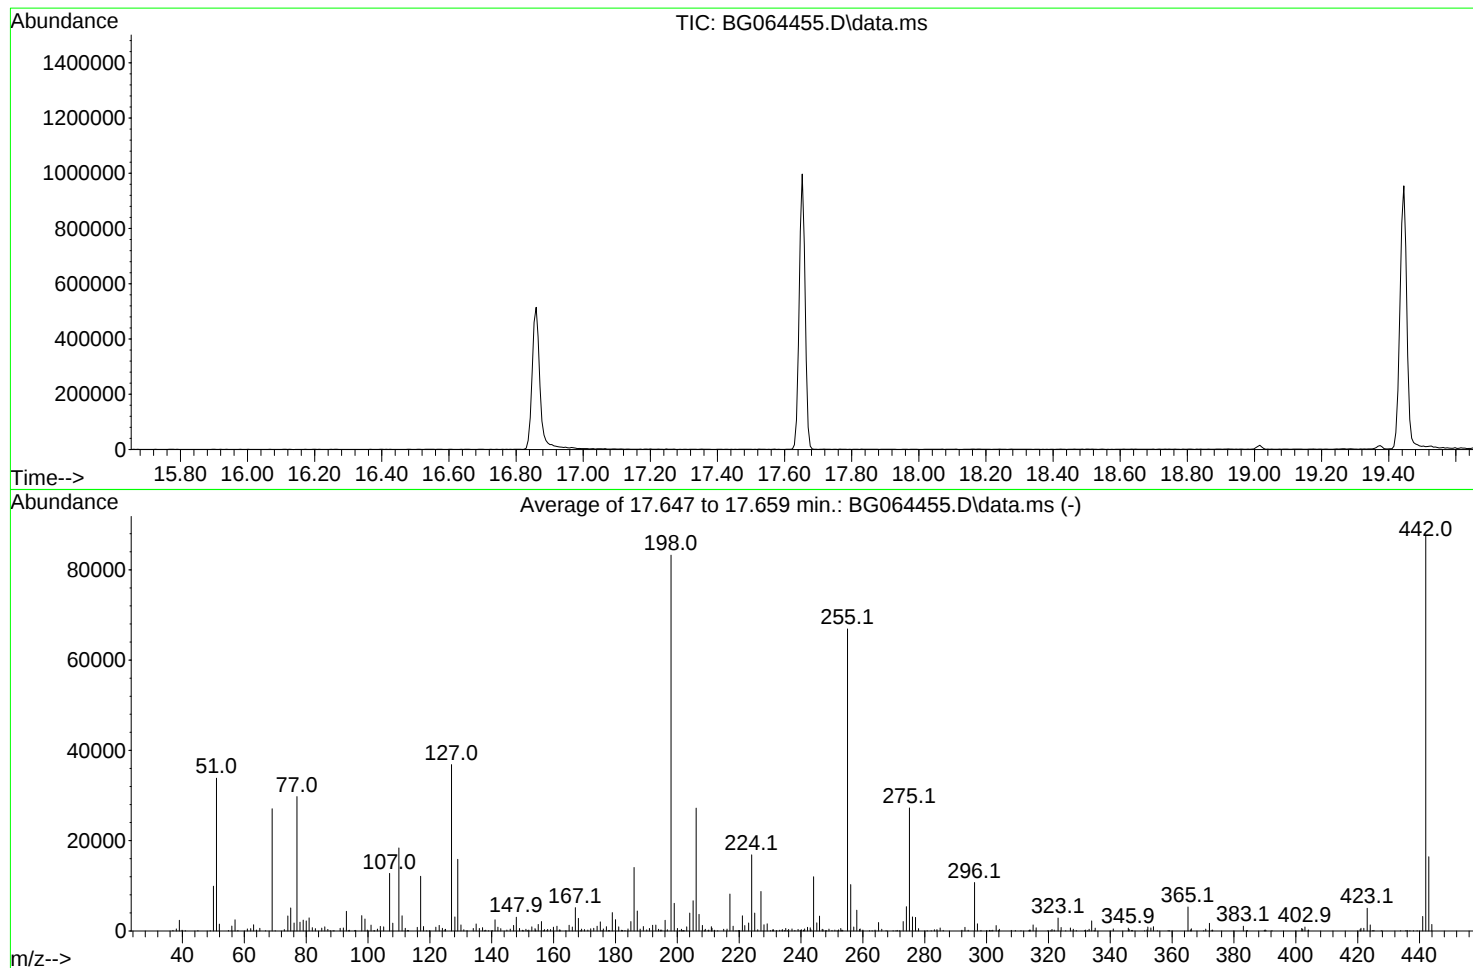

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	27067	PASS
70	69	0.00	2	0.2	61	PASS
197	198	0.00	2	0.3	261	PASS
198	198	100	100	100.0	83264	PASS
199	198	5	9	7.3	6101	PASS
365	198	1	100	6.3	5287	PASS
441	443	0.01	150	19.6	3224	PASS
442	442	100	100	100.0	87477	PASS
443	442	15	24	18.8	16428	PASS