

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092721\
 Data File : BG050279.D
 Acq On : 27 Sep 2021 16:12
 Operator : CG/JU
 Sample : PB139380BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK380

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.606	17	20	21	rBV2	1313	1144	0.11%	0.010%
2	3.653	24	28	32	rBV2	9247	15205	1.41%	0.139%
3	3.812	52	55	57	rVV3	894	1180	0.11%	0.011%
4	3.870	61	65	67	rVB3	1007	1398	0.13%	0.013%
5	3.894	67	69	71	rVB2	1987	1222	0.11%	0.011%
6	4.088	97	102	116	rBV	123117	250237	23.21%	2.294%
7	4.176	116	117	120	rVB3	1286	1129	0.10%	0.010%
8	4.417	154	158	164	rVB6	3475	5511	0.51%	0.051%
9	4.746	212	214	217	rBV	1288	1529	0.14%	0.014%
10	4.940	244	247	252	rBV2	927	1388	0.13%	0.013%
11	5.016	257	260	263	rVV2	842	1266	0.12%	0.012%
12	5.098	270	274	277	rBV	984	1239	0.11%	0.011%
13	5.269	300	303	306	rBV2	863	1367	0.13%	0.013%
14	5.897	408	410	413	rVV	1115	1144	0.11%	0.010%
15	6.379	487	492	495	rVB2	828	1329	0.12%	0.012%
16	7.419	661	669	678	rVB	177566	310213	28.77%	2.844%
17	7.601	693	700	710	rBV	128375	220604	20.46%	2.023%
18	7.813	729	736	745	rBV	171468	294832	27.34%	2.703%
19	8.289	809	817	824	rVB	137430	239699	22.23%	2.198%
20	8.788	900	902	907	rVB3	1163	1673	0.16%	0.015%
21	8.841	907	911	914	rBV2	746	1551	0.14%	0.014%
22	8.976	927	934	943	rVB2	203483	358544	33.25%	3.288%
23	9.458	1008	1016	1025	rVB	158127	283338	26.28%	2.598%
24	10.187	1131	1140	1147	rBV	115359	212465	19.70%	1.948%
25	10.721	1224	1231	1238	rVV	198829	357666	33.17%	3.280%
26	11.115	1289	1298	1308	rVB	172951	317590	29.45%	2.912%
27	11.238	1312	1319	1329	rVB	192262	356878	33.10%	3.272%
28	11.385	1339	1344	1348	rBV	705	1220	0.11%	0.011%
29	12.684	1554	1565	1569	rBV4	3334	8034	0.75%	0.074%
30	12.748	1572	1576	1580	rBV	884	1457	0.14%	0.013%
31	13.195	1649	1652	1657	rVB4	839	1146	0.11%	0.011%
32	13.530	1708	1709	1712	rBV3	1433	1254	0.12%	0.011%
33	13.688	1733	1736	1739	rBV2	1035	1136	0.11%	0.010%
34	14.299	1831	1840	1847	rBV	359933	526548	48.83%	4.828%
35	14.599	1884	1891	1899	rBV	390671	625923	58.05%	5.739%
36	14.746	1914	1916	1920	rVB2	1210	1097	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092721\
 Data File : BG050279.D
 Acq On : 27 Sep 2021 16:12
 Operator : CG/JU
 Sample : PB139380BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK380

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Title : SVOA CALIBRATION

37	14.904	1933	1943	1949	rBV	272142	439866	40.79%	4.033%
38	15.063	1963	1970	1979	rBV	165971	269918	25.03%	2.475%
39	15.169	1985	1988	1991	rBV2	872	1204	0.11%	0.011%
40	15.345	2015	2018	2021	rBV3	1103	1398	0.13%	0.013%
41	15.410	2026	2029	2033	rBV3	1115	1555	0.14%	0.014%
42	15.633	2065	2067	2072	rVB3	853	1342	0.12%	0.012%
43	15.845	2100	2103	2104	rBV2	1035	1113	0.10%	0.010%
44	15.892	2104	2111	2119	rVB	511956	783028	72.62%	7.180%
45	15.991	2122	2128	2137	rBV	129588	197039	18.27%	1.807%
46	16.127	2147	2151	2157	rBV4	2458	3761	0.35%	0.034%
47	16.497	2212	2214	2217	rVB2	1231	1327	0.12%	0.012%
48	16.532	2217	2220	2221	rVB2	1973	1415	0.13%	0.013%
49	16.679	2240	2245	2247	rVB4	1151	1829	0.17%	0.017%
50	16.896	2280	2282	2283	rBV2	1329	1176	0.11%	0.011%
51	17.020	2301	2303	2306	rVB3	1415	1579	0.15%	0.014%
52	17.120	2317	2320	2321	rBV2	1170	1136	0.11%	0.010%
53	17.178	2326	2330	2332	rBV3	1417	2077	0.19%	0.019%
54	17.384	2363	2365	2369	rVV3	1993	2492	0.23%	0.023%
55	17.437	2372	2374	2378	rVB5	2059	2276	0.21%	0.021%
56	17.478	2378	2381	2383	rBV4	1378	1477	0.14%	0.014%
57	17.519	2387	2388	2391	rBV3	1389	1231	0.11%	0.011%
58	17.648	2402	2410	2417	rBV	354175	546476	50.68%	5.011%
59	17.748	2419	2427	2435	rVV	572125	877281	81.36%	8.044%
60	17.866	2445	2447	2449	rBV3	2084	1509	0.14%	0.014%
61	17.995	2467	2469	2470	rBV2	1576	1199	0.11%	0.011%
62	18.036	2473	2476	2477	rBV2	1130	1269	0.12%	0.012%
63	18.095	2483	2486	2489	rBV4	2171	2997	0.28%	0.027%
64	18.154	2494	2496	2497	rBV2	1539	1220	0.11%	0.011%
65	18.283	2516	2518	2519	rVB	2448	1207	0.11%	0.011%
66	18.306	2519	2522	2524	rBV4	2555	2500	0.23%	0.023%
67	18.342	2526	2528	2531	rVB4	2241	1672	0.16%	0.015%
68	18.483	2550	2552	2554	rBV3	1852	1545	0.14%	0.014%
69	18.594	2570	2571	2573	rBV2	1622	1482	0.14%	0.014%
70	18.812	2606	2608	2610	rBV3	1821	1773	0.16%	0.016%
71	18.970	2633	2635	2636	rBV2	2510	1485	0.14%	0.014%
72	19.047	2646	2648	2650	rBV3	2271	2095	0.19%	0.019%
73	19.082	2652	2654	2655	rBV	2049	1311	0.12%	0.012%
74	19.176	2668	2670	2673	rBV3	3114	2617	0.24%	0.024%
75	19.470	2718	2720	2721	rBV	3574	2202	0.20%	0.020%
76	19.658	2747	2752	2754	rBV3	8780	14082	1.31%	0.129%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092721\
Data File : BG050279.D
Acq On : 27 Sep 2021 16:12
Operator : CG/JU
Sample : PB139380BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK380

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Title : SVOA CALIBRATION

77	20.022	2807	2814	2824	rBV	718099	1078306	100.00%	9.887%
78	21.955	3137	3143	3149	rVB	361649	625619	58.02%	5.736%
79	25.157	3680	3688	3701	rVB2	359972	1066774	98.93%	9.781%
80	25.398	3721	3729	3740	rVB2	189819	542043	50.27%	4.970%




Sum of corrected areas: 10906059

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092721\
Data File : BG050279.D
Acq On : 27 Sep 2021 16:12
Operator : CG/JU
Sample : PB139380BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK380

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

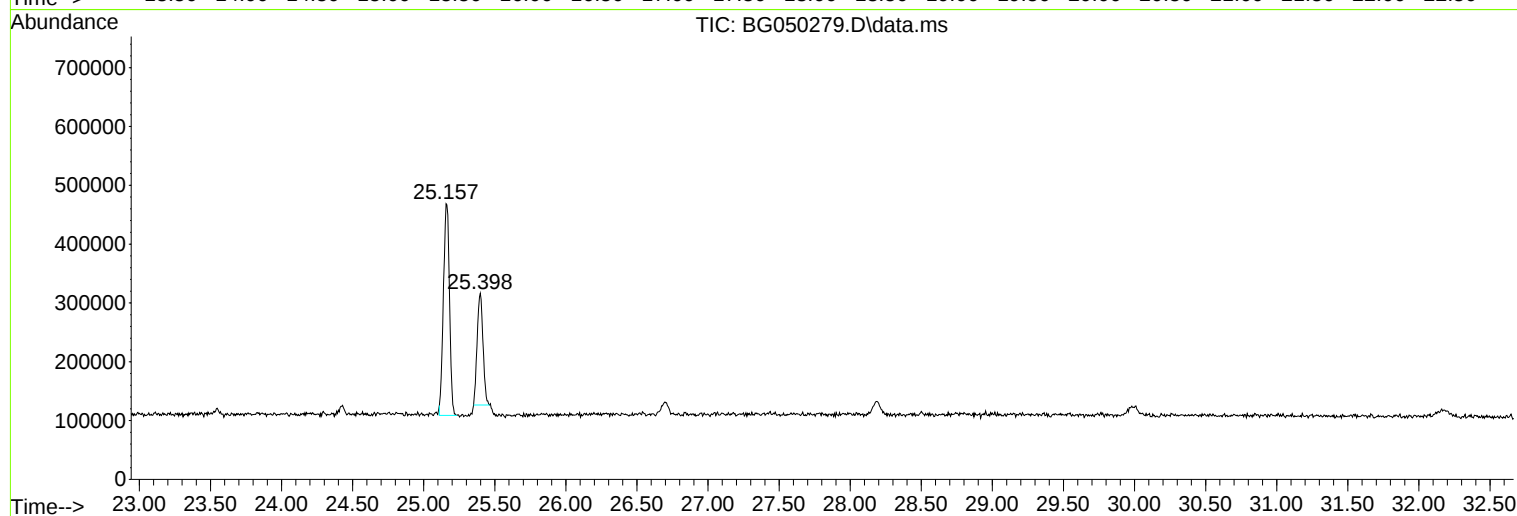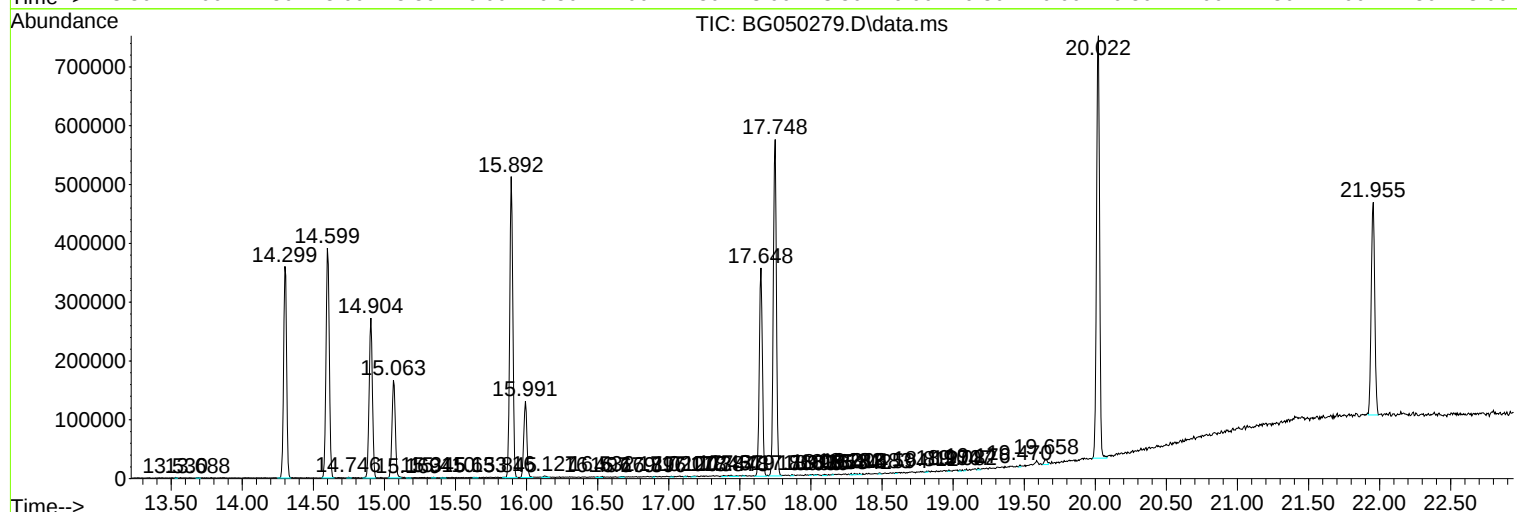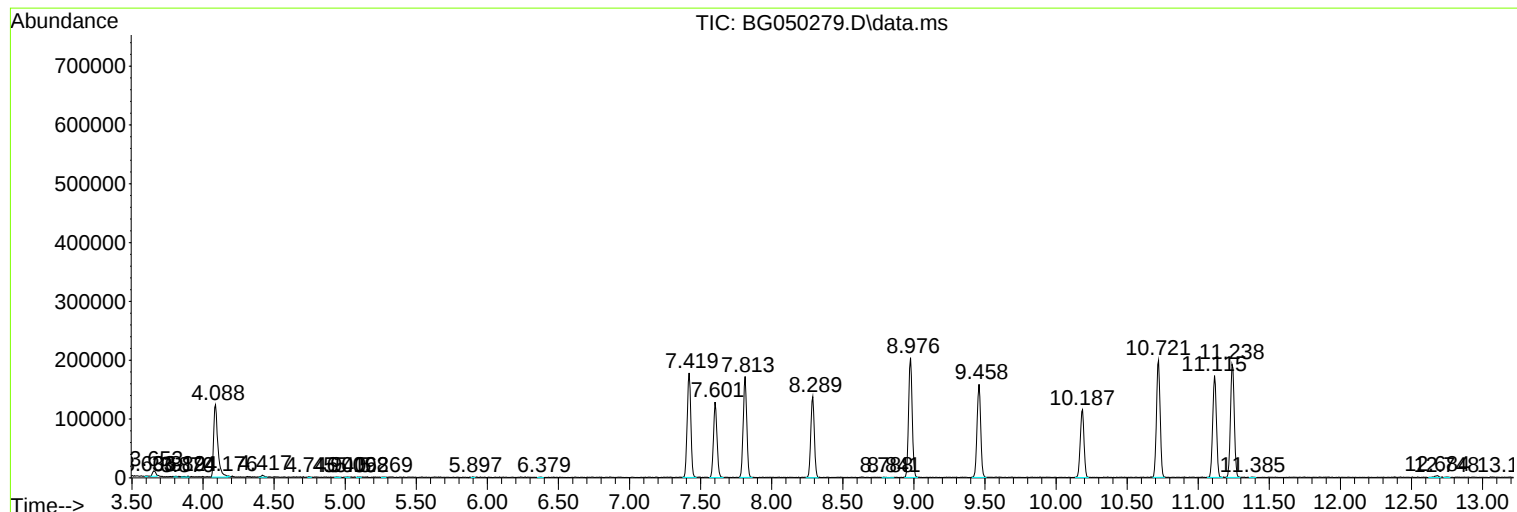

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092721\
Data File : BG050279.D
Acq On : 27 Sep 2021 16:12
Operator : CG/JU
Sample : PB139380BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK380

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092721\
Data File : BG050279.D
Acq On : 27 Sep 2021 16:12
Operator : CG/JU
Sample : PB139380BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK380

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
