

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
 Data File : BG063106.D
 Acq On : 28 Sep 2024 13:47
 Operator : RC/JU
 Sample : P3910-12DL2 30X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC32DL2

Quant Time: Sep 28 23:24:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 25 13:16:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.847	152	70101	20.000	ng/ul	0.00
20) Naphthalene-d8	10.637	136	310780	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.486	164	305539	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.236	188	786838	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.489	240	844983	20.000	ng/ul	# 0.00
88) Perylene-d12	24.527	264	982492	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	145	0.119	ng/uL	0.03
4) Pyridine-d5	3.710	84	631	0.212	ng/ul	-0.01
7) Phenol-d5	7.006	99	146	0.034	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	0.000	67	0	0.000	ng/ul	
11) 2-Chlorophenol-d4	7.382	132	376	0.088	ng/ul	0.00
15) 4-Methylphenol-d8	8.557	113	348	0.089	ng/ul	0.00
21) Nitrobenzene-d5	9.051	128	173	0.076	ng/ul	0.05
24) 2-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	10.261	165	69	0.011	ng/ul	0.00
31) 4-Chloroaniline-d4	10.796	131	55	0.008	ng/ul	0.02
46) Dimethylphthalate-d6	13.898	166	2586	0.106	ng/ul	0.00
49) Acenaphthylene-d8	14.186	160	3293	0.128	ng/ul	0.01
54) 4-Nitrophenol-d4	14.727	143	156	0.043	ng/ul	0.03
60) Fluorene-d10	15.485	176	2851	0.128	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.726	200	153	0.028	ng/ul	0.12
73) Anthracene-d10	17.335	188	7351	0.195	ng/ul	0.00
81) Pyrene-d10	19.633	212	7128	0.150	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.316	264	4050	0.077	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.895	266	14389	2.149	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
Data File : BG063106.D
Acq On : 28 Sep 2024 13:47
Operator : RC/JU
Sample : P3910-12DL2 30X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC32DL2

Quant Time: Sep 28 23:24:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 25 13:16:45 2024
Response via : Initial Calibration

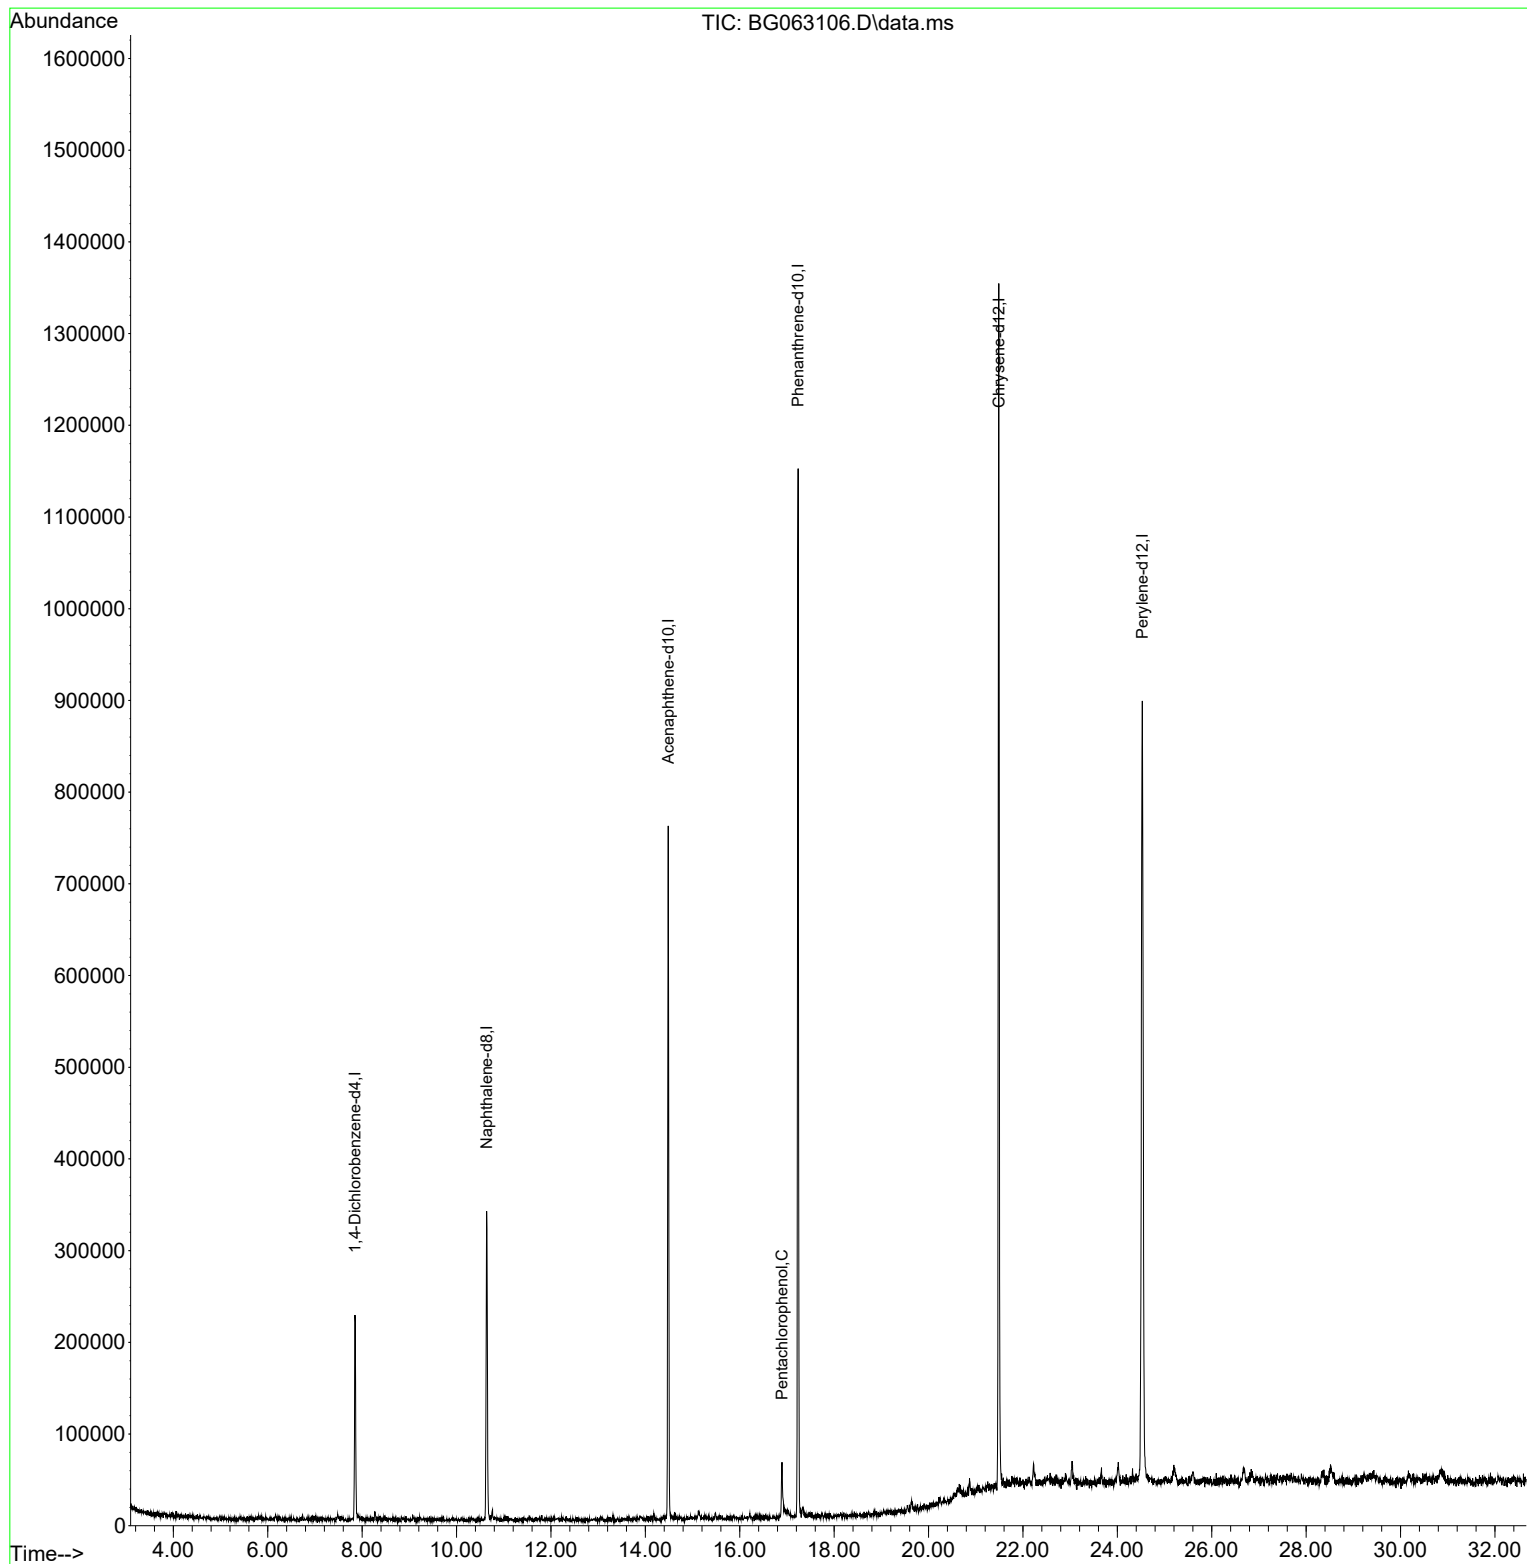

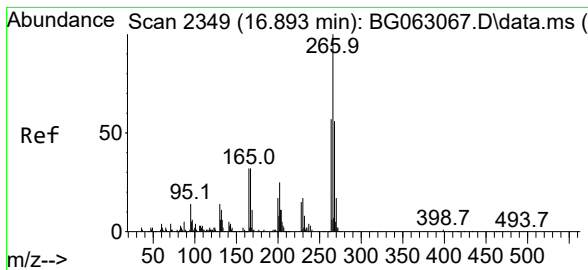

#71
 Pentachlorophenol
 Concen: 2.149 ng/ul
 RT: 16.895 min Scan# 21
 Delta R.T. 0.005 min
 Lab File: BG063106.D
 Acq: 28 Sep 2024 13:47

Instrument :
 BNA_G
 ClientSampleId :
 DDC32DL2

Tgt Ion	Ratio	Lower	Upper
266	100		
264	63.5	57.7	86.5
268	70.3	57.3	85.9

