

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
 Data File : BG063116.D
 Acq On : 28 Sep 2024 20:21
 Operator : RC/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020515

Quant Time: Sep 28 23:26:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 25 13:16:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	103304	20.000	ng/u1	0.00
20) Naphthalene-d8	10.637	136	435954	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.485	164	399782	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.235	188	1112016	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.489	240	1145380	20.000	ng/u1	# 0.00
88) Perylene-d12	24.526	264	1305380	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.316	96	14663	8.183	ng/uL	0.00
4) Pyridine-d5	3.721	84	98866	22.563	ng/u1	0.00
7) Phenol-d5	7.017	99	140787	22.065	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.176	67	55667	22.332	ng/u1	0.00
11) 2-Chlorophenol-d4	7.382	132	133496	21.294	ng/u1	0.00
15) 4-Methylphenol-d8	8.557	113	122842	21.327	ng/u1	0.00
21) Nitrobenzene-d5	9.003	128	62981	19.647	ng/u1	0.00
24) 2-Nitrophenol-d4	9.726	143	86715	21.181	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.261	165	170068	19.903	ng/u1	0.00
31) 4-Chloroaniline-d4	10.772	131	203720	20.318	ng/u1	0.00
46) Dimethylphthalate-d6	13.892	166	637611	20.059	ng/u1	0.00
49) Acenaphthylene-d8	14.174	160	669198	19.867	ng/u1	0.00
54) 4-Nitrophenol-d4	14.691	143	96253	20.078	ng/u1	0.00
60) Fluorene-d10	15.478	176	579542	19.899	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.602	200	137763	17.727	ng/u1	0.00
73) Anthracene-d10	17.335	188	1071650	20.087	ng/u1	0.00
81) Pyrene-d10	19.632	212	1359908	21.086	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.321	264	1391572	19.904	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.345	88	15139	7.157	ng/uL	94
5) Pyridine	3.739	79	97111	22.515	ng/u1#	82
6) Benzaldehyde	6.988	77	76342	25.762	ng/u1	95
8) Phenol	7.047	94	144010	22.430	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.270	93	91554	22.917	ng/u1	95
12) 2-Chlorophenol	7.411	128	127958	21.024	ng/u1	96
13) 2-Methylphenol	8.292	108	123447	21.873	ng/u1	92
14) 2,2'-oxybis(1-Chloropr...	8.369	45	78889	25.921	ng/u1	96
16) Acetophenone	8.663	105	189358	21.139	ng/u1	96
17) N-Nitroso-di-n-propyla...	8.651	70	80000	21.840	ng/u1#	92
18) 4-Methylphenol	8.621	108	141703	22.920	ng/u1	99
19) Hexachloroethane	8.927	117	47269	19.625	ng/u1	86
22) Nitrobenzene	9.044	77	122706	20.275	ng/u1#	89
23) Isophorone	9.562	82	246435	21.087	ng/u1	98
25) 2-Nitrophenol	9.755	139	84372	20.142	ng/u1	95
26) 2,4-Dimethylphenol	9.820	107	151351	20.077	ng/u1	92
27) Bis(2-Chloroethoxy)met...	10.043	93	128662	21.063	ng/u1#	97
29) 2,4-Dichlorophenol	10.290	162	168713	20.631	ng/u1	98
30) Naphthalene	10.690	128	447936	20.214	ng/u1	99
32) 4-Chloroaniline	10.795	127	191786	20.801	ng/u1	88
33) Hexachlorobutadiene	10.978	225	149701	18.825	ng/u1	92
34) Caprolactam	11.547	113	35620	15.573	ng/u1	95
35) 4-Chloro-3-methylphenol	11.929	107	154658	21.521	ng/u1	98
36) 2-Methylnaphthalene	12.300	142	364864	20.298	ng/u1	90

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
 Data File : BG063116.D
 Acq On : 28 Sep 2024 20:21
 Operator : RC/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD020515

Quant Time: Sep 28 23:26:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 25 13:16:45 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.523	142	367890	20.248	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.676	216	296681	19.103	ng/ul	99
40) Hexachlorocyclopentadiene	12.652	237	136842	15.505	ng/ul	97
41) 2,4,6-Trichlorophenol	12.916	196	181523	20.319	ng/ul	98
42) 2,4,5-Trichlorophenol	12.916	196	157307	16.021	ng/ul	96
43) 1,1'-Biphenyl	13.316	154	527353	19.923	ng/ul#	96
44) 2-Chloronaphthalene	13.357	162	431040	20.223	ng/ul	100
45) 2-Nitroaniline	13.557	65	82983	21.633	ng/ul	88
47) Dimethylphthalate	13.939	163	599906	19.680	ng/ul	99
48) 2,6-Dinitrotoluene	14.056	165	126286	20.119	ng/ul	97
50) Acenaphthylene	14.203	152	687616	20.370	ng/ul	98
51) 3-Nitroaniline	14.385	138	122082	23.045	ng/ul#	91
52) Acenaphthene	14.550	153	497490	21.159	ng/ul	96
53) 2,4-Dinitrophenol	14.603	184	87460	19.709	ng/ul#	82
55) 4-Nitrophenol	14.708	109	99949	17.223	ng/ul	91
56) Dibenzofuran	14.885	168	773468	20.559	ng/ul	95
57) 2,4-Dinitrotoluene	14.849	165	204089	20.408	ng/ul#	95
58) 2,3,4,6-Tetrachlorophenol	15.114	232	205019	19.543	ng/ul#	96
59) Diethylphthalate	15.308	149	598607	19.849	ng/ul	97
61) Fluorene	15.537	166	642744	20.731	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.531	204	380491	19.531	ng/ul	99
63) 4-Nitroaniline	15.555	138	124964	21.752	ng/ul	93
66) 4,6-Dinitro-2-methylph...	15.619	198	145966	17.715	ng/ul#	95
67) N-Nitrosodiphenylamine	15.743	169	579424	20.901	ng/ul	97
68) 4-Bromophenyl-phenylether	16.424	248	282494	20.700	ng/ul	96
69) Hexachlorobenzene	16.547	284	307217	20.204	ng/ul	96
70) Atrazine	16.694	200	274379	20.129	ng/ul	95
71) Pentachlorophenol	16.888	266	147959	15.638	ng/ul	94
72) Phenanthrene	17.276	178	1160195	20.239	ng/ul	99
74) Anthracene	17.370	178	1198301	20.328	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.281	216	315048	19.854	ng/ul	98
76) Pentachlorobenzene	14.808	250	349815	20.233	ng/ul	93
77) Carbazole	17.640	167	964056	20.436	ng/ul	98
78) Di-n-butylphthalate	18.204	149	1045548	20.409	ng/ul	97
80) Fluoranthene	19.297	202	1521335	21.045	ng/ul#	97
82) Pyrene	19.661	202	1608890	21.247	ng/ul#	97
83) Butylbenzylphthalate	20.555	149	455382	21.788	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.389	252	575673	21.264	ng/ul#	96
85) Benzo(a)anthracene	21.471	228	1625511	20.433	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.389	149	644695	21.571	ng/ul	97
87) Chrysene	21.536	228	1511563	20.469	ng/ul	99
89) Di-n-octyl phthalate	22.535	149	1094681	22.116	ng/ul	100
90) Benzo(b)fluoranthene	23.569	252	1618765	19.941	ng/ul	97
91) Benzo(k)fluoranthene	23.633	252	1635623	20.282	ng/ul#	98
93) Benzo(a)pyrene	24.385	252	1485045	19.987	ng/ul#	96
94) Indeno(1,2,3-cd)pyrene	27.958	276	1883877	20.594	ng/ul#	94
95) Dibenzo(a,h)anthracene	28.011	278	1529408	20.516	ng/ul#	99
96) Benzo(g,h,i)perylene	29.027	276	1402001	20.237	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
Data File : BG063116.D
Acq On : 28 Sep 2024 20:21
Operator : RC/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD020515

Quant Time: Sep 28 23:26:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 25 13:16:45 2024
Response via : Initial Calibration




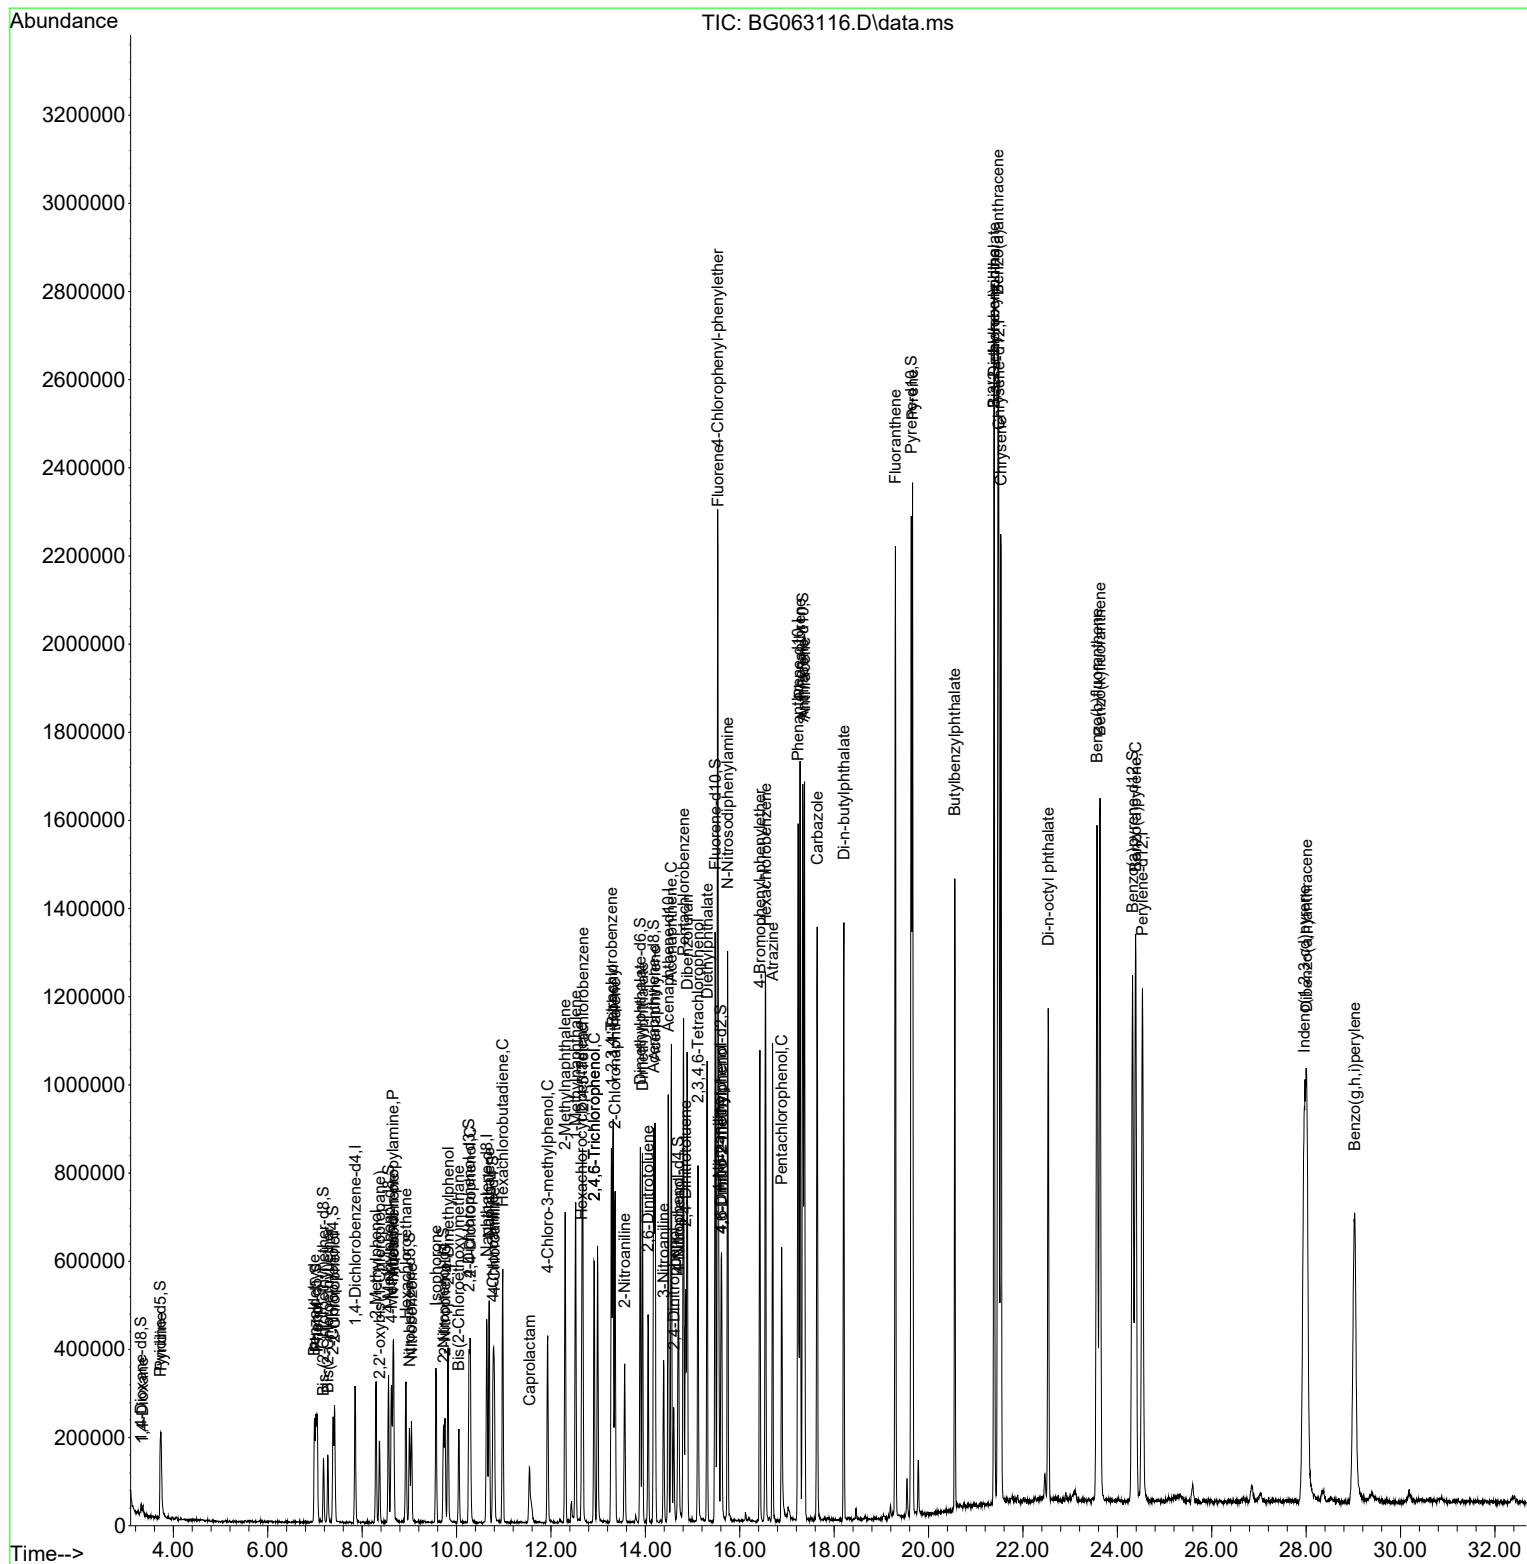




#2
1,4-Dioxane
Concen: 7.157 ng/uL
RT: 3.345 min Scan# 44
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion: 88 Resp: 15139
Ion Ratio Lower Upper
88 100
43 21.2 16.6 25.0
58 48.7 34.8 52.2



#5
Pyridine
Concen: 22.515 ng/uL
RT: 3.739 min Scan# 111
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion: 79 Resp: 97111
Ion Ratio Lower Upper
79 100
52 51.1 55.3 82.9#
51 31.6 30.5 45.7









#6
Benzaldehyde
Concen: 25.762 ng/ul
RT: 6.988 min Scan# 664
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion: 77 Resp: 76342
Ion Ratio Lower Upper
77 100
105 114.1 97.2 145.8
106 116.3 89.8 134.8

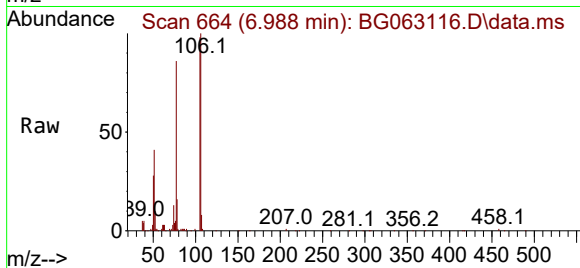

#8
Phenol
Concen: 22.430 ng/ul
RT: 7.047 min Scan# 674
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion: 94 Resp: 144010
Ion Ratio Lower Upper
94 100
65 24.8 20.1 30.1
66 43.5 34.6 51.8




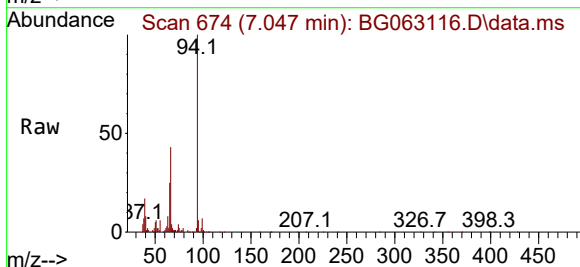




#10
Bis(2-Chloroethyl)ether
Concen: 22.917 ng/ul
RT: 7.270 min Scan# 712
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion: 93 Resp: 91554
Ion Ratio Lower Upper
93 100
63 64.4 47.2 70.8
95 31.6 25.3 37.9

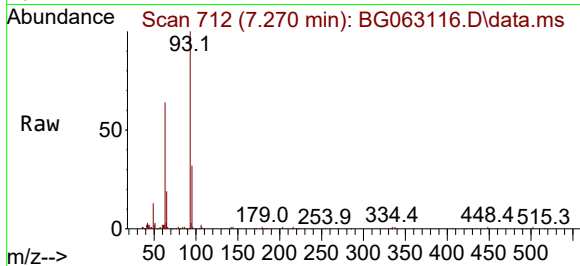

#12
2-Chlorophenol
Concen: 21.024 ng/ul
RT: 7.411 min Scan# 736
Delta R.T. -0.007 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:128 Resp: 127958
Ion Ratio Lower Upper
128 100
64 30.8 26.2 39.4
130 31.2 26.6 40.0

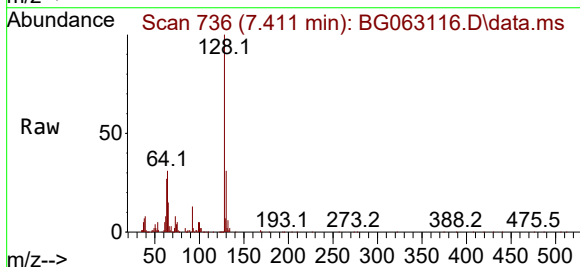



#13

2-Methylphenol

Concen: 21.873 ng/ul

RT: 8.292 min Scan# 886

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :





SSTD020515

Tgt Ion:108 Resp: 123447

Ion Ratio Lower Upper

108 100

107 83.5 72.6 109.0



#14

2,2'-oxybis(1-Chloropropane)

Concen: 25.921 ng/ul

RT: 8.369 min Scan# 899

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21




Tgt Ion: 45 Resp: 78889


Ion Ratio Lower Upper

45 100

77 24.3 21.7 32.5

79 16.9 13.0 19.6



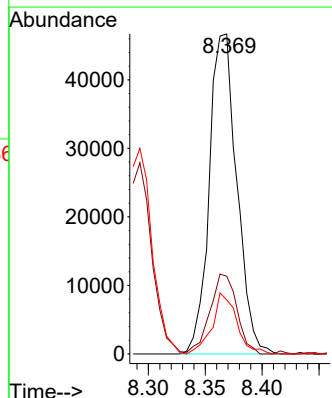





#16
Acetophenone
Concen: 21.139 ng/ul
RT: 8.663 min Scan# 949
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:105 Resp: 189358
Ion Ratio Lower Upper
105 100
77 65.4 54.2 81.4
51 20.4 19.6 29.4



#17
N-Nitroso-di-n-propylamine
Concen: 21.840 ng/ul
RT: 8.651 min Scan# 947
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion: 70 Resp: 80000
Ion Ratio Lower Upper
70 100
42 48.9 37.0 55.4
101 9.9 7.6 11.4
130 25.4 27.6 41.4#



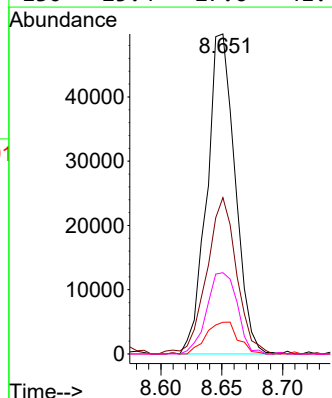





#18
4-Methylphenol
Concen: 22.920 ng/ul
RT: 8.621 min Scan# 941
Delta R.T. 0.005 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:108 Resp: 141703
Ion Ratio Lower Upper
108 100
107 104.8 83.0 124.4

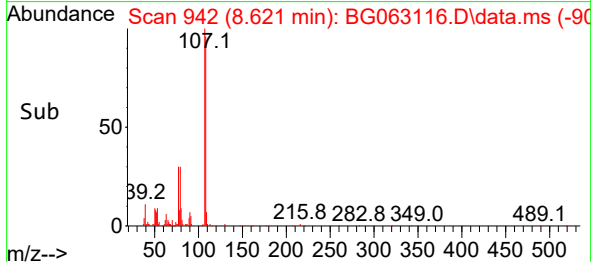

#19
Hexachloroethane
Concen: 19.625 ng/ul
RT: 8.927 min Scan# 994
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:117 Resp: 47269
Ion Ratio Lower Upper
117 100
201 200.0 143.8 215.8
199 97.2 89.1 133.7









#22
Nitrobenzene
Concen: 20.275 ng/ul
RT: 9.044 min Scan# 1013
Delta R.T. 0.005 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion: 77 Resp: 122706
Ion Ratio Lower Upper
77 100
123 56.4 37.6 56.4#
65 14.7 12.0 18.0



#23
Isophorone
Concen: 21.087 ng/ul
RT: 9.562 min Scan# 1102
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion: 82 Resp: 246435
Ion Ratio Lower Upper
82 100
95 10.9 10.0 15.0
138 23.9 19.5 29.3









#25
2-Nitrophenol
Concen: 20.142 ng/ul
RT: 9.755 min Scan# 1135
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:139 Resp: 84372
Ion Ratio Lower Upper
139 100
65 36.4 25.0 37.4
109 40.9 33.9 50.9



#26
2,4-Dimethylphenol
Concen: 20.077 ng/ul
RT: 9.820 min Scan# 1146
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:107 Resp: 151351
Ion Ratio Lower Upper
107 100
121 50.7 38.3 57.5
122 88.0 63.7 95.5









#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.063 ng/ul
 RT: 10.043 min Scan# 1184
 Delta R.T. -0.007 min
 Lab File: BG063116.D
 Acq: 28 Sep 2024 20:21




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020515


Tgt Ion: 93 Resp: 128662
 Ion Ratio Lower Upper
 93 100
 95 31.9 26.2 39.4
 123 13.8 8.7 13.1#



#29
 2,4-Dichlorophenol
 Concen: 20.631 ng/ul
 RT: 10.290 min Scan# 1226
 Delta R.T. -0.001 min
 Lab File: BG063116.D
 Acq: 28 Sep 2024 20:21

Tgt Ion:162 Resp: 168713
 Ion Ratio Lower Upper
 162 100
 164 66.4 52.6 78.8
 98 22.4 20.0 30.0









#30
Naphthalene
Concen: 20.214 ng/ul
RT: 10.690 min Scan# 1293
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:128 Resp: 447936
Ion Ratio Lower Upper
128 100
129 11.4 9.3 13.9
127 13.0 10.7 16.1

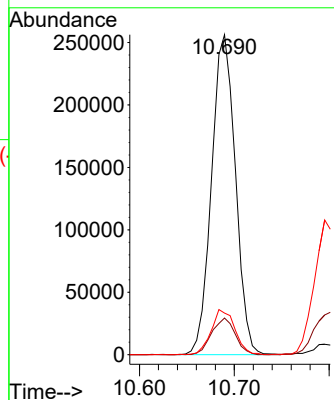

#32
4-Chloroaniline
Concen: 20.801 ng/ul
RT: 10.795 min Scan# 1312
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:127 Resp: 191786
Ion Ratio Lower Upper
127 100
129 29.4 29.4 44.0



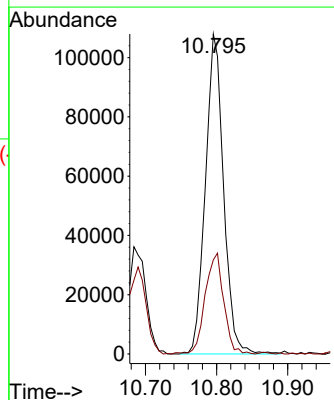





#33
Hexachlorobutadiene
Concen: 18.825 ng/ul
RT: 10.978 min Scan# 11
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:225 Resp: 149701
Ion Ratio Lower Upper
225 100
223 62.6 47.0 70.6
227 58.1 52.6 79.0



#34
Caprolactam
Concen: 15.573 ng/ul
RT: 11.547 min Scan# 1440
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:113 Resp: 35620
Ion Ratio Lower Upper
113 100
55 106.2 85.4 128.2
56 70.4 63.5 95.3









#35
4-Chloro-3-methylphenol
Concen: 21.521 ng/ul
RT: 11.929 min Scan# 1505
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:107 Resp: 154658
Ion Ratio Lower Upper
107 100
144 27.8 22.2 33.4
142 87.3 71.8 107.6



#36
2-Methylnaphthalene
Concen: 20.298 ng/ul
RT: 12.300 min Scan# 1568
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:142 Resp: 364864
Ion Ratio Lower Upper
142 100
141 85.4 75.8 113.8









#37
1-Methylnaphthalene
Concen: 20.248 ng/ul
RT: 12.523 min Scan# 1
Delta R.T. 0.005 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:142 Resp: 367890
Ion Ratio Lower Upper
142 100
141 93.4 73.4 110.0
116 4.3 3.0 4.6



#39
1,2,4,5-Tetrachlorobenzene
Concen: 19.103 ng/ul
RT: 12.676 min Scan# 1632
Delta R.T. 0.005 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:216 Resp: 296681
Ion Ratio Lower Upper
216 100
214 74.9 60.4 90.6
179 17.4 14.2 21.4
108 8.7 8.3 12.5









#40
Hexachlorocyclopentadiene
Concen: 15.505 ng/ul
RT: 12.652 min Scan# 1628
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:237 Resp: 136842
Ion Ratio Lower Upper
237 100
235 63.3 49.0 73.6
272 12.5 8.7 13.1



#41
2,4,6-Trichlorophenol
Concen: 20.319 ng/ul
RT: 12.916 min Scan# 1673
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:196 Resp: 181523
Ion Ratio Lower Upper
196 100
198 95.5 77.6 116.4
200 30.5 25.1 37.7









#42
2,4,5-Trichlorophenol
Concen: 16.021 ng/ul
RT: 12.916 min Scan# 1
Delta R.T. -0.072 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:196 Resp: 157307
Ion Ratio Lower Upper
196 100
198 95.5 74.0 111.0
200 30.5 22.1 33.1

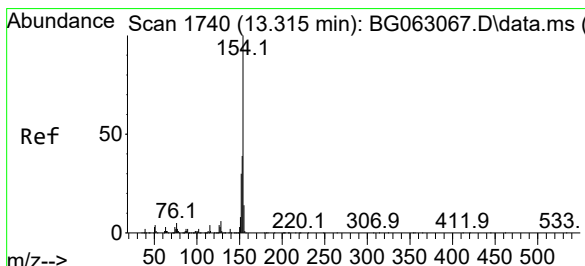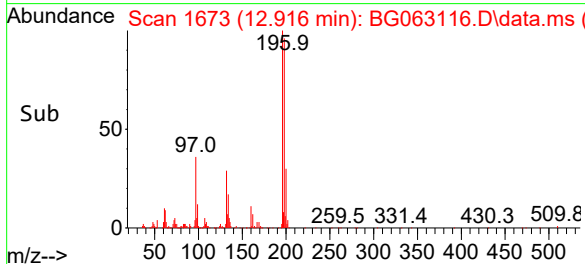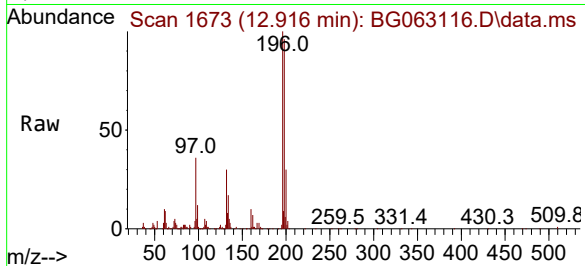

#43
1,1'-Biphenyl
Concen: 19.923 ng/ul
RT: 13.316 min Scan# 1741
Delta R.T. 0.005 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:154 Resp: 527353
Ion Ratio Lower Upper
154 100
153 43.1 32.6 48.8
76 6.6 4.1 6.1#

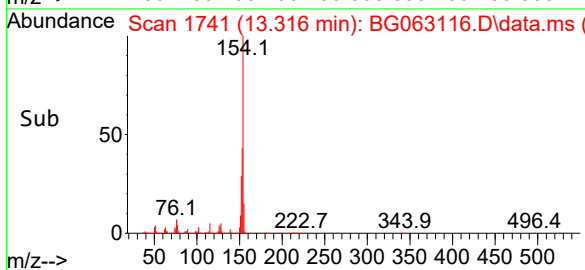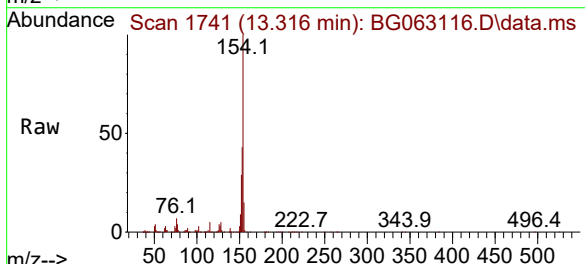



#44

2-Chloronaphthalene

Concen: 20.223 ng/ul

RT: 13.357 min Scan# 1

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:162 Resp: 431040

Ion Ratio Lower Upper

162 100

164 33.7 27.0 40.6

127 33.5 26.6 40.0

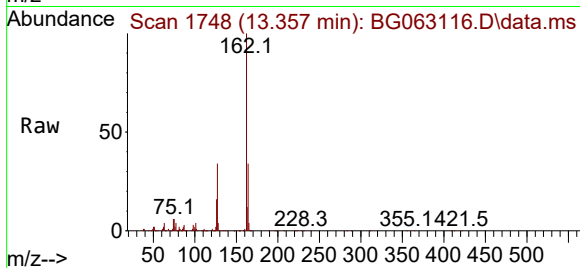

#45

2-Nitroaniline

Concen: 21.633 ng/ul

RT: 13.557 min Scan# 1782

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21




Tgt Ion: 65 Resp: 82983


Ion Ratio Lower Upper

65 100

92 70.8 67.4 101.0

138 153.8 135.4 203.2




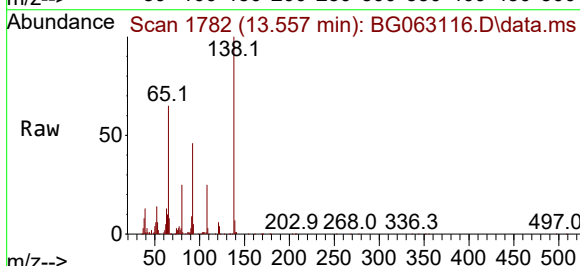


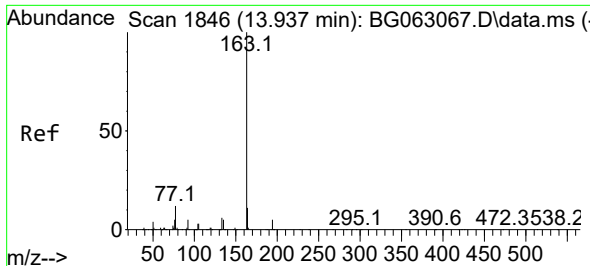

#47
Dimethylphthalate
Concen: 19.680 ng/ul
RT: 13.939 min Scan# 1846
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:163 Resp: 599906
Ion Ratio Lower Upper
163 100
194 4.4 3.5 5.3
164 11.0 8.3 12.5

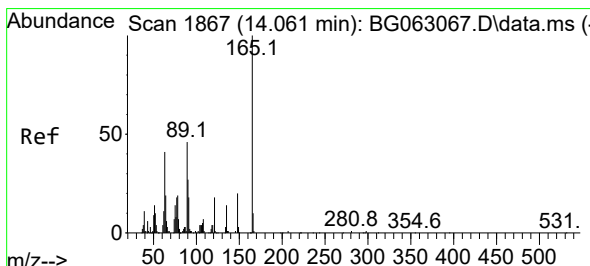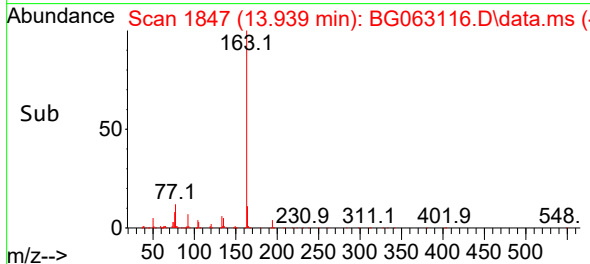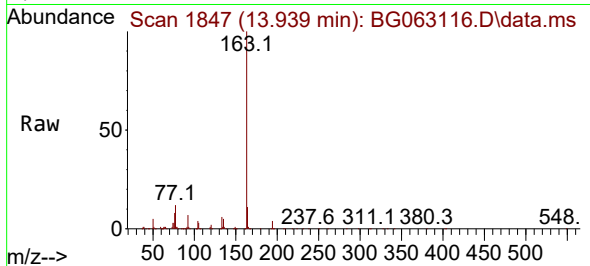

#48
2,6-Dinitrotoluene
Concen: 20.119 ng/ul
RT: 14.056 min Scan# 1867
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:165 Resp: 126286
Ion Ratio Lower Upper
165 100
89 42.5 34.9 52.3
121 13.7 13.6 20.4


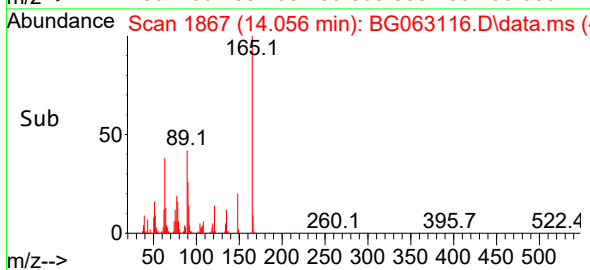

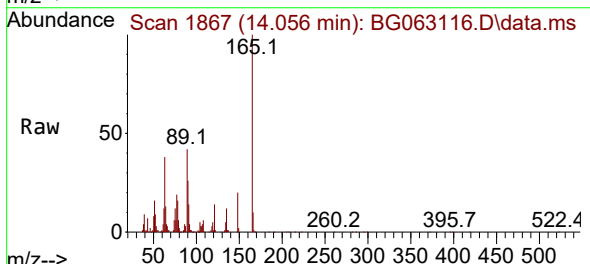




#50
Acenaphthylene
Concen: 20.370 ng/ul
RT: 14.203 min Scan# 1892
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:152 Resp: 687616
Ion Ratio Lower Upper
152 100
151 20.9 16.9 25.3
153 13.2 9.4 14.2

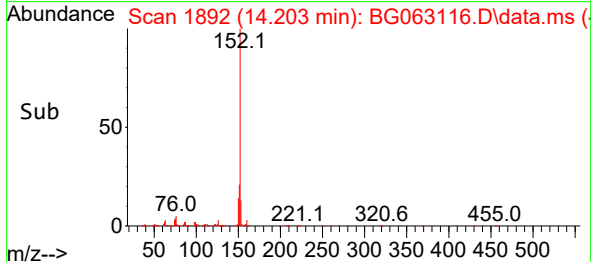

#51
3-Nitroaniline
Concen: 23.045 ng/ul
RT: 14.385 min Scan# 1923
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:138 Resp: 122082
Ion Ratio Lower Upper
138 100
108 9.4 5.8 8.8#
92 88.7 64.2 96.4




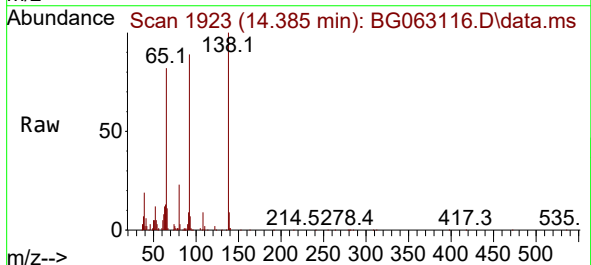




#52
Acenaphthene
Concen: 21.159 ng/ul
RT: 14.550 min Scan# 1951
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:153 Resp: 497490
Ion Ratio Lower Upper
153 100
152 49.9 36.9 55.3
154 85.5 70.2 105.4



#53
2,4-Dinitrophenol
Concen: 19.709 ng/ul
RT: 14.603 min Scan# 1960
Delta R.T. 0.005 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:184 Resp: 87460
Ion Ratio Lower Upper
184 100
63 30.4 35.8 53.8#
154 56.1 55.4 83.2



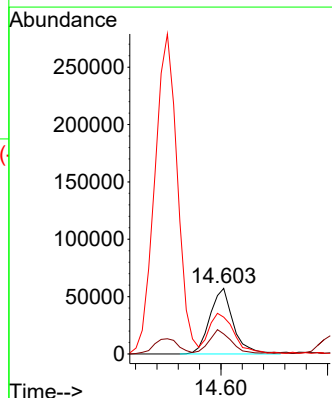





#55
4-Nitrophenol
Concen: 17.223 ng/ul
RT: 14.708 min Scan# 1977
Delta R.T. 0.005 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:	109	Resp:	99949
Ion Ratio	Lower	Upper	
109	100		
139	97.2	66.8	100.2
65	68.8	55.6	83.4



#56
Dibenzofuran
Concen: 20.559 ng/ul
RT: 14.885 min Scan# 2008
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:	168	Resp:	773468
Ion Ratio	Lower	Upper	
168	100		
139	36.2	26.8	40.2





#57

2,4-Dinitrotoluene

Concen: 20.408 ng/ul

RT: 14.849 min Scan# 2001

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:165 Resp: 204089

Ion Ratio Lower Upper

165 100

63 28.3 25.0 37.4

182 2.1 2.2 3.2#

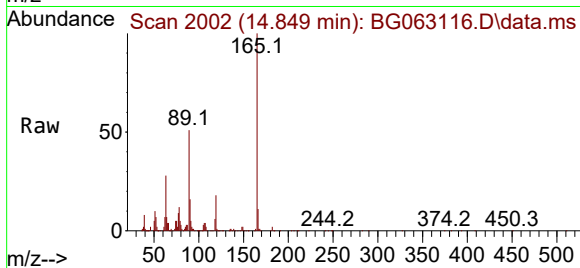

#58

2,3,4,6-Tetrachlorophenol

Concen: 19.543 ng/ul

RT: 15.114 min Scan# 2047

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Tgt Ion:232 Resp: 205019




Ion Ratio Lower Upper


232 100

131 33.6 25.8 38.6

130 0.0 1.9 2.9#

166 24.6 17.6 26.4




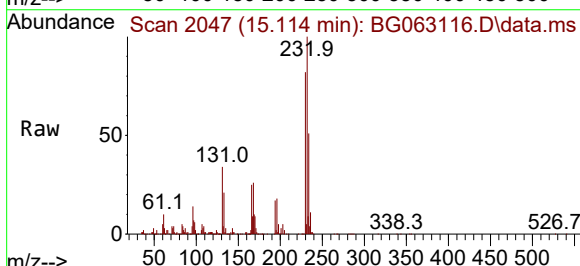




#59
Diethylphthalate
Concen: 19.849 ng/ul
RT: 15.308 min Scan# 2079
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:149 Resp: 598607
Ion Ratio Lower Upper
149 100
177 24.4 20.9 31.3
150 13.7 11.4 17.2



#61
Fluorene
Concen: 20.731 ng/ul
RT: 15.537 min Scan# 2119
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:166 Resp: 642744
Ion Ratio Lower Upper
166 100
165 99.1 80.2 120.4
167 12.8 9.5 14.3









#62
4-Chlorophenyl-phenylether
Concen: 19.531 ng/ul
RT: 15.531 min Scan# 2117
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:204 Resp: 380491
Ion Ratio Lower Upper
204 100
206 35.4 27.0 40.6
141 47.6 38.3 57.5



#63
4-Nitroaniline
Concen: 21.752 ng/ul
RT: 15.555 min Scan# 2122
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:138 Resp: 124964
Ion Ratio Lower Upper
138 100
92 43.6 33.5 50.3
108 115.8 85.0 127.6









#66
4,6-Dinitro-2-methylphenol
Concen: 17.715 ng/ul
RT: 15.619 min Scan# 2132
Delta R.T. 0.005 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:198 Resp: 145966
Ion Ratio Lower Upper
198 100
182 3.6 2.2 3.2#
77 16.3 11.3 16.9



#67
N-Nitrosodiphenylamine
Concen: 20.901 ng/ul
RT: 15.743 min Scan# 2154
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:169 Resp: 579424
Ion Ratio Lower Upper
169 100
168 66.2 55.8 83.8
167 36.2 28.6 42.8


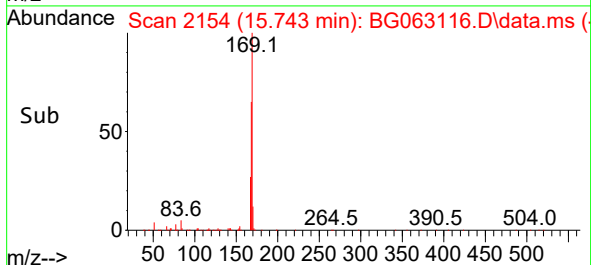






#68
4-Bromophenyl-phenylether
Concen: 20.700 ng/ul
RT: 16.424 min Scan# 21
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:248 Resp: 282494
Ion Ratio Lower Upper
248 100
250 99.7 75.1 112.7
141 55.5 44.6 66.8

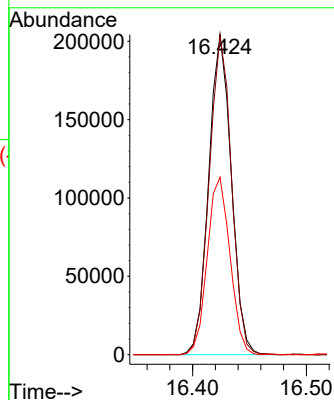

#69
Hexachlorobenzene
Concen: 20.204 ng/ul
RT: 16.547 min Scan# 2291
Delta R.T. 0.005 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:284 Resp: 307217
Ion Ratio Lower Upper
284 100
142 21.5 19.0 28.4
249 30.9 26.3 39.5

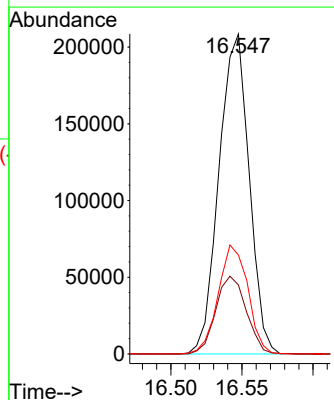



#70

Atrazine

Concen: 20.129 ng/ul

RT: 16.694 min Scan# 21

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:200 Resp: 274379

Ion Ratio Lower Upper

200 100

173 21.3 17.9 26.9

215 55.5 40.8 61.2



#71

Pentachlorophenol

Concen: 15.638 ng/ul

RT: 16.888 min Scan# 2349

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21




Tgt Ion:266 Resp: 147959


Ion Ratio Lower Upper

266 100

264 68.8 57.7 86.5

268 64.6 57.3 85.9

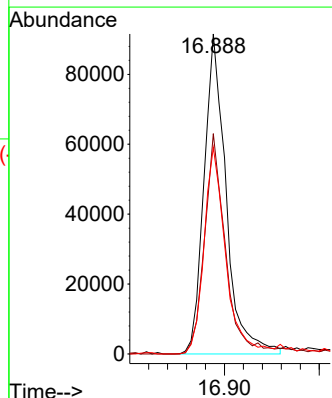



#72

Phenanthrene

Concen: 20.239 ng/ul

RT: 17.276 min Scan# 2414

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:178 Resp: 1160195

Ion Ratio Lower Upper

178 100

179 15.5 12.2 18.4

176 19.5 14.9 22.3



#74

Anthracene

Concen: 20.328 ng/ul

RT: 17.370 min Scan# 2431

Delta R.T. 0.005 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21




Tgt Ion:178 Resp: 1198301


Ion Ratio Lower Upper

178 100

179 15.4 12.1 18.1

176 18.9 14.1 21.1





#75

1,2,3,4-Tetrachlorobenzene

Concen: 19.854 ng/ul

RT: 13.281 min Scan# 1735

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:216 Resp: 315048

Ion Ratio Lower Upper

216 100

214 71.3 55.3 82.9

218 47.9 37.7 56.5

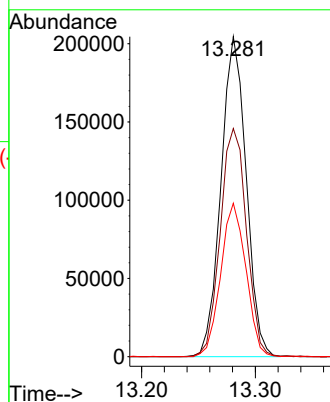

#76

Pentachlorobenzene

Concen: 20.233 ng/ul

RT: 14.808 min Scan# 1995

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21




Tgt Ion:250 Resp: 349815


Ion Ratio Lower Upper

250 100

248 57.7 52.7 79.1

252 62.1 47.5 71.3









#77
 Carbazole
 Concen: 20.436 ng/ul
 RT: 17.640 min Scan# 2476
 Delta R.T. -0.001 min
 Lab File: BG063116.D
 Acq: 28 Sep 2024 20:21




Instrument :
 BNA_G
 ClientSampleId :
 SSTD020515


Tgt Ion:167 Resp: 964056
 Ion Ratio Lower Upper
 167 100
 166 22.1 18.5 27.7
 139 11.8 9.7 14.5



#78
 Di-n-butylphthalate
 Concen: 20.409 ng/ul
 RT: 18.204 min Scan# 2573
 Delta R.T. 0.005 min
 Lab File: BG063116.D
 Acq: 28 Sep 2024 20:21

Tgt Ion:149 Resp: 1045548
 Ion Ratio Lower Upper
 149 100
 150 10.1 7.1 10.7
 104 4.9 4.3 6.5



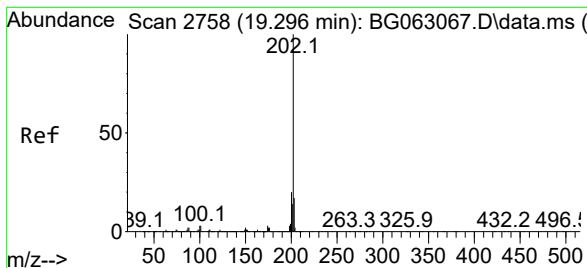

#80

Fluoranthene

Concen: 21.045 ng/ul

RT: 19.297 min Scan# 21

Delta R.T. 0.005 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:202 Resp: 1521335

Ion Ratio Lower Upper

202 100

101 4.1 2.7 4.1#

100 3.7 1.9 2.9#

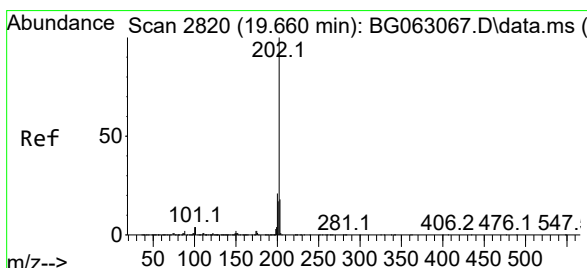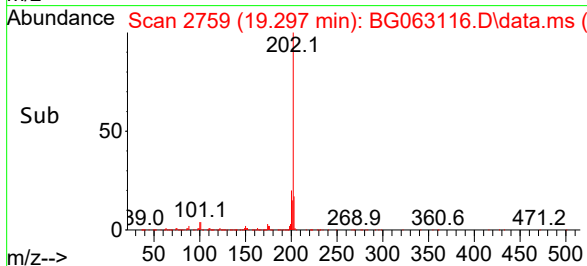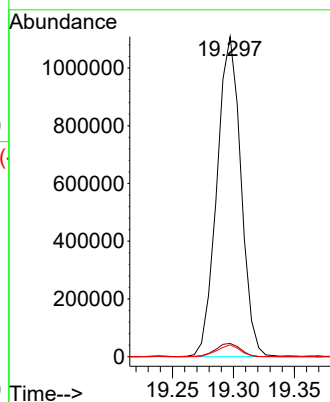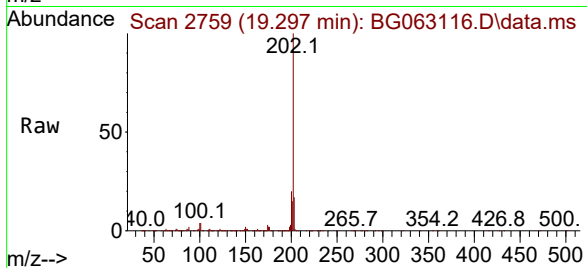

#82

Pyrene

Concen: 21.247 ng/ul

RT: 19.661 min Scan# 2821

Delta R.T. 0.005 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21




Tgt Ion:202 Resp: 1608890


Ion Ratio Lower Upper

202 100

101 4.9 3.1 4.7#

100 4.1 2.4 3.6#

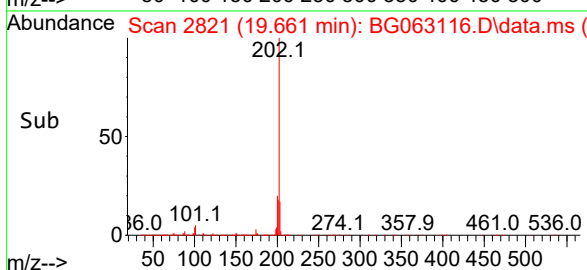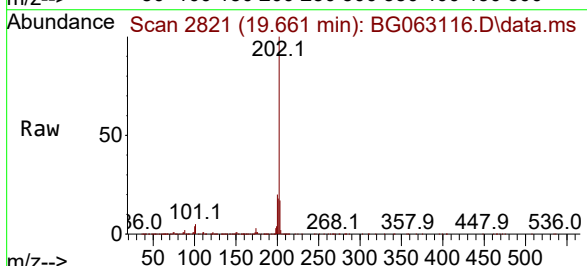



#83

Butylbenzylphthalate

Concen: 21.788 ng/ul

RT: 20.555 min Scan# 2972

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:149 Resp: 455382

Ion Ratio Lower Upper

149 100

91 55.9 42.2 63.2

206 26.6 24.4 36.6

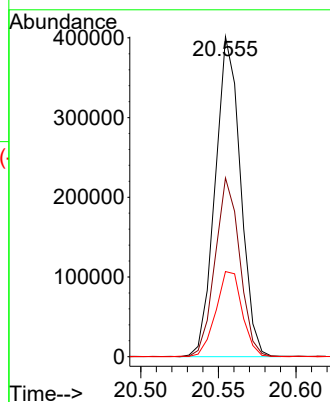

#84

3,3'-Dichlorobenzidine

Concen: 21.264 ng/ul

RT: 21.389 min Scan# 3115

Delta R.T. -0.001 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21




Tgt Ion:252 Resp: 575673


Ion Ratio Lower Upper

252 100

254 64.6 49.3 73.9

126 5.7 3.7 5.5#

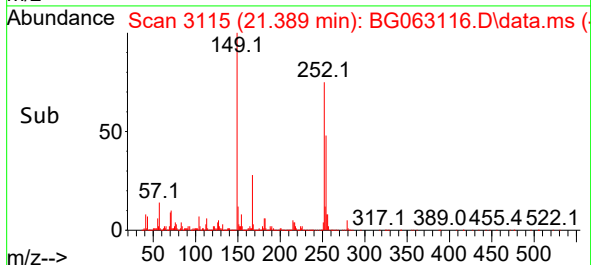



#85

Benzo(a)anthracene

Concen: 20.433 ng/ul

RT: 21.471 min Scan# 3128

Delta R.T. 0.005 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:228 Resp: 1625511

Ion Ratio Lower Upper

228 100

229 19.8 15.5 23.3

226 29.4 22.6 34.0



#86

Bis(2-ethylhexyl)phthalate

Concen: 21.571 ng/ul

RT: 21.389 min Scan# 3115

Delta R.T. 0.005 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21




Tgt Ion:149 Resp: 644695


Ion Ratio Lower Upper

149 100

167 28.0 20.8 31.2

279 5.4 4.4 6.6









#87
Chrysene
Concen: 20.469 ng/ul
RT: 21.536 min Scan# 3139
Delta R.T. 0.005 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21




Instrument :
BNA_G
ClientSampleId :
SSTD020515


Tgt Ion:228 Resp: 1511563
Ion Ratio Lower Upper
228 100
226 29.8 23.9 35.9
229 19.0 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 22.116 ng/ul
RT: 22.535 min Scan# 3310
Delta R.T. -0.001 min
Lab File: BG063116.D
Acq: 28 Sep 2024 20:21

Tgt Ion:149 Resp: 1094681

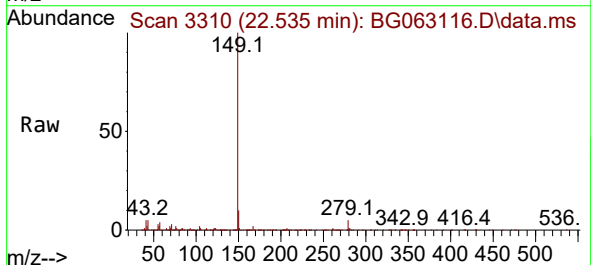



#90

Benzo(b)fluoranthene

Concen: 19.941 ng/ul

RT: 23.569 min Scan# 34

Delta R.T. 0.005 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:252 Resp: 1618765

Ion Ratio Lower Upper

252 100

253 20.9 17.9 26.9

125 3.9 2.7 4.1



#91

Benzo(k)fluoranthene

Concen: 20.282 ng/ul

RT: 23.633 min Scan# 3497

Delta R.T. 0.005 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21




Tgt Ion:252 Resp: 1635623


Ion Ratio Lower Upper

252 100

253 21.3 17.7 26.5

125 4.4 2.6 3.8#





#93

Benzo(a)pyrene

Concen: 19.987 ng/ul

RT: 24.385 min Scan# 3

Delta R.T. 0.005 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:252 Resp: 1485045

Ion Ratio Lower Upper

252 100

253 22.7 16.7 25.1

125 4.1 2.6 3.8#



#94

Indeno(1,2,3-cd)pyrene

Concen: 20.594 ng/ul

RT: 27.958 min Scan# 4233

Delta R.T. 0.016 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21




Tgt Ion:276 Resp: 1883877


Ion Ratio Lower Upper

276 100

138 9.1 5.7 8.5#

277 23.9 16.9 25.3



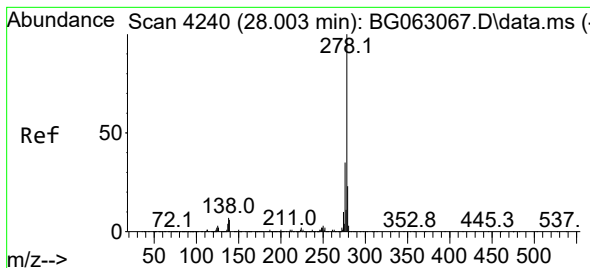

#95

Dibenzo(a,h)anthracene

Concen: 20.516 ng/ul

RT: 28.011 min Scan# 41

Delta R.T. 0.010 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Instrument :

BNA_G

ClientSampleId :

SSTD020515





Tgt Ion:278 Resp: 1529408

Ion Ratio Lower Upper

278 100

139 7.0 4.5 6.7#

279 23.1 18.6 28.0

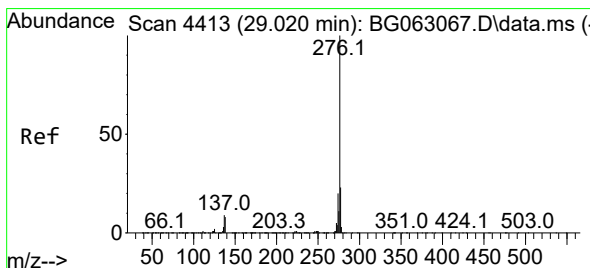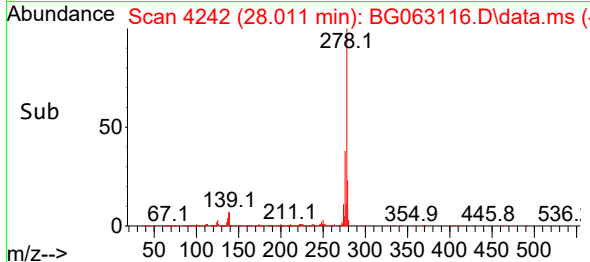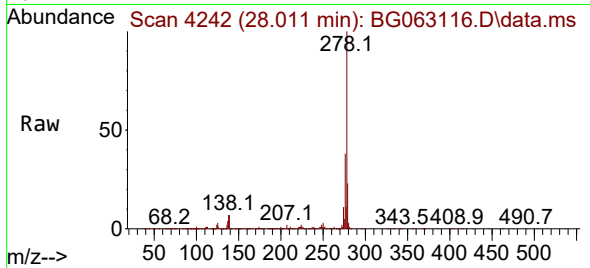

#96

Benzo(g,h,i)perylene

Concen: 20.237 ng/ul

RT: 29.027 min Scan# 4415

Delta R.T. 0.010 min

Lab File: BG063116.D

Acq: 28 Sep 2024 20:21

Tgt Ion:276 Resp: 1402001

Ion Ratio Lower Upper

276 100

138 8.4 5.6 8.4

277 23.0 19.2 28.8

