

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
 Data File : BG063095.D
 Acq On : 28 Sep 2024 5:41
 Operator : RC/JU
 Sample : P3927-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DDC80

Quant Time: Sep 28 06:17:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 25 13:16:45 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.847	152	76251	20.000	ng/u1	0.00
20) Naphthalene-d8	10.637	136	343370	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.486	164	314276	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.236	188	792338	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.489	240	820995	20.000	ng/u1	# 0.00
88) Perylene-d12	24.521	264	962537	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	3652	2.761	ng/uL	0.00
4) Pyridine-d5	3.722	84	56680	17.525	ng/u1	0.00
7) Phenol-d5	7.018	99	82482	17.513	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.177	67	31978	17.380	ng/u1	0.00
11) 2-Chlorophenol-d4	7.382	132	75792	16.379	ng/u1	0.00
15) 4-Methylphenol-d8	8.557	113	78193	18.391	ng/u1	0.00
21) Nitrobenzene-d5	8.998	128	39999	15.842	ng/u1	0.00
24) 2-Nitrophenol-d4	9.727	143	53485	16.586	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.261	165	113590	16.878	ng/u1	0.00
31) 4-Chloroaniline-d4	10.773	131	124175	15.724	ng/u1	0.00
46) Dimethylphthalate-d6	13.892	166	450060	18.011	ng/u1	0.00
49) Acenaphthylene-d8	14.174	160	467956	17.672	ng/u1	0.00
54) 4-Nitrophenol-d4	14.691	143	58069	15.408	ng/u1	0.00
60) Fluorene-d10	15.479	176	415721	18.157	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.602	200	78558	14.187	ng/u1	0.00
73) Anthracene-d10	17.335	188	739056	19.442	ng/u1	0.00
81) Pyrene-d10	19.627	212	929054	20.097	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.315	264	991247	19.228	ng/u1	0.00
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.114	232	117599	14.260	ng/u1	96
71) Pentachlorophenol	16.907	266	3612480	535.844	ng/u1	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
Data File : BG063095.D
Acq On : 28 Sep 2024 5:41
Operator : RC/JU
Sample : P3927-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DDC80

Quant Time: Sep 28 06:17:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 25 13:16:45 2024
Response via : Initial Calibration

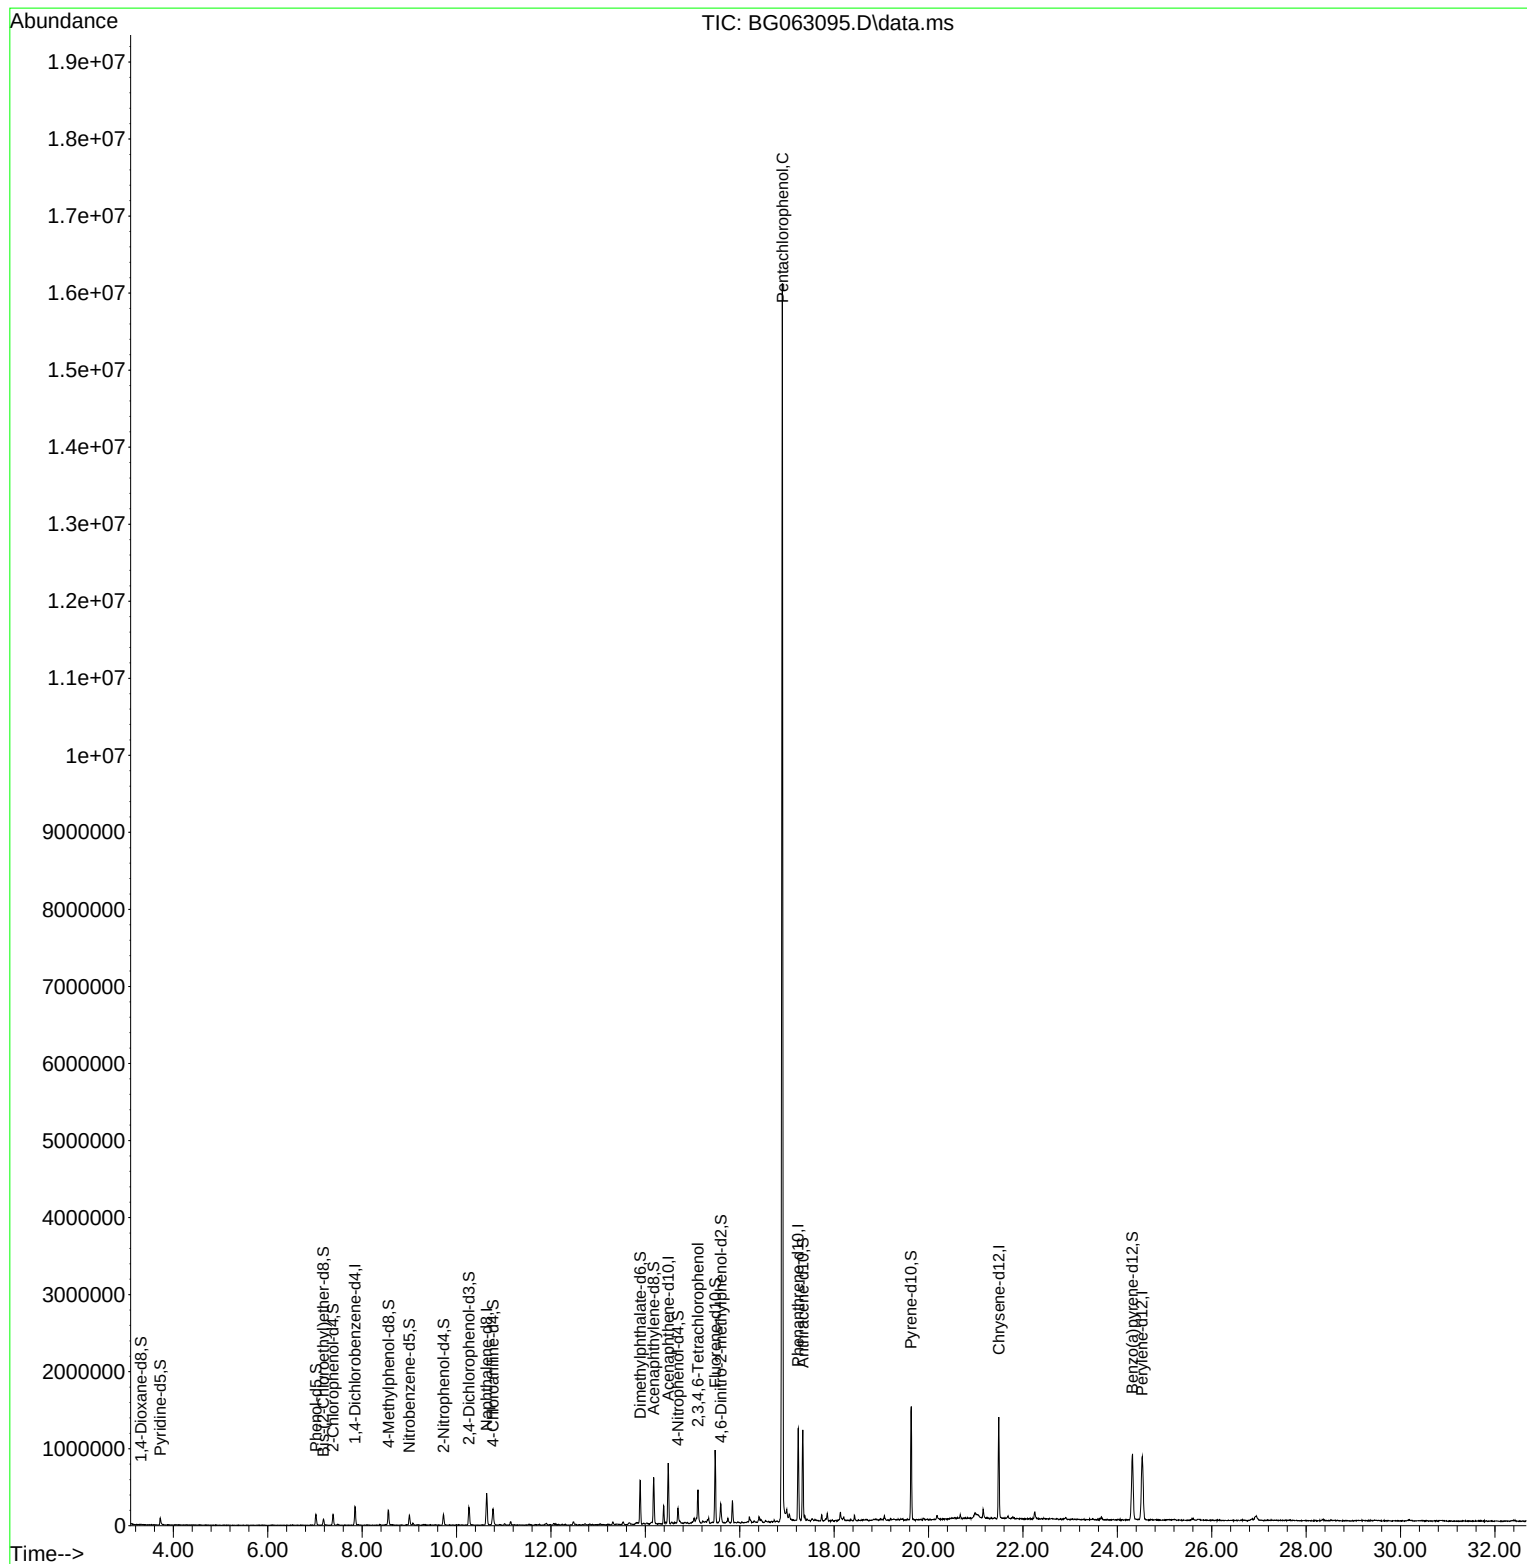




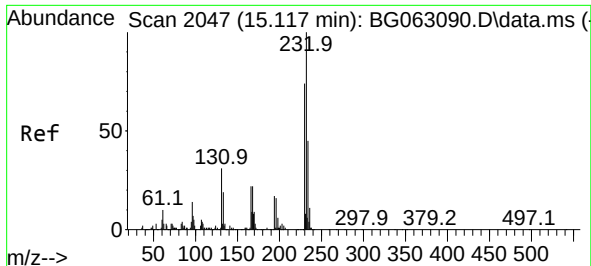


#58
2,3,4,6-Tetrachlorophenol
Concen: 14.260 ng/ul
RT: 15.114 min Scan# 2047
Delta R.T. -0.001 min
Lab File: BG063095.D
Acq: 28 Sep 2024 5:41

Instrument :
BNA_G
ClientSampleId :
DDC80

Tgt Ion:232 Resp: 117599

Ion	Ratio	Lower	Upper
232	100		
131	28.8	25.8	38.6
130	1.9	1.9	2.9
166	21.2	17.6	26.4

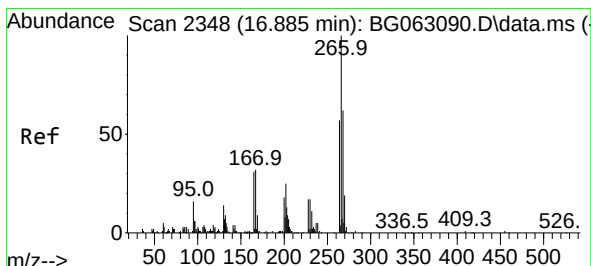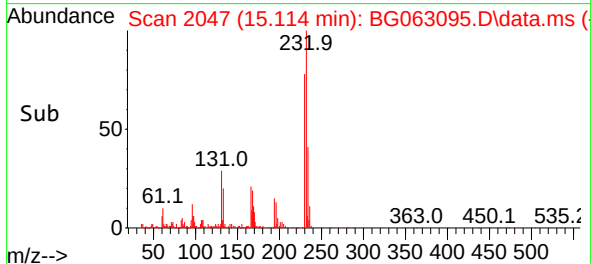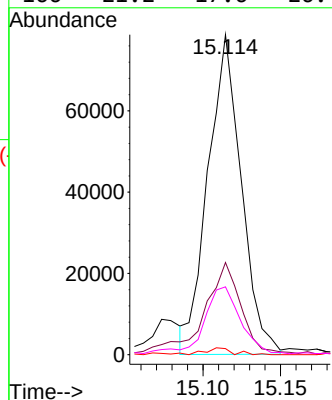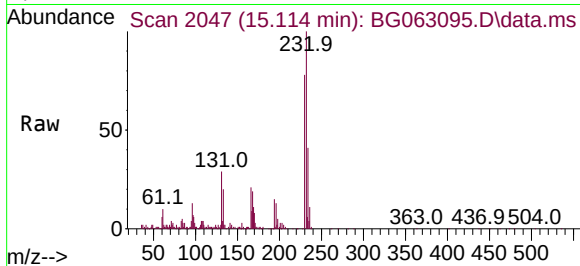

#71
Pentachlorophenol
Concen: 535.844 ng/ul
RT: 16.907 min Scan# 2352
Delta R.T. 0.017 min
Lab File: BG063095.D
Acq: 28 Sep 2024 5:41

Tgt Ion:266 Resp: 3612480

Ion	Ratio	Lower	Upper
266	100		
264	65.9	57.7	86.5
268	67.3	57.3	85.9

