

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
 Data File : BG063076.D
 Acq On : 27 Sep 2024 16:30
 Operator : RC/JU
 Sample : PB163375BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK375

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.320	36	39	41	rVB2	8798	8837	0.23%	0.030%
2	3.720	104	107	116	rBV	157245	252873	6.58%	0.871%
3	4.196	185	188	192	rBV4	6010	8710	0.23%	0.030%
4	4.472	233	235	239	rBV3	5736	6307	0.16%	0.022%
5	4.865	300	302	306	rVB3	4635	5745	0.15%	0.020%
6	5.371	384	388	391	rBV3	3656	8109	0.21%	0.028%
7	7.016	663	668	677	rBV2	222179	387137	10.08%	1.334%
8	7.180	691	696	703	rBV	160870	250999	6.54%	0.865%
9	7.245	705	707	712	rVB2	4516	5556	0.14%	0.019%
10	7.292	712	715	717	rBV2	5231	5355	0.14%	0.018%
11	7.380	724	730	737	rBV	253674	428883	11.17%	1.478%
12	7.645	771	775	778	rBV2	5565	7316	0.19%	0.025%
13	7.850	801	810	822	rBV	245321	416543	10.85%	1.435%
14	8.167	860	864	867	rBV	3920	6478	0.17%	0.022%
15	8.555	924	930	937	rBV2	320507	541798	14.11%	1.867%
16	9.002	998	1006	1013	rBV2	225069	403486	10.51%	1.390%
17	9.724	1122	1129	1138	rBV2	210546	396086	10.31%	1.365%
18	10.265	1213	1221	1235	rBV	375989	700493	18.24%	2.413%
19	10.641	1277	1285	1294	rBV	343809	616357	16.05%	2.124%
20	10.776	1300	1308	1316	rBV	325604	611250	15.92%	2.106%
21	10.999	1342	1346	1351	rVB	4090	6375	0.17%	0.022%
22	11.922	1500	1503	1506	rBV2	5595	7779	0.20%	0.027%
23	12.175	1544	1546	1550	rVB2	4837	5216	0.14%	0.018%
24	12.245	1550	1558	1566	rBV3	6733	22027	0.57%	0.076%
25	12.686	1627	1633	1634	rBV	4716	6389	0.17%	0.022%
26	12.962	1678	1680	1682	rBV	6472	6874	0.18%	0.024%
27	13.273	1732	1733	1736	rBV2	4885	5300	0.14%	0.018%
28	13.367	1746	1749	1751	rBV2	7385	6477	0.17%	0.022%
29	13.890	1832	1838	1848	rVB	848072	1232226	32.08%	4.245%
30	14.178	1879	1887	1894	rBV	925547	1458408	37.97%	5.025%
31	14.284	1902	1905	1909	rVB3	4339	5348	0.14%	0.018%
32	14.348	1912	1916	1920	rBV3	4799	6358	0.17%	0.022%
33	14.484	1932	1939	1946	rBV	717304	1123783	29.26%	3.872%
34	14.689	1969	1974	1984	rBV	274896	478489	12.46%	1.649%
35	15.112	2044	2046	2050	rBV2	4324	5821	0.15%	0.020%
36	15.482	2102	2109	2116	rBV	1391093	2092407	54.48%	7.209%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
 Data File : BG063076.D
 Acq On : 27 Sep 2024 16:30
 Operator : RC/JU
 Sample : PB163375BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK375

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
 Title : SVOA CALIBRATION

37	15.600	2123	2129	2139	rBV	321521	503834	13.12%	1.736%
38	15.712	2146	2148	2154	rBV4	7397	11540	0.30%	0.040%
39	15.853	2168	2172	2174	rVB2	4463	5970	0.16%	0.021%
40	15.876	2174	2176	2179	rVB	5660	6048	0.16%	0.021%
41	16.158	2222	2224	2227	rBV2	4754	5335	0.14%	0.018%
42	16.264	2238	2242	2247	rVB4	7753	13593	0.35%	0.047%
43	16.599	2297	2299	2302	rVB2	5936	5202	0.14%	0.018%
44	16.816	2332	2336	2338	rBV2	4811	5174	0.13%	0.018%
45	16.916	2351	2353	2359	rVB5	5325	6767	0.18%	0.023%
46	17.022	2367	2371	2374	rBV4	5382	9189	0.24%	0.032%
47	17.233	2401	2407	2417	rVB	1198476	1789883	46.60%	6.167%
48	17.333	2417	2424	2436	rBV	1834940	2703053	70.38%	9.313%
49	17.574	2463	2465	2468	rBV2	5087	6575	0.17%	0.023%
50	17.797	2500	2503	2505	rVB2	6589	6626	0.17%	0.023%
51	17.903	2518	2521	2524	rBV4	5775	7897	0.21%	0.027%
52	19.196	2737	2741	2746	rVB4	28655	35921	0.94%	0.124%
53	19.266	2750	2753	2759	rVB	27127	33444	0.87%	0.115%
54	19.560	2799	2803	2808	rBV7	9057	22005	0.57%	0.076%
55	19.630	2808	2815	2822	rBV	2679275	3623401	94.34%	12.484%
56	21.487	3125	3131	3141	rVB2	1508824	2346455	61.10%	8.084%
57	24.319	3603	3613	3627	rVB2	1447886	3840615	100.00%	13.232%
58	24.531	3639	3649	3662	rVB	932069	2499165	65.07%	8.610%




Sum of corrected areas: 29025287

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
Data File : BG063076.D
Acq On : 27 Sep 2024 16:30
Operator : RC/JU
Sample : PB163375BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK375

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

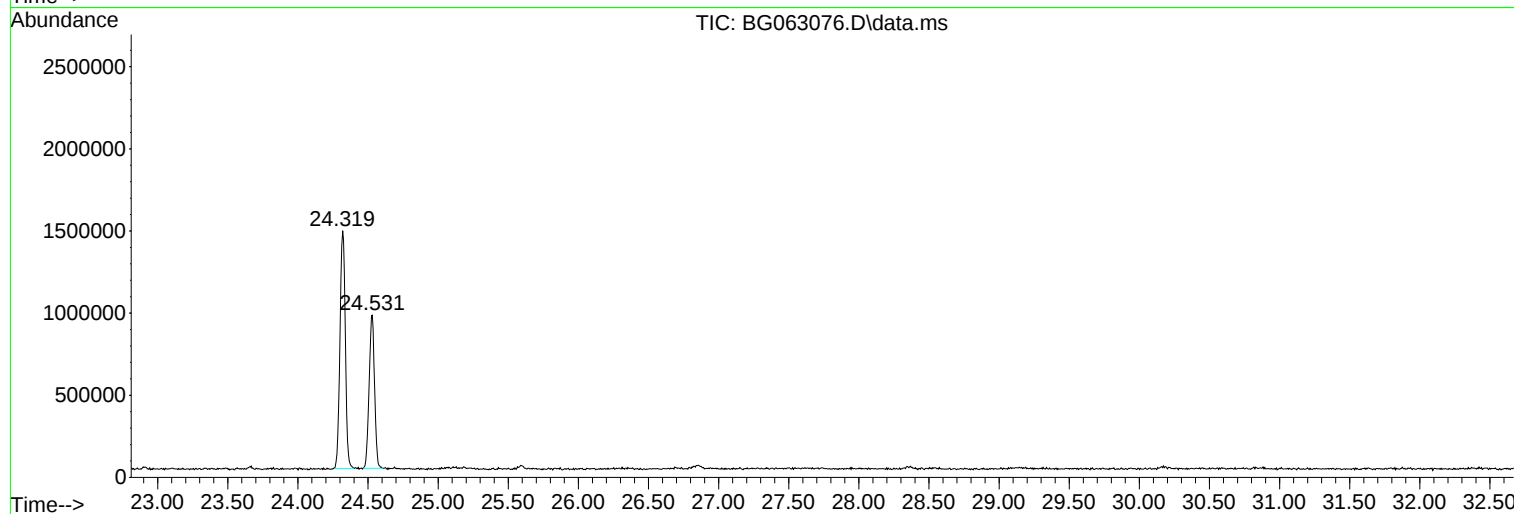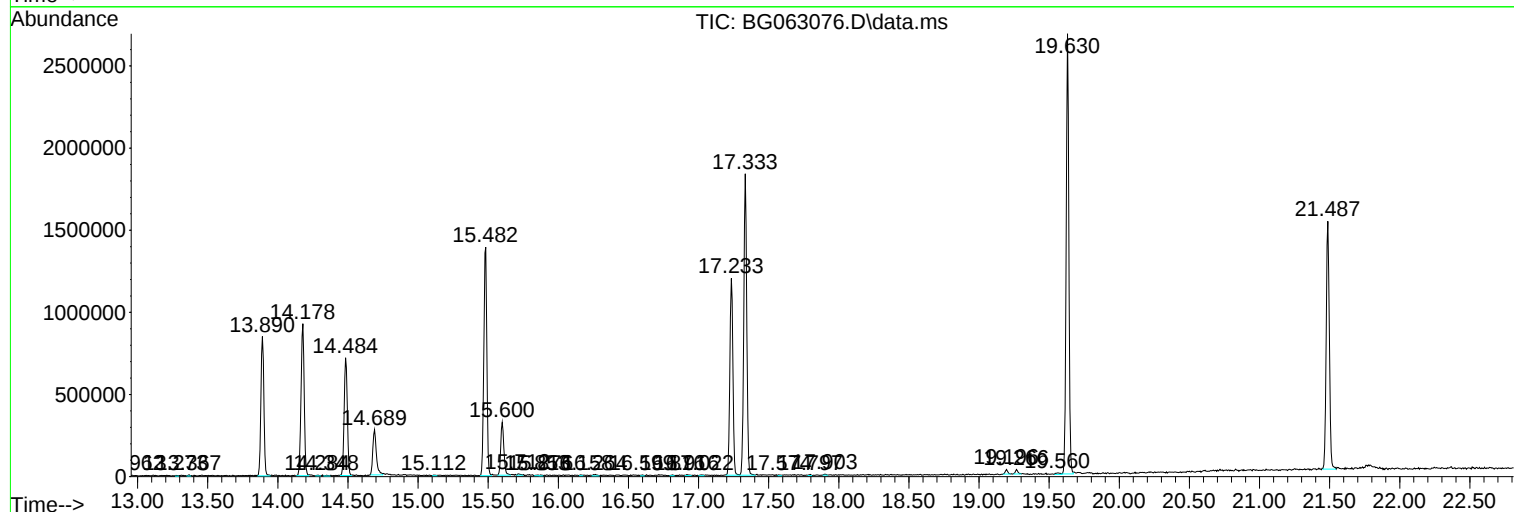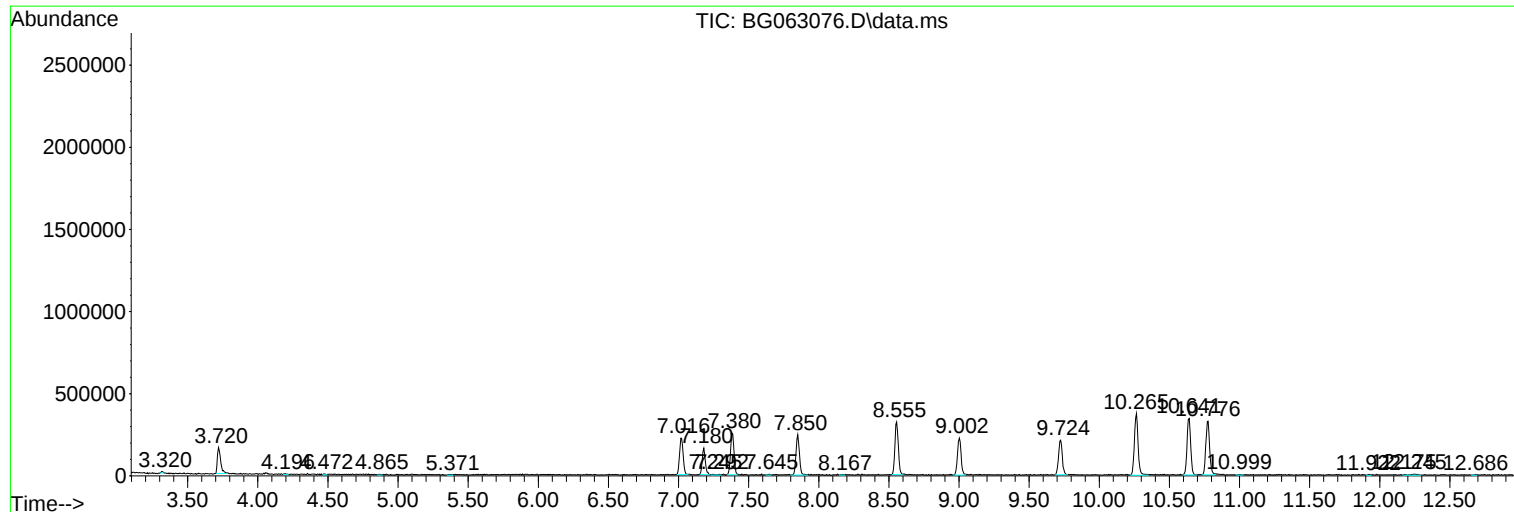

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
Data File : BG063076.D
Acq On : 27 Sep 2024 16:30
Operator : RC/JU
Sample : PB163375BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK375

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092724\
Data File : BG063076.D
Acq On : 27 Sep 2024 16:30
Operator : RC/JU
Sample : PB163375BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK375

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG092524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------